

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051121\
 Data File : P0077731.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2021 6:43
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 5/13/2021 10:49:42 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 13:32:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 15:14:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.645	1392717	447730	20.062	26.628 #
2) SA Decachlor...	9.989	8.847	1116246	581330	21.245	32.963m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051121\
Data File : P0077731.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2021 6:43
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
5/13/2021 10:49:42 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 13:32:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 15:14:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

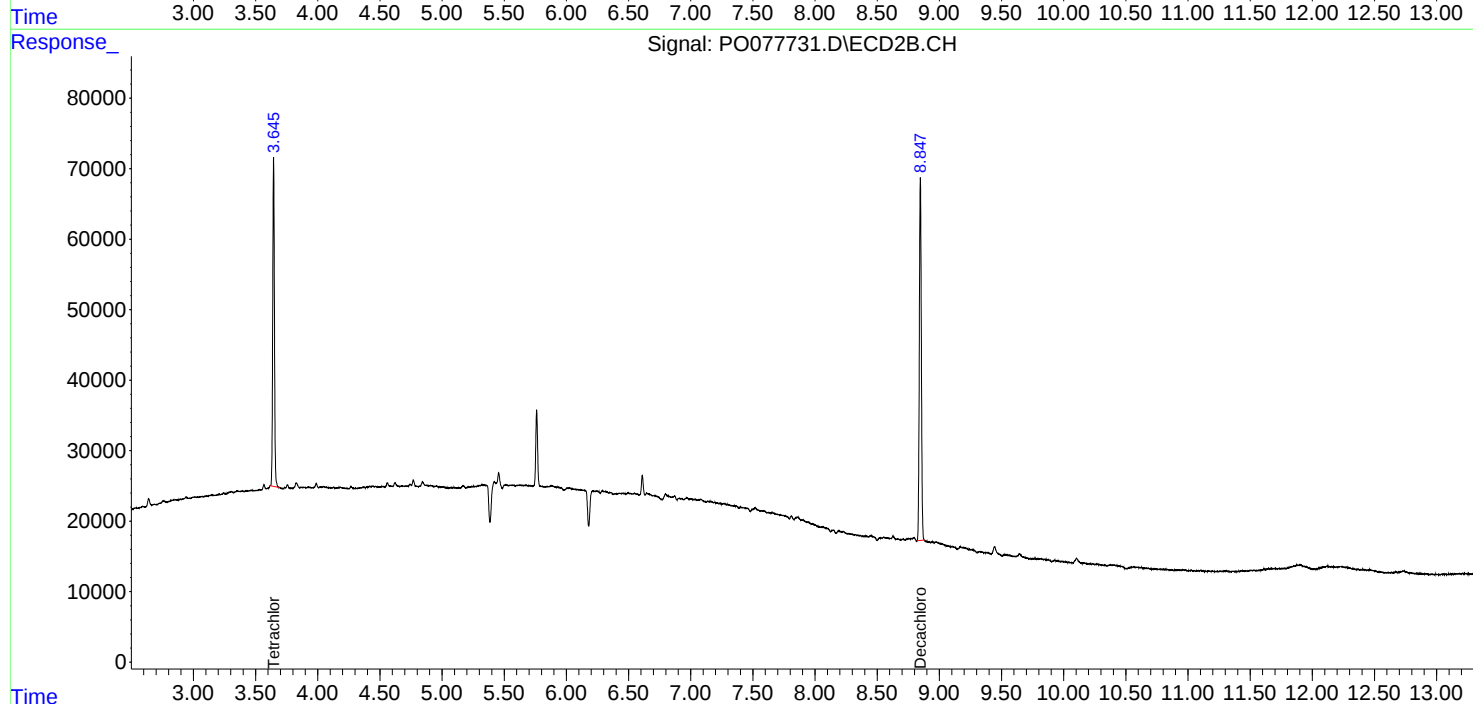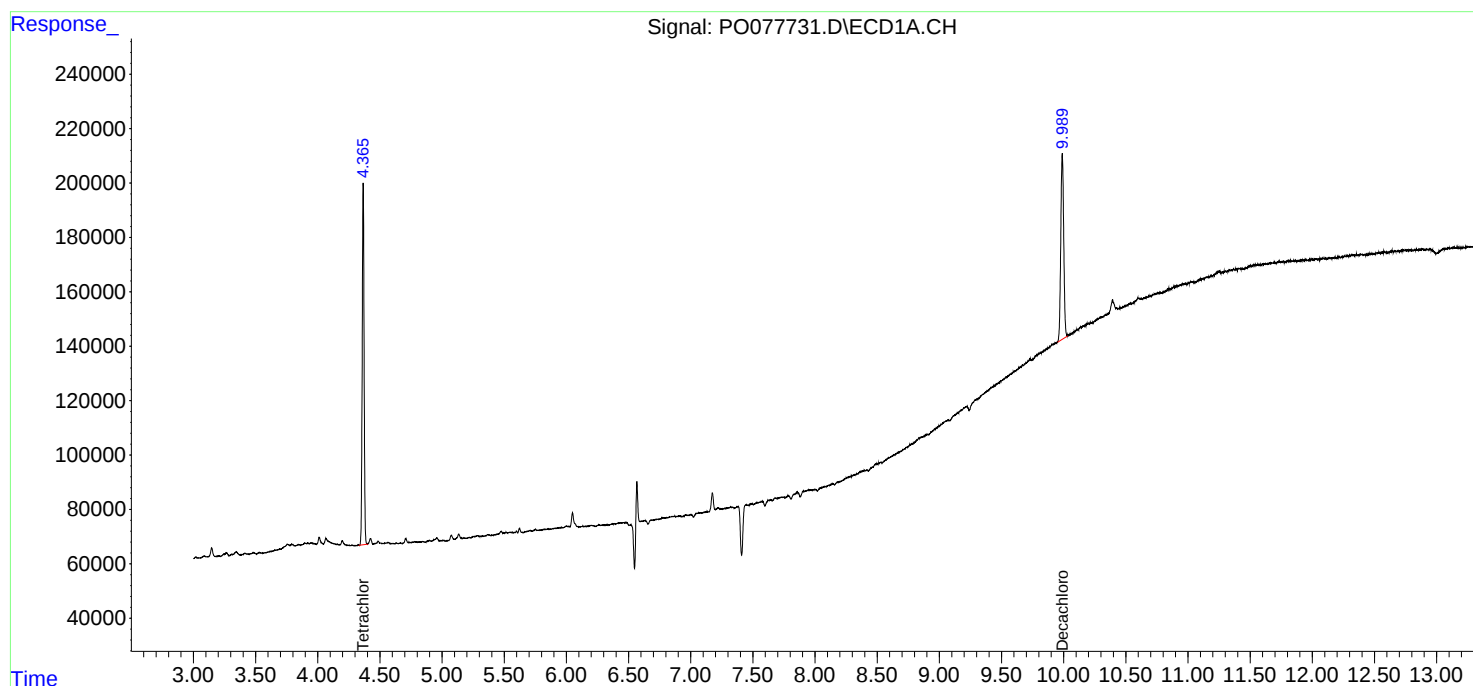

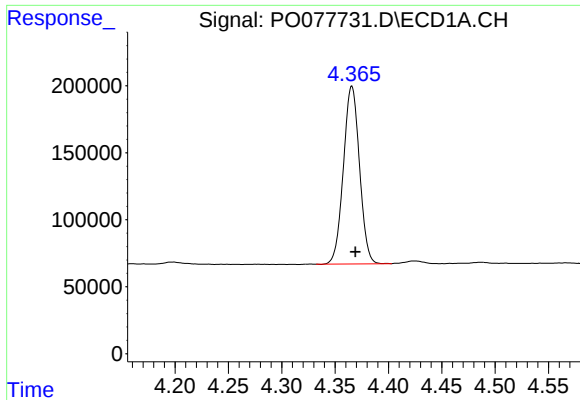


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.003 min
Response: 1392717
Conc: 20.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
5/13/2021 10:49:42 AM

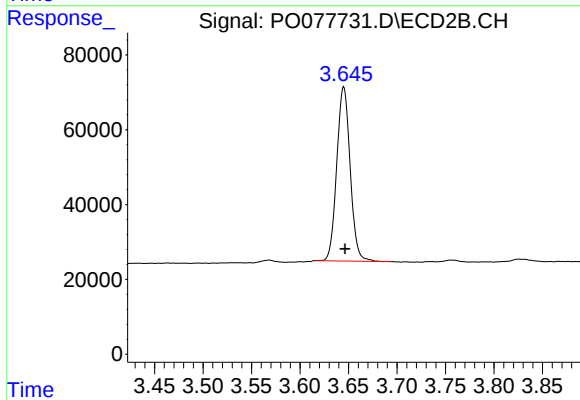


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.001 min
Response: 447730
Conc: 26.63 ng/ml

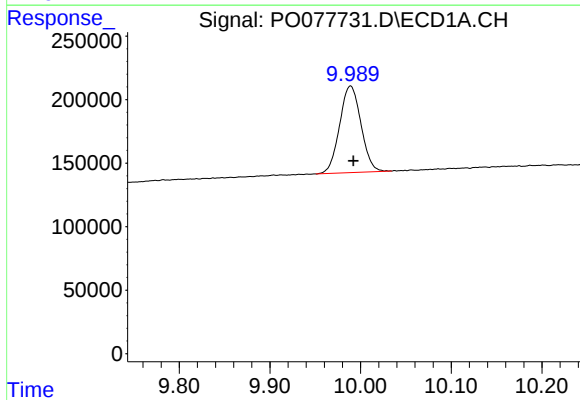

#2 Decachlorobiphenyl

R.T.: 9.989 min
Delta R.T.: -0.003 min
Response: 1116246
Conc: 21.24 ng/ml

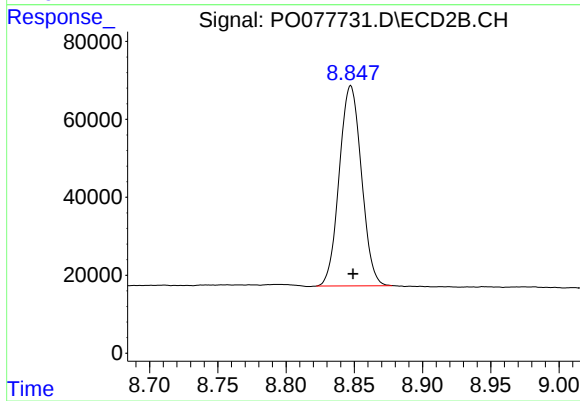

#2 Decachlorobiphenyl

R.T.: 8.847 min
Delta R.T.: -0.002 min
Response: 581330
Conc: 32.96 ng/ml m