

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051121\
 Data File : P0077739.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2021 9:01
 Operator : DD\AJ
 Sample : M2262-08
 Misc : AR1262 LOQ 50 PPB
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 LOQ-WATER-02-QT2-2021

Manual Integrations
 APPROVED

Ankita
 5/13/2021 10:49:46 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 13:38:34 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051121.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue May 11 15:14:32 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.366	3.645	1107949	373644	15.960	22.222 #
2) SA Decachlor...	9.989	8.847	905498	492589	17.234	27.931 #
Target Compounds						
36) L8 AR-1262-1	7.948	6.970	189401	46431	49.384	71.862 #
37) L8 AR-1262-2	8.487	7.518	304698	154260	44.262	69.710 #
38) L8 AR-1262-3	8.758	7.801	196516	63327	44.068m	70.774 #
39) L8 AR-1262-4	8.837	7.864	152216	117739	46.655	70.594 #
40) L8 AR-1262-5	9.390	8.359	89280	55118	38.474	68.445 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051121\
Data File : PO077739.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2021 9:01
Operator : DD\AJ
Sample : M2262-08
Misc : AR1262 LOQ 50 PPB
ALS Vial : 54 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
LOQ-WATER-02-QT2-2021


Manual Integrations
APPROVED

Ankita
5/13/2021 10:49:46 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 13:38:34 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051121.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue May 11 15:14:32 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

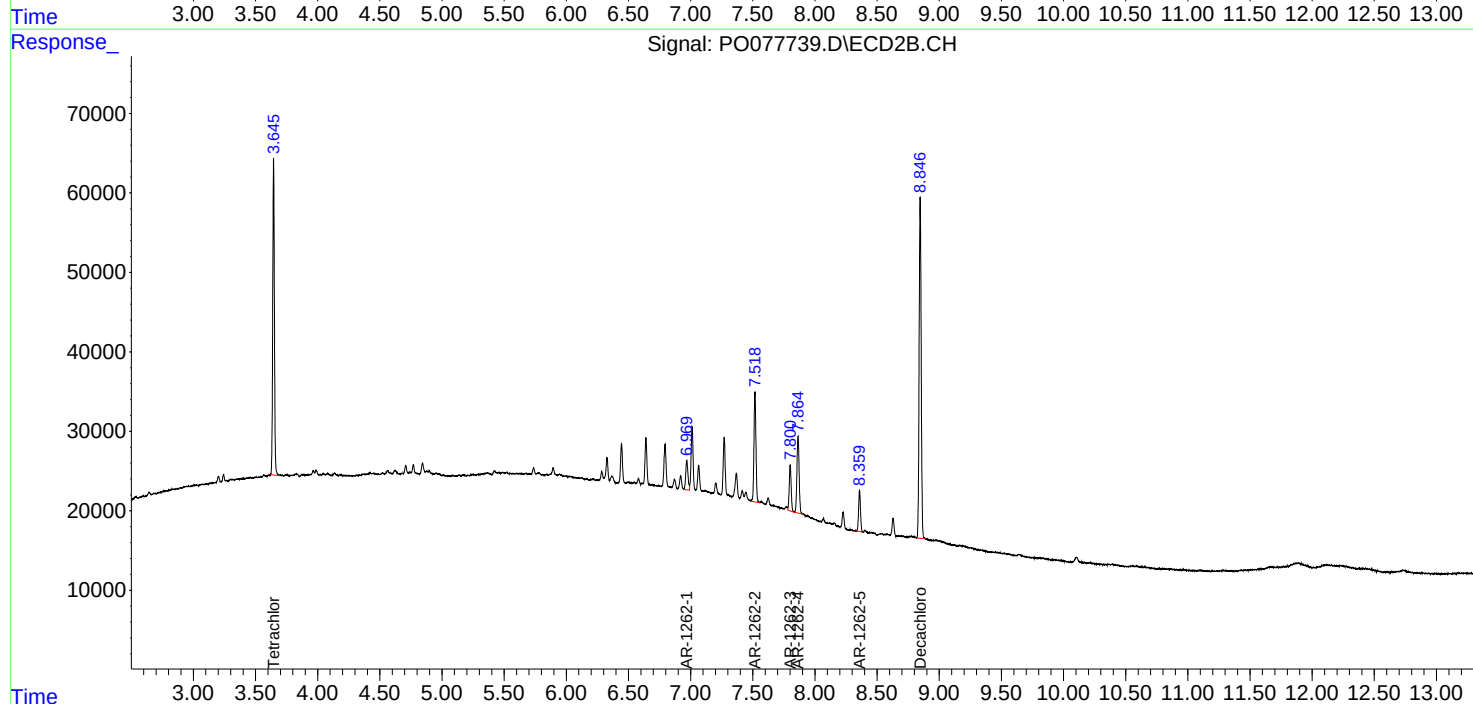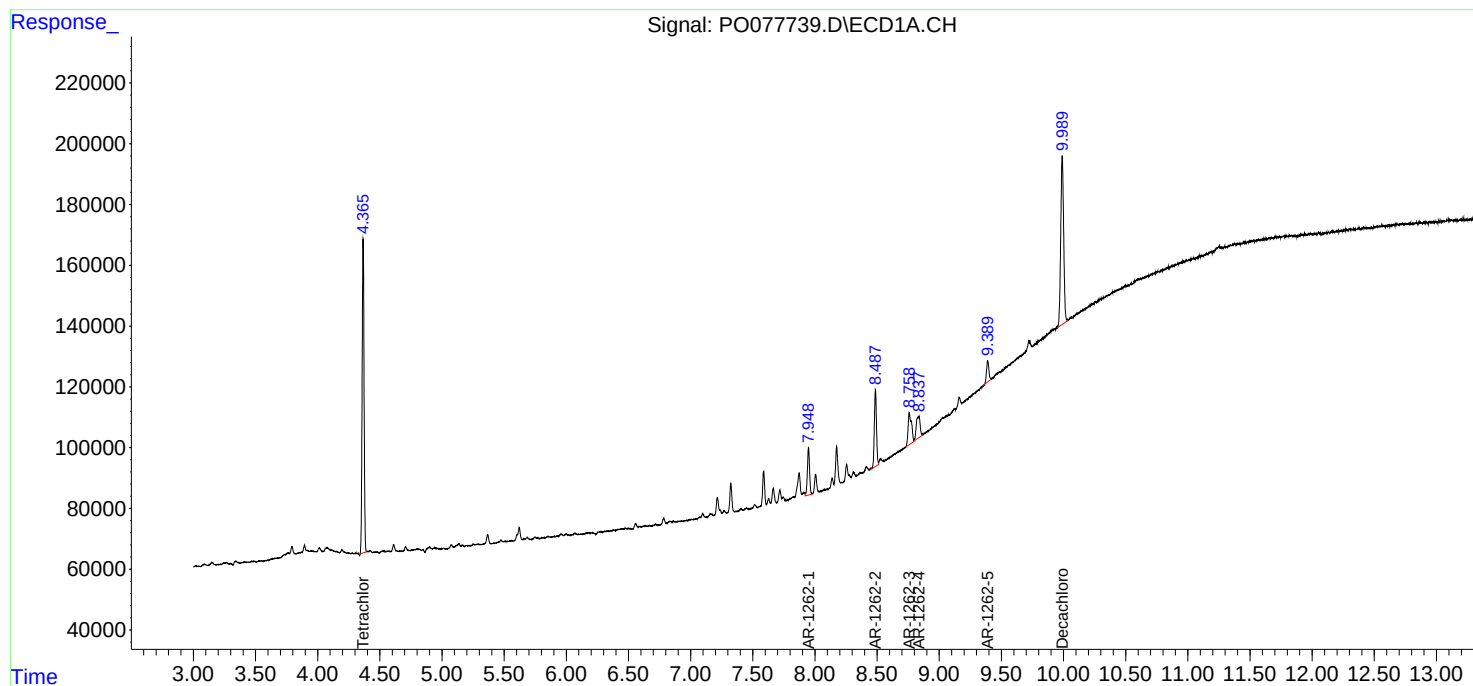

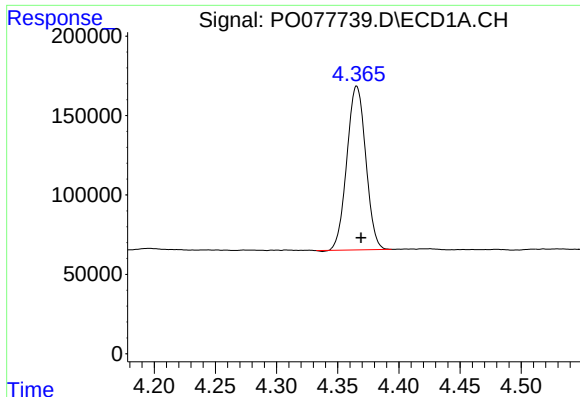


#1 Tetrachloro-m-xylene

R.T.: 4.366 min
Delta R.T.: -0.003 min
Response: 1107949
Conc: 15.96 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT2-2021


Manual Integrations
APPROVED

Ankita
5/13/2021 10:49:46 AM

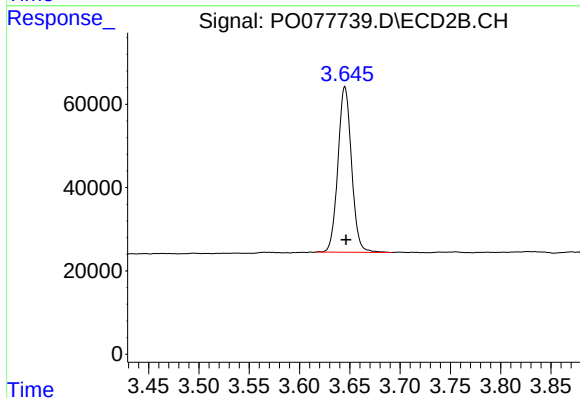


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.001 min
Response: 373644
Conc: 22.22 ng/ml

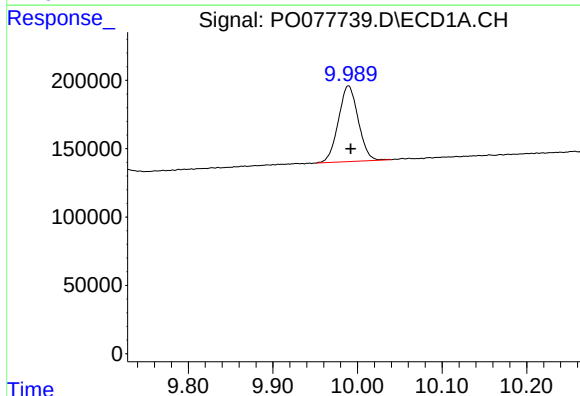


#2 Decachlorobiphenyl

R.T.: 9.989 min
Delta R.T.: -0.003 min
Response: 905498
Conc: 17.23 ng/ml

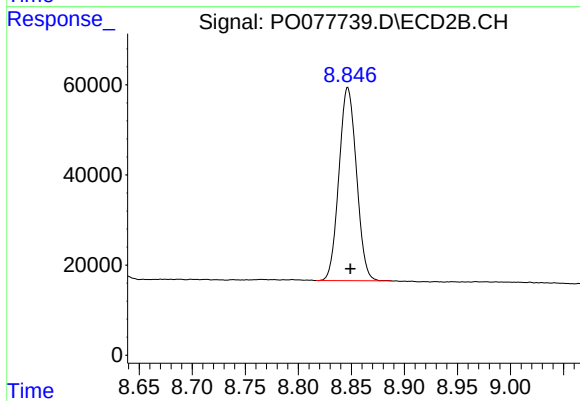

#2 Decachlorobiphenyl

R.T.: 8.847 min
Delta R.T.: -0.002 min
Response: 492589
Conc: 27.93 ng/ml

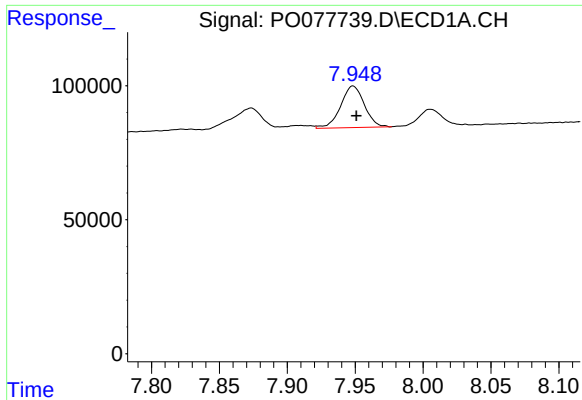


#36 AR-1262-1

R.T.: 7.948 min
Delta R.T.: -0.003 min
Response: 189401
Conc: 49.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT2-2021


Manual Integrations
APPROVED

Ankita
5/13/2021 10:49:46 AM

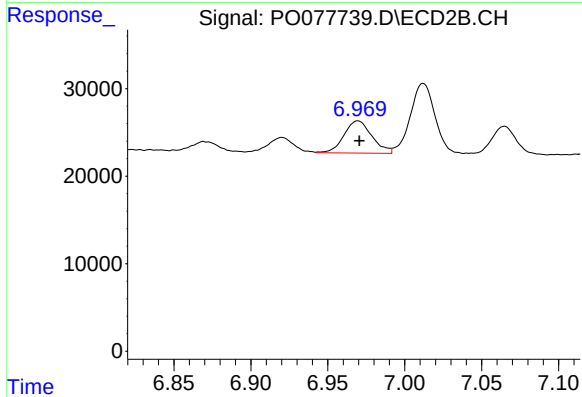


#36 AR-1262-1

R.T.: 6.970 min
Delta R.T.: 0.000 min
Response: 46431
Conc: 71.86 ng/ml

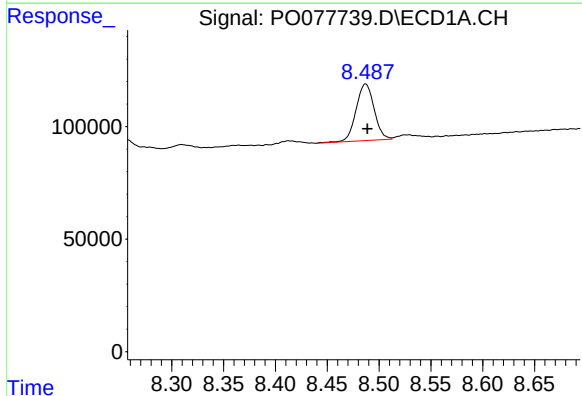


#37 AR-1262-2

R.T.: 8.487 min
Delta R.T.: -0.002 min
Response: 304698
Conc: 44.26 ng/ml

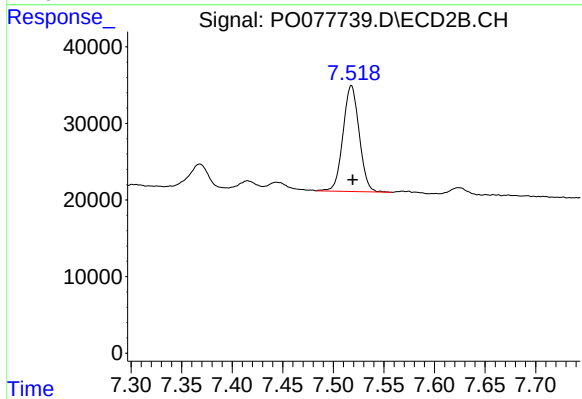

#37 AR-1262-2

R.T.: 7.518 min
Delta R.T.: -0.001 min
Response: 154260
Conc: 69.71 ng/ml

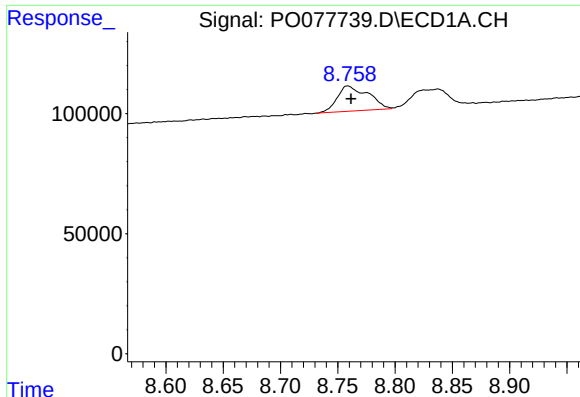


#38 AR-1262-3

R.T.: 8.758 min
Delta R.T.: -0.003 min
Response: 196516
Conc: 44.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT2-2021


Manual Integrations
APPROVED

Ankita
5/13/2021 10:49:46 AM

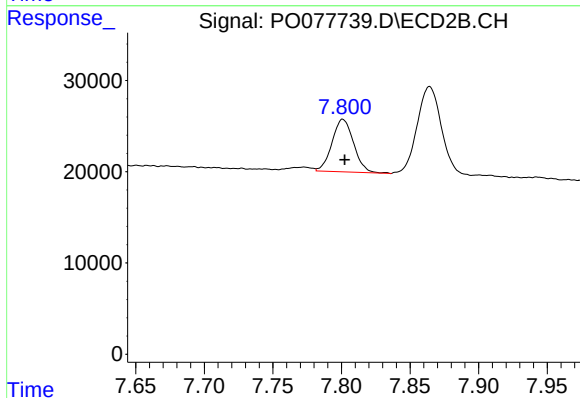


#38 AR-1262-3

R.T.: 7.801 min
Delta R.T.: -0.001 min
Response: 63327
Conc: 70.77 ng/ml

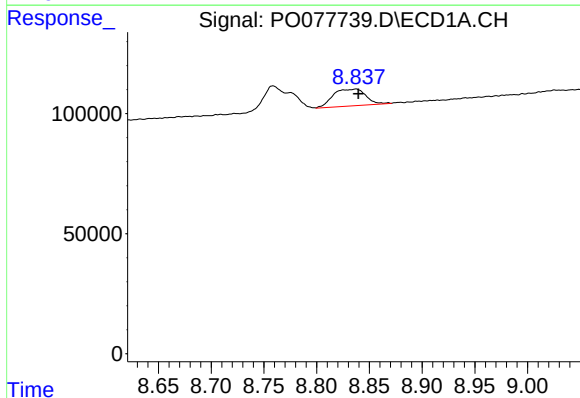


#39 AR-1262-4

R.T.: 8.837 min
Delta R.T.: -0.002 min
Response: 152216
Conc: 46.66 ng/ml

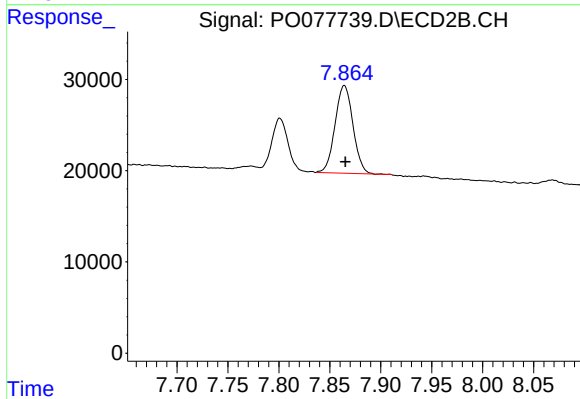

#39 AR-1262-4

R.T.: 7.864 min
Delta R.T.: 0.000 min
Response: 117739
Conc: 70.59 ng/ml

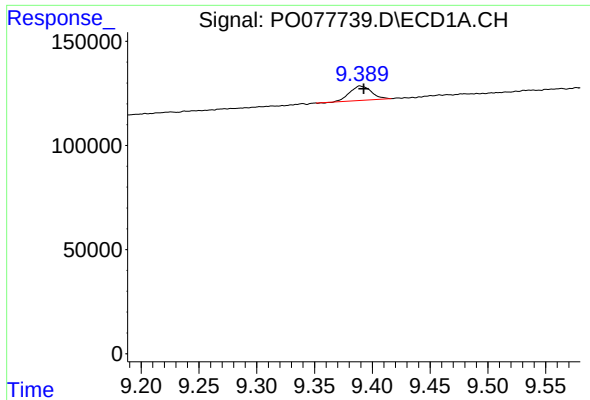


#40 AR-1262-5

R.T.: 9.390 min
Delta R.T.: -0.003 min
Response: 89280
Conc: 38.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
LOQ-WATER-02-QT2-2021

Manual Integrations
APPROVED

Ankita
5/13/2021 10:49:46 AM

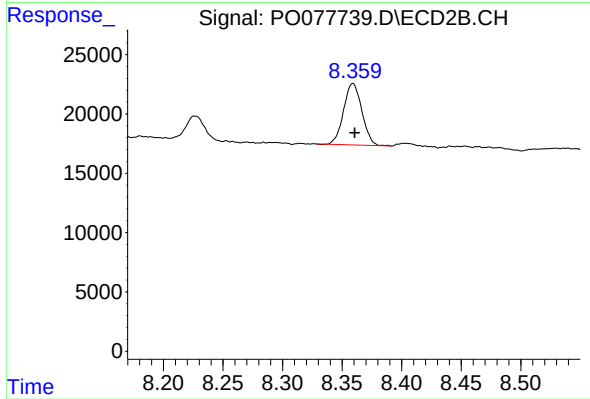

#40 AR-1262-5

R.T.: 8.359 min
Delta R.T.: -0.002 min
Response: 55118
Conc: 68.44 ng/ml