

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051123\
 Data File : P0094964.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 13:45
 Operator : YP/AJ
 Sample : 02692-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ERME-LIQUID-0509

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/12/2023
 Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 04:35:16 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.409	3.624	97022935	77328687	28.167m	57.792 #
2) SA Decachlor...	10.255	8.627	58036278	22795144	23.914	20.252

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051123\
Data File : PO094964.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 13:45
Operator : YP/AJ
Sample : 02692-03
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
ERME-LIQUID-0509


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/12/2023
Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 04:35:16 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

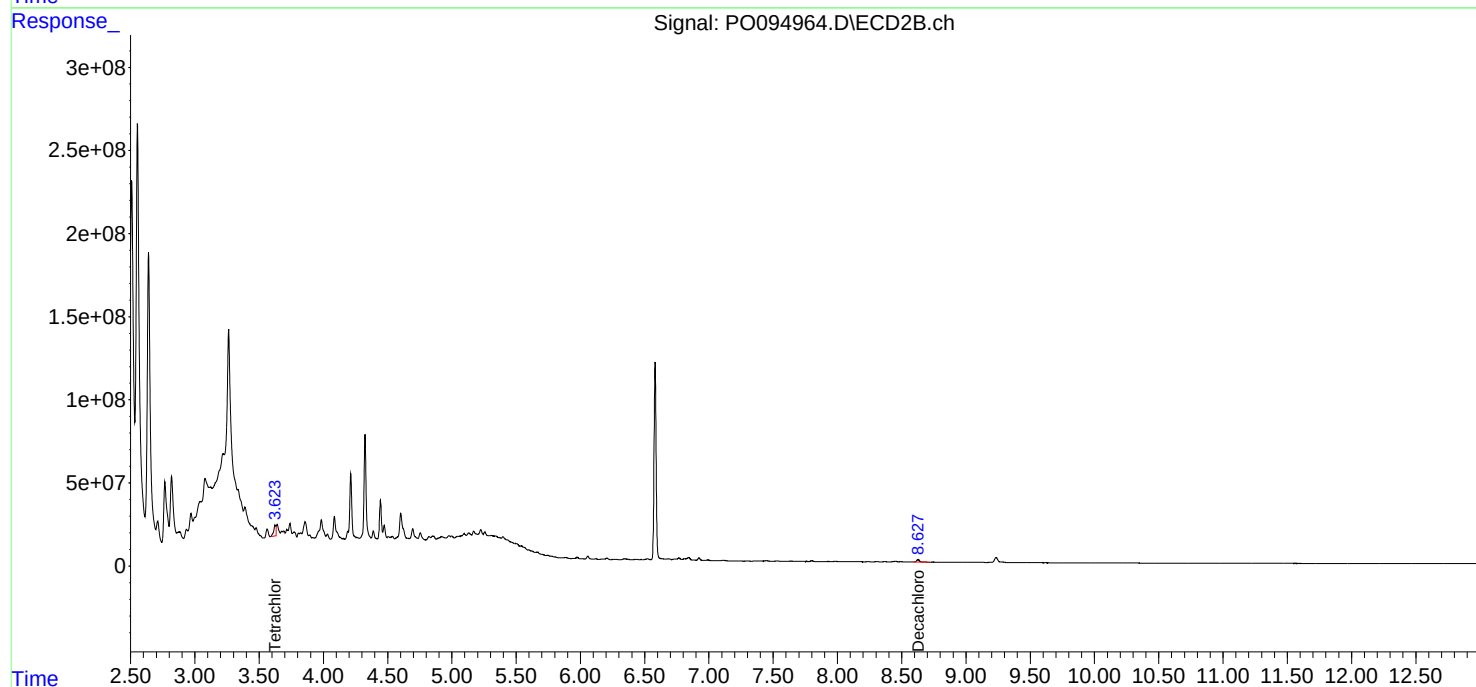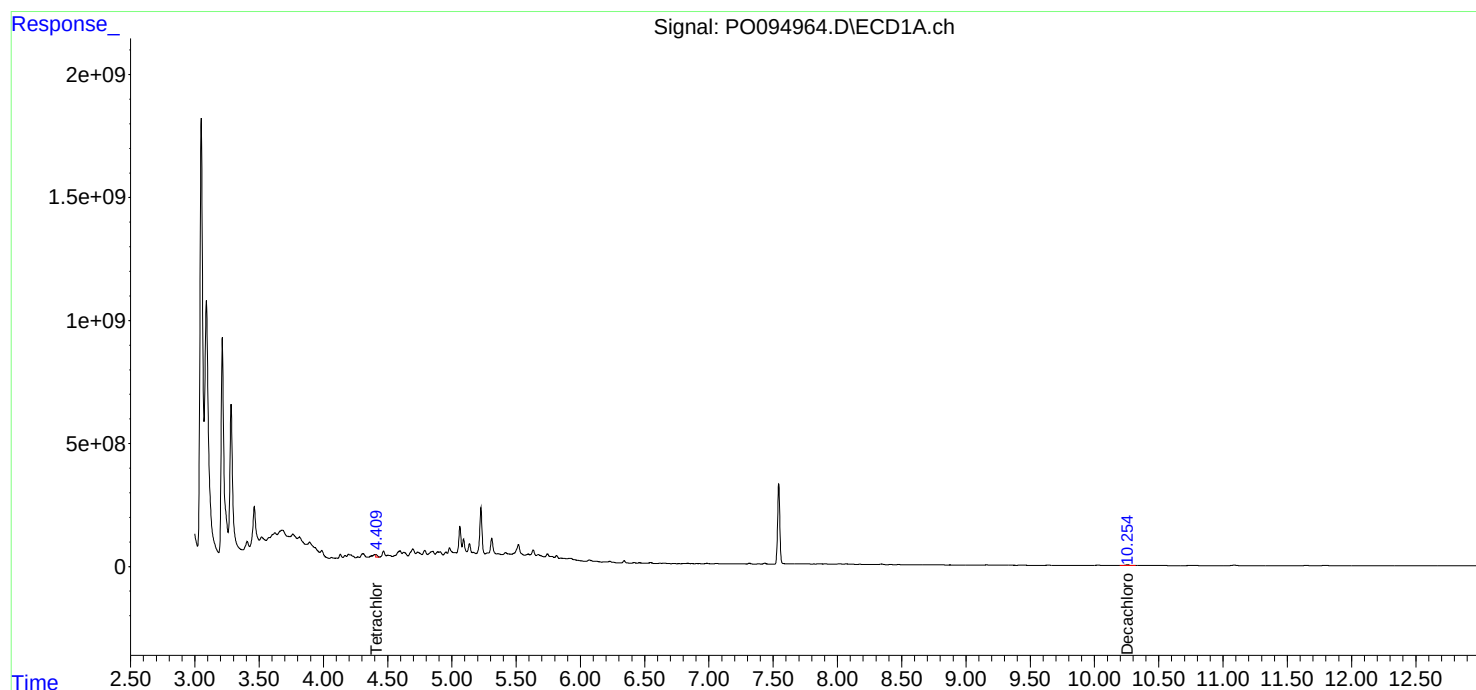

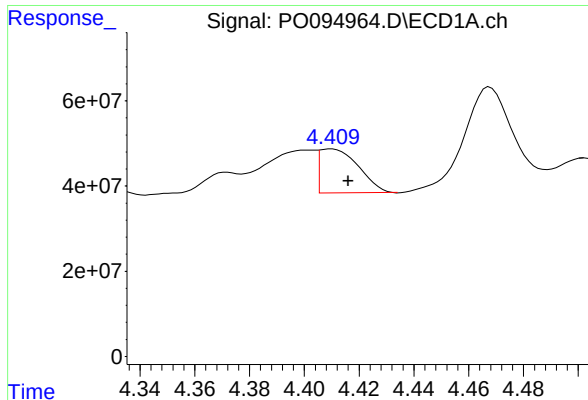

#1 Tetrachloro-m-xylene

R.T.: 4.409 min
Delta R.T.: -0.007 min
Response: 97022935
Conc: 28.17 ng/ml


Instrument :

ECD_O

ClientSampleId :
ERME-LIQUID-0509


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/12/2023
Supervised By :Ankita Jodhani 05/16/2023

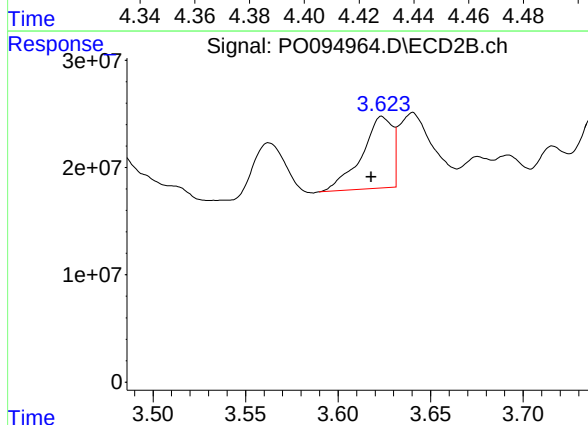


#1 Tetrachloro-m-xylene

R.T.: 3.624 min
Delta R.T.: 0.006 min
Response: 77328687
Conc: 57.79 ng/ml

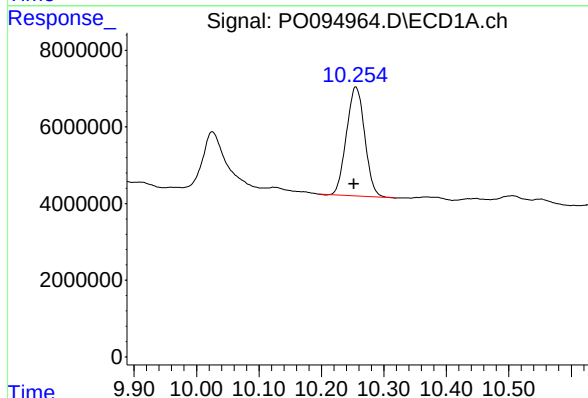

#2 Decachlorobiphenyl

R.T.: 10.255 min
Delta R.T.: 0.003 min
Response: 58036278
Conc: 23.91 ng/ml

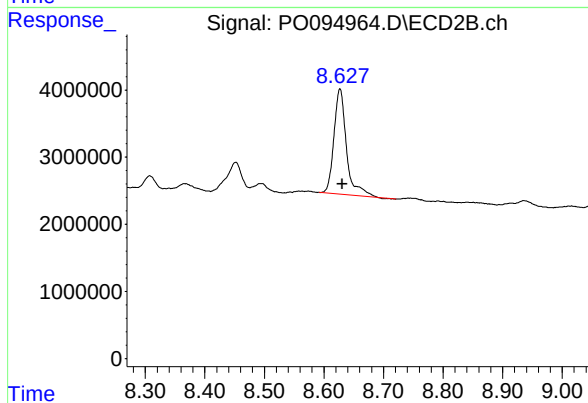

#2 Decachlorobiphenyl

R.T.: 8.627 min
Delta R.T.: -0.004 min
Response: 22795144
Conc: 20.25 ng/ml