

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051123\
 Data File : P0094966.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 14:19
 Operator : YP/AJ
 Sample : 02743-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DRUM-A-SLUDGE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/12/2023
 Supervised By : Ankita Jodhani 05/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 04:36:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.415	3.616	52196310	27145960	15.153	20.288 #
2) SA Decachlor...	10.253	8.626	31781289	13878220	13.096m	12.330

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051123\
Data File : PO094966.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 14:19
Operator : YP/AJ
Sample : 02743-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DRUM-A-SLUDGE


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/12/2023
Supervised By : Ankita Jodhani 05/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 04:36:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

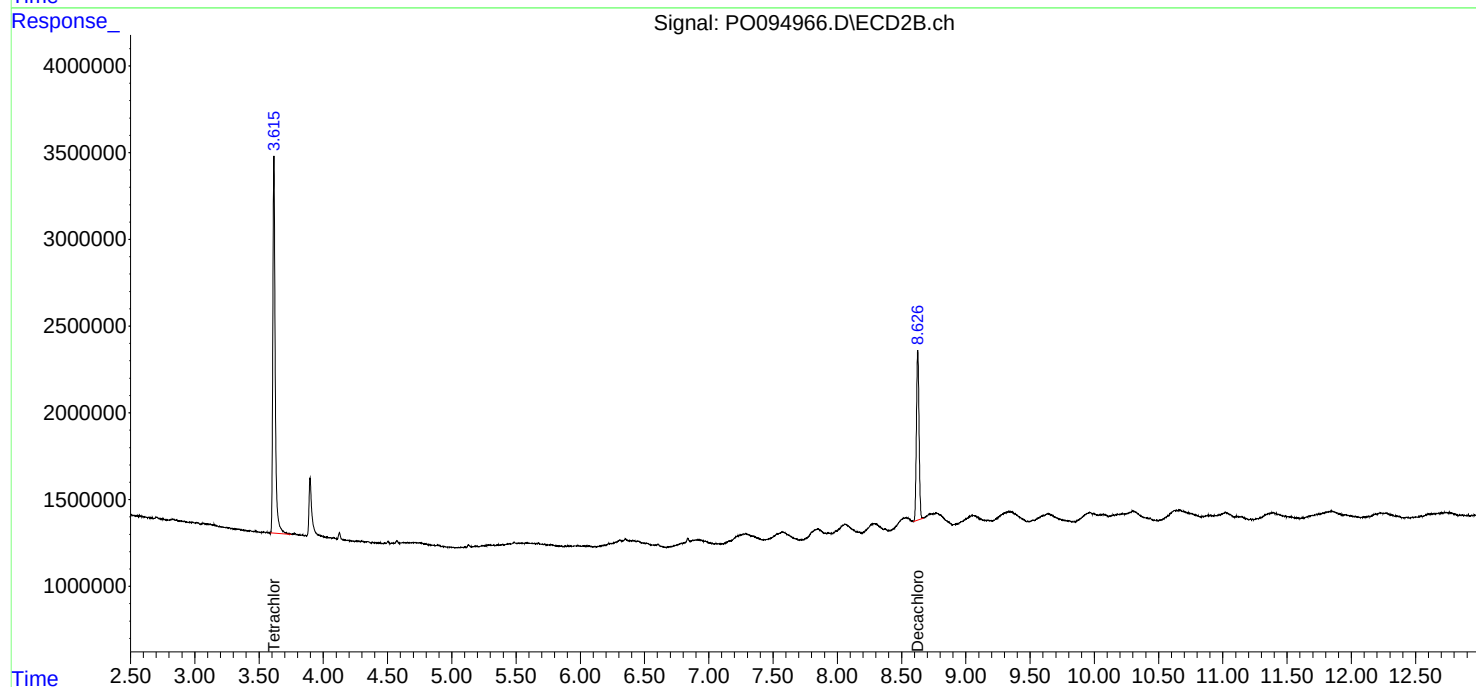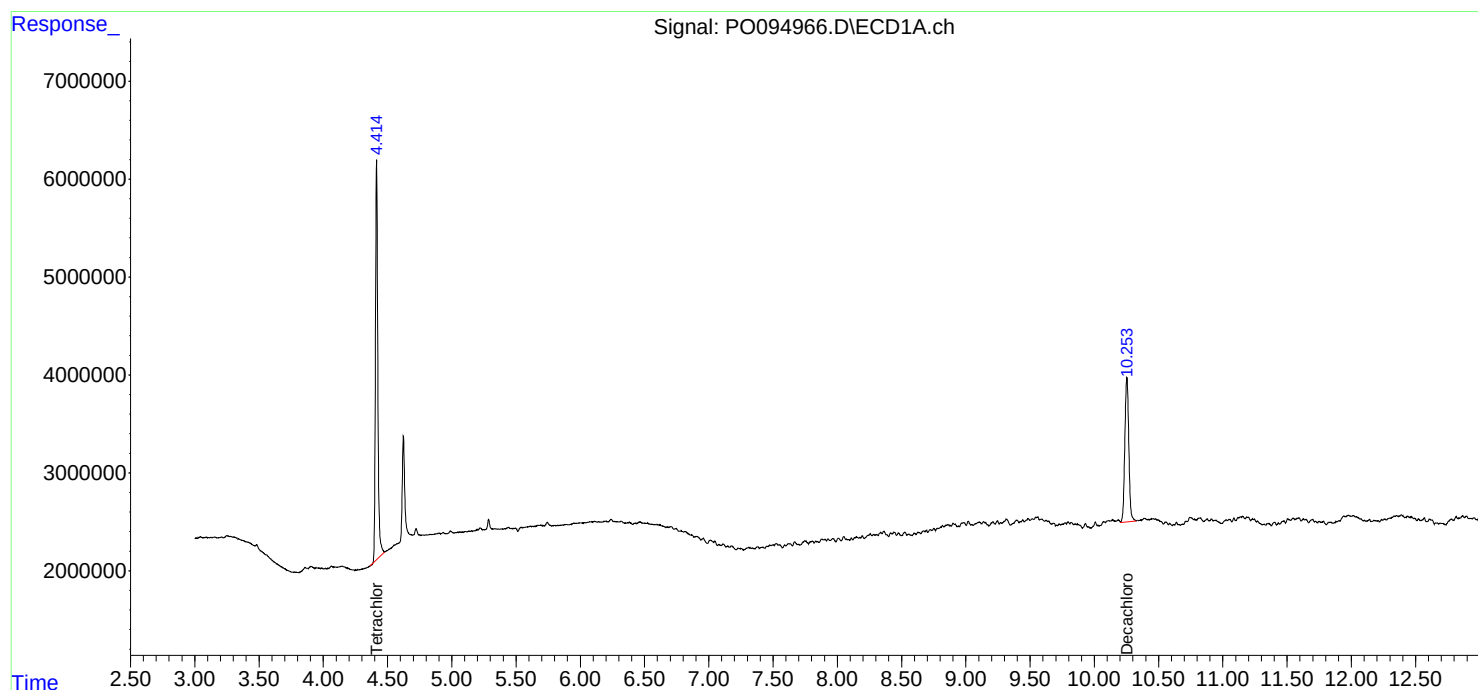

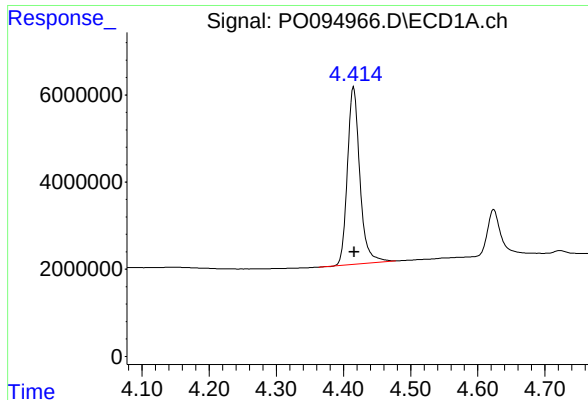


#1 Tetrachloro-m-xylene

R.T.: 4.415 min
Delta R.T.: -0.001 min
Response: 52196310
Conc: 15.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
DRUM-A-SLUDGE


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/12/2023
Supervised By :Ankita Jodhani 05/12/2023

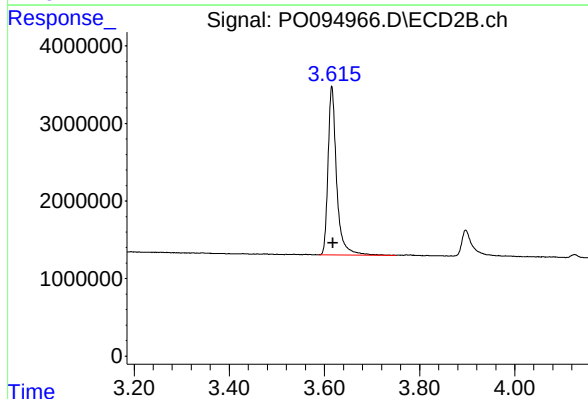


#1 Tetrachloro-m-xylene

R.T.: 3.616 min
Delta R.T.: -0.002 min
Response: 27145960
Conc: 20.29 ng/ml

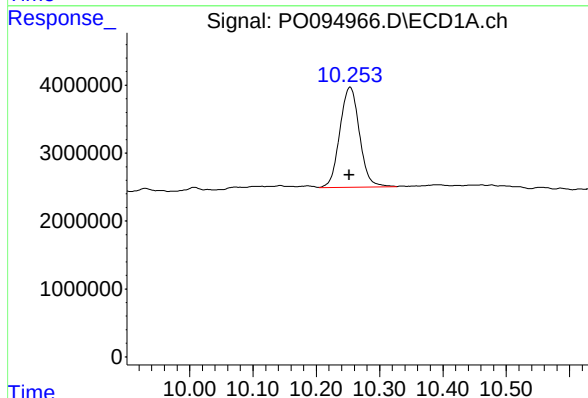

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: 0.000 min
Response: 31781289
Conc: 13.10 ng/ml m

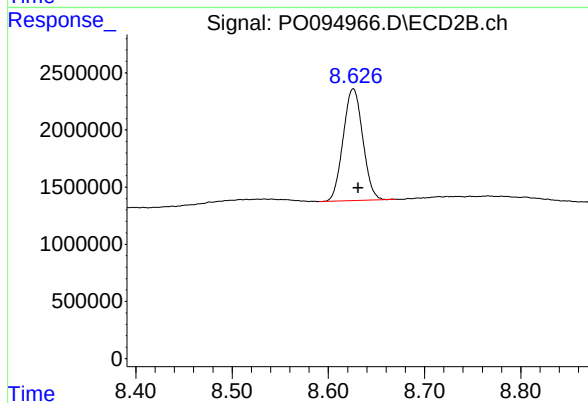

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.005 min
Response: 13878220
Conc: 12.33 ng/ml