

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051123\
 Data File : P0094977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 May 2023 18:15
 Operator : YP/AJ
 Sample : 02747-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB-03-0-2-20230510

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 05/12/2023
 Supervised By : Ankita Jodhani 05/12/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 04:42:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.414	3.615	70406540	27650814	20.440	20.665
2) SA Decachlor...	10.253	8.626	55010437	23518848	22.667	20.895m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051123\
Data File : PO094977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 May 2023 18:15
Operator : YP/AJ
Sample : 02747-01
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
SB-03-0-2-20230510


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 05/12/2023
Supervised By : Ankita Jodhani 05/12/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 04:42:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

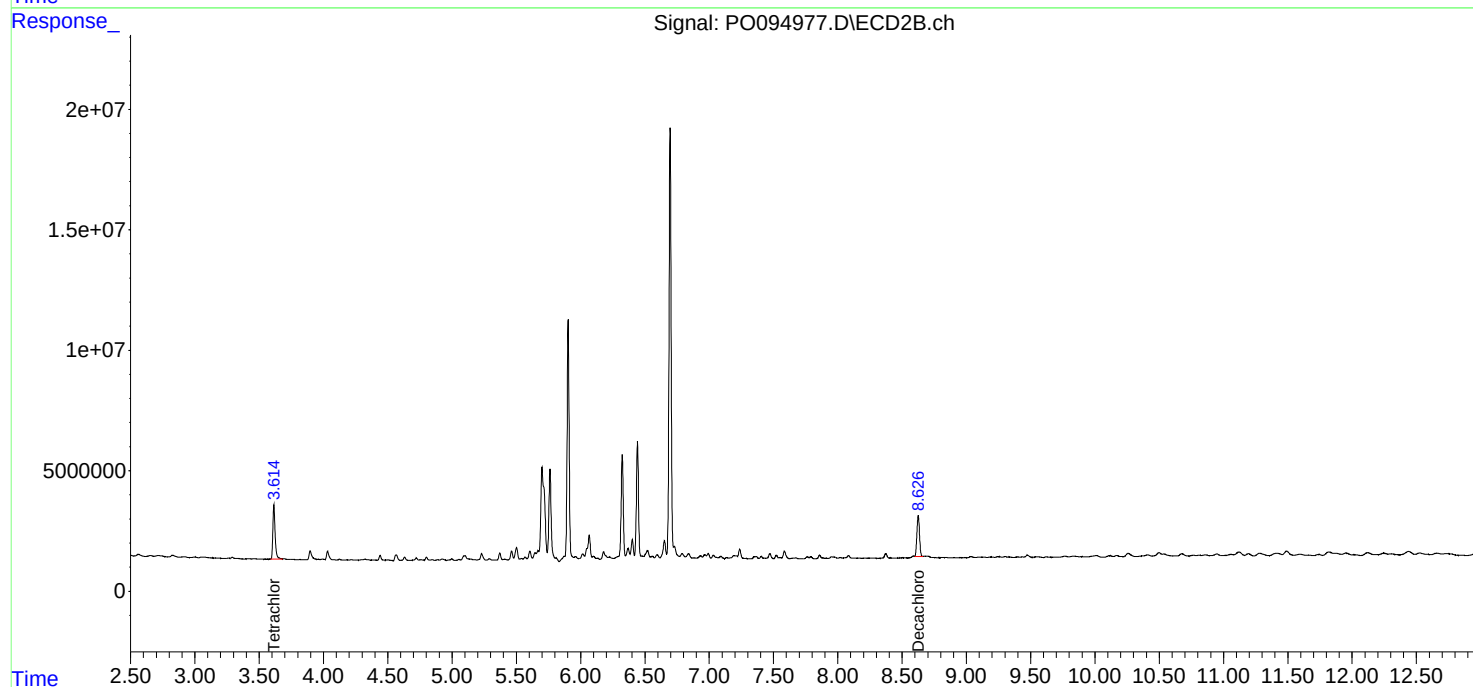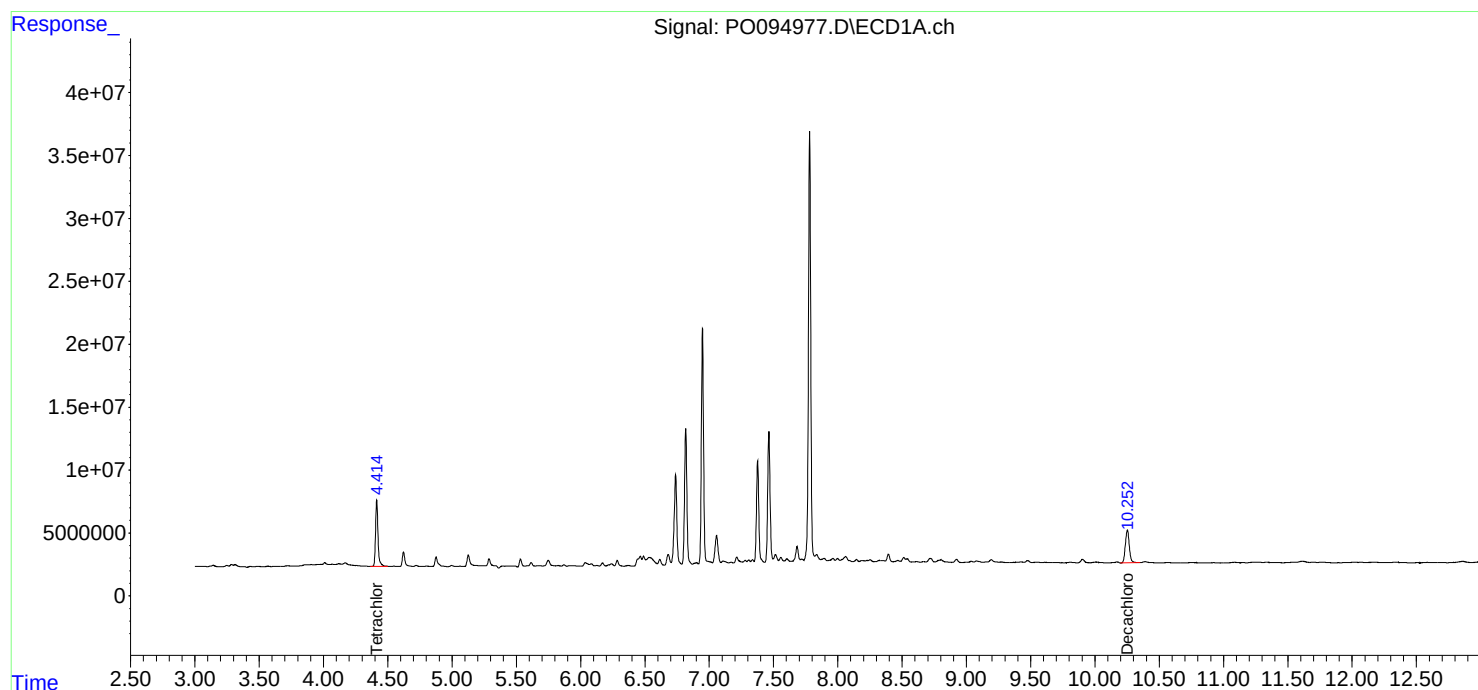

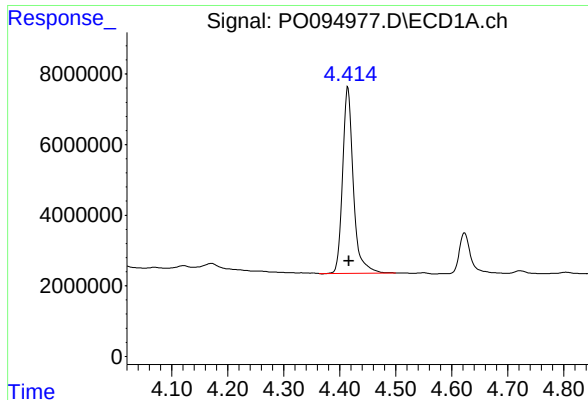


#1 Tetrachloro-m-xylene

R.T.: 4.414 min
Delta R.T.: -0.002 min
Response: 70406540
Conc: 20.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB-03-0-2-20230510


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 05/12/2023
Supervised By :Ankita Jodhani 05/12/2023

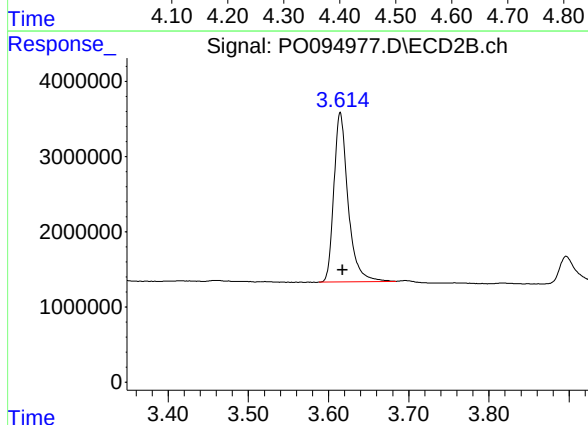


#1 Tetrachloro-m-xylene

R.T.: 3.615 min
Delta R.T.: -0.003 min
Response: 27650814
Conc: 20.66 ng/ml

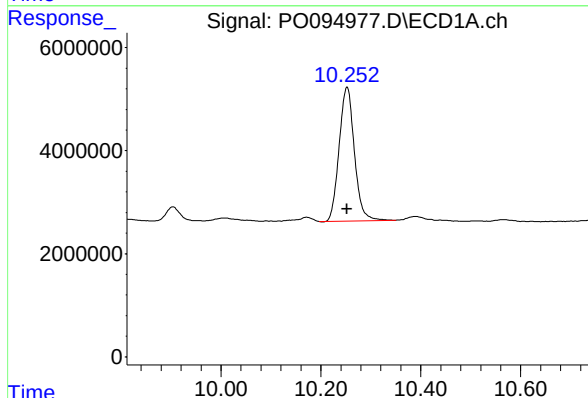

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: 0.000 min
Response: 55010437
Conc: 22.67 ng/ml

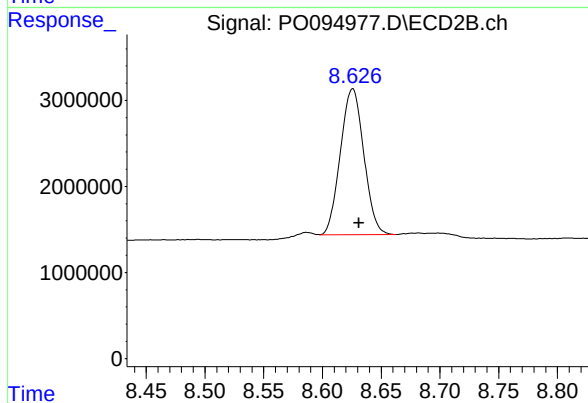

#2 Decachlorobiphenyl

R.T.: 8.626 min
Delta R.T.: -0.006 min
Response: 23518848
Conc: 20.89 ng/ml m