

Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051219\
 Data File : P0056151.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2019 14:15
 Operator : SM/SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Ankita
 5/15/2019 12:27:40 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 21:48:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.264	3.581	628440	583710	21.000	20.667
2)	SA Decachlor...	9.851	8.524	825938	608083	22.074	22.486m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051219\
Data File : PO056151.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2019 14:15
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
5/15/2019 12:27:40 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 21:48:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

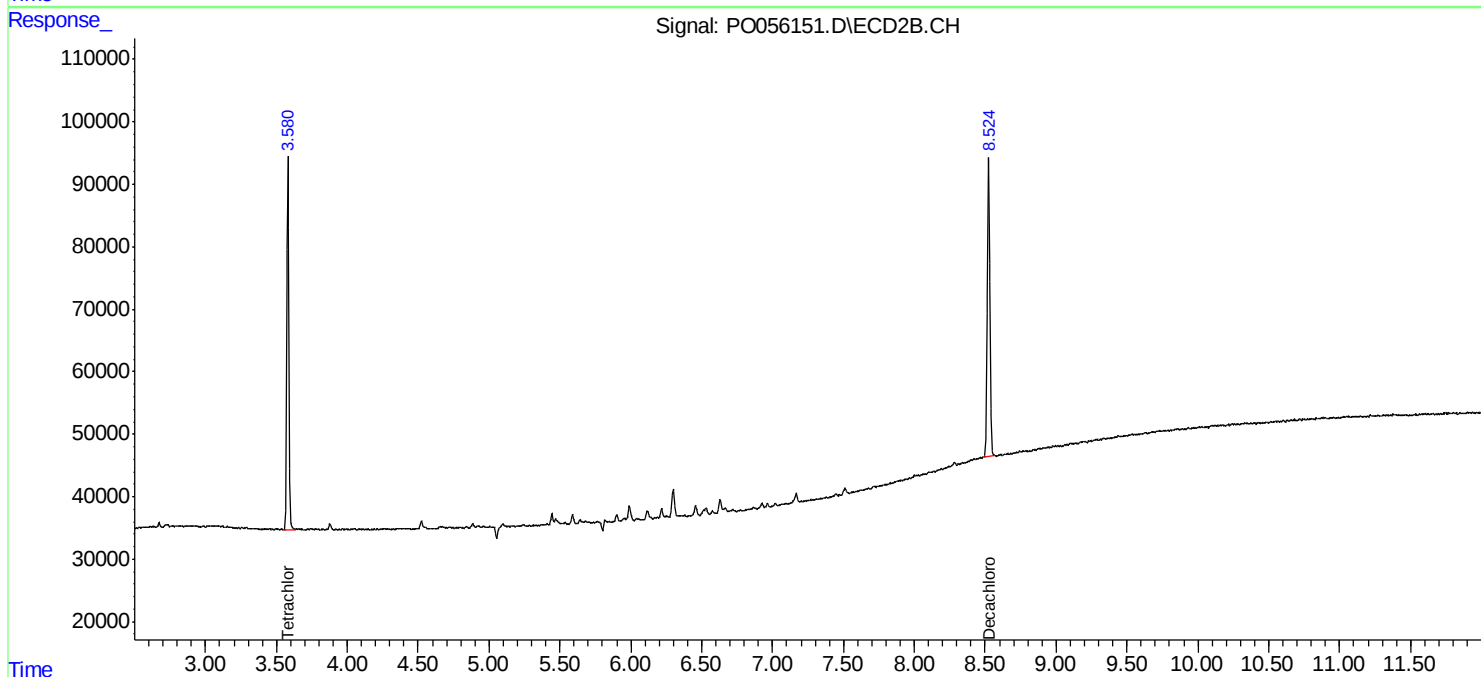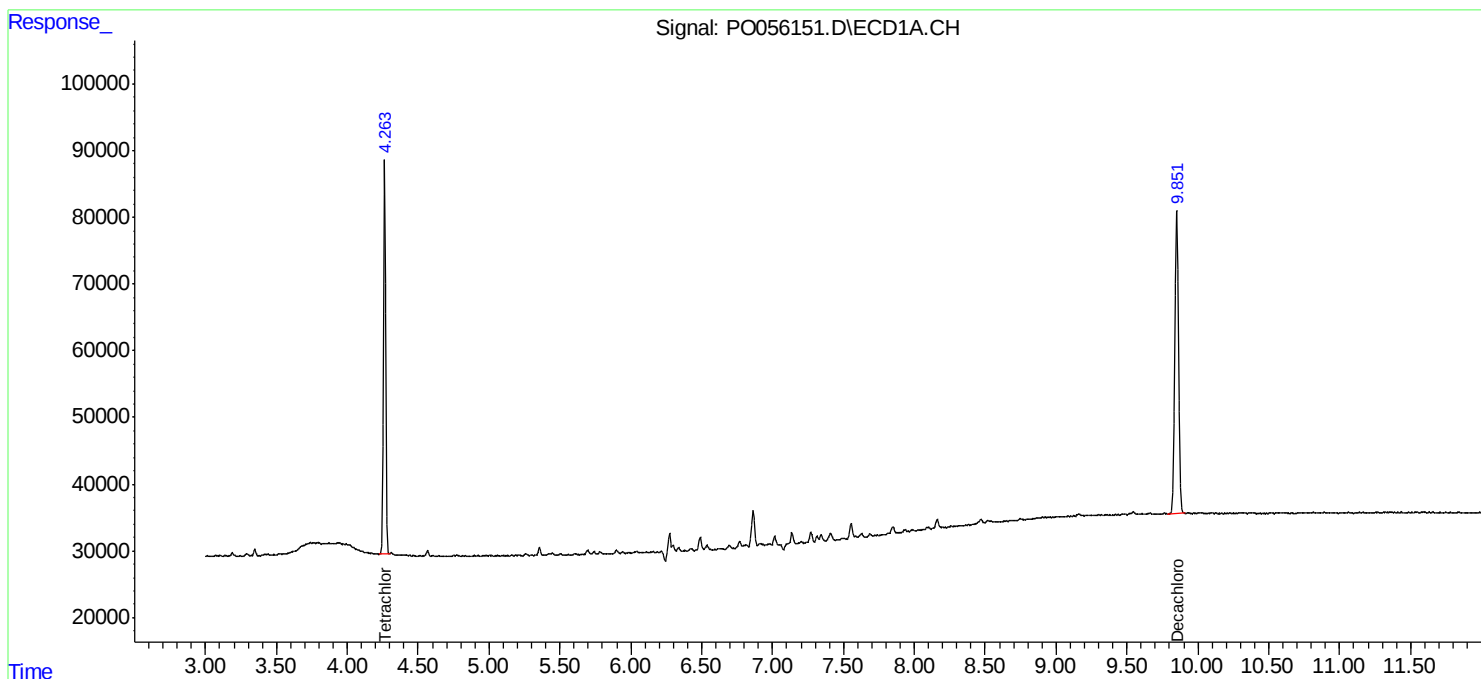

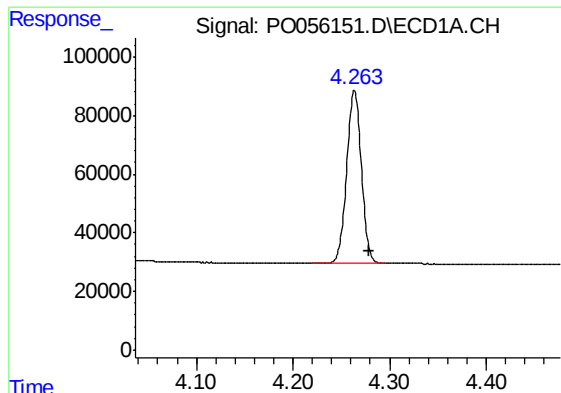


#1 Tetrachloro-m-xylene

R.T.: 4.264 min
Delta R.T.: -0.015 min
Response: 628440
Conc: 21.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Ankita
5/15/2019 12:27:40 PM

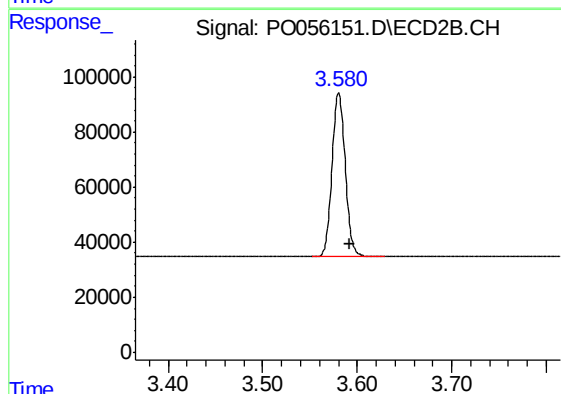


#1 Tetrachloro-m-xylene

R.T.: 3.581 min
Delta R.T.: -0.012 min
Response: 583710
Conc: 20.67 ng/ml

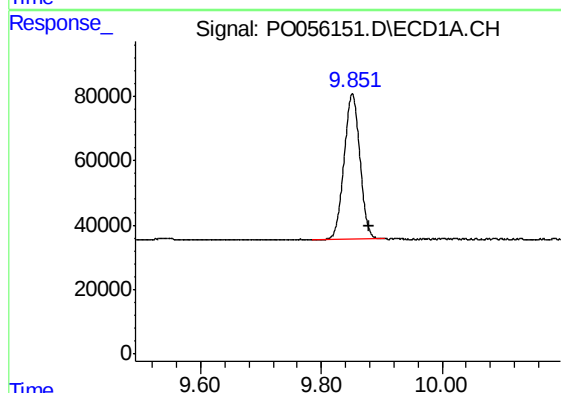

#2 Decachlorobiphenyl

R.T.: 9.851 min
Delta R.T.: -0.028 min
Response: 825938
Conc: 22.07 ng/ml

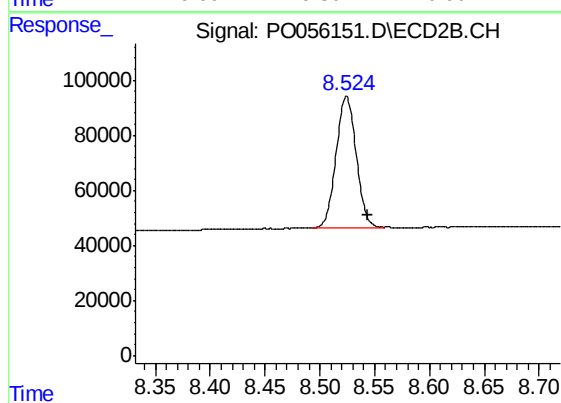

#2 Decachlorobiphenyl

R.T.: 8.524 min
Delta R.T.: -0.020 min
Response: 608083
Conc: 22.49 ng/ml m