

Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051219\
Data File : P0056155.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2019 15:23
Operator : SM/SJ
Sample : K2767-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
P026-SS009-1824-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 22:25:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.263	3.580	748823	701697	25.023	24.845
2) SA Decachlor...	9.852	8.524	884772	647338	23.646	23.937

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : \\74.0.250.170\terastorage\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051219\
Data File : PO056155.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2019 15:23
Operator : SM/SJ
Sample : K2767-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
P026-SS009-1824-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 22:25:08 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

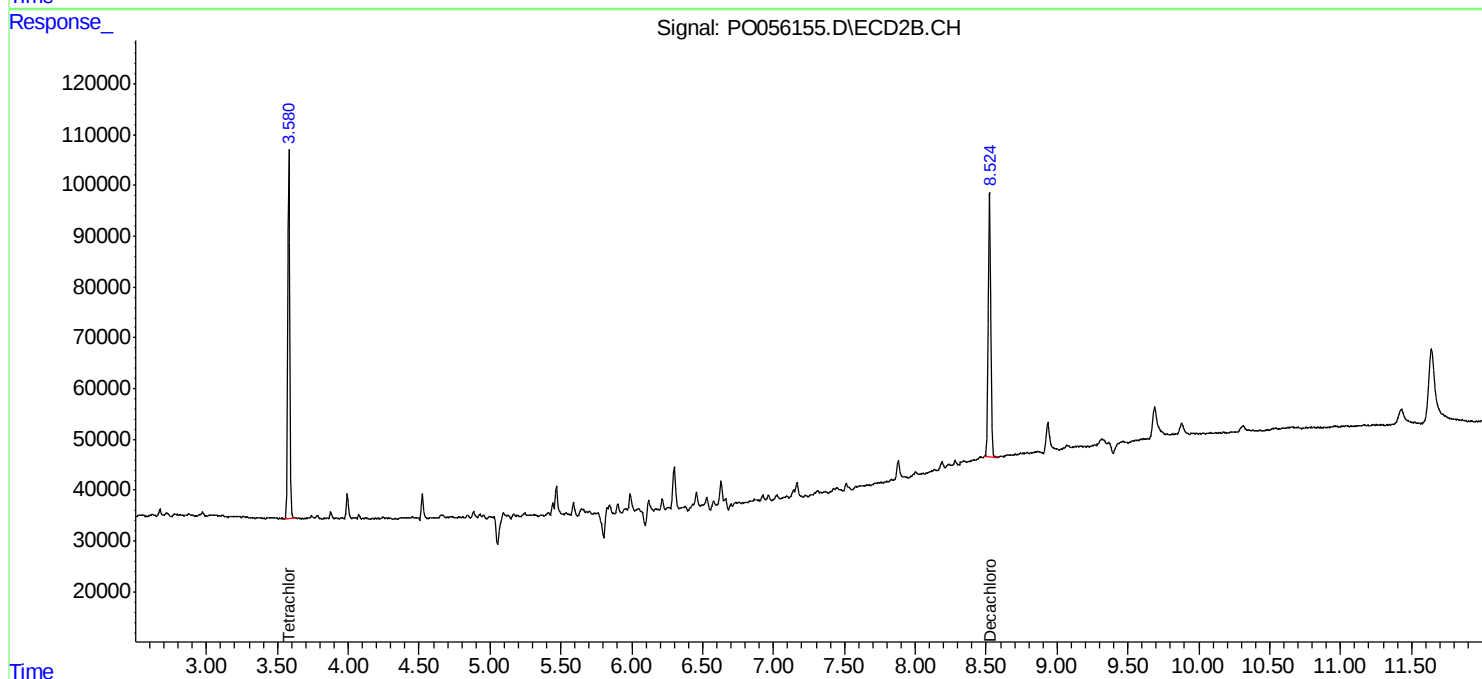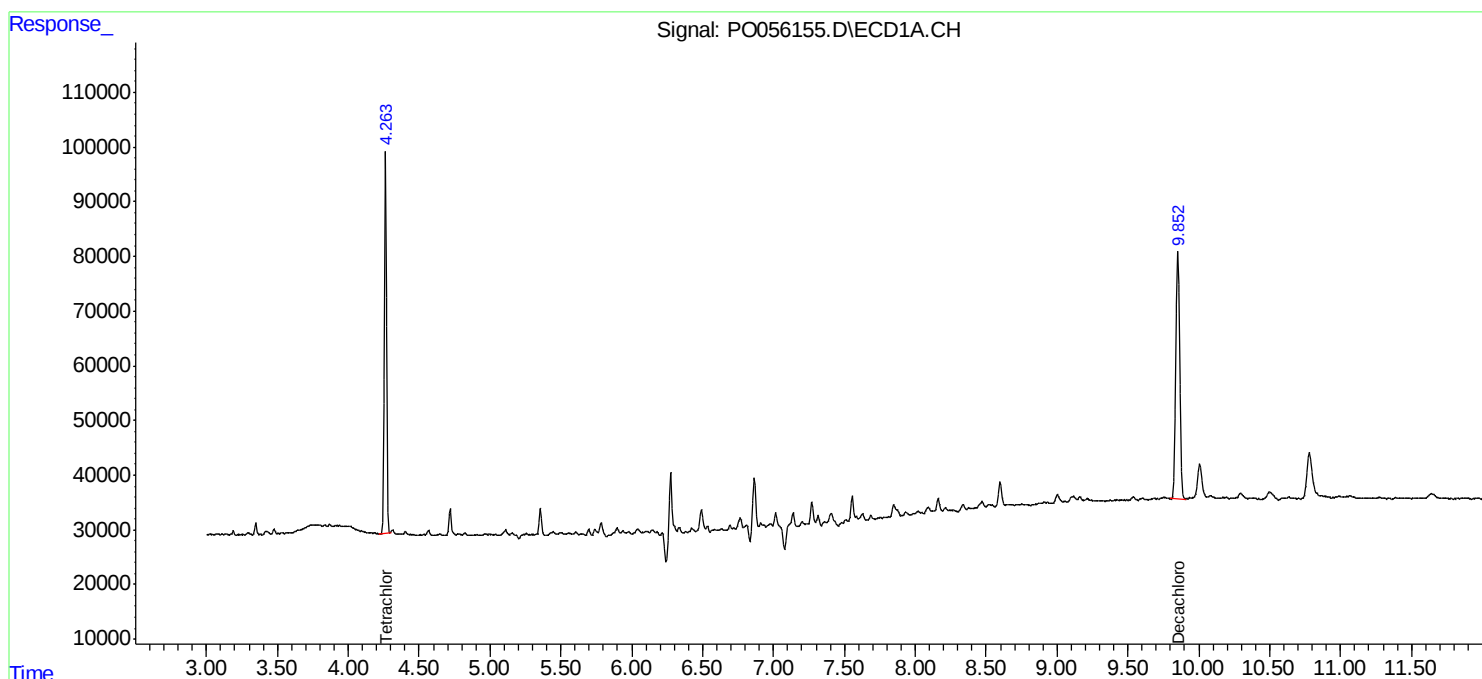


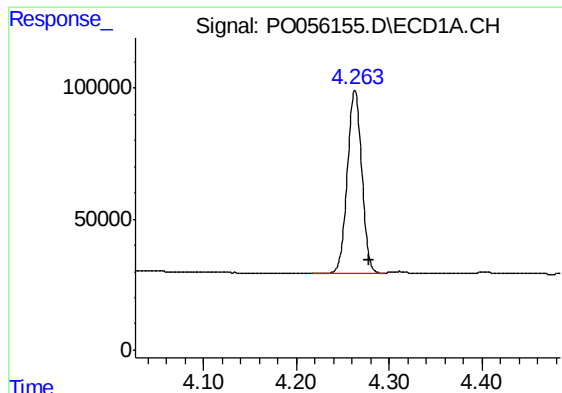

#1 Tetrachloro-m-xylene


R.T.: 4.263 min
Delta R.T.: -0.016 min
Response: 748823
Conc: 25.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
P026-SS009-1824-01

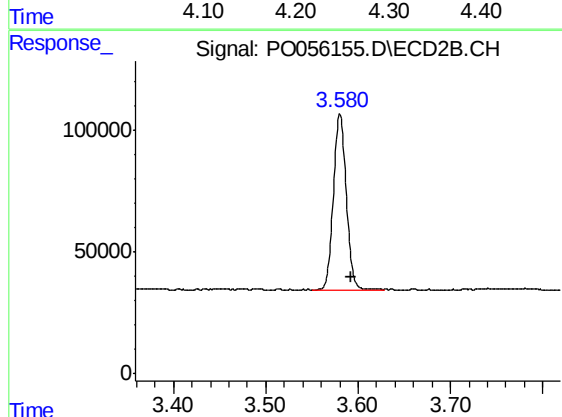


#1 Tetrachloro-m-xylene

R.T.: 3.580 min
Delta R.T.: -0.013 min
Response: 701697
Conc: 24.84 ng/ml

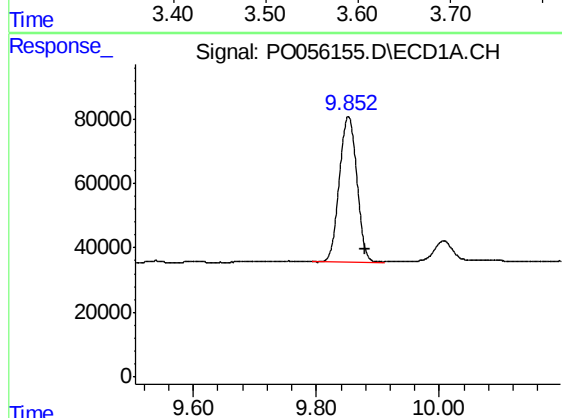

#2 Decachlorobiphenyl

R.T.: 9.852 min
Delta R.T.: -0.027 min
Response: 884772
Conc: 23.65 ng/ml

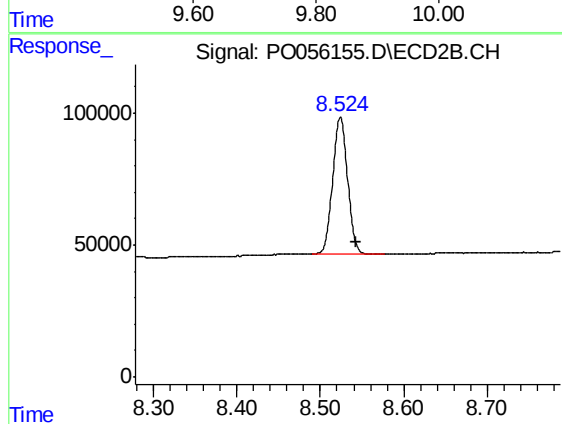

#2 Decachlorobiphenyl

R.T.: 8.524 min
Delta R.T.: -0.020 min
Response: 647338
Conc: 23.94 ng/ml