

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051220\
 Data File : P0068301.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2020 11:33
 Operator : DD\AJ
 Sample : L2182-09
 Misc : AR1242 25PPB MDL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/13/2020 2:22:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 23:42:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.905	3.932	663715	802789	23.665	23.395
2) SA Decachlor...	10.862	9.206	884762	917555	22.234m	23.833
Target Compounds						
16) L4 AR-1242-1	6.226	5.184	26009	31835	29.561	29.315
17) L4 AR-1242-2	6.249	5.205	35782	49867	29.929	35.161
18) L4 AR-1242-3	6.313	5.394	27053	25527	36.210	32.034
19) L4 AR-1242-4	6.421	5.492	15724	27746	25.678m	35.912 #
20) L4 AR-1242-5	7.200	6.052	13656	27142	18.490m	26.913m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051220\
Data File : PO068301.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2020 11:33
Operator : DD\AJ
Sample : L2182-09
Misc : AR1242 25PPB MDL
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 23:42:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

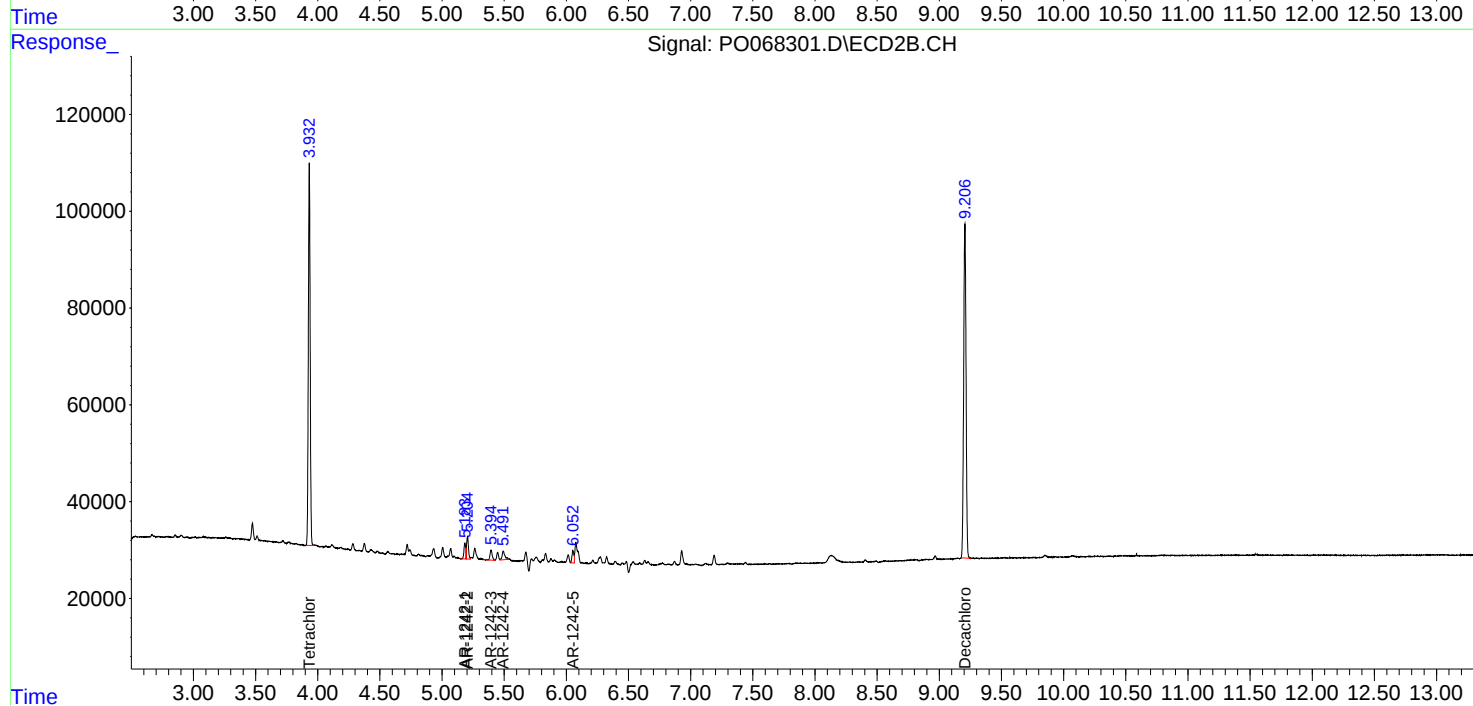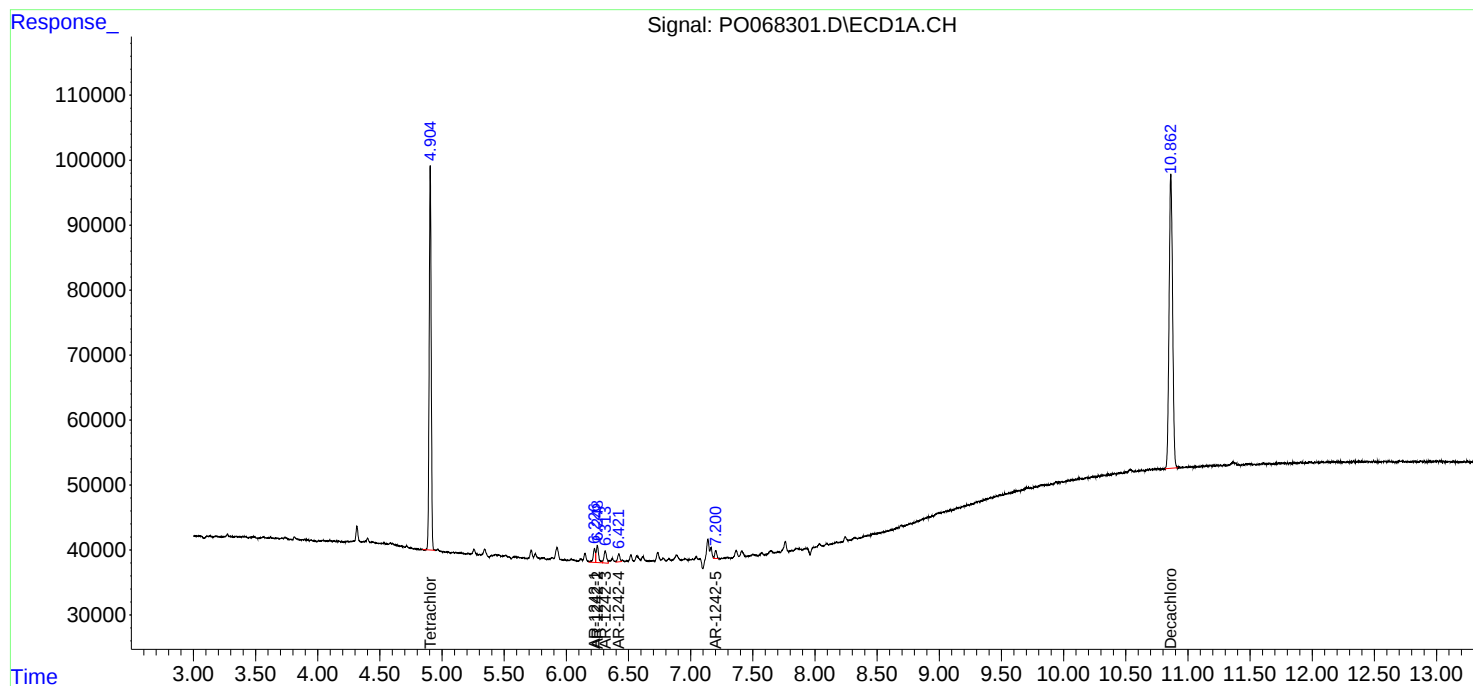

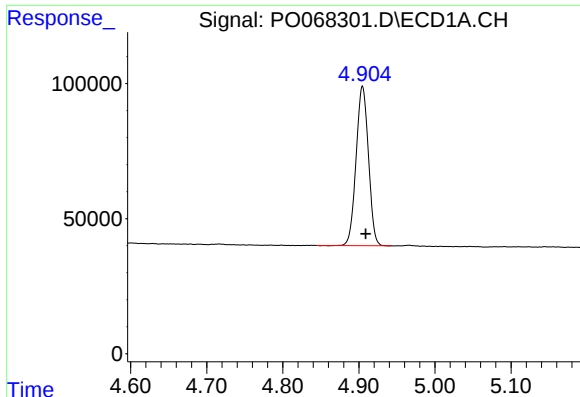


#1 Tetrachloro-m-xylene

R.T.: 4.905 min
Delta R.T.: -0.004 min
Response: 663715
Conc: 23.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:44 PM

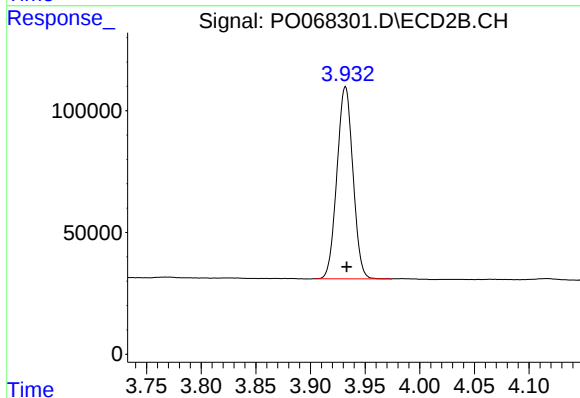


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.001 min
Response: 802789
Conc: 23.40 ng/ml

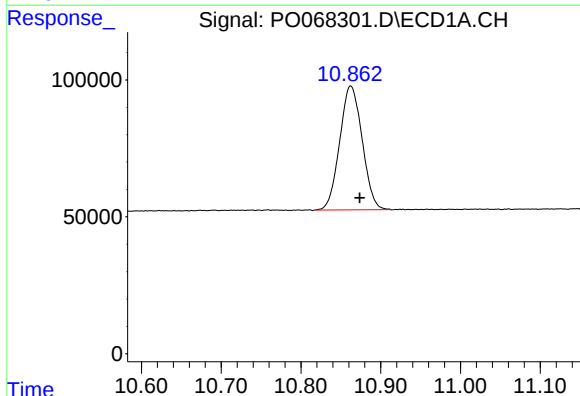


#2 Decachlorobiphenyl

R.T.: 10.862 min
Delta R.T.: -0.012 min
Response: 884762
Conc: 22.23 ng/ml m

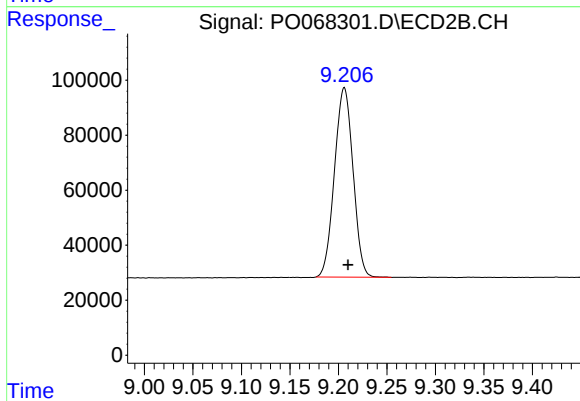

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.004 min
Response: 917555
Conc: 23.83 ng/ml

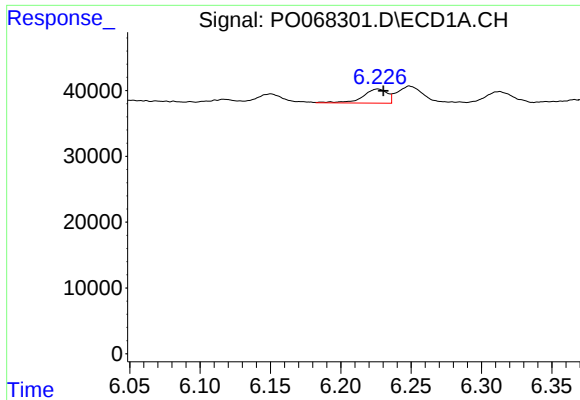


#16 AR-1242-1

R.T.: 6.226 min
Delta R.T.: -0.004 min
Response: 26009
Conc: 29.56 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:44 PM

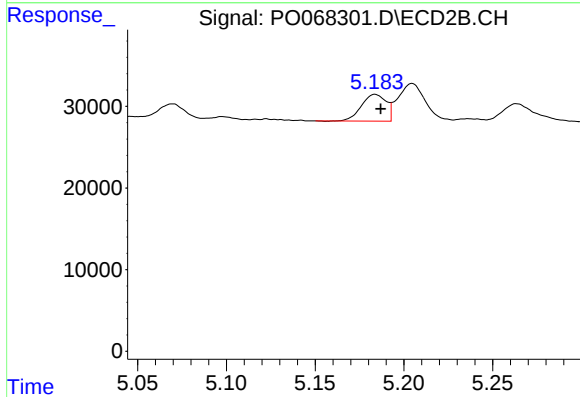


#16 AR-1242-1

R.T.: 5.184 min
Delta R.T.: -0.003 min
Response: 31835
Conc: 29.31 ng/ml

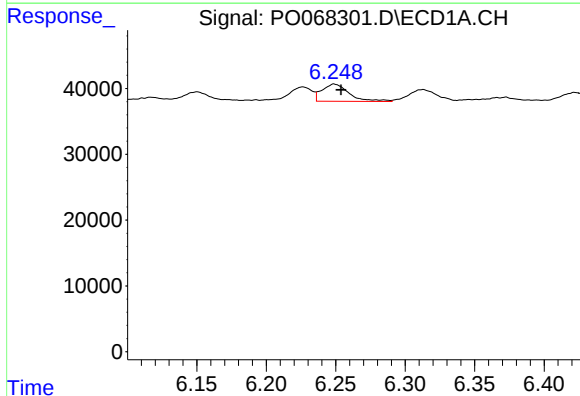


#17 AR-1242-2

R.T.: 6.249 min
Delta R.T.: -0.005 min
Response: 35782
Conc: 29.93 ng/ml

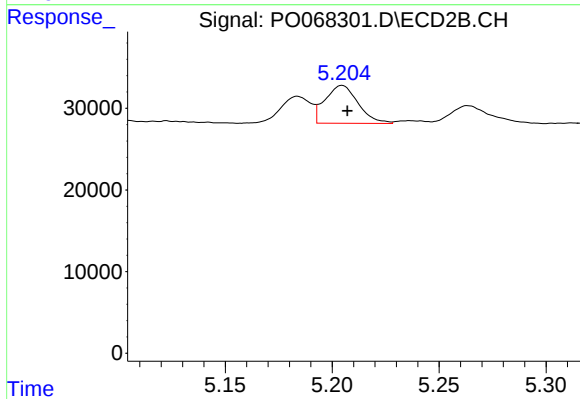

#17 AR-1242-2

R.T.: 5.205 min
Delta R.T.: -0.002 min
Response: 49867
Conc: 35.16 ng/ml

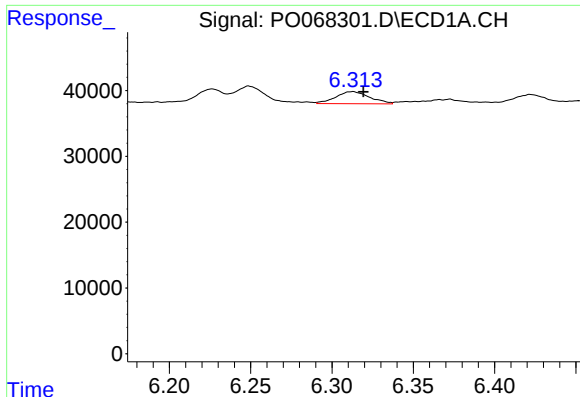


#18 AR-1242-3

R.T.: 6.313 min
Delta R.T.: -0.007 min
Response: 27053
Conc: 36.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:44 PM

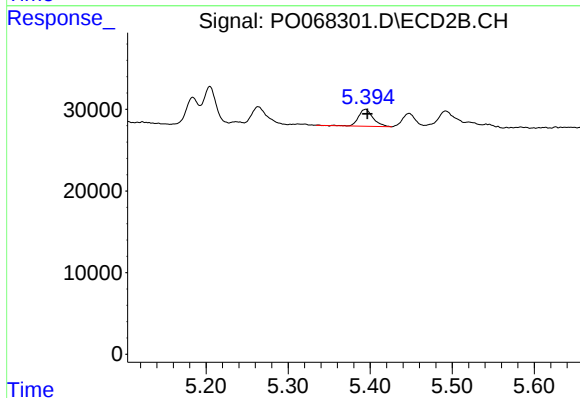


#18 AR-1242-3

R.T.: 5.394 min
Delta R.T.: -0.002 min
Response: 25527
Conc: 32.03 ng/ml

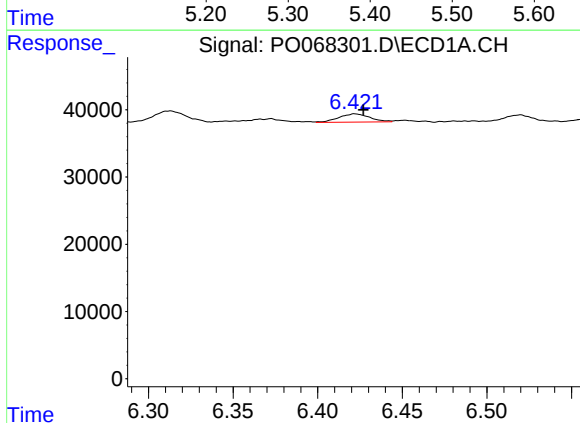


#19 AR-1242-4

R.T.: 6.421 min
Delta R.T.: -0.006 min
Response: 15724
Conc: 25.68 ng/ml m

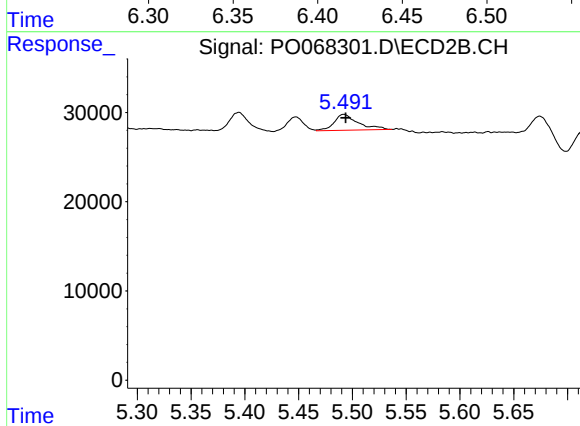

#19 AR-1242-4

R.T.: 5.492 min
Delta R.T.: -0.002 min
Response: 27746
Conc: 35.91 ng/ml

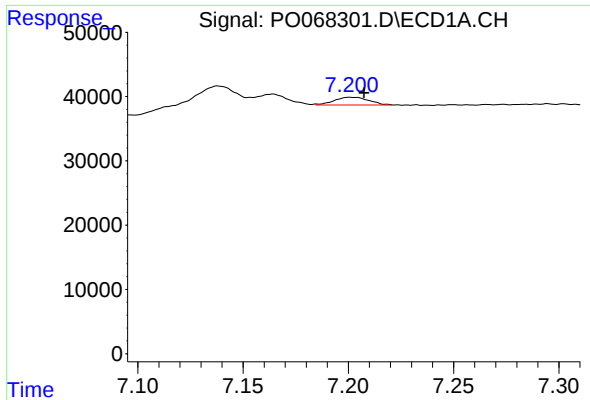


#20 AR-1242-5

R.T.: 7.200 min
Delta R.T.: -0.007 min
Response: 13656
Conc: 18.49 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020

Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:44 PM

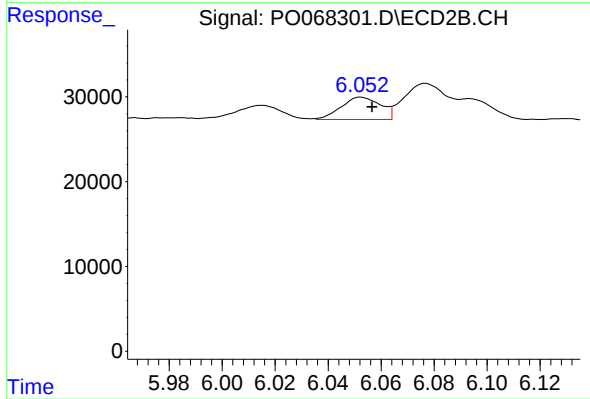

#20 AR-1242-5

R.T.: 6.052 min
Delta R.T.: -0.005 min
Response: 27142
Conc: 26.91 ng/ml m