

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051220\
 Data File : P0068302.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2020 11:50
 Operator : DD\AJ
 Sample : L2182-09
 Misc : AR1248 25PPB MDL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/13/2020 2:22:45 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 23:42:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.905	3.932	633641	752669	22.593	21.935
2)	SA Decachlor...	10.864	9.207	849740	885249	21.354m	22.994
Target Compounds							
21)	L5 AR-1248-1	6.226	5.184	20351	26425	30.701	32.557
22)	L5 AR-1248-2	6.519	5.447	26315	32584	31.563	30.676
23)	L5 AR-1248-3	6.735	5.492	29207	41177	29.693m	38.519 #
24)	L5 AR-1248-4	7.164	5.674	31267	32119	26.506m	24.890m
25)	L5 AR-1248-5	7.201	6.096	24896	60932	22.352m	46.837 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051220\
Data File : P0068302.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2020 11:50
Operator : DD\AJ
Sample : L2182-09
Misc : AR1248 25PPB MDL
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:45 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 23:42:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

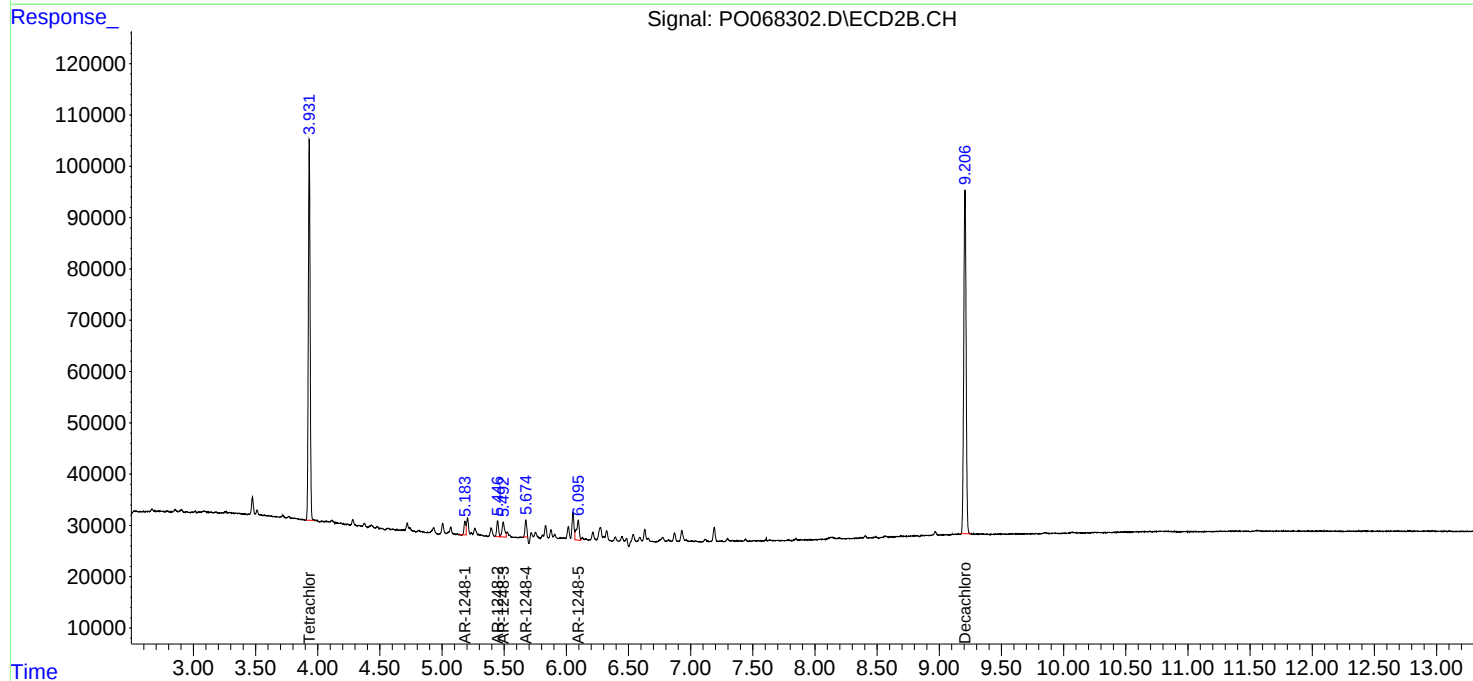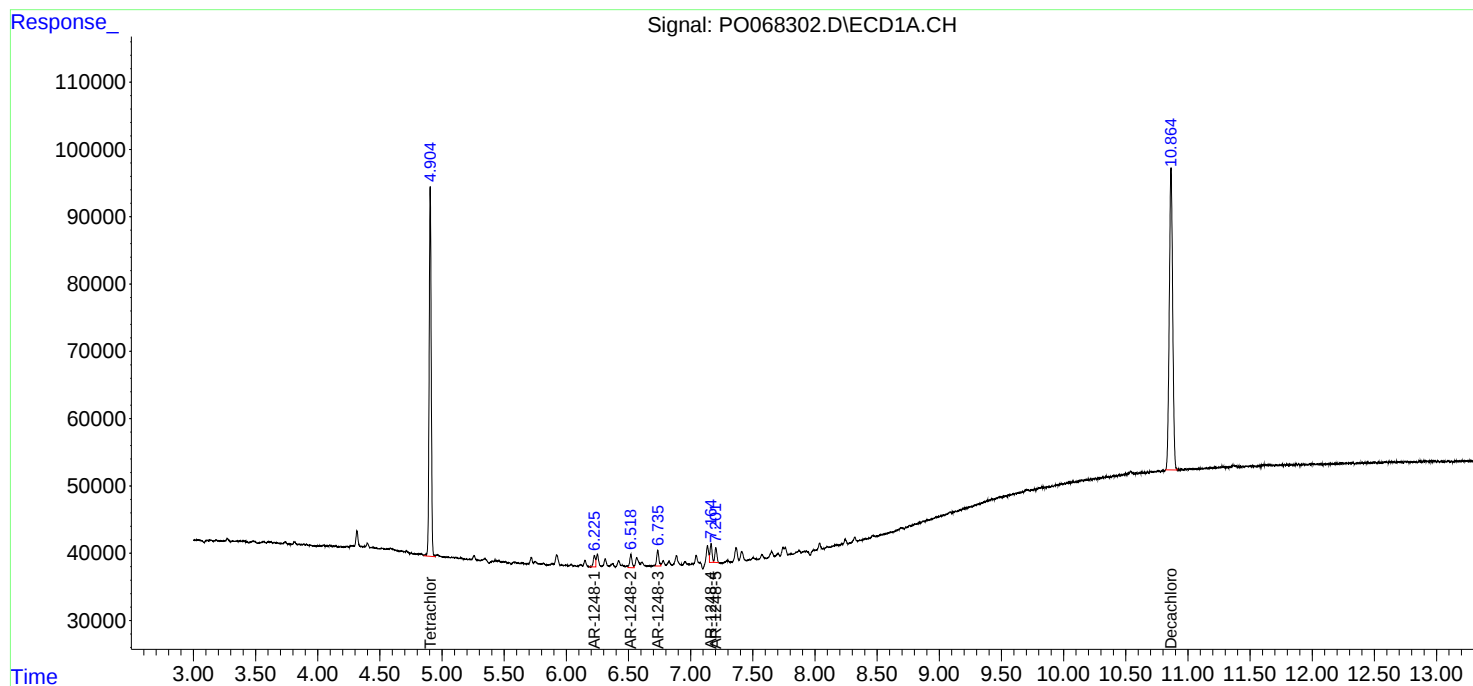

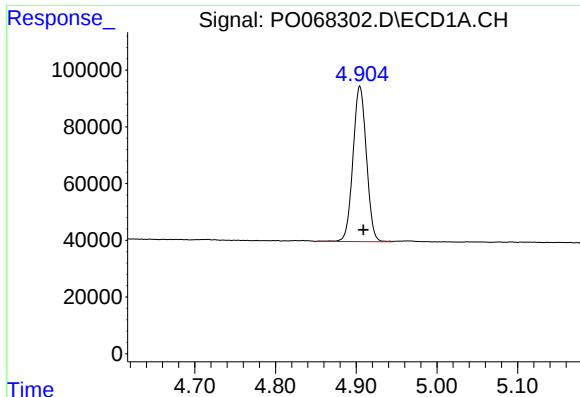


#1 Tetrachloro-m-xylene

R.T.: 4.905 min
Delta R.T.: -0.004 min
Response: 633641
Conc: 22.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:45 PM

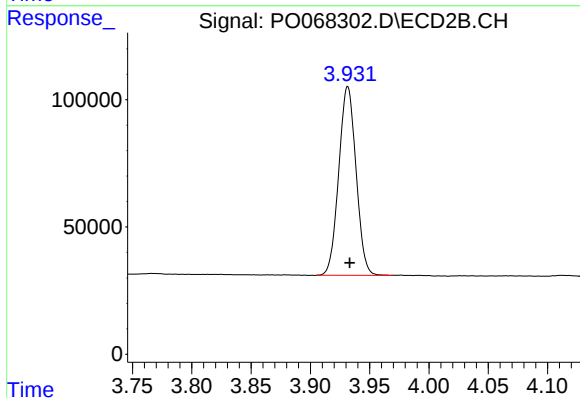


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.002 min
Response: 752669
Conc: 21.93 ng/ml

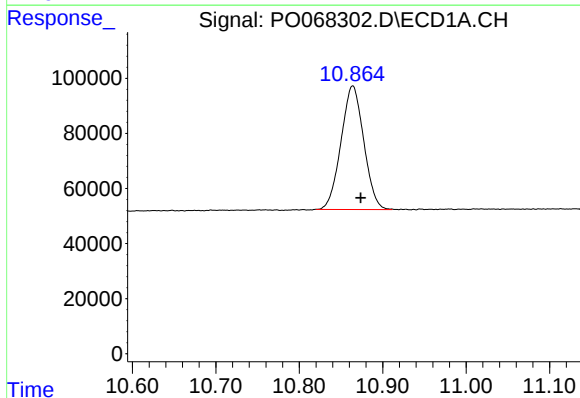


#2 Decachlorobiphenyl

R.T.: 10.864 min
Delta R.T.: -0.010 min
Response: 849740
Conc: 21.35 ng/ml m

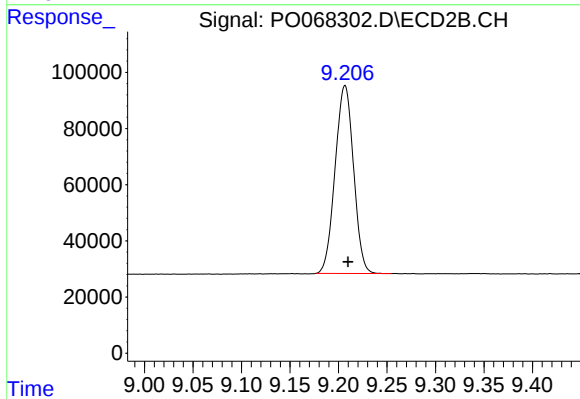

#2 Decachlorobiphenyl

R.T.: 9.207 min
Delta R.T.: -0.003 min
Response: 885249
Conc: 22.99 ng/ml

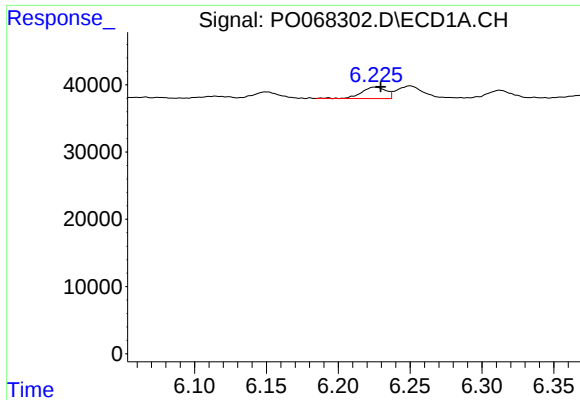


#21 AR-1248-1

R.T.: 6.226 min
Delta R.T.: -0.004 min
Response: 20351
Conc: 30.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:45 PM

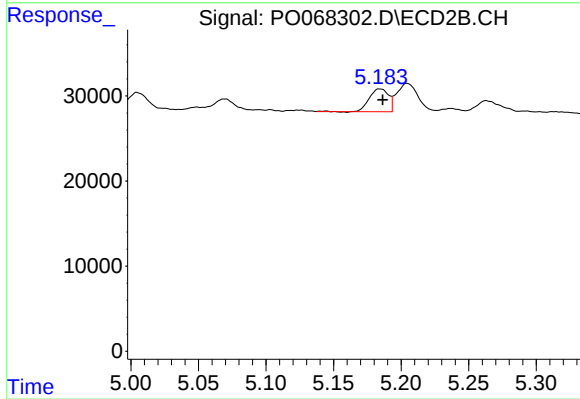


#21 AR-1248-1

R.T.: 5.184 min
Delta R.T.: -0.002 min
Response: 26425
Conc: 32.56 ng/ml

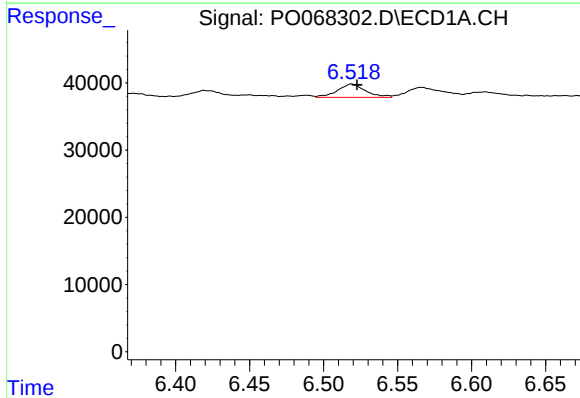


#22 AR-1248-2

R.T.: 6.519 min
Delta R.T.: -0.003 min
Response: 26315
Conc: 31.56 ng/ml

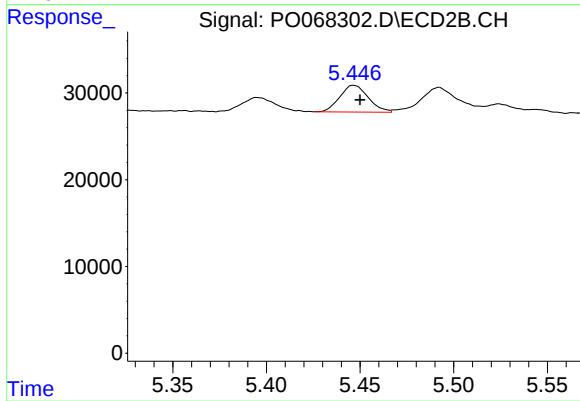

#22 AR-1248-2

R.T.: 5.447 min
Delta R.T.: -0.003 min
Response: 32584
Conc: 30.68 ng/ml

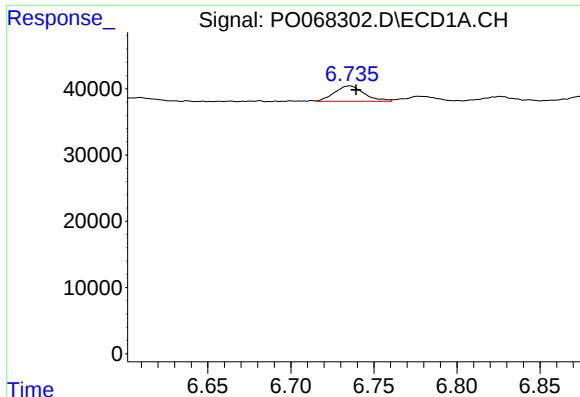


#23 AR-1248-3

R.T.: 6.735 min
Delta R.T.: -0.004 min
Response: 29207
Conc: 29.69 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:45 PM

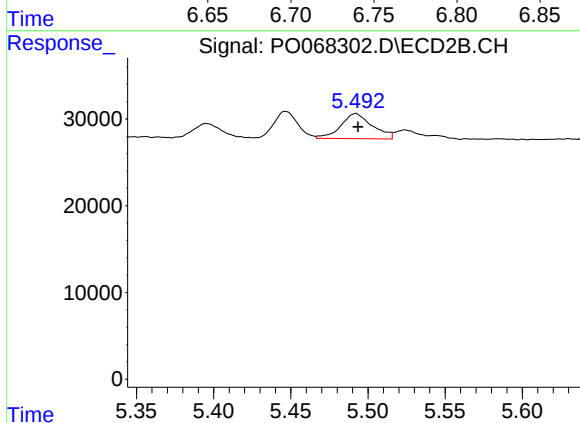


#23 AR-1248-3

R.T.: 5.492 min
Delta R.T.: -0.001 min
Response: 41177
Conc: 38.52 ng/ml

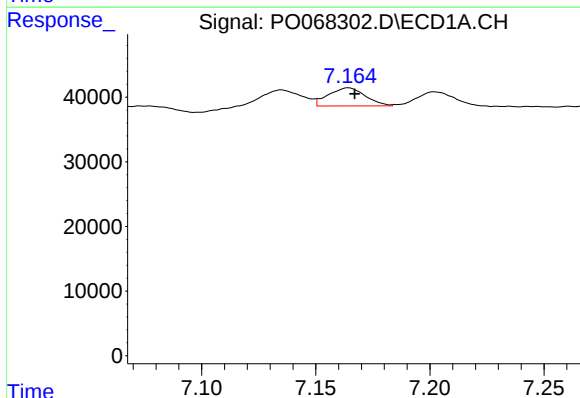


#24 AR-1248-4

R.T.: 7.164 min
Delta R.T.: -0.003 min
Response: 31267
Conc: 26.51 ng/ml m

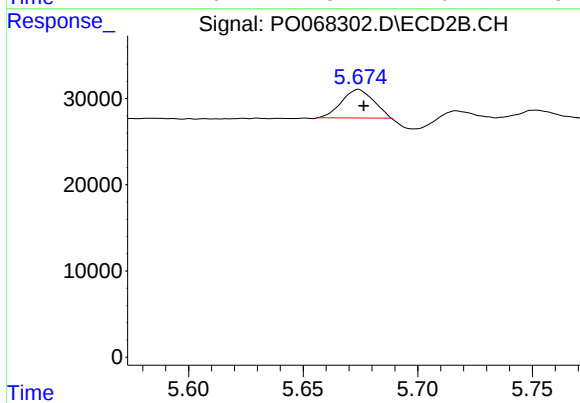

#24 AR-1248-4

R.T.: 5.674 min
Delta R.T.: -0.003 min
Response: 32119
Conc: 24.89 ng/ml m

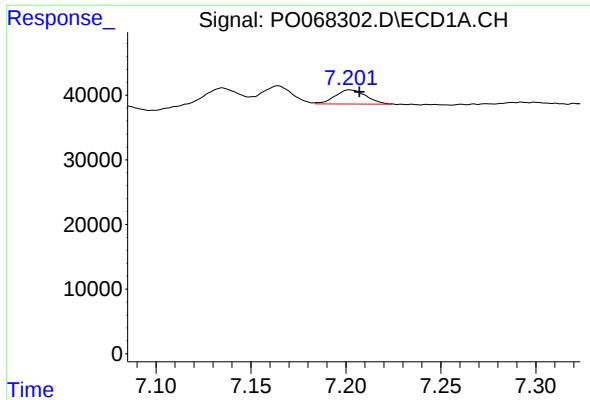


#25 AR-1248-5

R.T.: 7.201 min
Delta R.T.: -0.006 min
Response: 24896
Conc: 22.35 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020

Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:45 PM

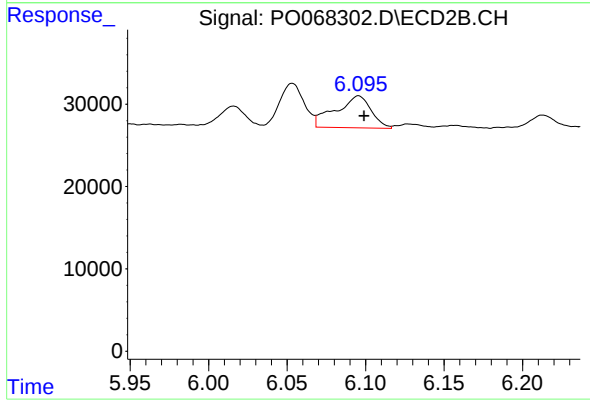

#25 AR-1248-5

R.T.: 6.096 min
Delta R.T.: -0.003 min
Response: 60932
Conc: 46.84 ng/ml