

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051220\
 Data File : P0068304.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2020 12:24
 Operator : DD\AJ
 Sample : L2182-09
 Misc : AR1262 25PPB MDL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/13/2020 2:22:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 23:43:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.905	3.932	649238	778769	23.149	22.695
2) SA Decachlor...	10.863	9.206	867027	905999	21.788m	23.533
Target Compounds						
36) L8 AR-1262-1	8.535	7.297	56065	45567	28.024	32.032
37) L8 AR-1262-2	9.085	7.848	101883	137338	28.263	29.551
38) L8 AR-1262-3	9.389	8.134	66567	75040	25.646m	38.863m#
39) L8 AR-1262-4	9.481	8.197	51480	112038	24.916	31.898 #
40) L8 AR-1262-5	10.135	8.692	37450	52181	24.513	30.248

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051220\
Data File : P0068304.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2020 12:24
Operator : DD\AJ
Sample : L2182-09
Misc : AR1262 25PPB MDL
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleID :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:48 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 23:43:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

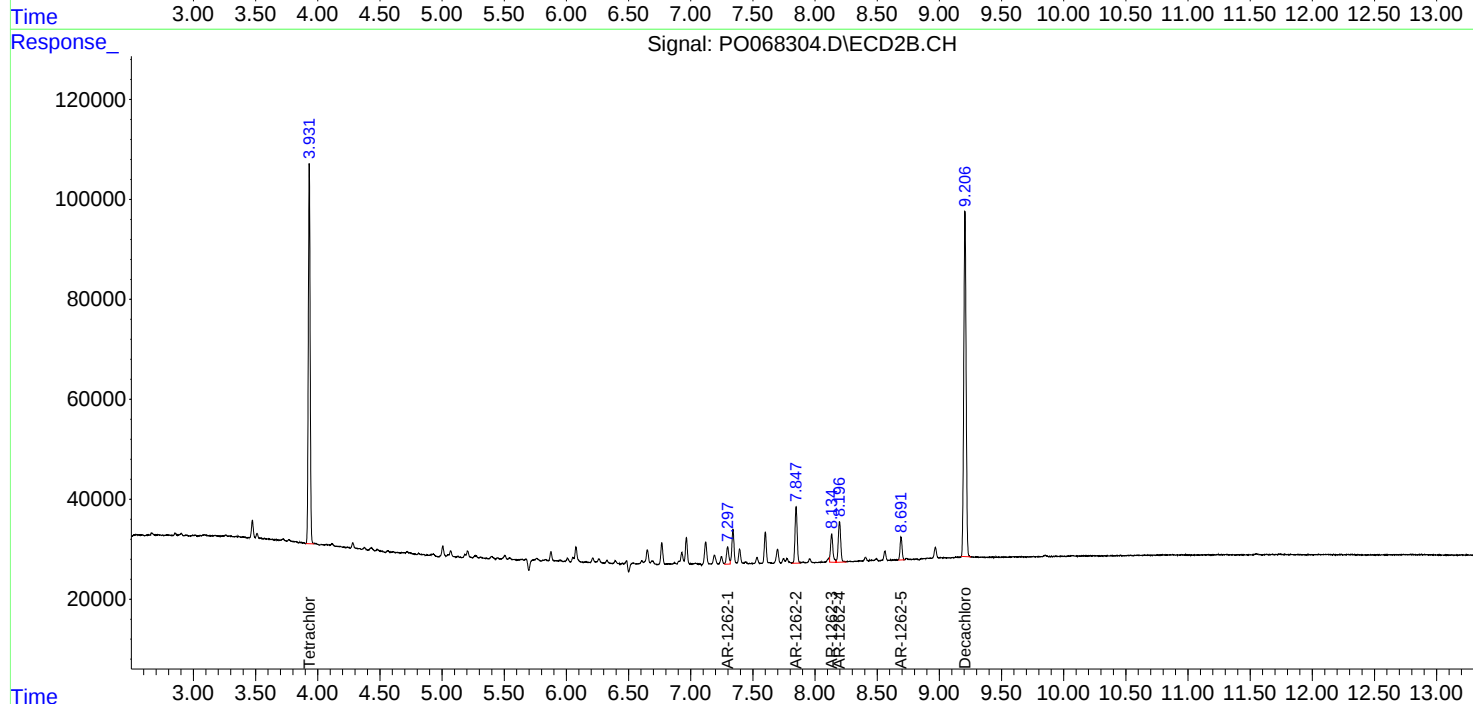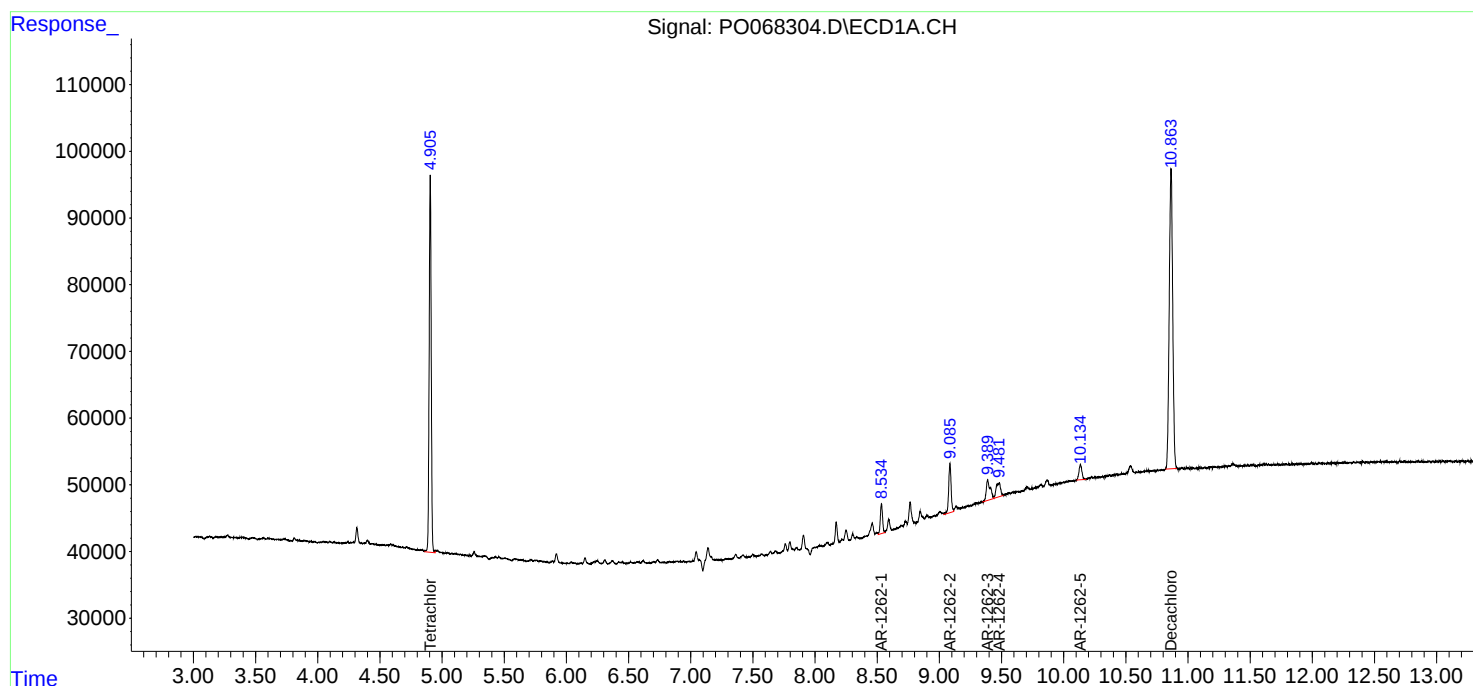

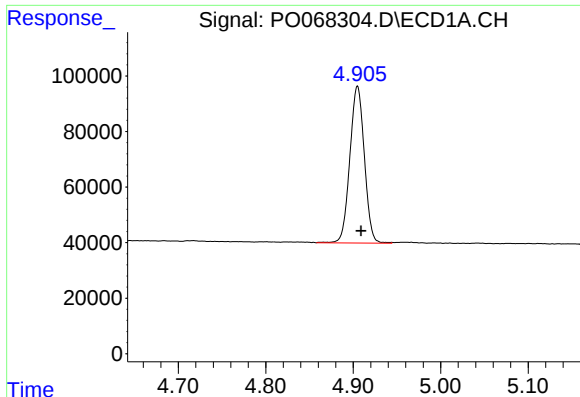


#1 Tetrachloro-m-xylene

R.T.: 4.905 min
Delta R.T.: -0.004 min
Response: 649238
Conc: 23.15 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:48 PM

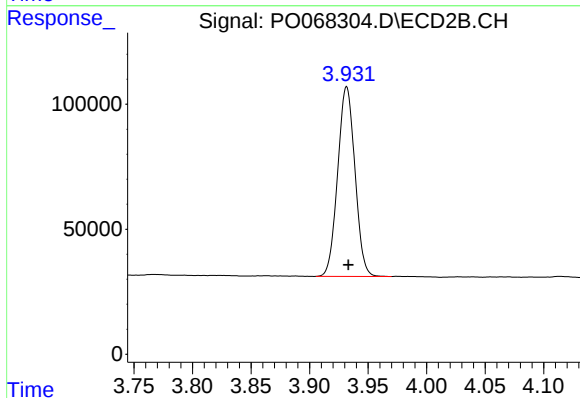


#1 Tetrachloro-m-xylene

R.T.: 3.932 min
Delta R.T.: -0.001 min
Response: 778769
Conc: 22.70 ng/ml

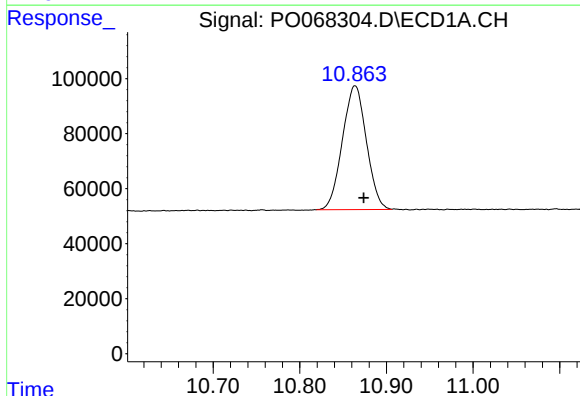


#2 Decachlorobiphenyl

R.T.: 10.863 min
Delta R.T.: -0.010 min
Response: 867027
Conc: 21.79 ng/ml m

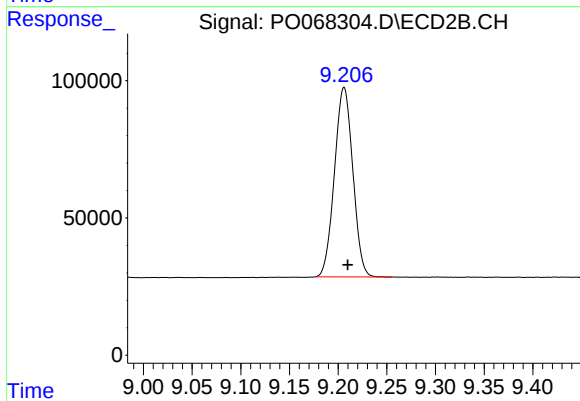

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.004 min
Response: 905999
Conc: 23.53 ng/ml

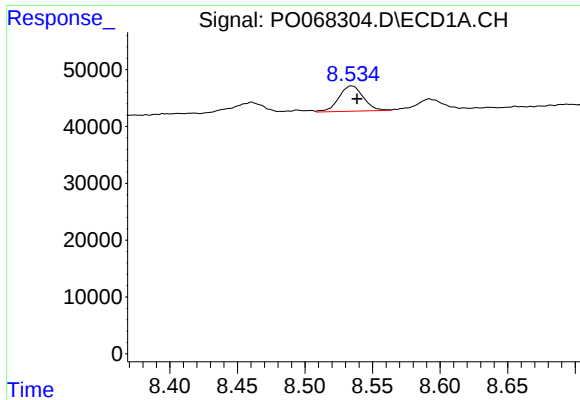


#36 AR-1262-1

R.T.: 8.535 min
Delta R.T.: -0.004 min
Response: 56065
Conc: 28.02 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:48 PM

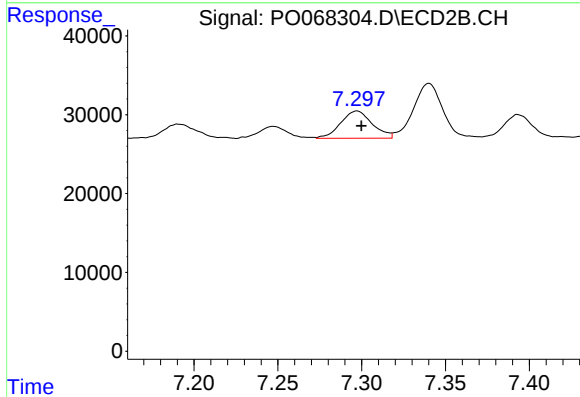


#36 AR-1262-1

R.T.: 7.297 min
Delta R.T.: -0.003 min
Response: 45567
Conc: 32.03 ng/ml

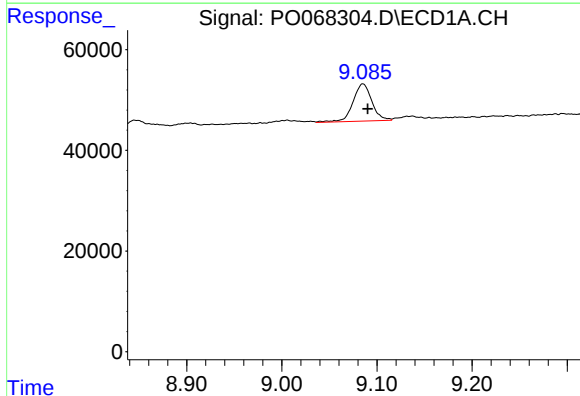


#37 AR-1262-2

R.T.: 9.085 min
Delta R.T.: -0.005 min
Response: 101883
Conc: 28.26 ng/ml

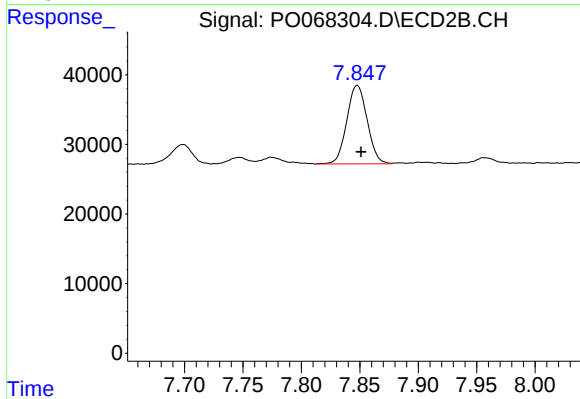

#37 AR-1262-2

R.T.: 7.848 min
Delta R.T.: -0.003 min
Response: 137338
Conc: 29.55 ng/ml

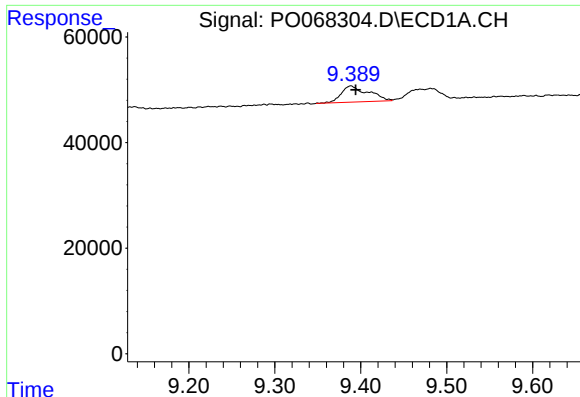


#38 AR-1262-3

R.T.: 9.389 min
Delta R.T.: -0.006 min
Response: 66567
Conc: 25.65 ng/ml m

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:48 PM

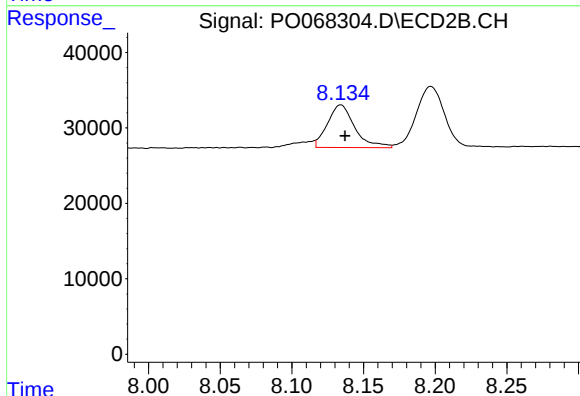


#38 AR-1262-3

R.T.: 8.134 min
Delta R.T.: -0.003 min
Response: 75040
Conc: 38.86 ng/ml m

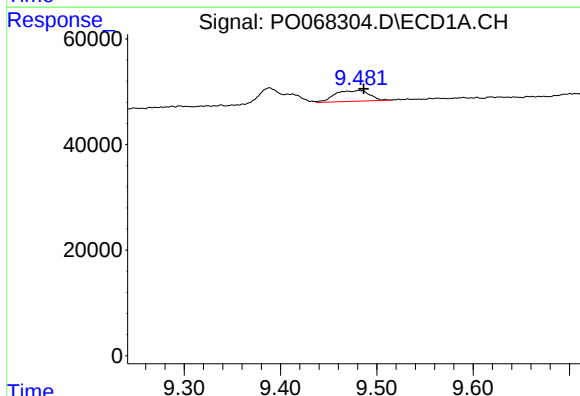


#39 AR-1262-4

R.T.: 9.481 min
Delta R.T.: -0.005 min
Response: 51480
Conc: 24.92 ng/ml

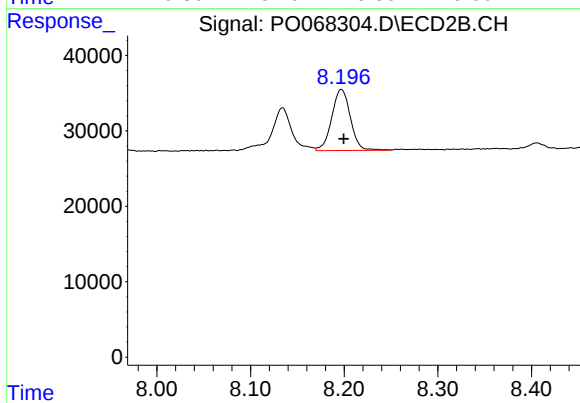

#39 AR-1262-4

R.T.: 8.197 min
Delta R.T.: -0.003 min
Response: 112038
Conc: 31.90 ng/ml

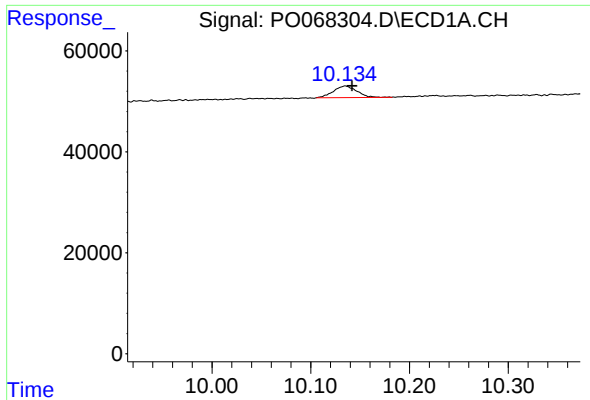


#40 AR-1262-5

R.T.: 10.135 min
Delta R.T.: -0.007 min
Response: 37450
Conc: 24.51 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020

Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:48 PM

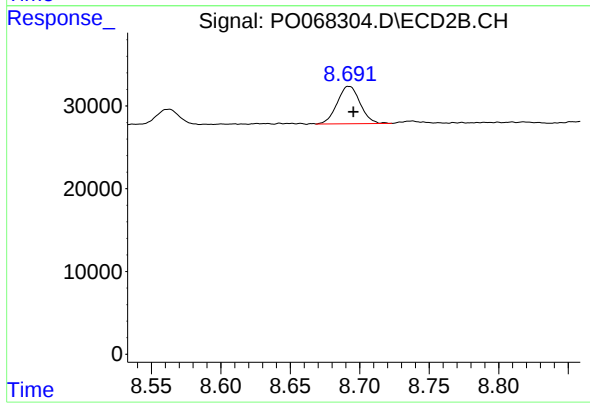

#40 AR-1262-5

R.T.: 8.692 min
Delta R.T.: -0.003 min
Response: 52181
Conc: 30.25 ng/ml