

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051220\
 Data File : P0068305.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2020 12:41
 Operator : DD\AJ
 Sample : L2182-09
 Misc : AR1268 25PPB MDL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 MDL-WATER-03-QT2-2020

Manual Integrations
 APPROVED

Sohil
 5/13/2020 2:22:53 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 23:44:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0050820.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 08 13:29:29 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.905	3.931	447257	535812	15.947	15.615
2)	SA Decachlor...	10.863	9.206	662337	706552	16.645m	18.352
Target Compounds							
41)	L9 AR-1268-1	9.388	8.133	126831	205336	26.637	36.488 #
42)	L9 AR-1268-2	9.483	8.198	122925	161252	26.872	31.520
43)	L9 AR-1268-3	9.703	8.405	110379	133768	27.911	31.551
44)	L9 AR-1268-4	10.134	8.693	47154	68187	26.420	33.693 #
45)	L9 AR-1268-5	10.537	8.968	342781	410322	26.402	31.160

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051220\
Data File : P0068305.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2020 12:41
Operator : DD\AJ
Sample : L2182-09
Misc : AR1268 25PPB MDL
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:53 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 23:44:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050820.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 08 13:29:29 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

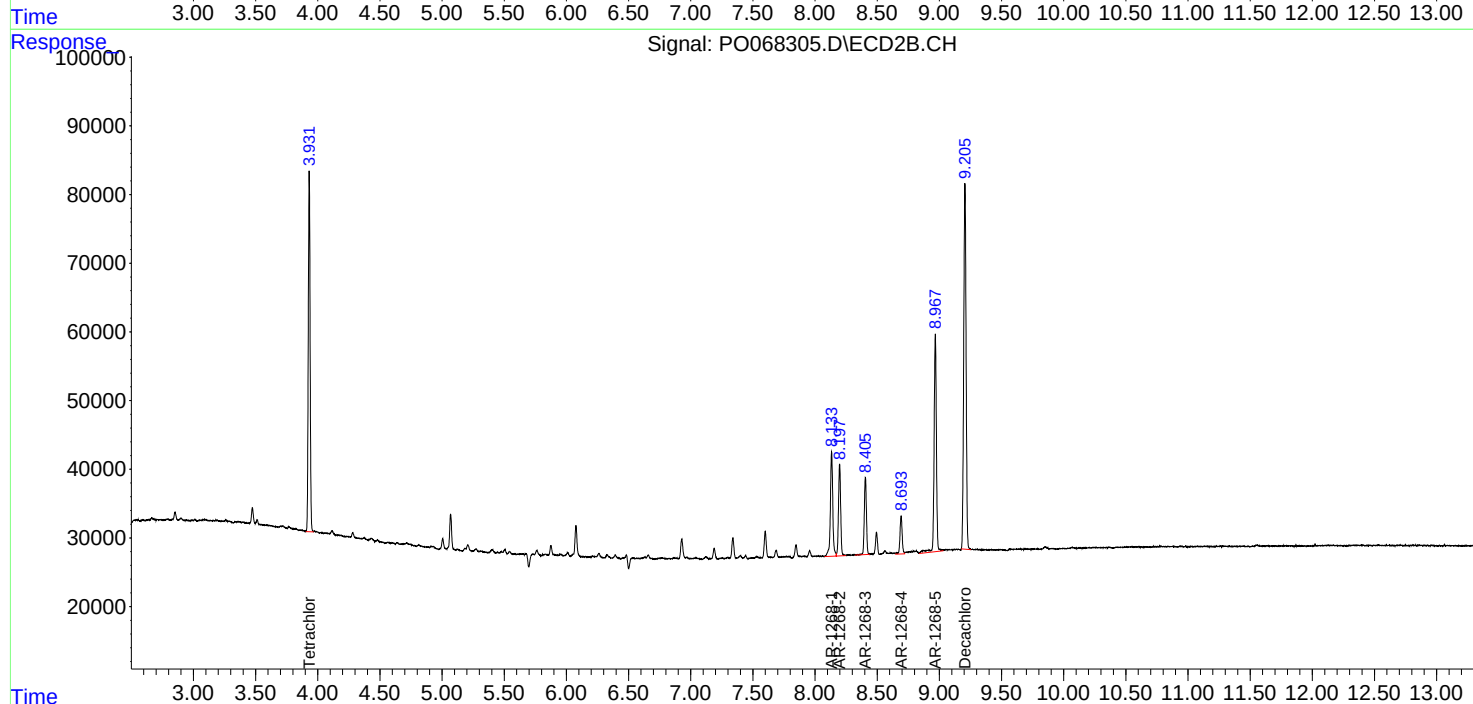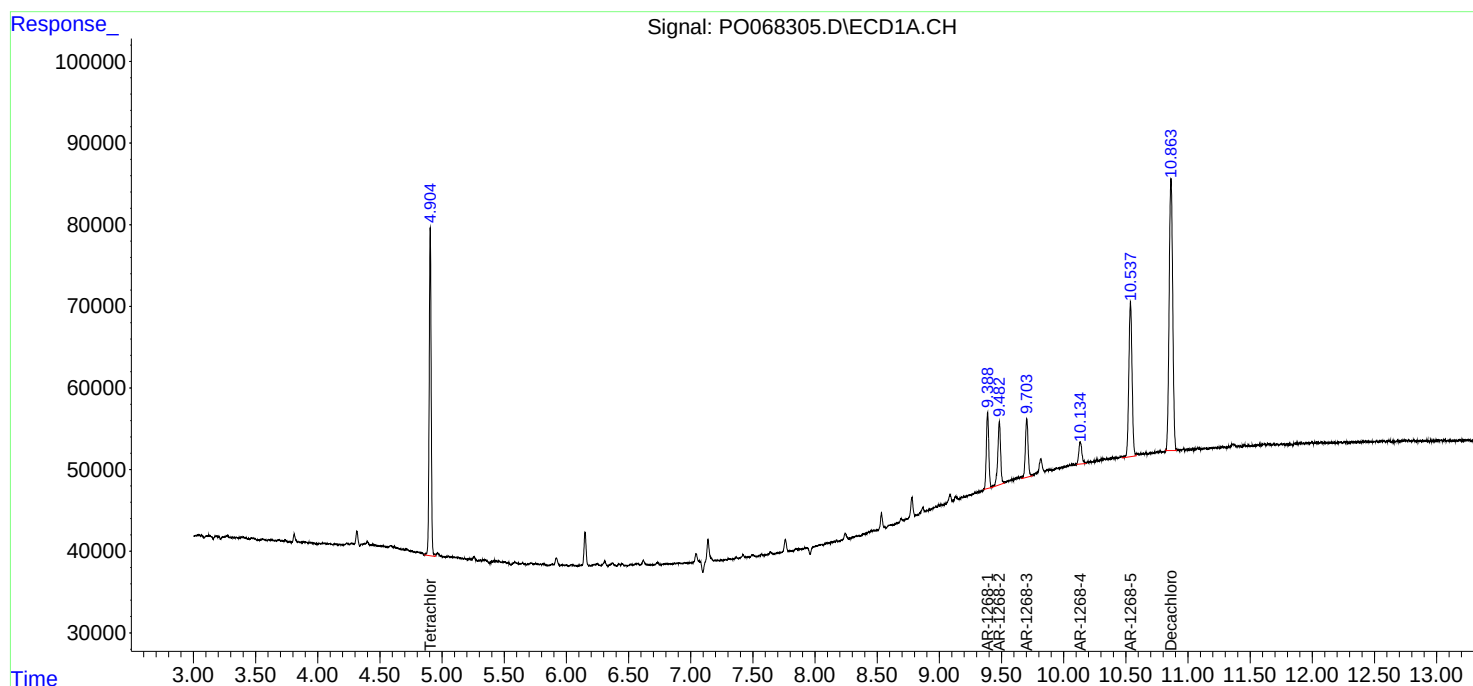

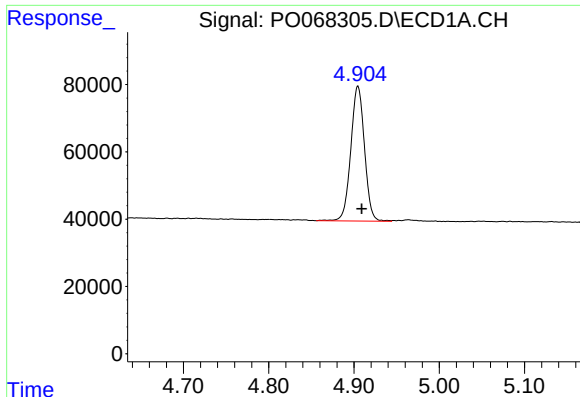


#1 Tetrachloro-m-xylene

R.T.: 4.905 min
Delta R.T.: -0.004 min
Response: 447257
Conc: 15.95 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:53 PM

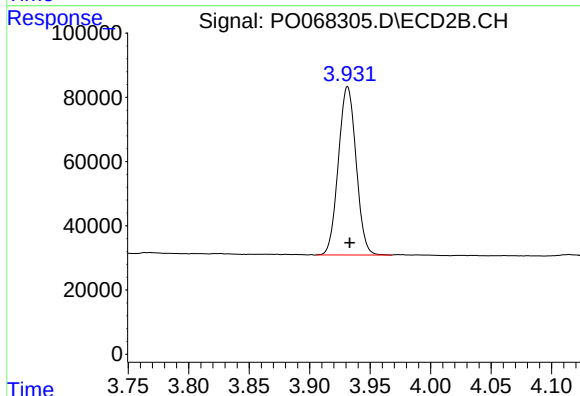


#1 Tetrachloro-m-xylene

R.T.: 3.931 min
Delta R.T.: -0.002 min
Response: 535812
Conc: 15.61 ng/ml

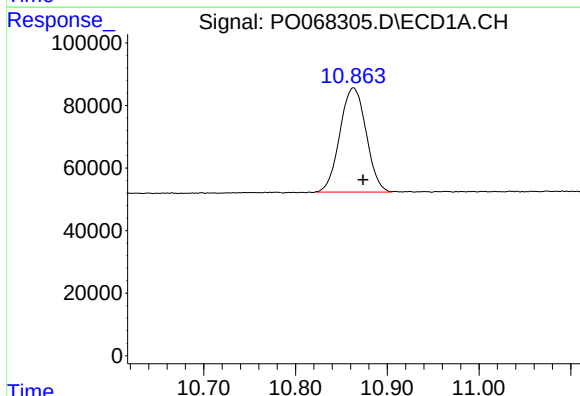


#2 Decachlorobiphenyl

R.T.: 10.863 min
Delta R.T.: -0.011 min
Response: 662337
Conc: 16.64 ng/ml m

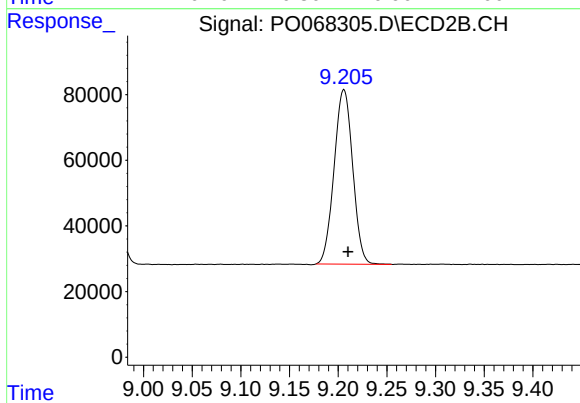

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.004 min
Response: 706552
Conc: 18.35 ng/ml

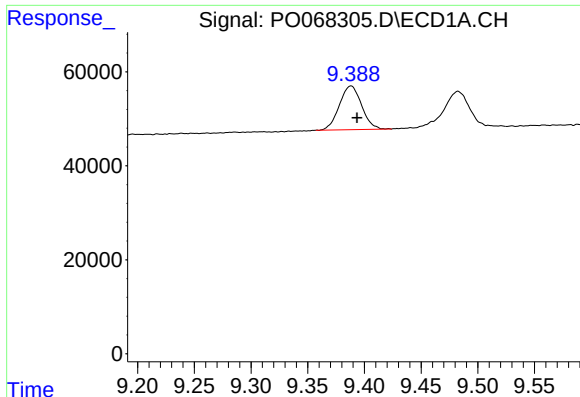


#41 AR-1268-1

R.T.: 9.388 min
Delta R.T.: -0.005 min
Response: 126831
Conc: 26.64 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020


Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:53 PM

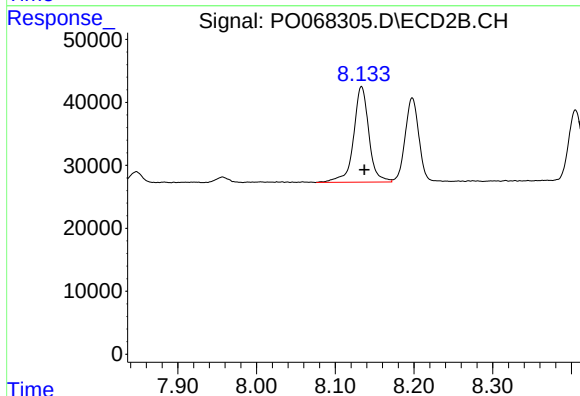


#41 AR-1268-1

R.T.: 8.133 min
Delta R.T.: -0.004 min
Response: 205336
Conc: 36.49 ng/ml

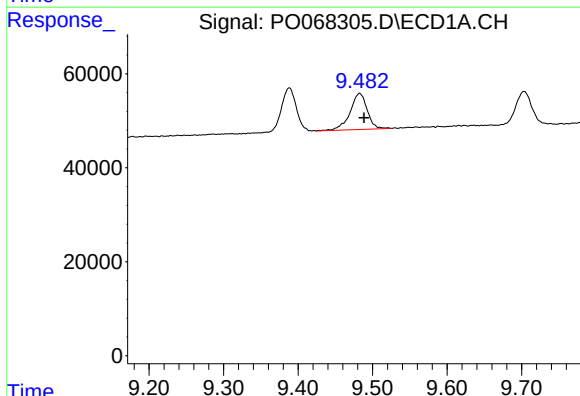


#42 AR-1268-2

R.T.: 9.483 min
Delta R.T.: -0.006 min
Response: 122925
Conc: 26.87 ng/ml

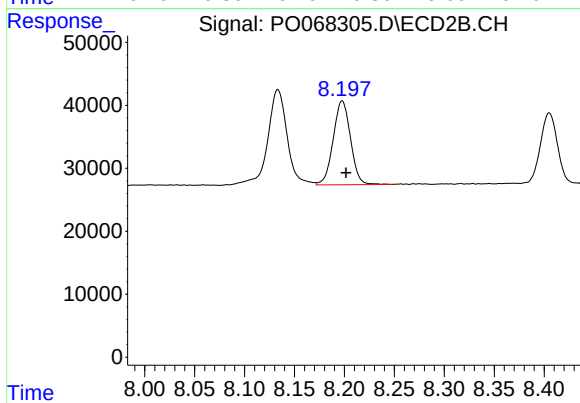

#42 AR-1268-2

R.T.: 8.198 min
Delta R.T.: -0.004 min
Response: 161252
Conc: 31.52 ng/ml

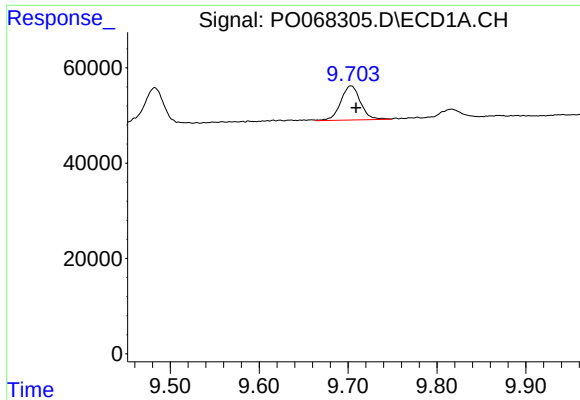


#43 AR-1268-3

R.T.: 9.703 min
Delta R.T.: -0.006 min
Response: 110379
Conc: 27.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020

Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:53 PM

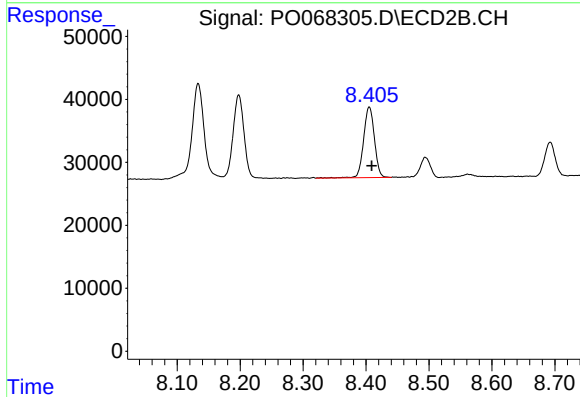


#43 AR-1268-3

R.T.: 8.405 min
Delta R.T.: -0.004 min
Response: 133768
Conc: 31.55 ng/ml


#44 AR-1268-4

R.T.: 10.134 min
Delta R.T.: -0.008 min
Response: 47154
Conc: 26.42 ng/ml

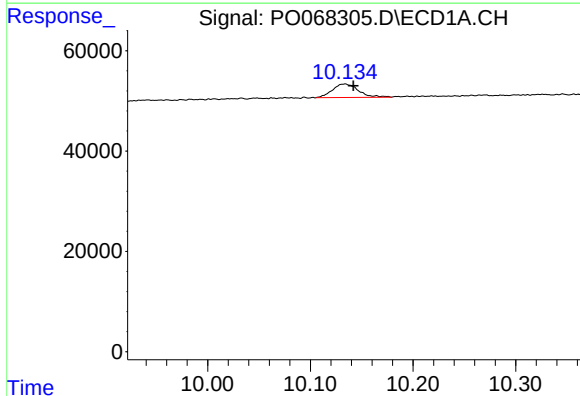

#44 AR-1268-4

R.T.: 8.693 min
Delta R.T.: -0.003 min
Response: 68187
Conc: 33.69 ng/ml

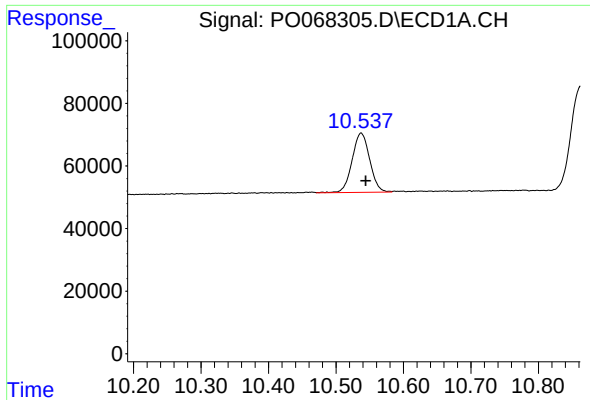


#45 AR-1268-5

R.T.: 10.537 min
Delta R.T.: -0.007 min
Response: 342781
Conc: 26.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2020

Manual Integrations
APPROVED

Sohil
5/13/2020 2:22:53 PM

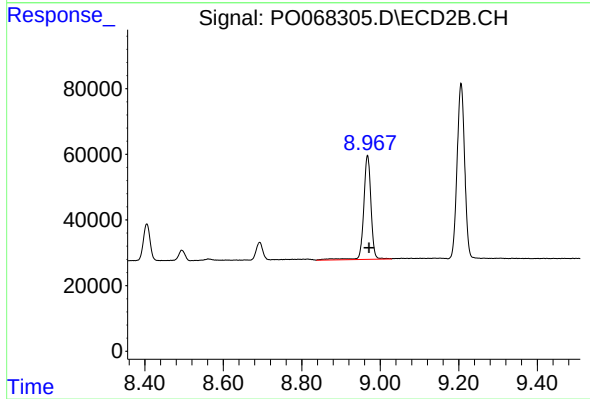

#45 AR-1268-5

R.T.: 8.968 min
Delta R.T.: -0.004 min
Response: 410322
Conc: 31.16 ng/ml