

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
 Data File : P0085994.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2022 22:46
 Operator : YP\AJ
 Sample : N2771-02 10X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-BC226656-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 07:12:31 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.478	3.680	211525	79727	2.083	1.829
2)	SA Decachlor...	10.327	8.747	133196	62185	2.513	1.832 #
Target Compounds							
3)	L1 AR-1016-1	5.654	4.799	33376	11587	10.444	7.419 #
4)	L1 AR-1016-2	5.684	4.799	5620	11587	1.264	5.533 #
5)	L1 AR-1016-3	5.740	4.997	17163	6438	6.259	5.824
6)	L1 AR-1016-4	5.885f	4.997	23143	6438	10.441	6.983 #
7)	L1 AR-1016-5	6.141	5.241	22064	4658	10.648	4.125 #
8)	L2 AR-1221-1	0.000	3.911	0	6643	N.D.	12.919 #
9)	L2 AR-1221-2	4.815	0.000	6633	0	7.266	N.D. #
10)	L2 AR-1221-3	4.888	0.000	22851	0	8.479	N.D. #
11)	L3 AR-1232-1	4.888	0.000	22851	0	11.163	N.D. #
12)	L3 AR-1232-2	5.350f	4.799	15694	11587	16.664	14.214
13)	L3 AR-1232-3	5.684	4.997	5620	6438	3.198	15.592 #
14)	L3 AR-1232-4	5.885f	0.000	23143	0	26.604	N.D. #
15)	L3 AR-1232-5	5.937	5.241	13116	4658	19.807	11.121 #
16)	L4 AR-1242-1	5.654	4.799	33376	11587	12.278	8.772 #
17)	L4 AR-1242-2	5.684	4.799	5620	11587	1.495	6.608 #
18)	L4 AR-1242-3	5.740	4.997	17163	6438	7.305	6.846
19)	L4 AR-1242-4	5.885f	0.000	23143	0	12.210	N.D. #
20)	L4 AR-1242-5	6.544f	5.568	1638	3951	0.895	3.474 #
21)	L5 AR-1248-1	5.654	4.799	33376	11587	16.524	11.933 #
22)	L5 AR-1248-2	5.937	4.997	13116	6438	4.862	4.840
23)	L5 AR-1248-3	6.141	0.000	22064	0	7.436	N.D. #
24)	L5 AR-1248-4	6.544	5.241	1638	4658	0.509	2.909 #
25)	L5 AR-1248-5	6.544f	0.000	1638	0	0.526	N.D. #
26)	L6 AR-1254-1	6.523	5.568	13673	3951	4.063	1.569 #
27)	L6 AR-1254-2	6.750	5.786f	24313	10619	4.941	4.849
28)	L6 AR-1254-3	7.112	0.000	11037	0	2.185	N.D. #
29)	L6 AR-1254-4	7.366	6.325f	4153	15672	1.115	7.084 #
30)	L6 AR-1254-5	7.819	6.798	21122	7921	5.421	2.678 #
31)	L7 AR-1260-1	7.241f	6.276	11359	10612	3.753	5.452 #
32)	L7 AR-1260-2	7.535	6.487	19834	19228	5.483	8.181 #
33)	L7 AR-1260-3	7.896	0.000	21353	0	7.736	N.D. #
34)	L7 AR-1260-4	8.124	7.098	1717	6910	0.509	3.838 #
35)	L7 AR-1260-5	8.454	7.338	45061	14812	7.302	3.419 #
36)	L8 AR-1262-1	7.896	6.837	21353	9820	4.721	3.250 #
37)	L8 AR-1262-2	8.454	7.338	45061	14812	5.757	2.696 #
38)	L8 AR-1262-3	8.771	7.623	39035	30519	11.916	14.478
39)	L8 AR-1262-4	8.855	7.688	1394	27026	0.603	6.818 #
40)	L8 AR-1262-5	0.000	8.184	0	13419	N.D.	7.491 #
41)	L9 AR-1268-1	8.771	7.623	39035	30519	4.471	5.002

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
Data File : P0085994.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2022 22:46
Operator : YP\AJ
Sample : N2771-02 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:12:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.855	7.688	1394	27026	0.174	4.923 #
43)	L9 AR-1268-3	9.162f	7.899	6030	2257	0.909	0.496 #
44)	L9 AR-1268-4	0.000	8.184	0	13419	N.D.	6.873 #
45)	L9 AR-1268-5	0.000	8.482	0	20228	N.D.	1.380 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
Data File : P0085994.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2022 22:46
Operator : YP\AJ
Sample : N2771-02 10X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:12:31 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

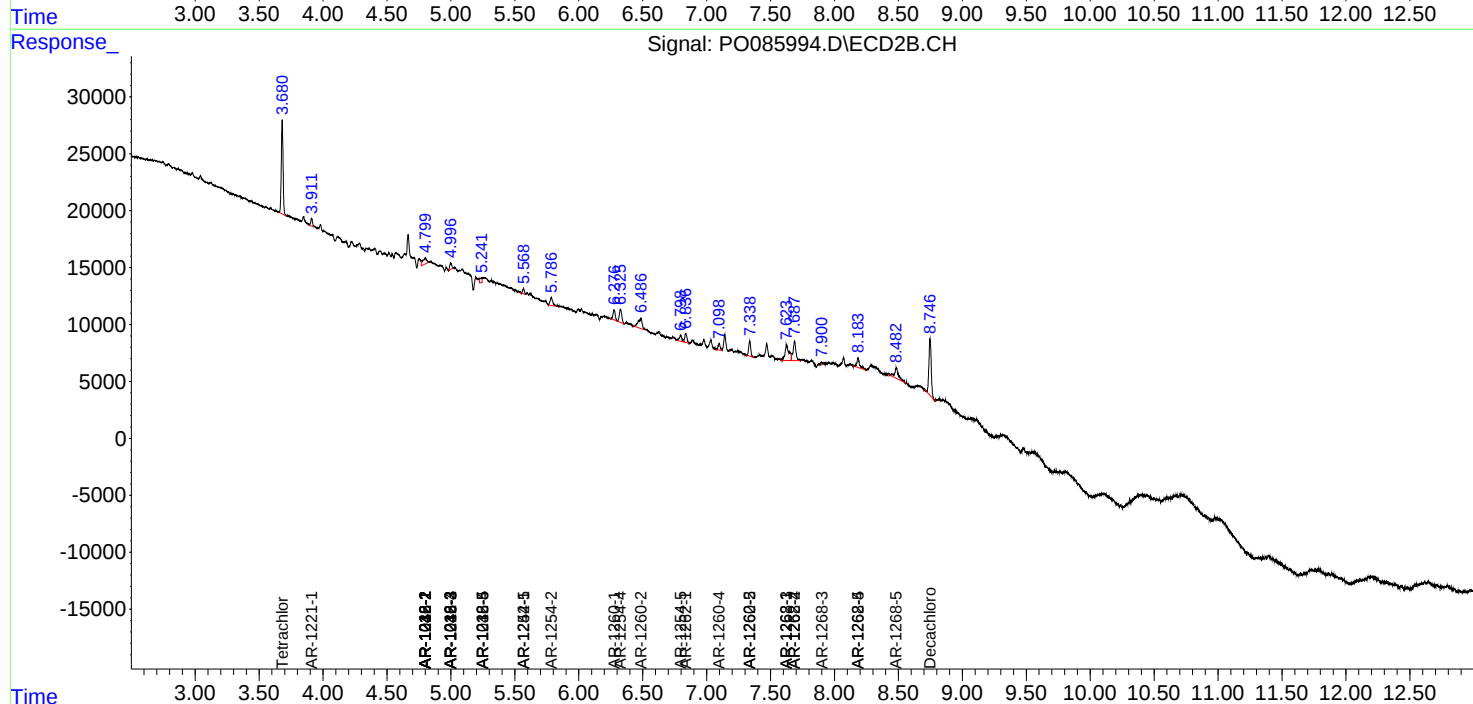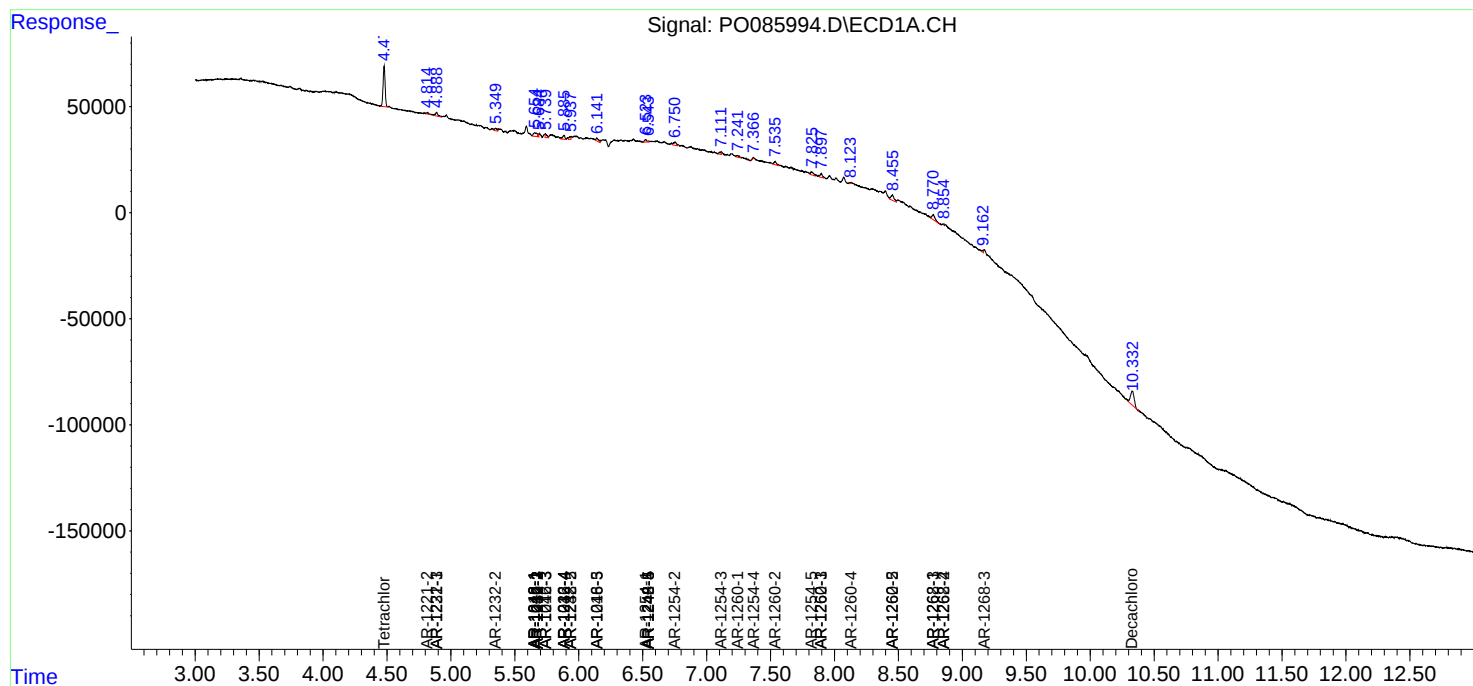


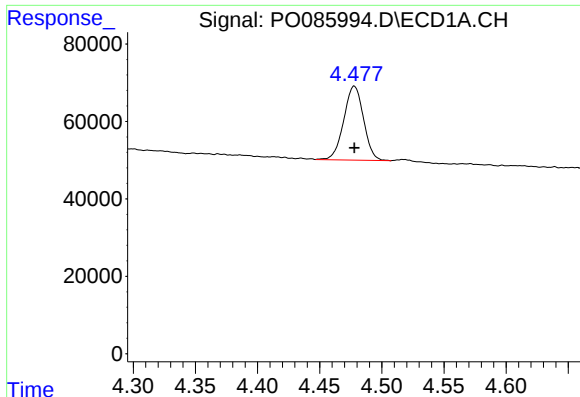

#1 Tetrachloro-m-xylene


R.T.: 4.478 min
Delta R.T.: 0.000 min
Response: 211525
Conc: 2.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

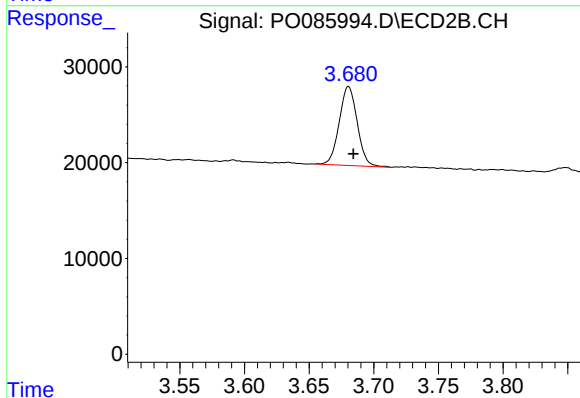


#1 Tetrachloro-m-xylene

R.T.: 3.680 min
Delta R.T.: -0.004 min
Response: 79727
Conc: 1.83 ng/ml

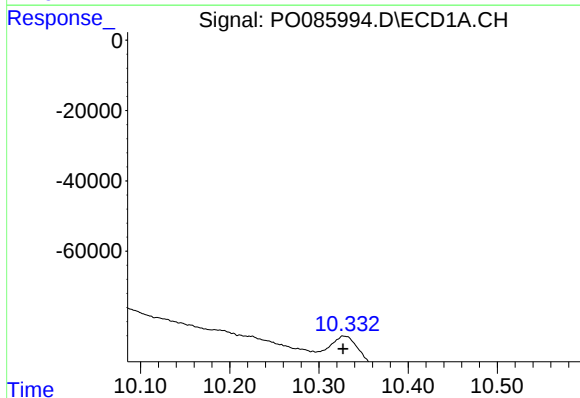


#2 Decachlorobiphenyl

R.T.: 10.327 min
Delta R.T.: 0.000 min
Response: 133196
Conc: 2.51 ng/ml

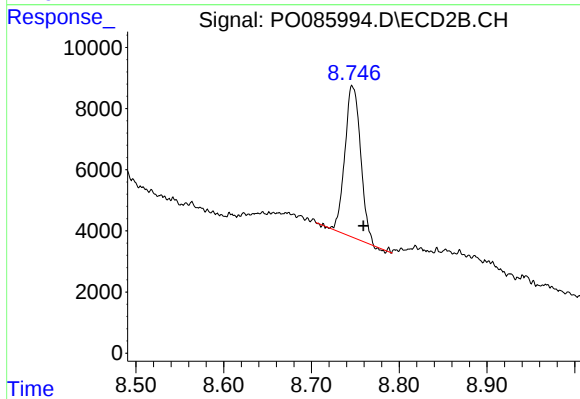

#2 Decachlorobiphenyl


R.T.: 8.747 min
Delta R.T.: -0.013 min
Response: 62185
Conc: 1.83 ng/ml

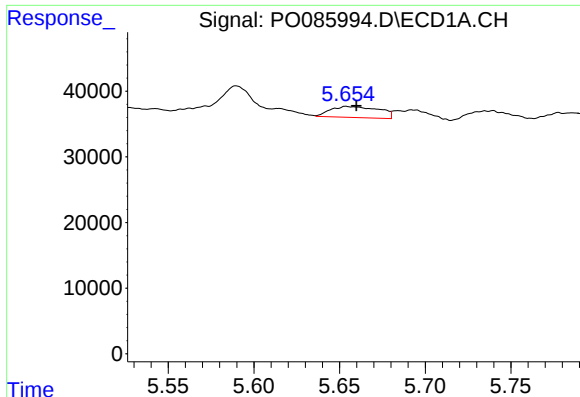

#3 AR-1016-1


R.T.: 5.654 min
Delta R.T.: -0.006 min
Response: 33376
Conc: 10.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

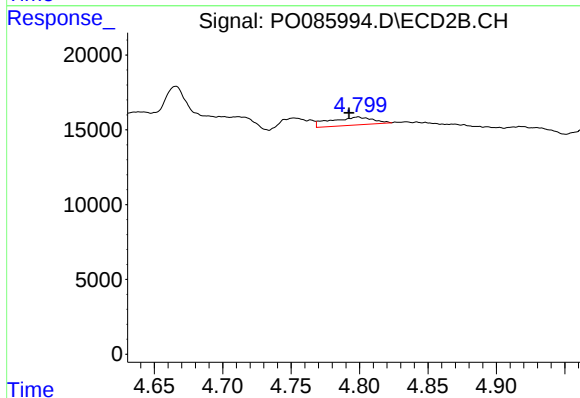


#3 AR-1016-1

R.T.: 4.799 min
Delta R.T.: 0.007 min
Response: 11587
Conc: 7.42 ng/ml

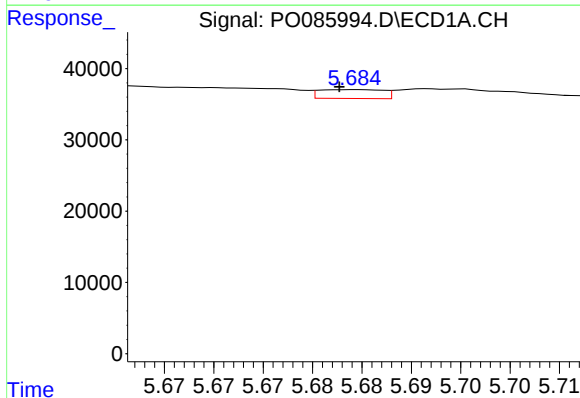


#4 AR-1016-2

R.T.: 5.684 min
Delta R.T.: 0.002 min
Response: 5620
Conc: 1.26 ng/ml

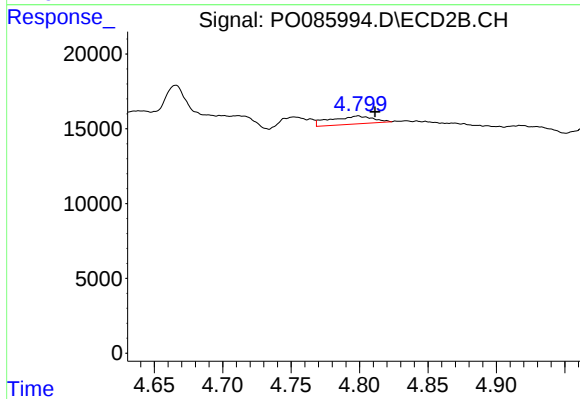

#4 AR-1016-2


R.T.: 4.799 min
Delta R.T.: -0.012 min
Response: 11587
Conc: 5.53 ng/ml

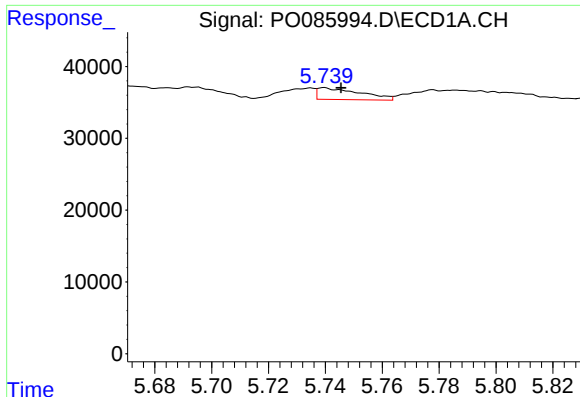

#5 AR-1016-3


R.T.: 5.740 min
Delta R.T.: -0.006 min
Response: 17163
Conc: 6.26 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

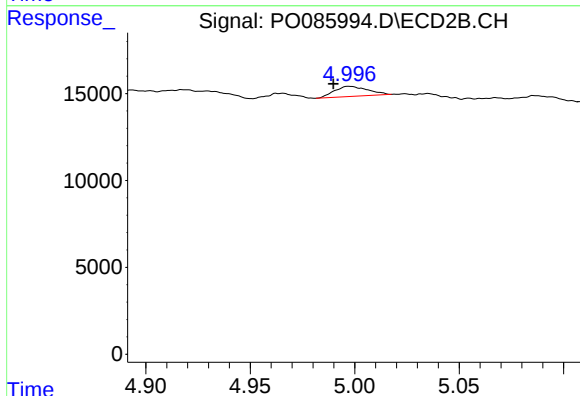


#5 AR-1016-3

R.T.: 4.997 min
Delta R.T.: 0.007 min
Response: 6438
Conc: 5.82 ng/ml

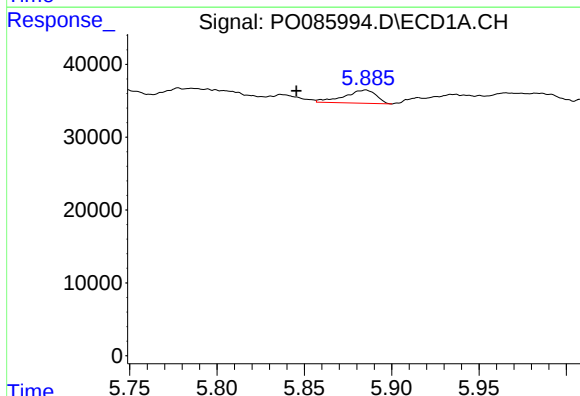


#6 AR-1016-4

R.T.: 5.885 min
Delta R.T.: 0.040 min
Response: 23143
Conc: 10.44 ng/ml

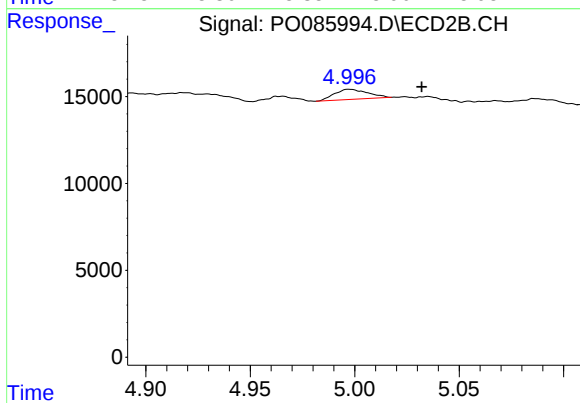

#6 AR-1016-4


R.T.: 4.997 min
Delta R.T.: -0.035 min
Response: 6438
Conc: 6.98 ng/ml

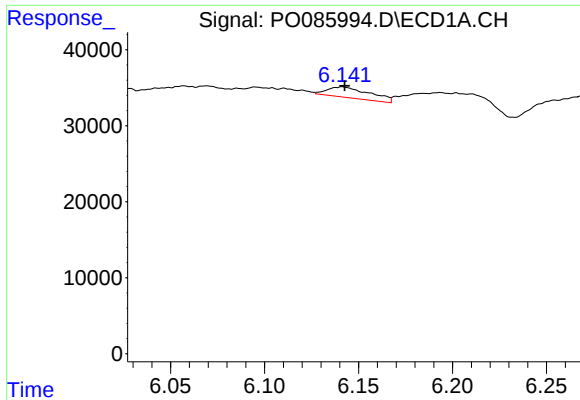

#7 AR-1016-5


R.T.: 6.141 min
Delta R.T.: -0.001 min
Response: 22064
Conc: 10.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

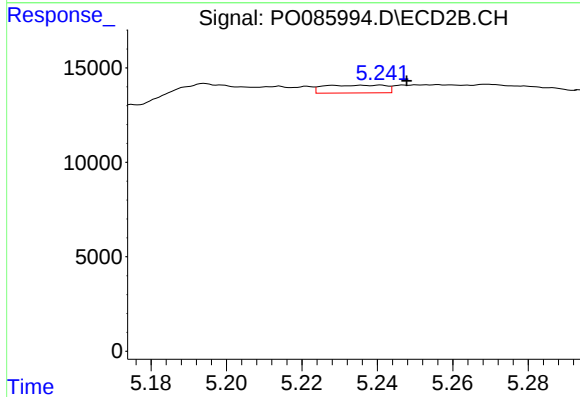


#7 AR-1016-5

R.T.: 5.241 min
Delta R.T.: -0.007 min
Response: 4658
Conc: 4.13 ng/ml

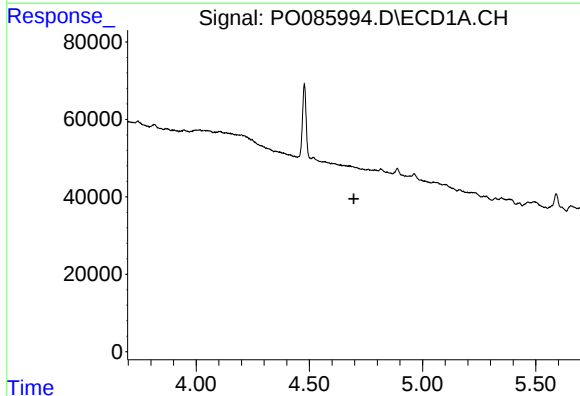


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.696 min
Response: 0
Conc: N.D.

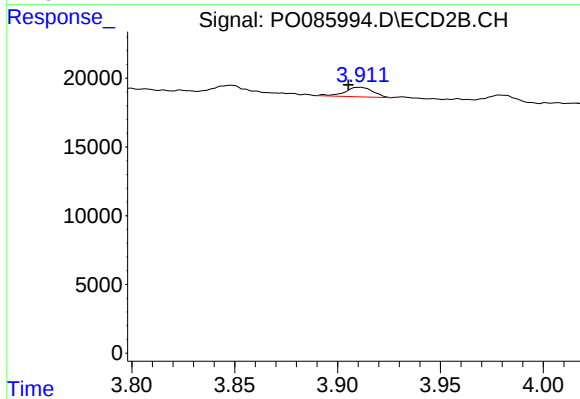

#8 AR-1221-1


R.T.: 3.911 min
Delta R.T.: 0.006 min
Response: 6643
Conc: 12.92 ng/ml

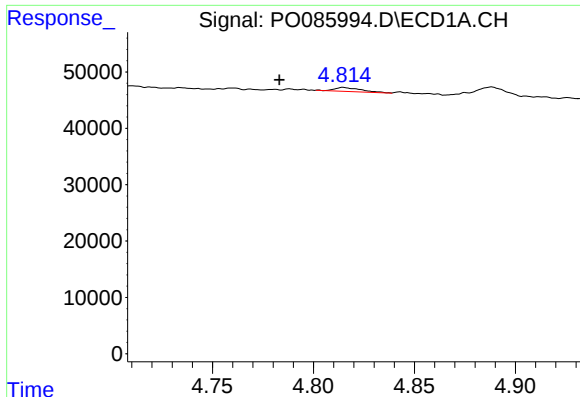

#9 AR-1221-2


R.T.: 4.815 min
Delta R.T.: 0.031 min
Response: 6633
Conc: 7.27 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

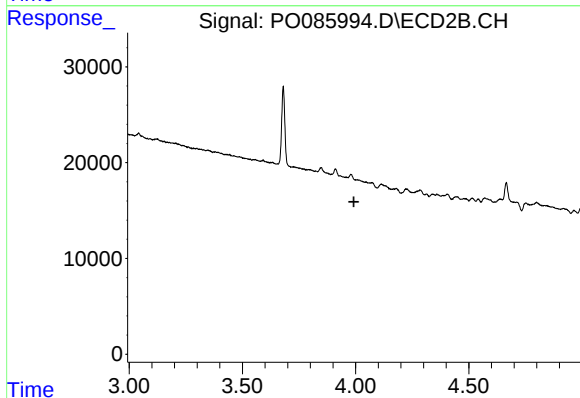


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.993 min
Response: 0
Conc: N.D.

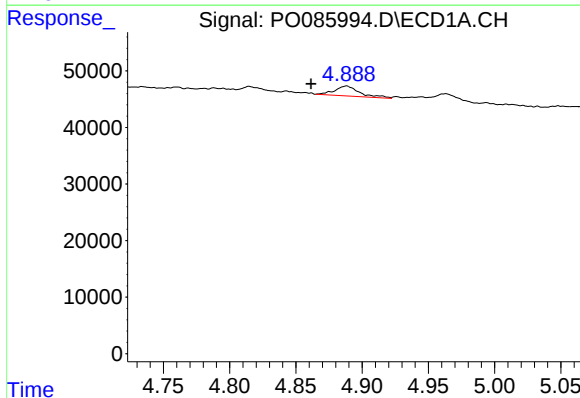


#10 AR-1221-3

R.T.: 4.888 min
Delta R.T.: 0.027 min
Response: 22851
Conc: 8.48 ng/ml

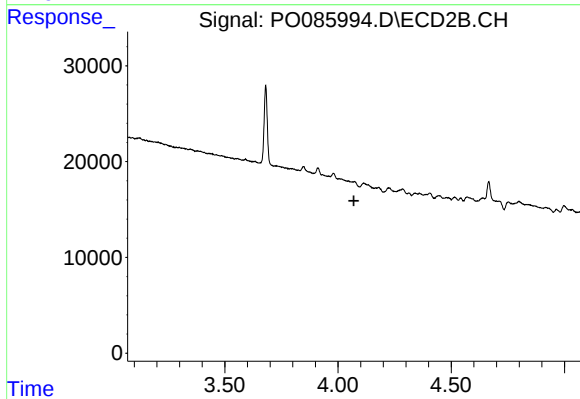

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.070 min
Response: 0
Conc: N.D.

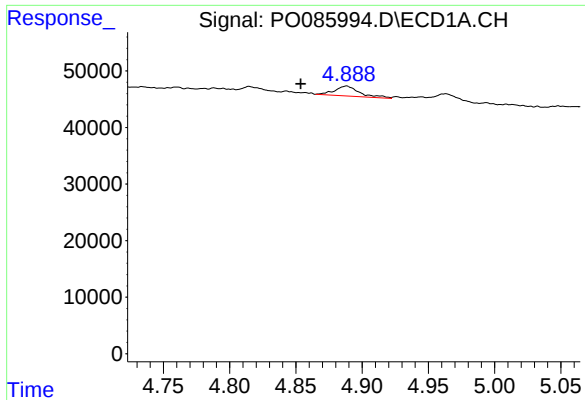

#11 AR-1232-1


R.T.: 4.888 min
Delta R.T.: 0.035 min
Response: 22851
Conc: 11.16 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

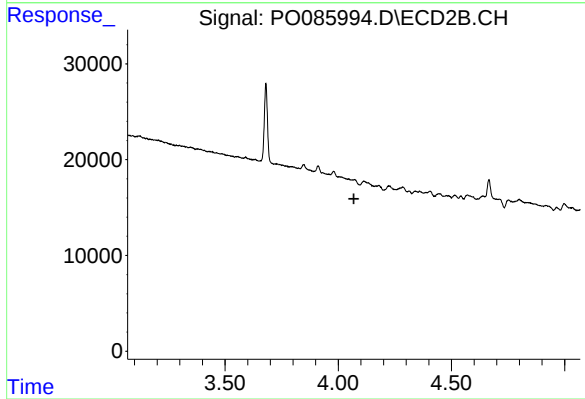


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.069 min
Response: 0
Conc: N.D.

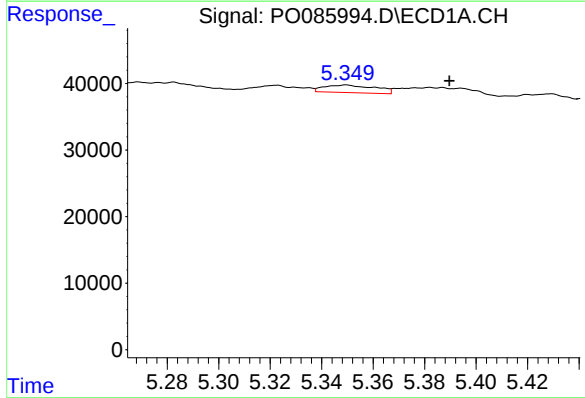


#12 AR-1232-2

R.T.: 5.350 min
Delta R.T.: -0.040 min
Response: 15694
Conc: 16.66 ng/ml

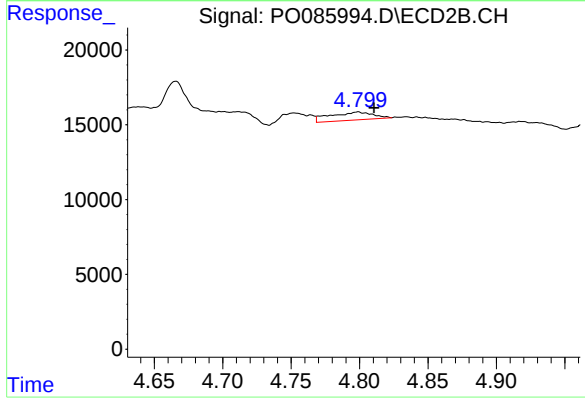

#12 AR-1232-2


R.T.: 4.799 min
Delta R.T.: -0.012 min
Response: 11587
Conc: 14.21 ng/ml

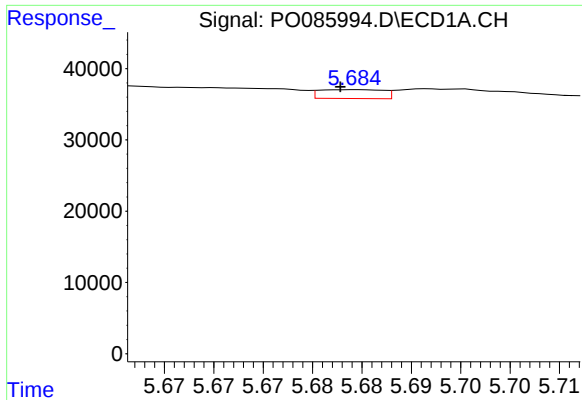

#13 AR-1232-3


R.T.: 5.684 min
Delta R.T.: 0.002 min
Response: 5620
Conc: 3.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

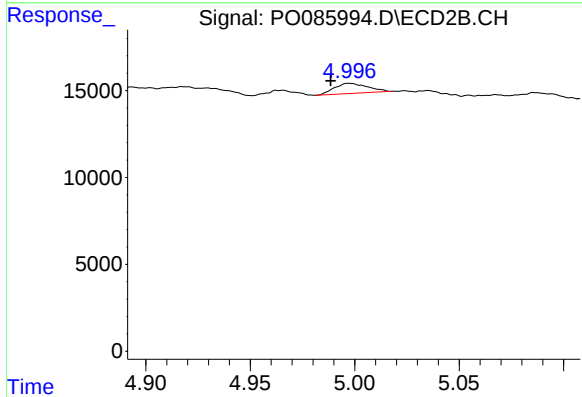


#13 AR-1232-3

R.T.: 4.997 min
Delta R.T.: 0.009 min
Response: 6438
Conc: 15.59 ng/ml

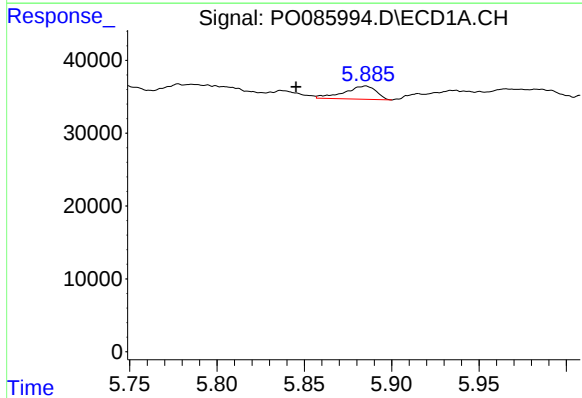


#14 AR-1232-4

R.T.: 5.885 min
Delta R.T.: 0.040 min
Response: 23143
Conc: 26.60 ng/ml

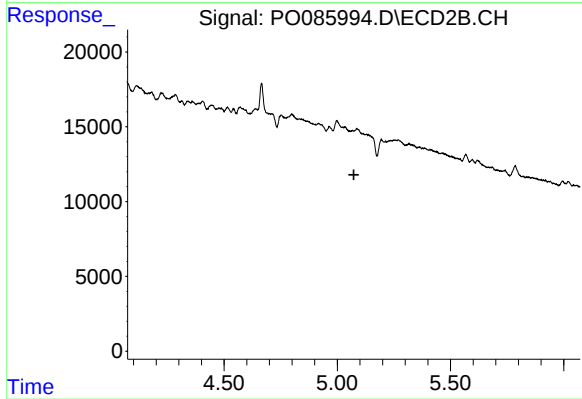

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 5.073 min
Response: 0
Conc: N.D.

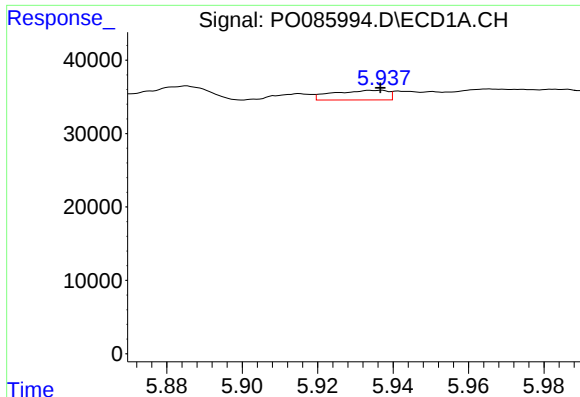

#15 AR-1232-5


R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 13116
Conc: 19.81 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

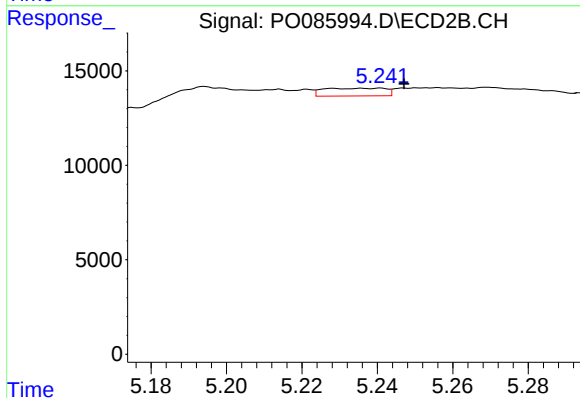


#15 AR-1232-5

R.T.: 5.241 min
Delta R.T.: -0.006 min
Response: 4658
Conc: 11.12 ng/ml

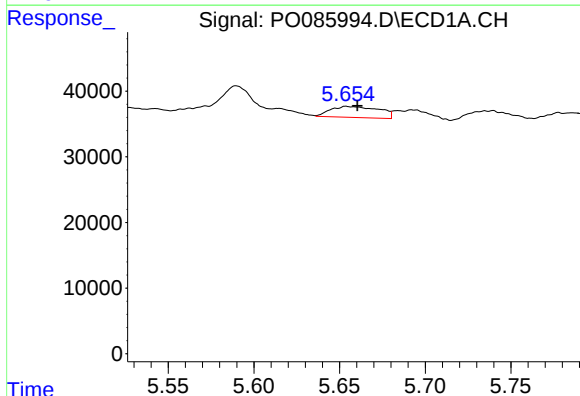


#16 AR-1242-1

R.T.: 5.654 min
Delta R.T.: -0.007 min
Response: 33376
Conc: 12.28 ng/ml

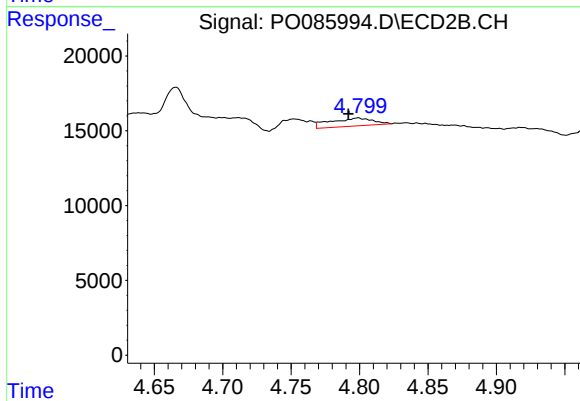

#16 AR-1242-1


R.T.: 4.799 min
Delta R.T.: 0.007 min
Response: 11587
Conc: 8.77 ng/ml

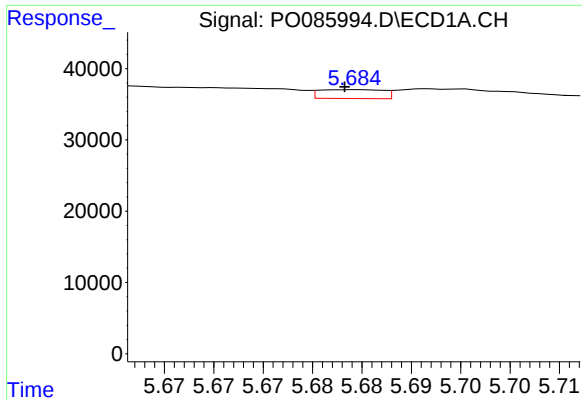

#17 AR-1242-2


R.T.: 5.684 min
Delta R.T.: 0.001 min
Response: 5620
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

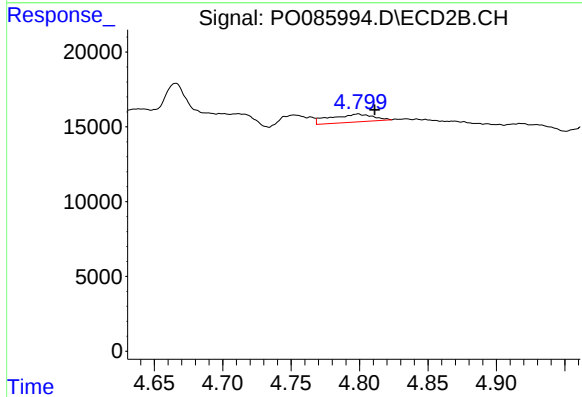


#17 AR-1242-2

R.T.: 4.799 min
Delta R.T.: -0.012 min
Response: 11587
Conc: 6.61 ng/ml

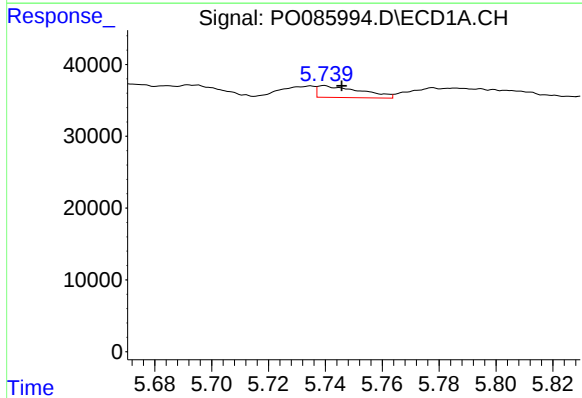


#18 AR-1242-3

R.T.: 5.740 min
Delta R.T.: -0.006 min
Response: 17163
Conc: 7.30 ng/ml

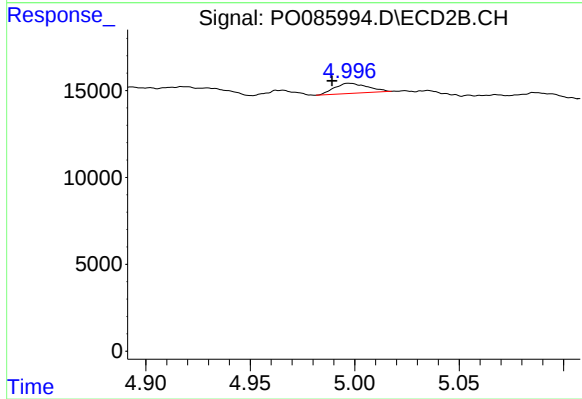

#18 AR-1242-3


R.T.: 4.997 min
Delta R.T.: 0.008 min
Response: 6438
Conc: 6.85 ng/ml

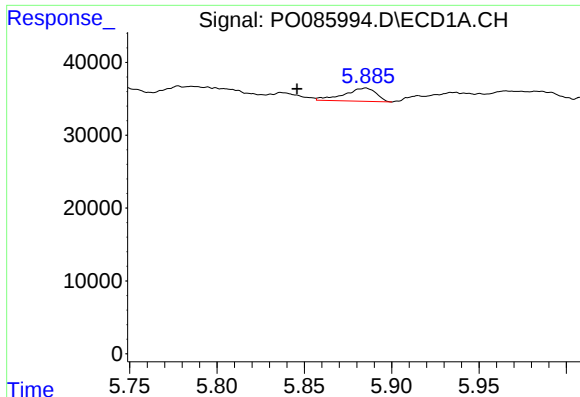

#19 AR-1242-4


R.T.: 5.885 min
Delta R.T.: 0.039 min
Response: 23143
Conc: 12.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

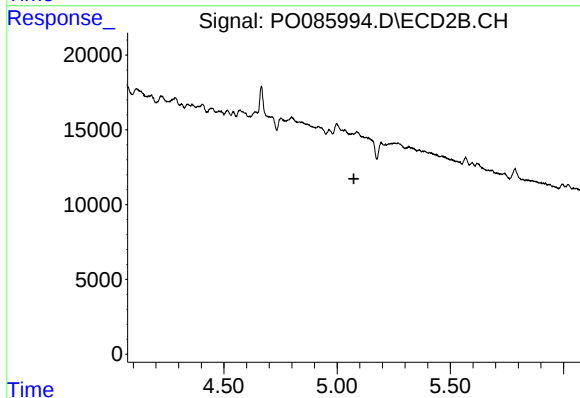


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.074 min
Response: 0
Conc: N.D.

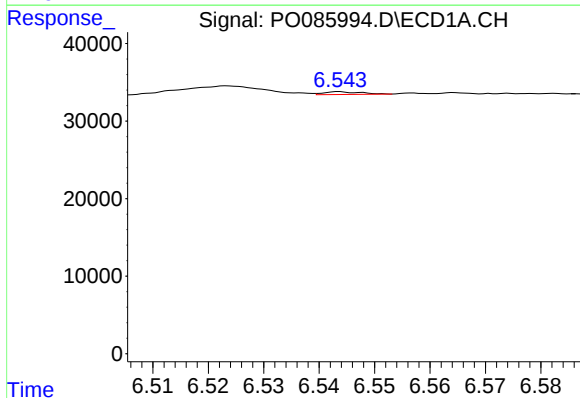


#20 AR-1242-5

R.T.: 6.544 min
Delta R.T.: -0.044 min
Response: 1638
Conc: 0.89 ng/ml

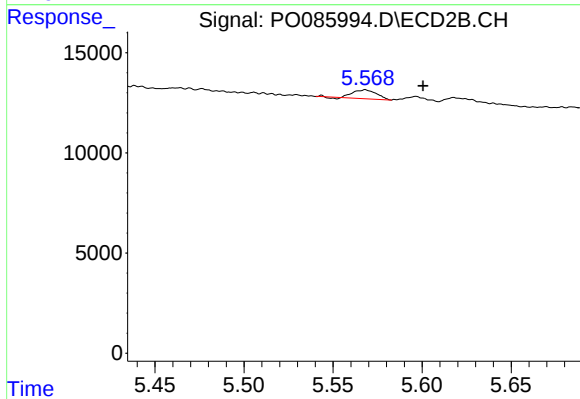

#20 AR-1242-5


R.T.: 5.568 min
Delta R.T.: -0.032 min
Response: 3951
Conc: 3.47 ng/ml

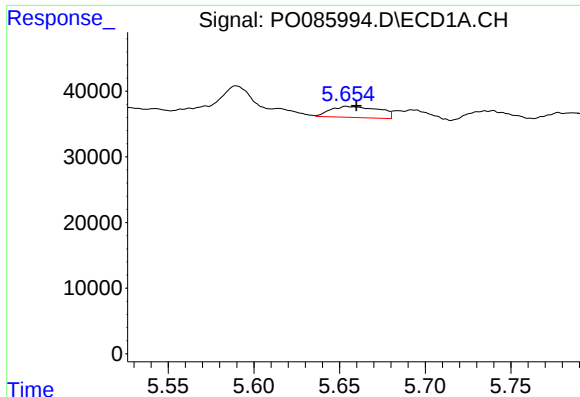

#21 AR-1248-1


R.T.: 5.654 min
Delta R.T.: -0.006 min
Response: 33376
Conc: 16.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

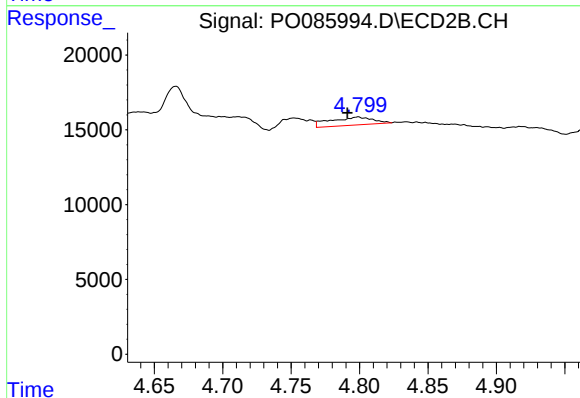


#21 AR-1248-1

R.T.: 4.799 min
Delta R.T.: 0.008 min
Response: 11587
Conc: 11.93 ng/ml

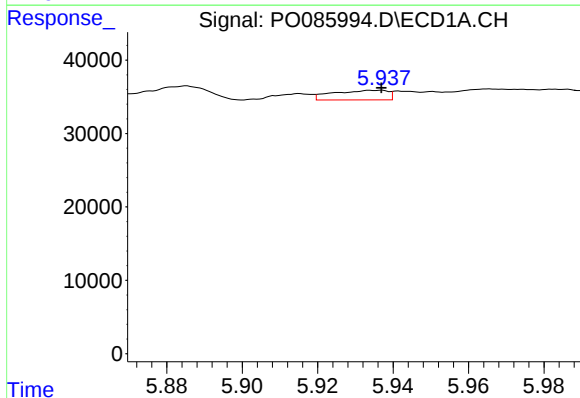


#22 AR-1248-2

R.T.: 5.937 min
Delta R.T.: 0.000 min
Response: 13116
Conc: 4.86 ng/ml

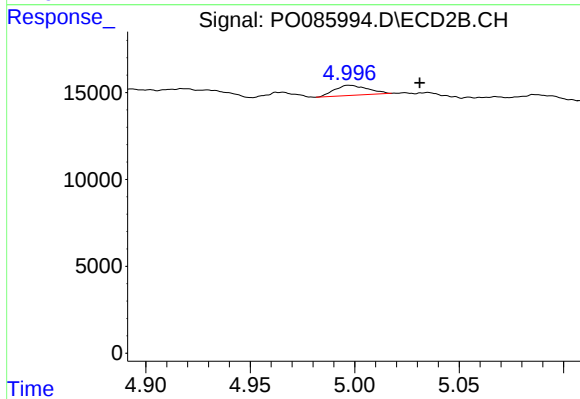

#22 AR-1248-2


R.T.: 4.997 min
Delta R.T.: -0.034 min
Response: 6438
Conc: 4.84 ng/ml

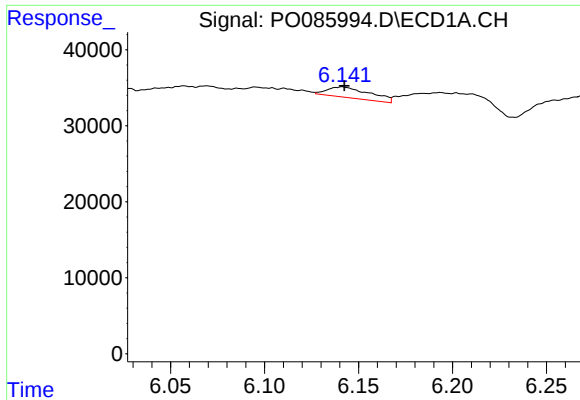

#23 AR-1248-3


R.T.: 6.141 min
Delta R.T.: -0.001 min
Response: 22064
Conc: 7.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

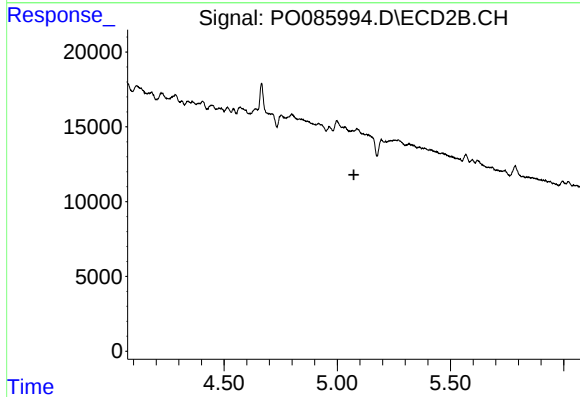


#23 AR-1248-3

R.T.: 0.000 min
Exp R.T. : 5.073 min
Response: 0
Conc: N.D.

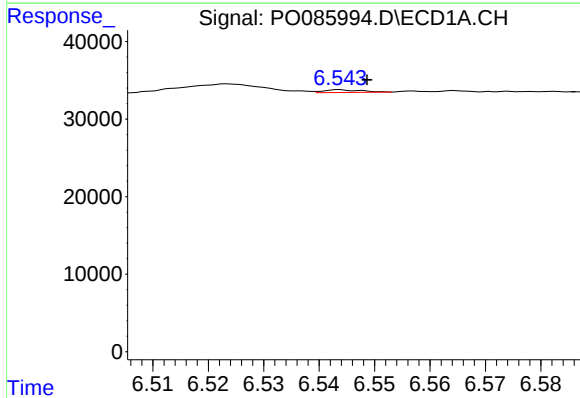


#24 AR-1248-4

R.T.: 6.544 min
Delta R.T.: -0.005 min
Response: 1638
Conc: 0.51 ng/ml

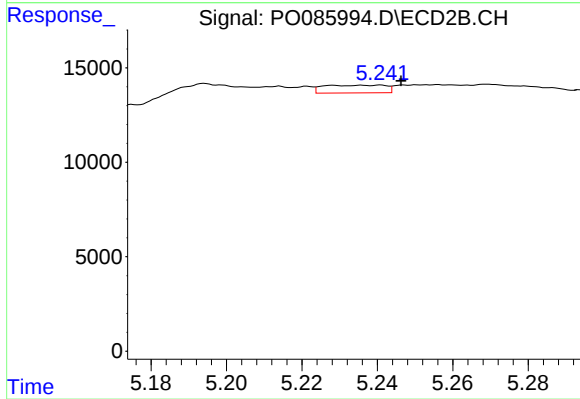

#24 AR-1248-4


R.T.: 5.241 min
Delta R.T.: -0.005 min
Response: 4658
Conc: 2.91 ng/ml

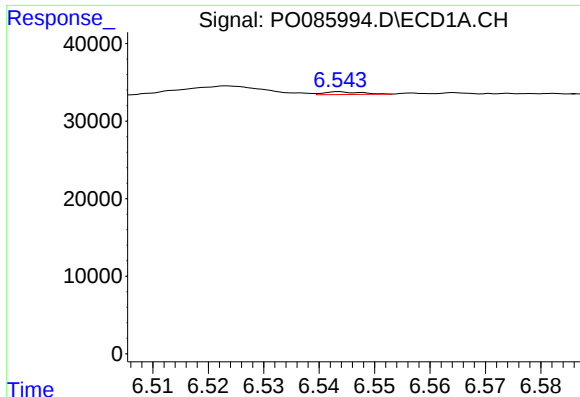

#25 AR-1248-5


R.T.: 6.544 min
Delta R.T.: -0.044 min
Response: 1638
Conc: 0.53 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

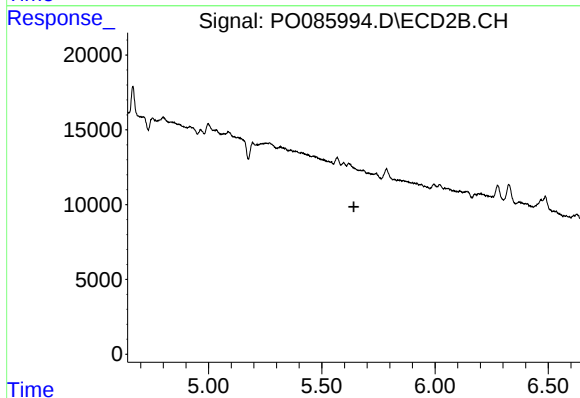


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 5.642 min
Response: 0
Conc: N.D.

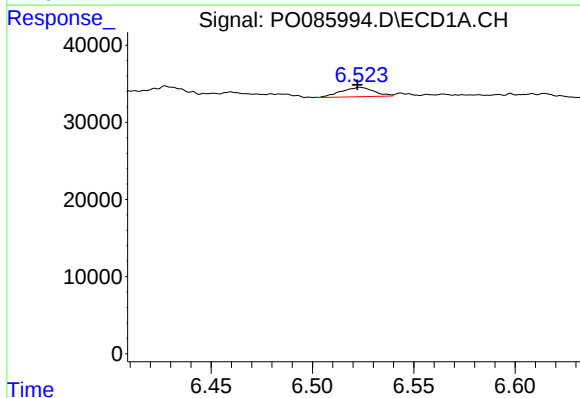


#26 AR-1254-1

R.T.: 6.523 min
Delta R.T.: 0.001 min
Response: 13673
Conc: 4.06 ng/ml

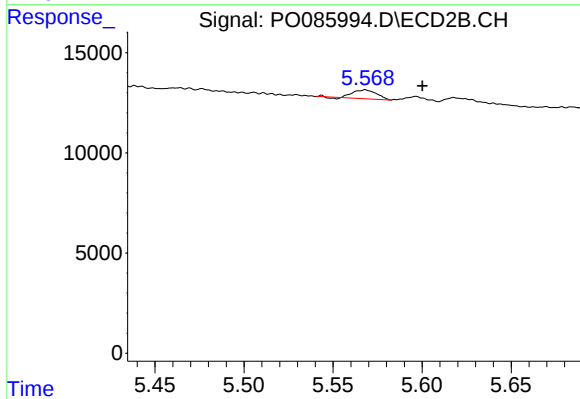

#26 AR-1254-1


R.T.: 5.568 min
Delta R.T.: -0.032 min
Response: 3951
Conc: 1.57 ng/ml

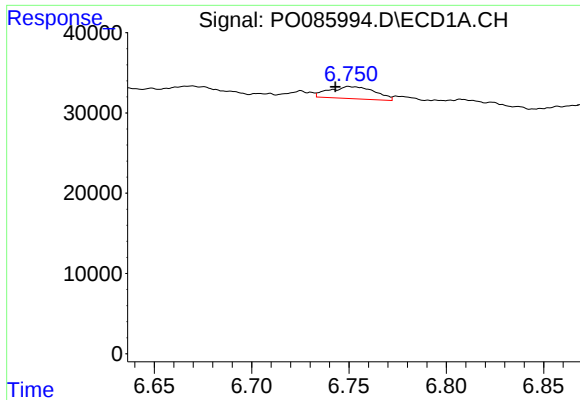

#27 AR-1254-2


R.T.: 6.750 min
Delta R.T.: 0.007 min
Response: 24313
Conc: 4.94 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

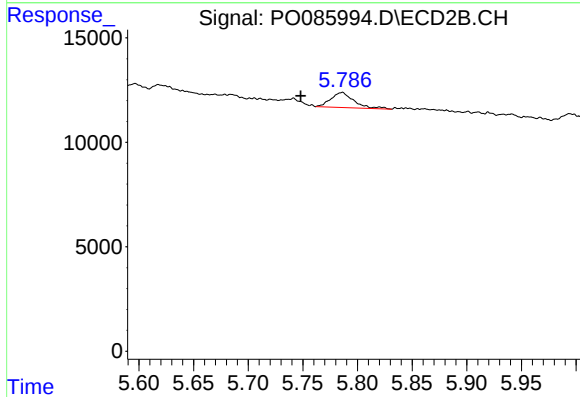


#27 AR-1254-2

R.T.: 5.786 min
Delta R.T.: 0.038 min
Response: 10619
Conc: 4.85 ng/ml

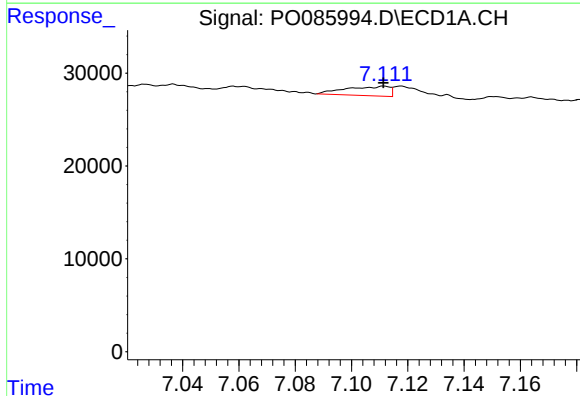


#28 AR-1254-3

R.T.: 7.112 min
Delta R.T.: 0.000 min
Response: 11037
Conc: 2.18 ng/ml

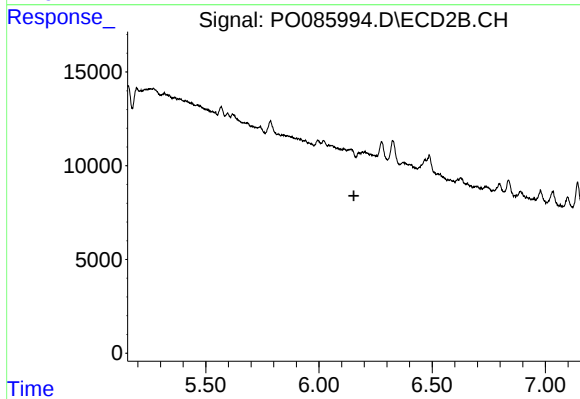

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.154 min
Response: 0
Conc: N.D.

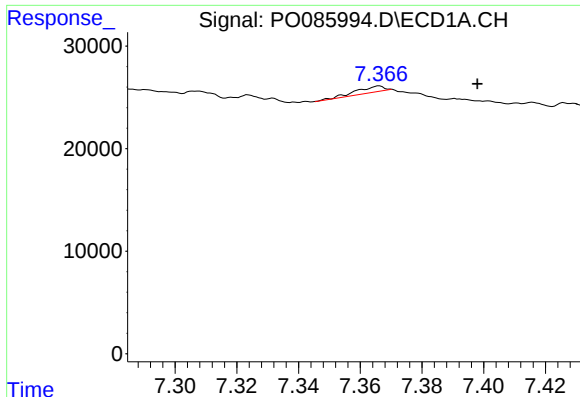

#29 AR-1254-4


R.T.: 7.366 min
Delta R.T.: -0.032 min
Response: 4153
Conc: 1.11 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

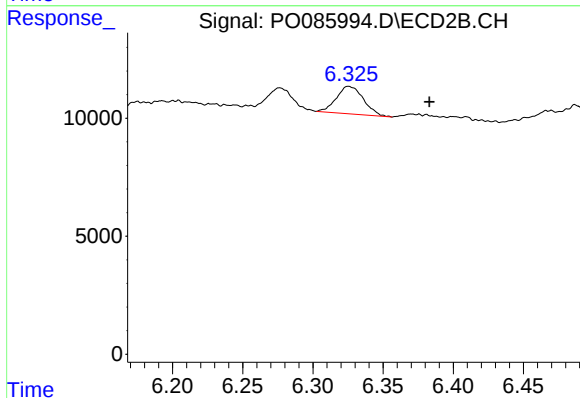


#29 AR-1254-4

R.T.: 6.325 min
Delta R.T.: -0.058 min
Response: 15672
Conc: 7.08 ng/ml

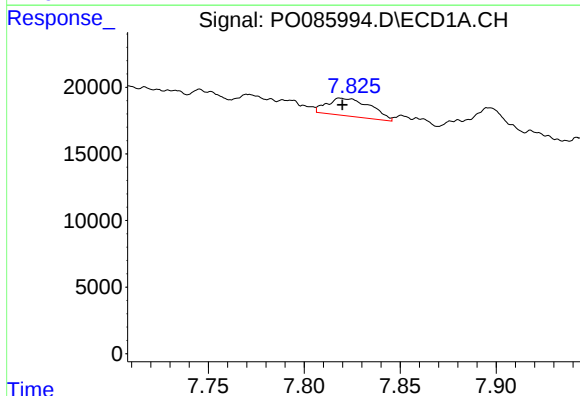


#30 AR-1254-5

R.T.: 7.819 min
Delta R.T.: -0.001 min
Response: 21122
Conc: 5.42 ng/ml

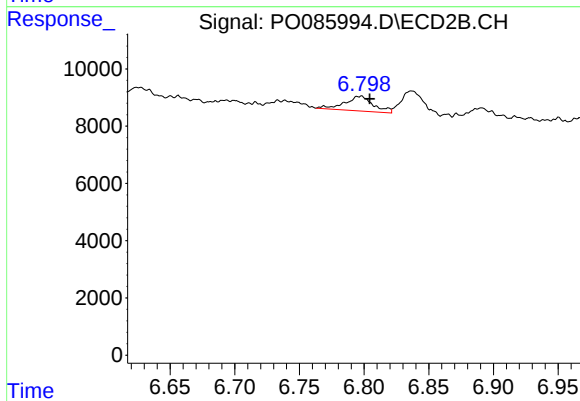

#30 AR-1254-5


R.T.: 6.798 min
Delta R.T.: -0.007 min
Response: 7921
Conc: 2.68 ng/ml

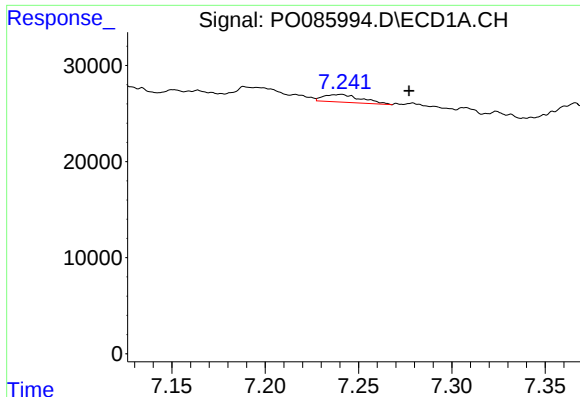

#31 AR-1260-1


R.T.: 7.241 min
Delta R.T.: -0.036 min
Response: 11359
Conc: 3.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

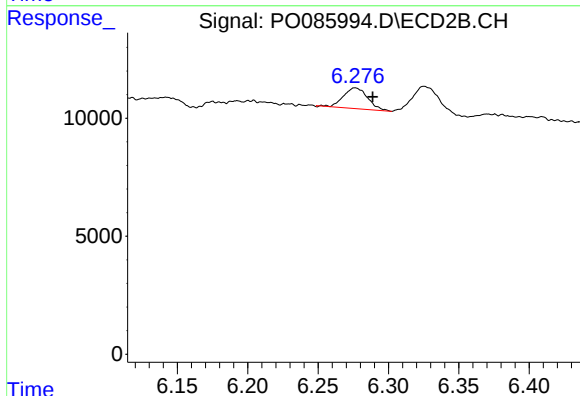


#31 AR-1260-1

R.T.: 6.276 min
Delta R.T.: -0.012 min
Response: 10612
Conc: 5.45 ng/ml

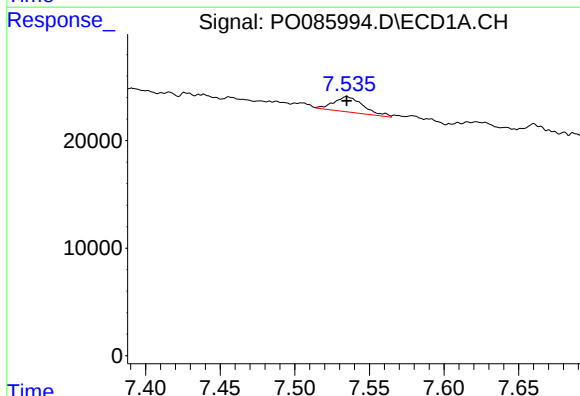


#32 AR-1260-2

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 19834
Conc: 5.48 ng/ml

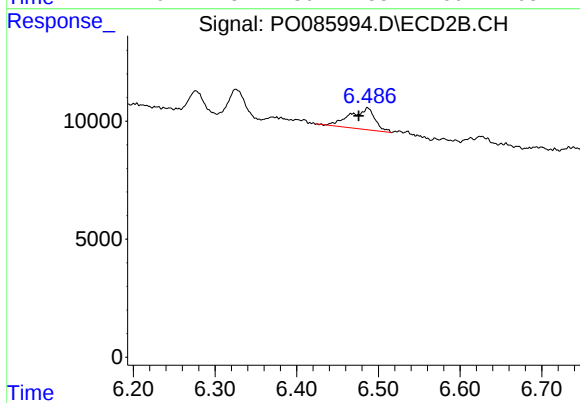

#32 AR-1260-2


R.T.: 6.487 min
Delta R.T.: 0.011 min
Response: 19228
Conc: 8.18 ng/ml

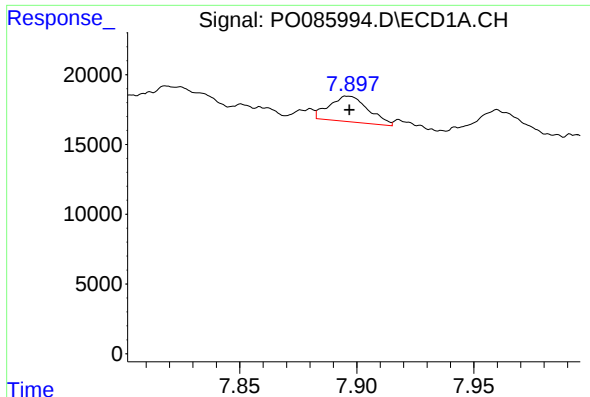

#33 AR-1260-3


R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 21353
Conc: 7.74 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

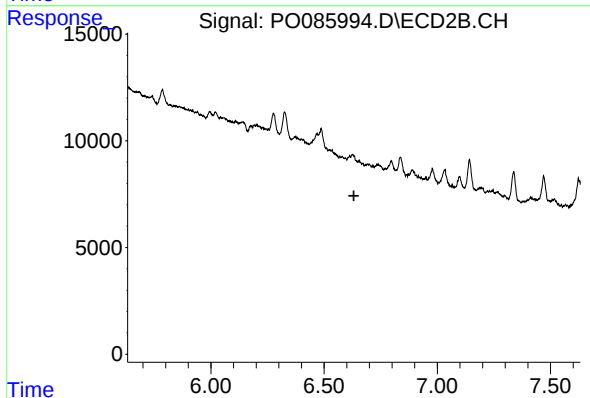


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

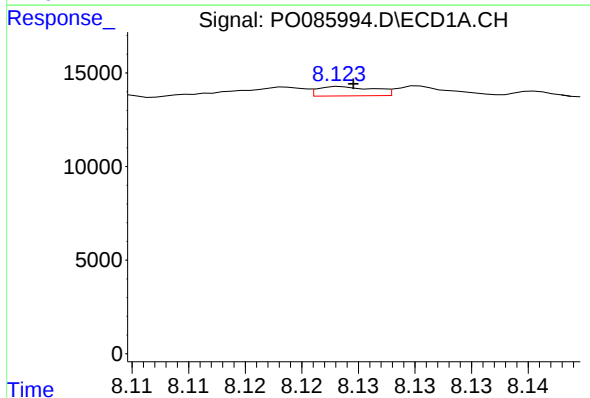


#34 AR-1260-4

R.T.: 8.124 min
Delta R.T.: -0.001 min
Response: 1717
Conc: 0.51 ng/ml

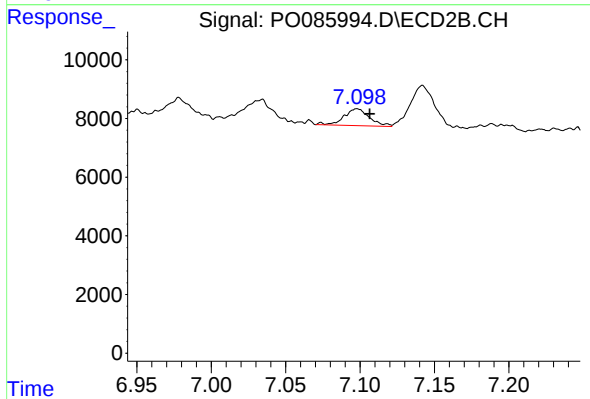

#34 AR-1260-4


R.T.: 7.098 min
Delta R.T.: -0.008 min
Response: 6910
Conc: 3.84 ng/ml

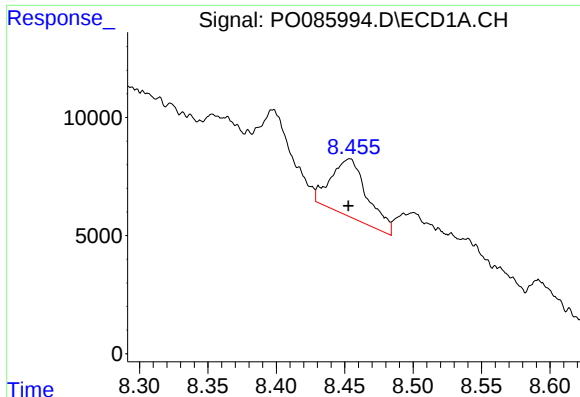

#35 AR-1260-5


R.T.: 8.454 min
Delta R.T.: 0.001 min
Response: 45061
Conc: 7.30 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

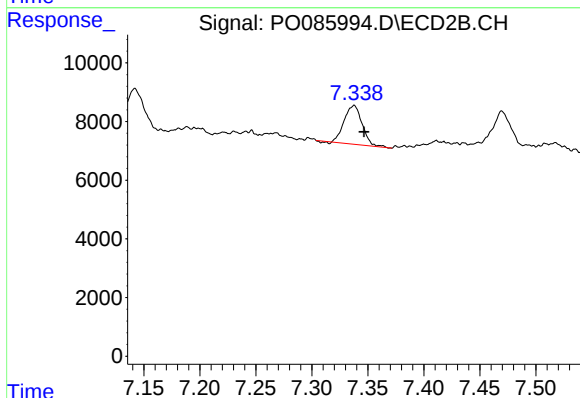


#35 AR-1260-5

R.T.: 7.338 min
Delta R.T.: -0.009 min
Response: 14812
Conc: 3.42 ng/ml

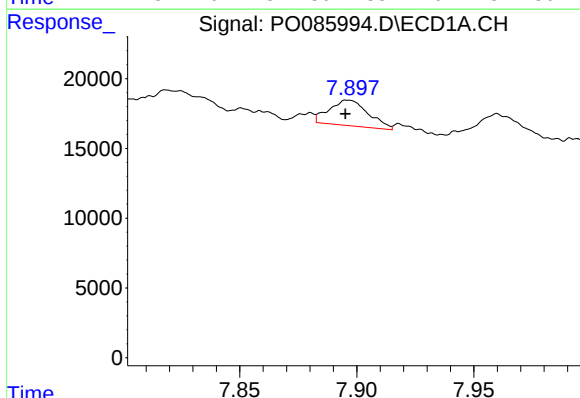


#36 AR-1262-1

R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 21353
Conc: 4.72 ng/ml

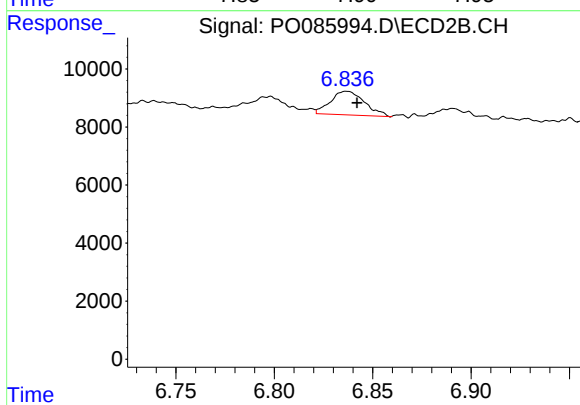

#36 AR-1262-1


R.T.: 6.837 min
Delta R.T.: -0.005 min
Response: 9820
Conc: 3.25 ng/ml

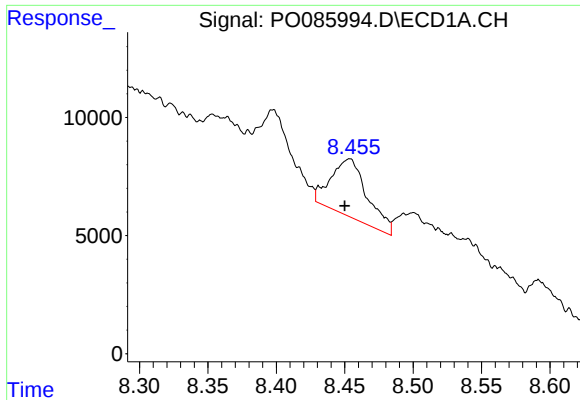

#37 AR-1262-2


R.T.: 8.454 min
Delta R.T.: 0.004 min
Response: 45061
Conc: 5.76 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

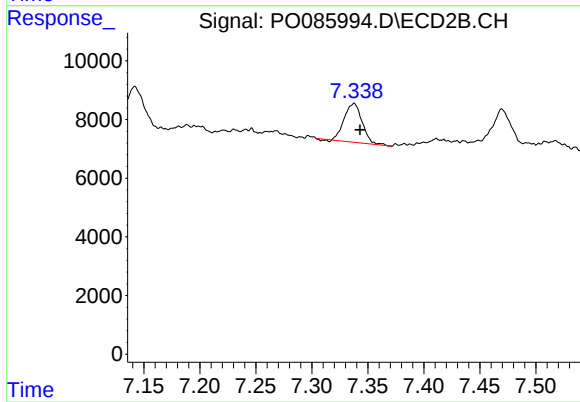


#37 AR-1262-2

R.T.: 7.338 min
Delta R.T.: -0.005 min
Response: 14812
Conc: 2.70 ng/ml

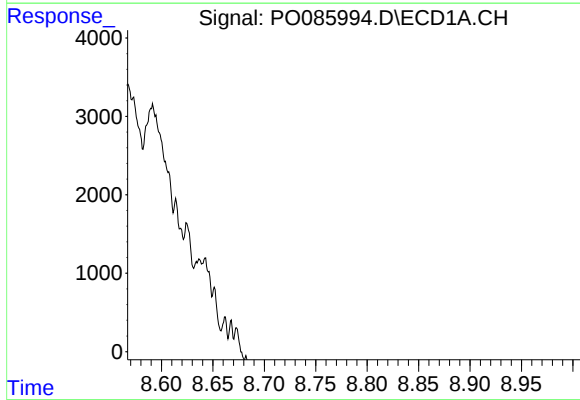


#38 AR-1262-3

R.T.: 8.771 min
Delta R.T.: -0.002 min
Response: 39035
Conc: 11.92 ng/ml

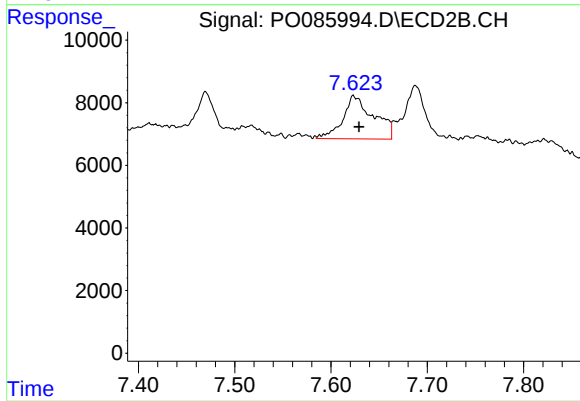

#38 AR-1262-3


R.T.: 7.623 min
Delta R.T.: -0.006 min
Response: 30519
Conc: 14.48 ng/ml

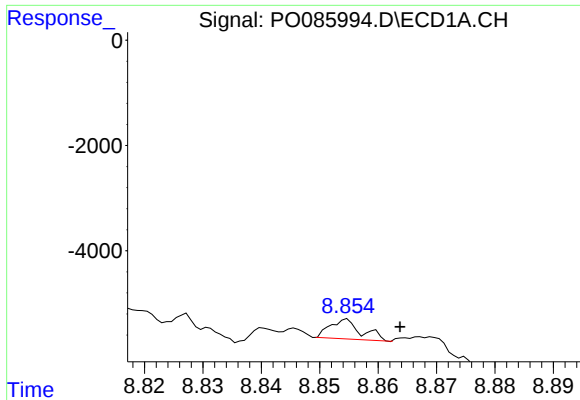

#39 AR-1262-4


R.T.: 8.855 min
Delta R.T.: -0.009 min
Response: 1394
Conc: 0.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

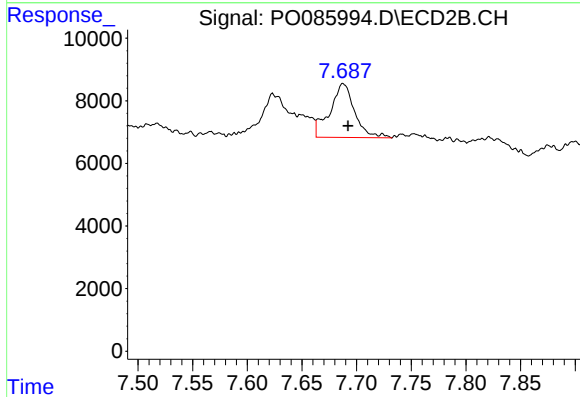


#39 AR-1262-4

R.T.: 7.688 min
Delta R.T.: -0.004 min
Response: 27026
Conc: 6.82 ng/ml

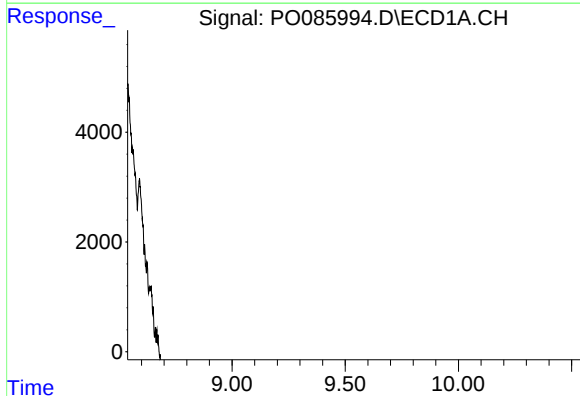


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.539 min
Response: 0
Conc: N.D.

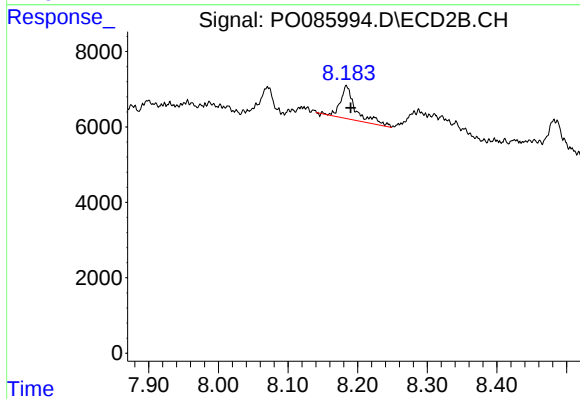

#40 AR-1262-5


R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 13419
Conc: 7.49 ng/ml

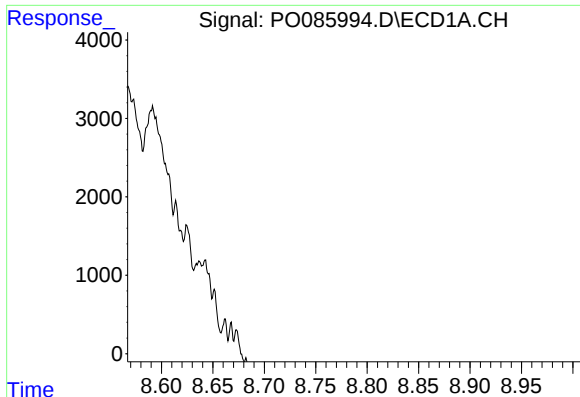

#41 AR-1268-1


R.T.: 8.771 min
Delta R.T.: 0.000 min
Response: 39035
Conc: 4.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

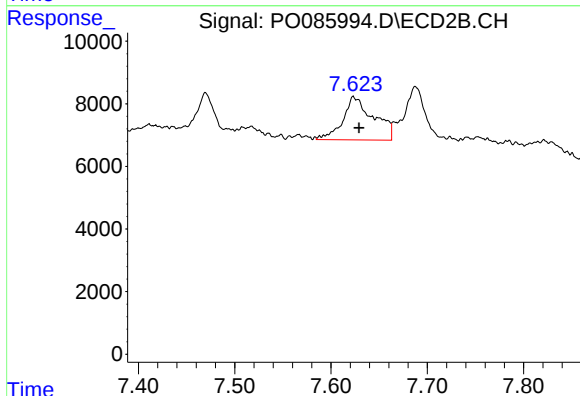


#41 AR-1268-1

R.T.: 7.623 min
Delta R.T.: -0.006 min
Response: 30519
Conc: 5.00 ng/ml

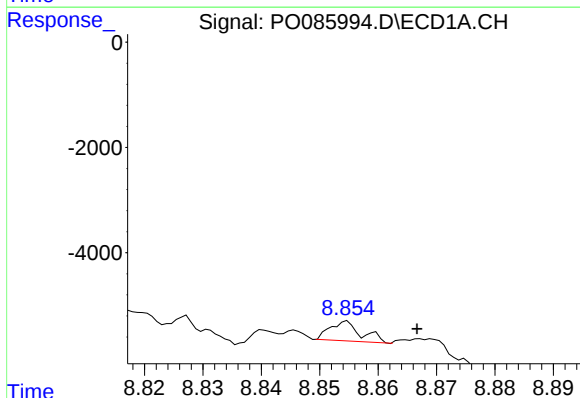


#42 AR-1268-2

R.T.: 8.855 min
Delta R.T.: -0.012 min
Response: 1394
Conc: 0.17 ng/ml

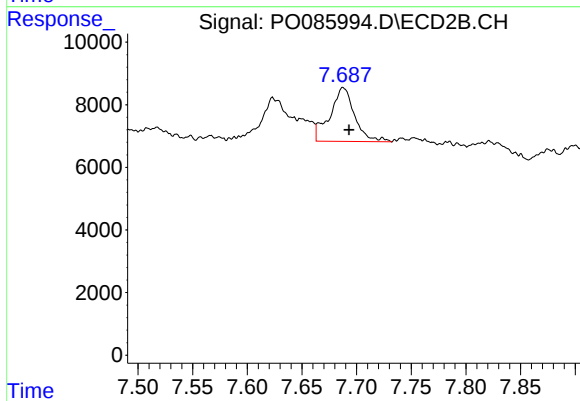

#42 AR-1268-2


R.T.: 7.688 min
Delta R.T.: -0.005 min
Response: 27026
Conc: 4.92 ng/ml

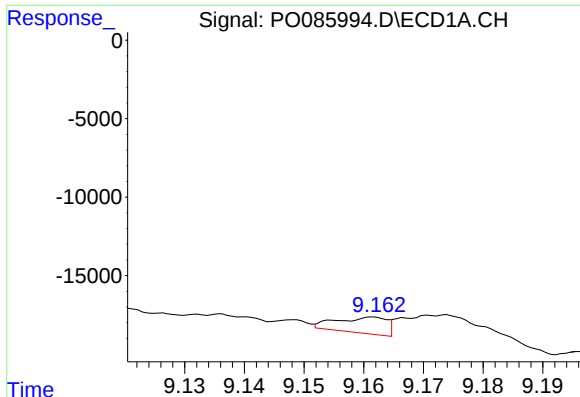

#43 AR-1268-3


R.T.: 9.162 min
Delta R.T.: 0.058 min
Response: 6030
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

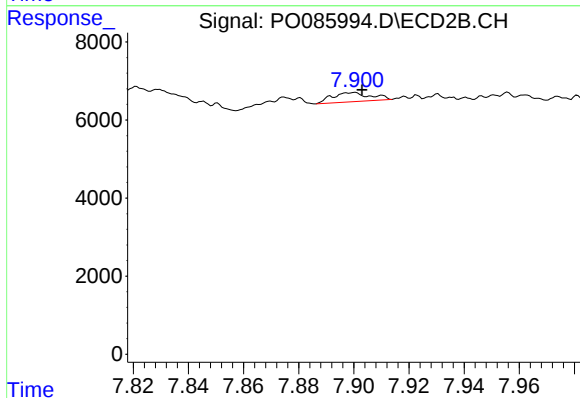


#43 AR-1268-3

R.T.: 7.899 min
Delta R.T.: -0.004 min
Response: 2257
Conc: 0.50 ng/ml

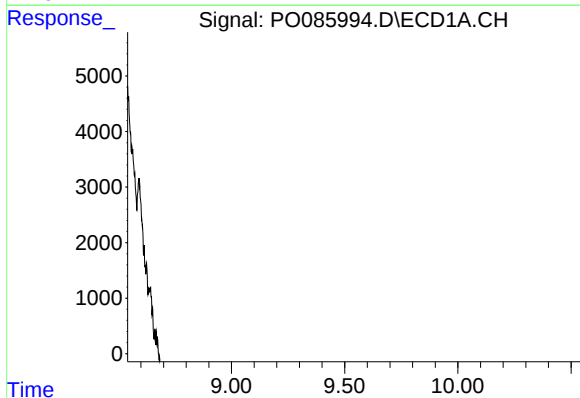


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.541 min
Response: 0
Conc: N.D.

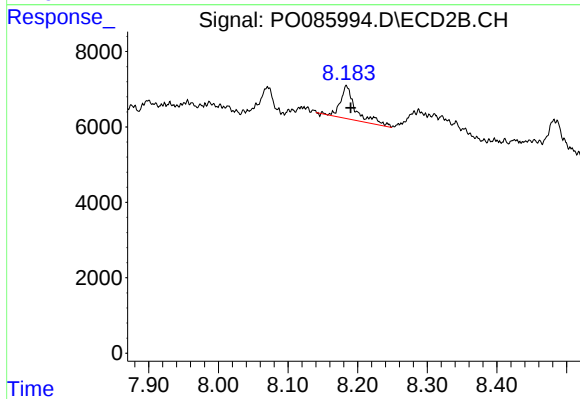

#44 AR-1268-4


R.T.: 8.184 min
Delta R.T.: -0.006 min
Response: 13419
Conc: 6.87 ng/ml

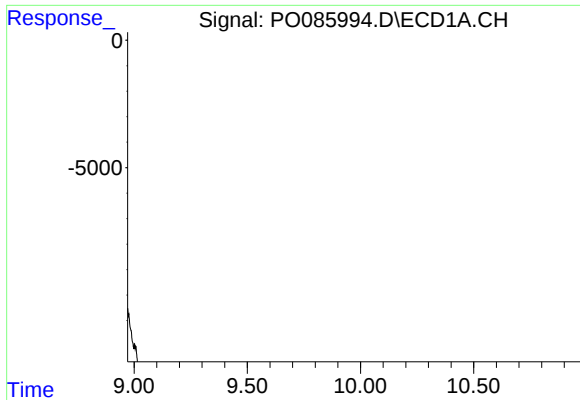

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-1

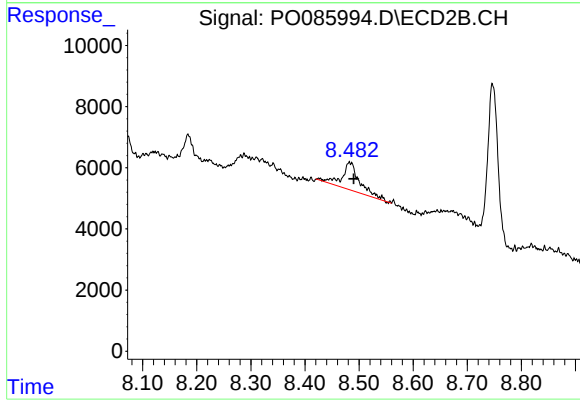

#45 AR-1268-5

R.T.: 8.482 min
Delta R.T.: -0.008 min
Response: 20228
Conc: 1.38 ng/ml