

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
 Data File : P0085997.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2022 23:35
 Operator : YP\AJ
 Sample : N2771-05 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-BC226656-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 07:13:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.480	3.682	181902	73366	1.791	1.683
2)	SA Decachlor...	10.329	8.750	101981	55240	1.924	1.628
Target Compounds							
3)	L1 AR-1016-1	5.594f	0.000	20172	0	6.312	N.D. #
5)	L1 AR-1016-3	5.760	0.000	5452	0	1.988	N.D. #
16)	L4 AR-1242-1	5.594f	0.000	20172	0	7.421	N.D. #
18)	L4 AR-1242-3	5.760	0.000	5452	0	2.320	N.D. #
20)	L4 AR-1242-5	6.591	0.000	1992	0	1.088	N.D. #
21)	L5 AR-1248-1	5.594f	0.000	20172	0	9.987	N.D. #
24)	L5 AR-1248-4	6.522	0.000	12799	0	3.976	N.D. #
25)	L5 AR-1248-5	6.591	0.000	1992	0	0.640	N.D. #
26)	L6 AR-1254-1	6.522	0.000	12799	0	3.803	N.D. #
27)	L6 AR-1254-2	6.743	0.000	7588	0	1.542	N.D. #
28)	L6 AR-1254-3	7.112	6.156	14015	7007	2.774	1.983 #
29)	L6 AR-1254-4	7.412	0.000	15368	0	4.126	N.D. #
30)	L6 AR-1254-5	7.817	0.000	13565	0	3.481	N.D. #
31)	L7 AR-1260-1	7.268	0.000	11390	0	3.763	N.D. #
32)	L7 AR-1260-2	7.545	6.533f	8964	12608	2.478	5.364 #
36)	L8 AR-1262-1	0.000	6.895f	0	11975	N.D.	3.963 #
38)	L8 AR-1262-3	0.000	7.588f	0	6819	N.D.	3.235 #
40)	L8 AR-1262-5	0.000	8.234f	0	5493	N.D.	3.066 #
41)	L9 AR-1268-1	0.000	7.588f	0	6819	N.D.	1.117 #
43)	L9 AR-1268-3	0.000	7.917	0	10034	N.D.	2.207 #
44)	L9 AR-1268-4	0.000	8.234f	0	5493	N.D.	2.813 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
Data File : P0085997.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2022 23:35
Operator : YP\AJ
Sample : N2771-05 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:13:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

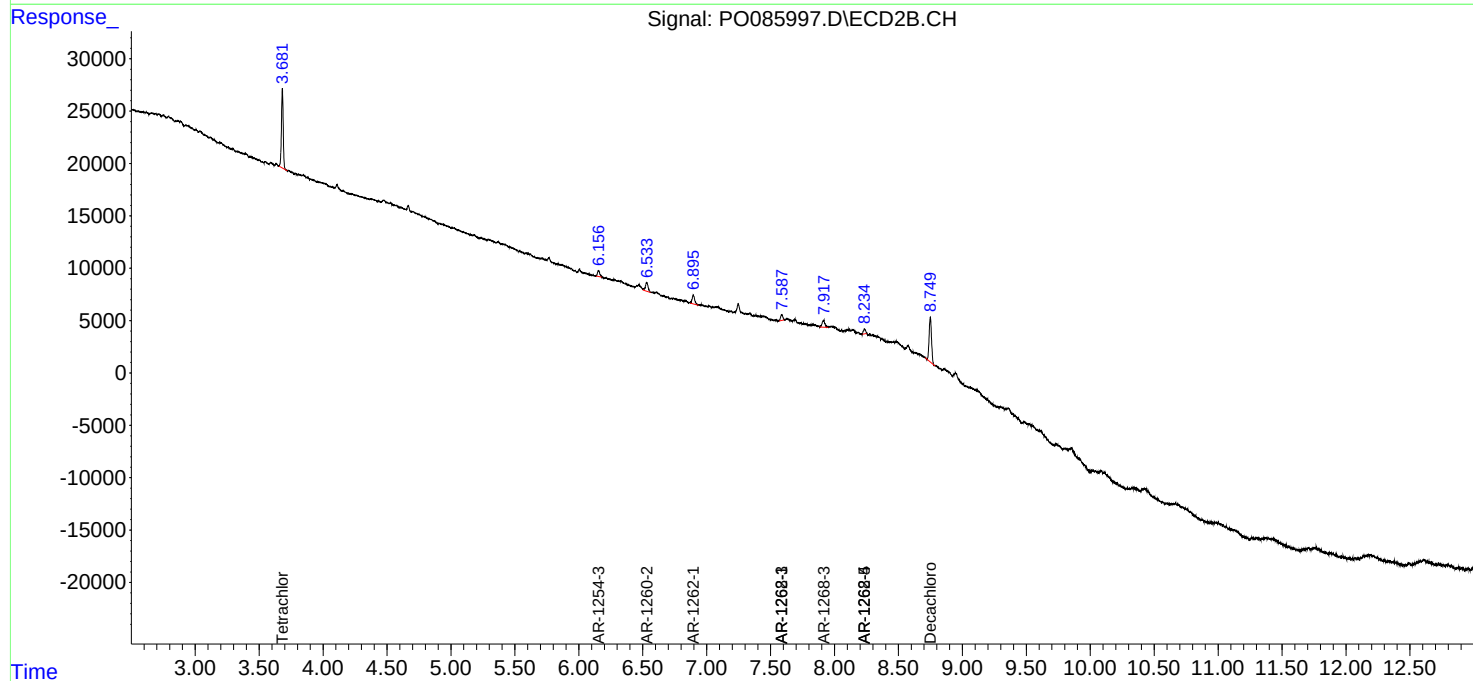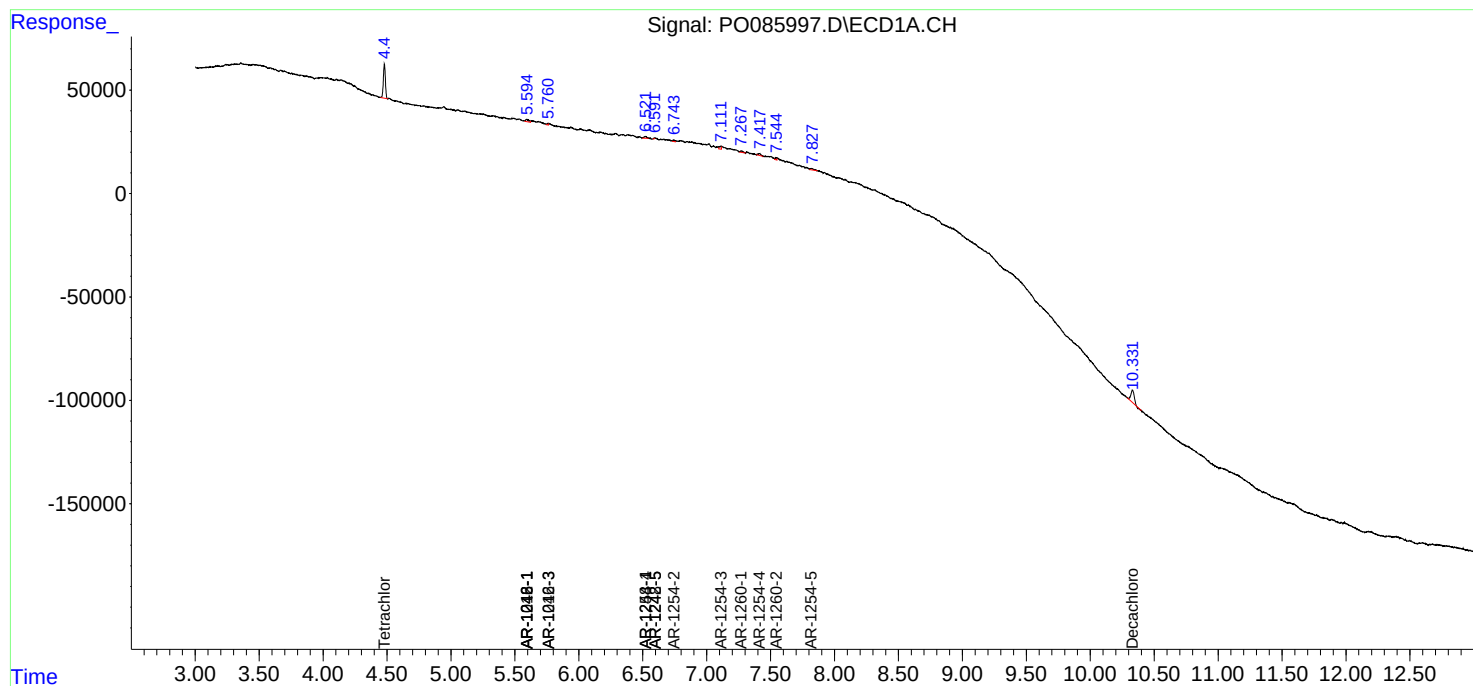


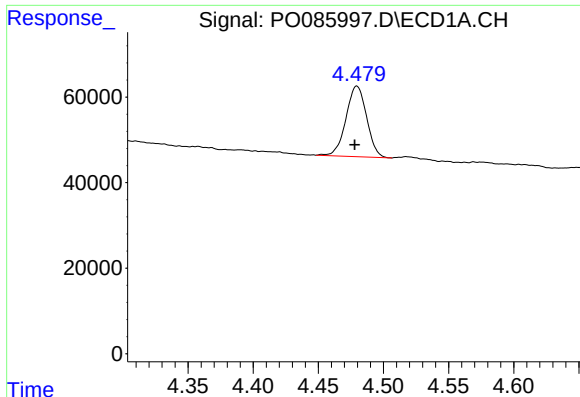

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.002 min
Response: 181902
Conc: 1.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

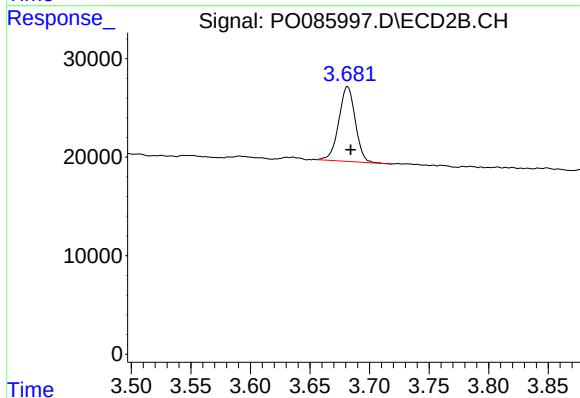


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.003 min
Response: 73366
Conc: 1.68 ng/ml

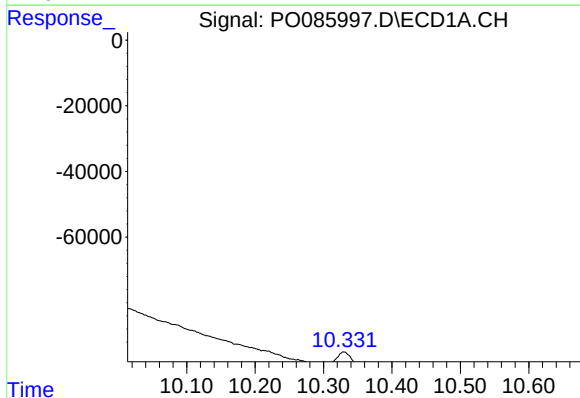


#2 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: 0.002 min
Response: 101981
Conc: 1.92 ng/ml

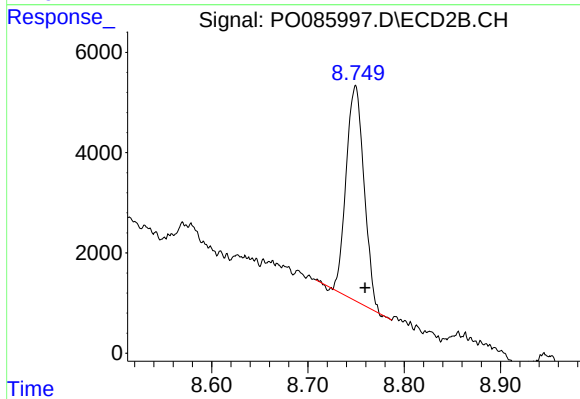

#2 Decachlorobiphenyl


R.T.: 8.750 min
Delta R.T.: -0.010 min
Response: 55240
Conc: 1.63 ng/ml

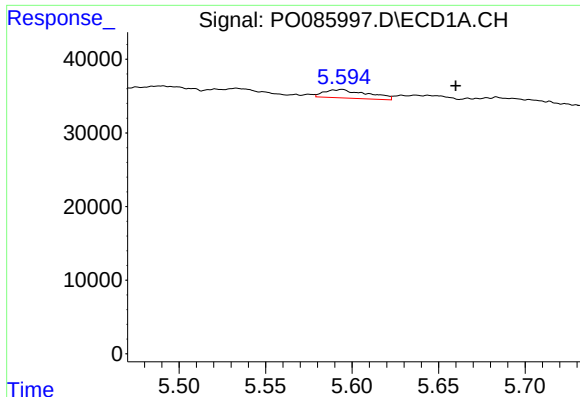

#3 AR-1016-1


R.T.: 5.594 min
Delta R.T.: -0.066 min
Response: 20172
Conc: 6.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

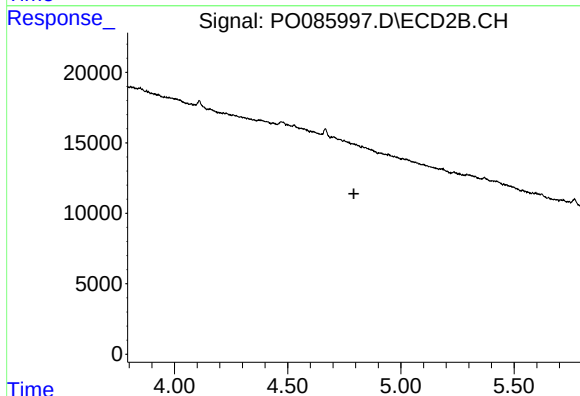


#3 AR-1016-1

R.T.: 0.000 min
Exp R.T. : 4.792 min
Response: 0
Conc: N.D.

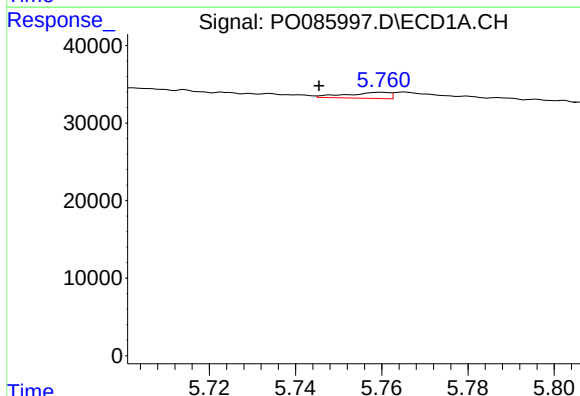


#5 AR-1016-3

R.T.: 5.760 min
Delta R.T.: 0.015 min
Response: 5452
Conc: 1.99 ng/ml

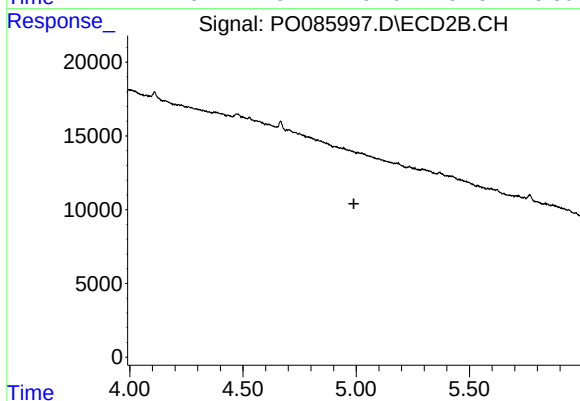

#5 AR-1016-3


R.T.: 0.000 min
Exp R.T. : 4.990 min
Response: 0
Conc: N.D.

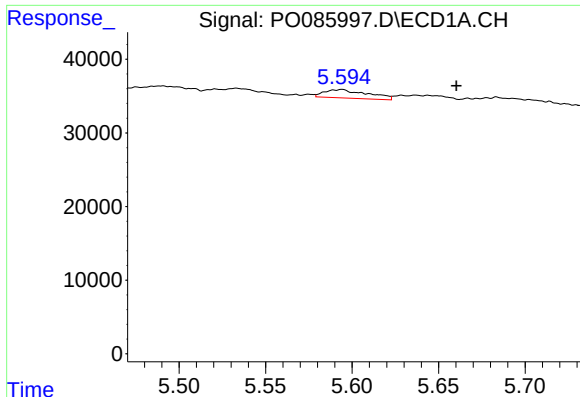

#16 AR-1242-1


R.T.: 5.594 min
Delta R.T.: -0.066 min
Response: 20172
Conc: 7.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

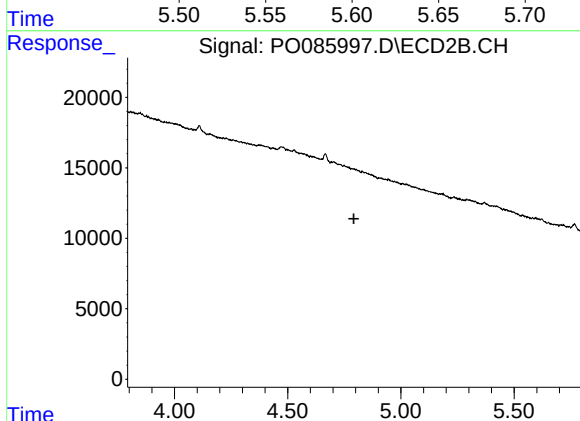


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 4.792 min
Response: 0
Conc: N.D.

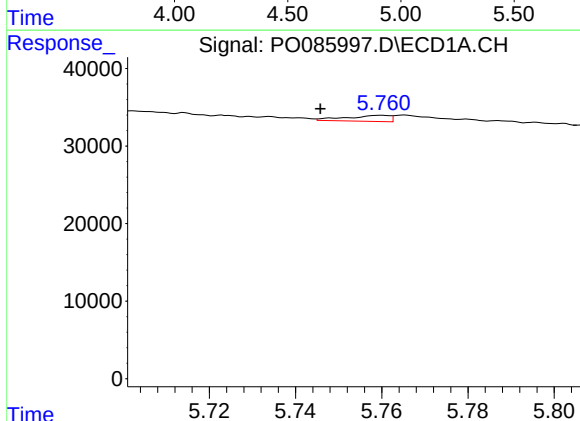


#18 AR-1242-3

R.T.: 5.760 min
Delta R.T.: 0.014 min
Response: 5452
Conc: 2.32 ng/ml

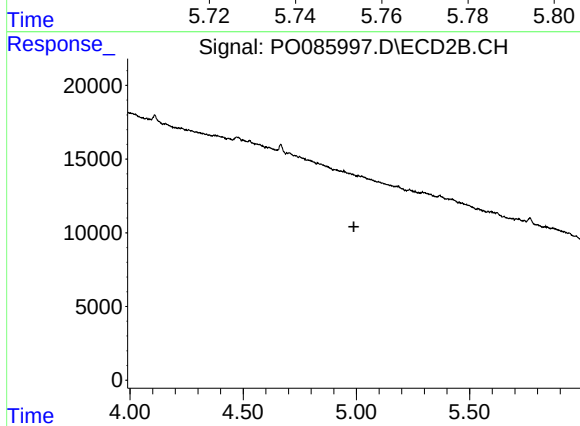

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

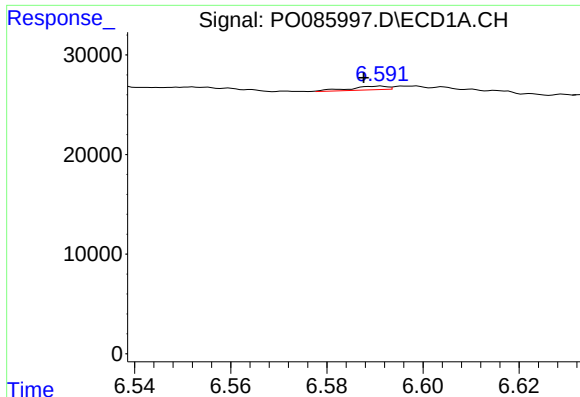

#20 AR-1242-5


R.T.: 6.591 min
Delta R.T.: 0.004 min
Response: 1992
Conc: 1.09 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

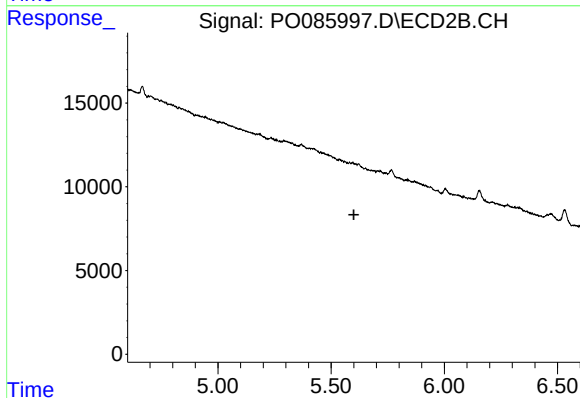


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 5.600 min
Response: 0
Conc: N.D.

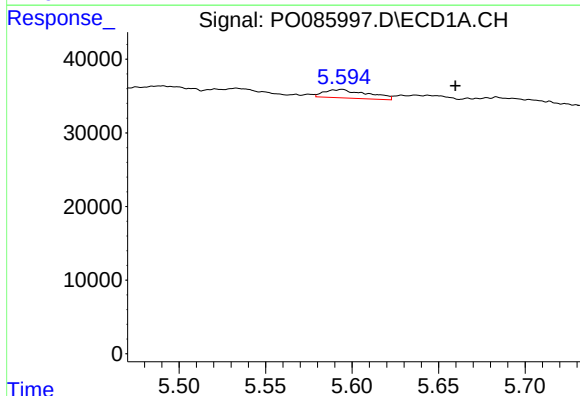


#21 AR-1248-1

R.T.: 5.594 min
Delta R.T.: -0.065 min
Response: 20172
Conc: 9.99 ng/ml

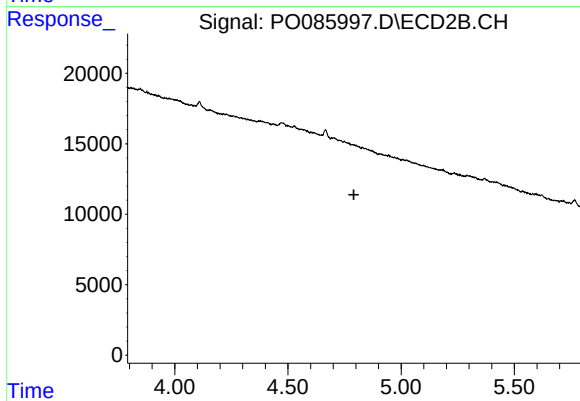

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T. : 4.791 min
Response: 0
Conc: N.D.

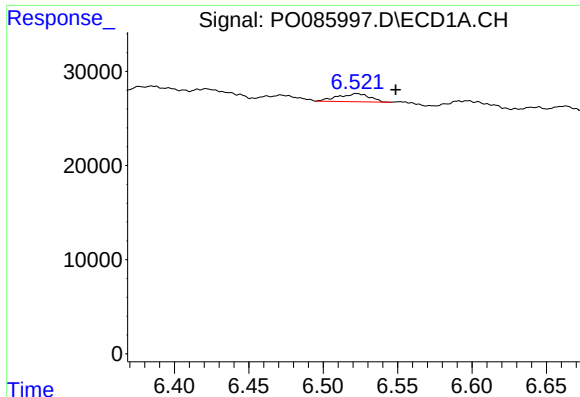

#24 AR-1248-4


R.T.: 6.522 min
Delta R.T.: -0.027 min
Response: 12799
Conc: 3.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

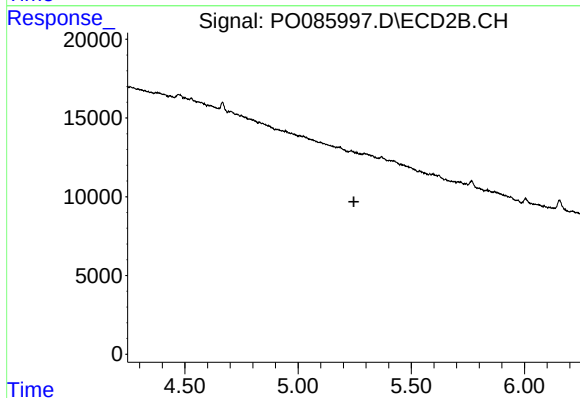


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.246 min
Response: 0
Conc: N.D.

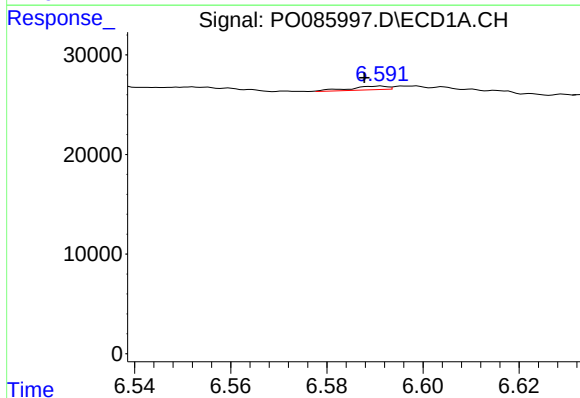


#25 AR-1248-5

R.T.: 6.591 min
Delta R.T.: 0.003 min
Response: 1992
Conc: 0.64 ng/ml

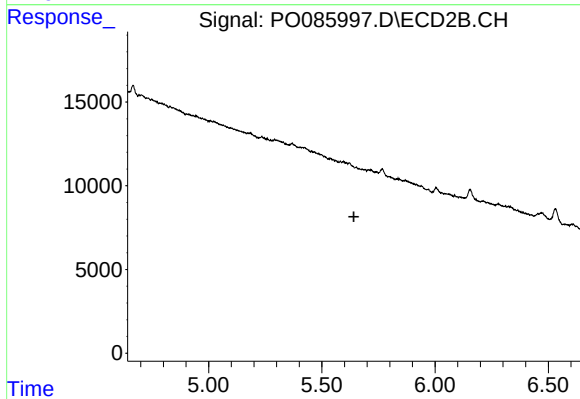

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.642 min
Response: 0
Conc: N.D.

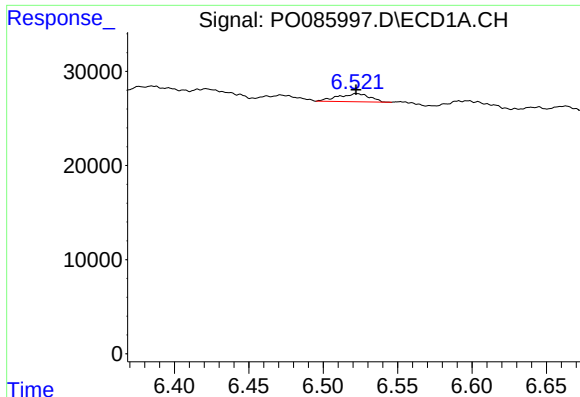

#26 AR-1254-1


R.T.: 6.522 min
Delta R.T.: 0.000 min
Response: 12799
Conc: 3.80 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

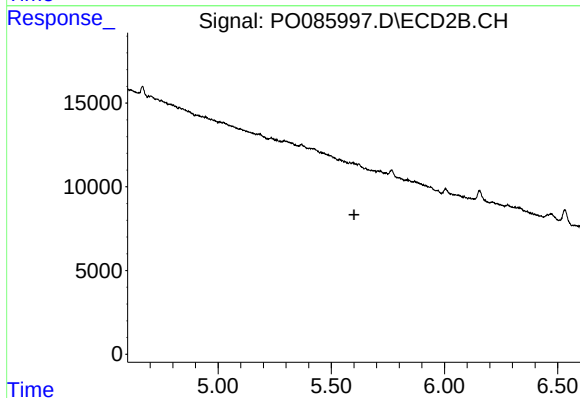


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.600 min
Response: 0
Conc: N.D.

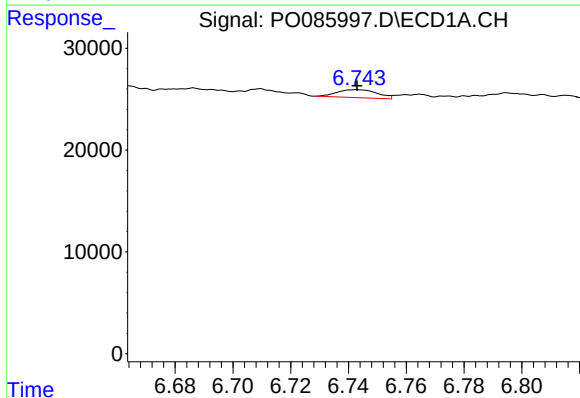


#27 AR-1254-2

R.T.: 6.743 min
Delta R.T.: 0.000 min
Response: 7588
Conc: 1.54 ng/ml

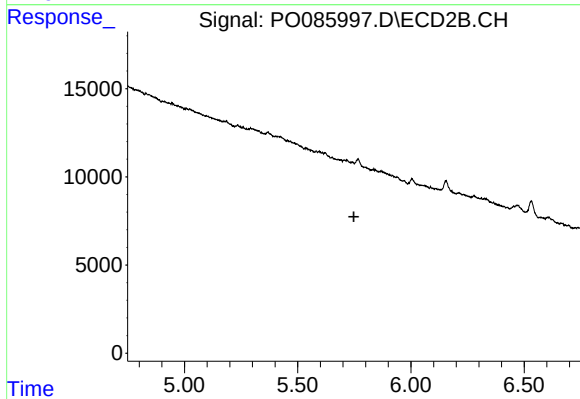

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T. : 5.748 min
Response: 0
Conc: N.D.

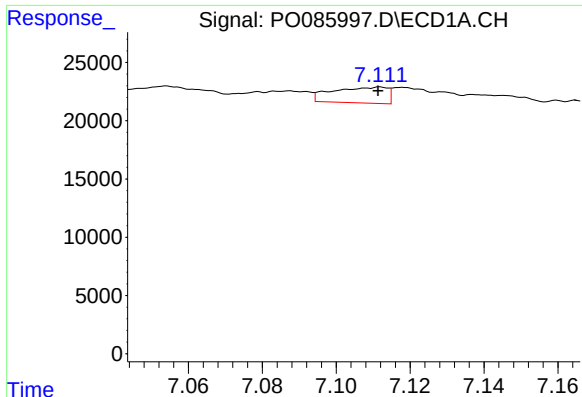

#28 AR-1254-3


R.T.: 7.112 min
Delta R.T.: 0.000 min
Response: 14015
Conc: 2.77 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

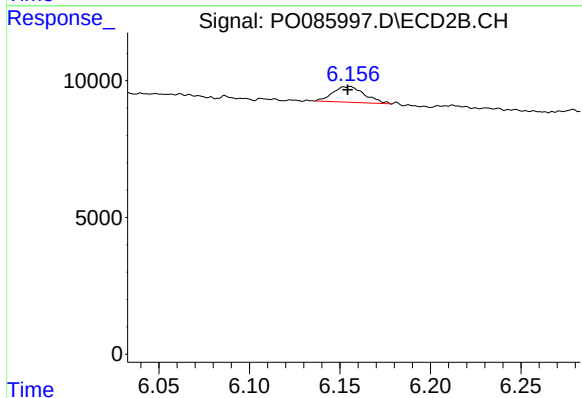


#28 AR-1254-3

R.T.: 6.156 min
Delta R.T.: 0.002 min
Response: 7007
Conc: 1.98 ng/ml

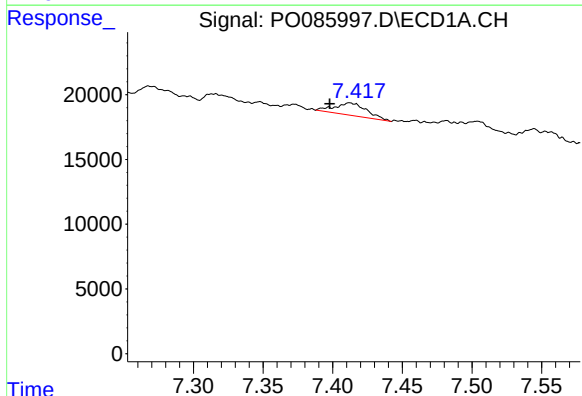


#29 AR-1254-4

R.T.: 7.412 min
Delta R.T.: 0.014 min
Response: 15368
Conc: 4.13 ng/ml

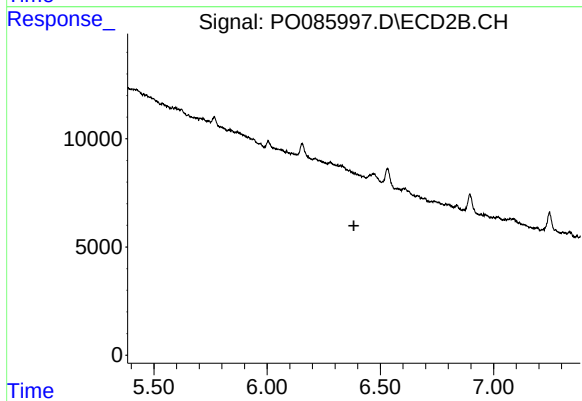

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T. : 6.383 min
Response: 0
Conc: N.D.

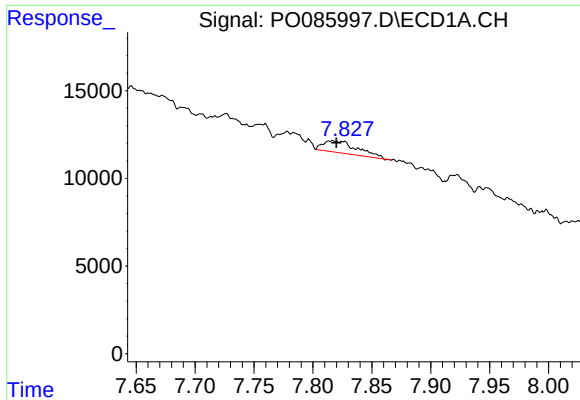

#30 AR-1254-5


R.T.: 7.817 min
Delta R.T.: -0.003 min
Response: 13565
Conc: 3.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

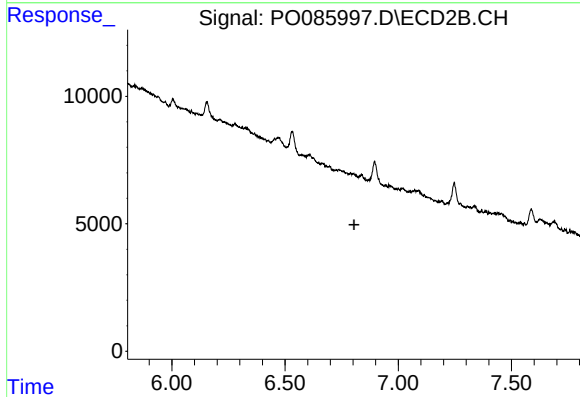


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 6.804 min
Response: 0
Conc: N.D.

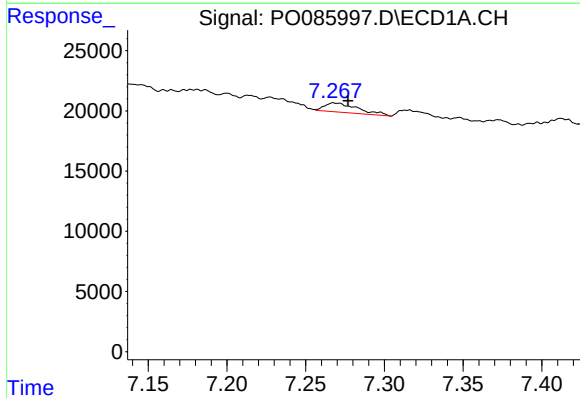


#31 AR-1260-1

R.T.: 7.268 min
Delta R.T.: -0.009 min
Response: 11390
Conc: 3.76 ng/ml

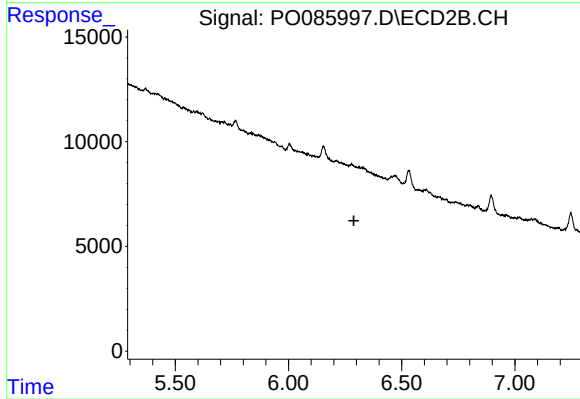

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T. : 6.289 min
Response: 0
Conc: N.D.

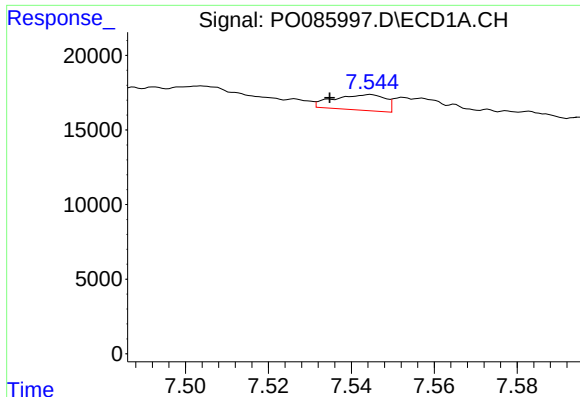

#32 AR-1260-2


R.T.: 7.545 min
Delta R.T.: 0.010 min
Response: 8964
Conc: 2.48 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

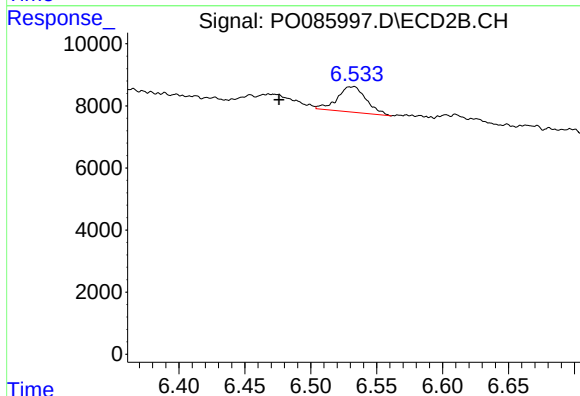


#32 AR-1260-2

R.T.: 6.533 min
Delta R.T.: 0.057 min
Response: 12608
Conc: 5.36 ng/ml

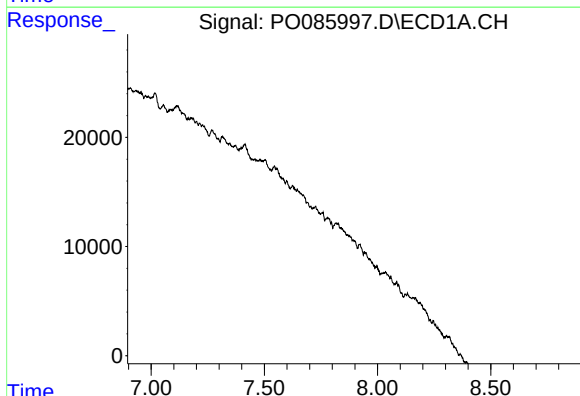


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.895 min
Response: 0
Conc: N.D.

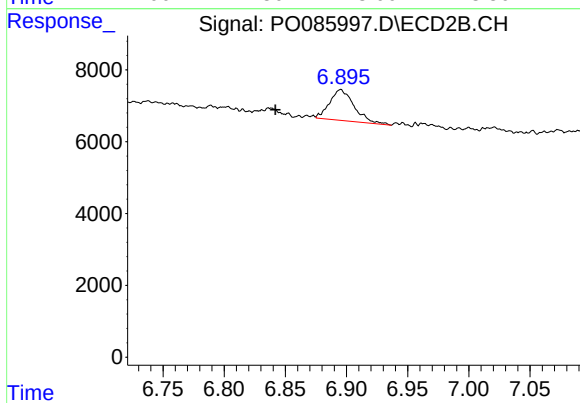

#36 AR-1262-1


R.T.: 6.895 min
Delta R.T.: 0.053 min
Response: 11975
Conc: 3.96 ng/ml

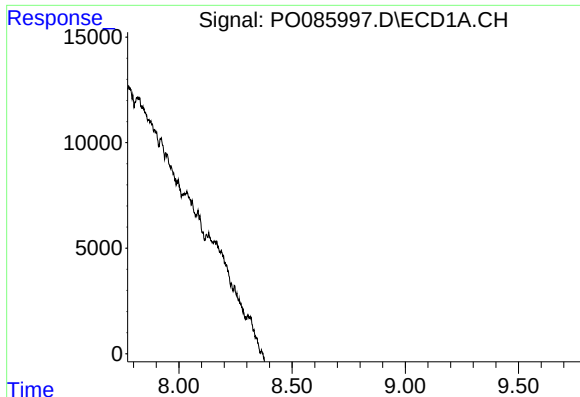

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.773 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

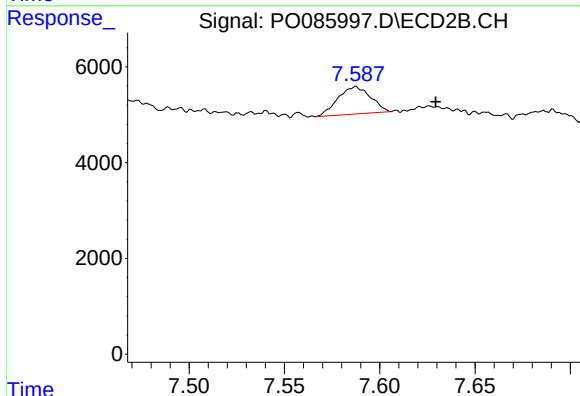


#38 AR-1262-3

R.T.: 7.588 min
Delta R.T.: -0.042 min
Response: 6819
Conc: 3.23 ng/ml

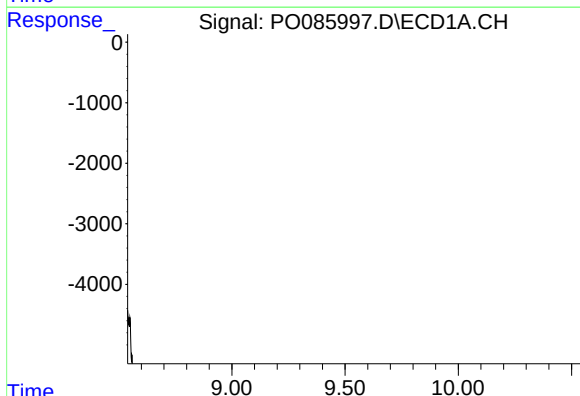


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.539 min
Response: 0
Conc: N.D.

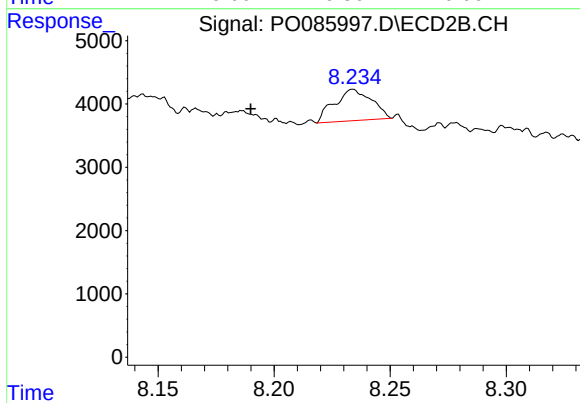

#40 AR-1262-5


R.T.: 8.234 min
Delta R.T.: 0.044 min
Response: 5493
Conc: 3.07 ng/ml

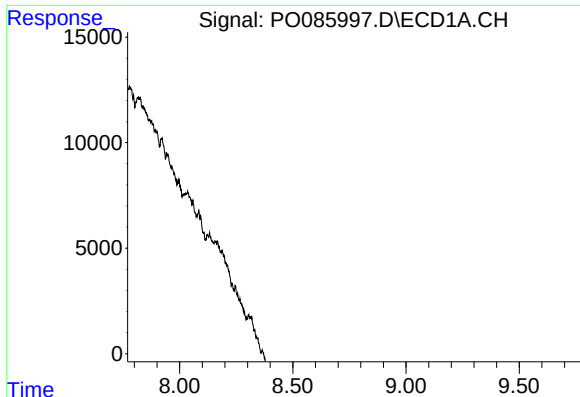

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.770 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

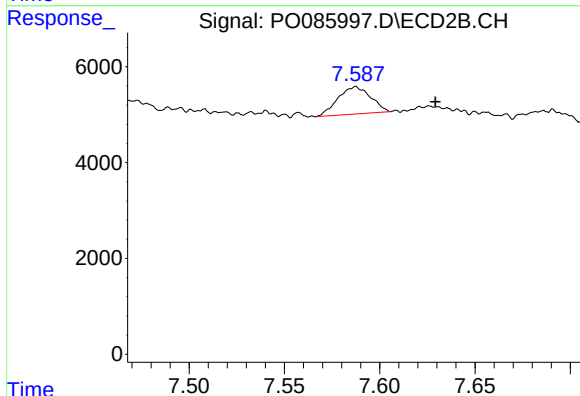


#41 AR-1268-1

R.T.: 7.588 min
Delta R.T.: -0.042 min
Response: 6819
Conc: 1.12 ng/ml

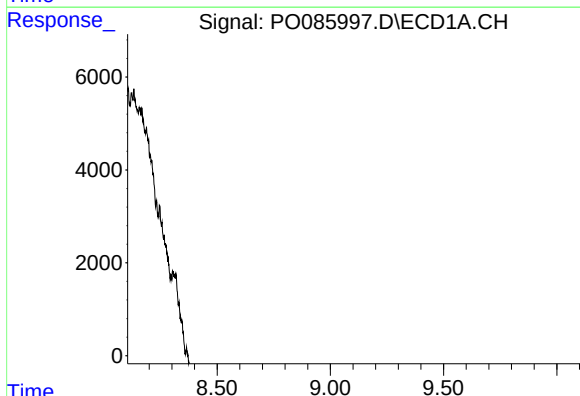


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.104 min
Response: 0
Conc: N.D.

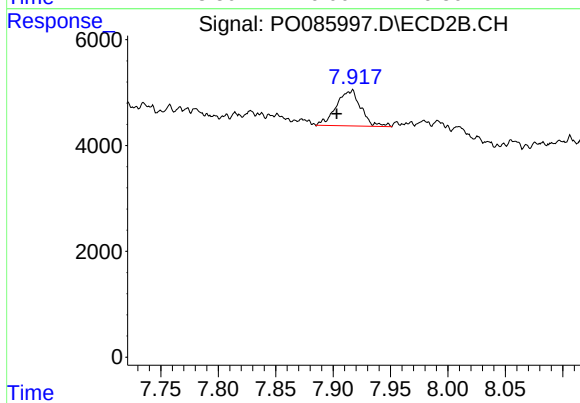

#43 AR-1268-3


R.T.: 7.917 min
Delta R.T.: 0.014 min
Response: 10034
Conc: 2.21 ng/ml

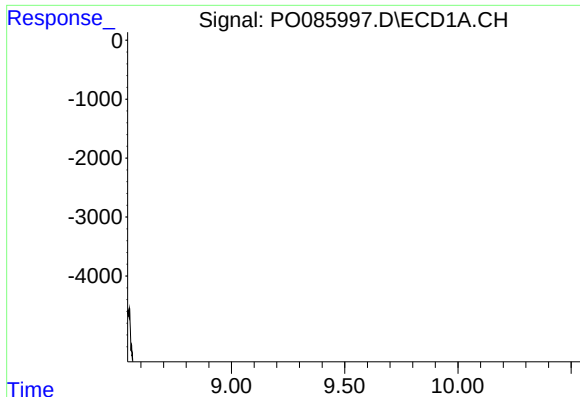

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.541 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

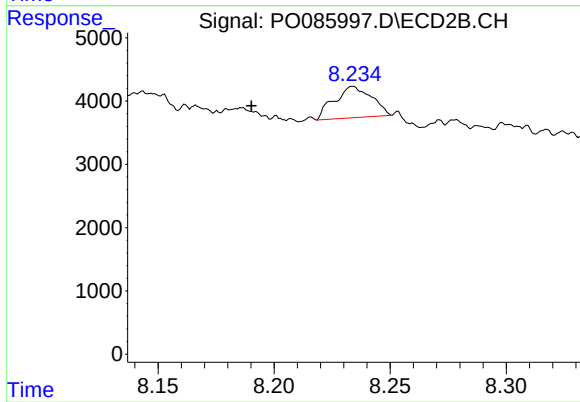

#44 AR-1268-4

R.T.: 8.234 min
Delta R.T.: 0.044 min
Response: 5493
Conc: 2.81 ng/ml