

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
 Data File : P0085998.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2022 23:51
 Operator : YP\AJ
 Sample : N2771-06 10X
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-BC226656-5

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 07:14:00 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	3.682	216376	74002	2.131	1.698
2)	SA Decachlor...	10.330	8.748	119445	54056	2.254	1.593 #
Target Compounds							
3)	L1 AR-1016-1	0.000	4.795	0	9380	N.D.	6.006 #
4)	L1 AR-1016-2	0.000	4.795	0	9380	N.D.	4.479 #
5)	L1 AR-1016-3	5.777	5.001	18084	5135	6.595	4.646 #
6)	L1 AR-1016-4	5.884f	5.001	14468	5135	6.527	5.571
7)	L1 AR-1016-5	0.000	5.193f	0	1131	N.D.	1.002 #
8)	L2 AR-1221-1	4.687	3.911	49180	15485	40.169	30.113 #
9)	L2 AR-1221-2	4.813	3.980	78208	25561	85.676	66.325
10)	L2 AR-1221-3	4.889	4.119f	54403	3853	20.186	3.173 #
11)	L3 AR-1232-1	4.889f	4.119f	54403	3853	26.575	4.169 #
12)	L3 AR-1232-2	5.352f	4.795	6644	9380	7.054	11.507 #
13)	L3 AR-1232-3	0.000	5.001	0	5135	N.D.	12.438 #
14)	L3 AR-1232-4	5.884f	0.000	14468	0	16.631	N.D. #
15)	L3 AR-1232-5	5.938	5.193f	3091	1131	4.668	2.701 #
16)	L4 AR-1242-1	0.000	4.795	0	9380	N.D.	7.101 #
17)	L4 AR-1242-2	0.000	4.795	0	9380	N.D.	5.349 #
18)	L4 AR-1242-3	5.777	5.001	18084	5135	7.697	5.461 #
19)	L4 AR-1242-4	5.884f	0.000	14468	0	7.633	N.D. #
20)	L4 AR-1242-5	6.524f	5.570	4839	5180	2.644	4.555 #
21)	L5 AR-1248-1	0.000	4.795	0	9380	N.D.	9.660 #
22)	L5 AR-1248-2	5.938	5.001	3091	5135	1.146	3.861 #
24)	L5 AR-1248-4	6.524	5.193f	4839	1131	1.503	0.707 #
25)	L5 AR-1248-5	6.524f	0.000	4839	0	1.555	N.D. #
26)	L6 AR-1254-1	6.524	5.570	4839	5180	1.438	2.057 #
27)	L6 AR-1254-2	6.750	5.785f	11995	7987	2.438	3.647 #
29)	L6 AR-1254-4	0.000	6.328f	0	14169	N.D.	6.405 #
30)	L6 AR-1254-5	7.821	6.796	20093	7826	5.157	2.646 #
31)	L7 AR-1260-1	7.263	6.279	4041	13353	1.335	6.860 #
32)	L7 AR-1260-2	7.535	6.474	28261	5830	7.812	2.480 #
33)	L7 AR-1260-3	7.900	0.000	16134	0	5.846	N.D. #
34)	L7 AR-1260-4	8.073f	7.098	32092	6238	9.512	3.464 #
35)	L7 AR-1260-5	8.459	7.338	28742	19701	4.658	4.548
36)	L8 AR-1262-1	7.900	6.839	16134	8105	3.567	2.683
37)	L8 AR-1262-2	8.459	7.338	28742	19701	3.672	3.586
38)	L8 AR-1262-3	8.775	7.626	46880	16120	14.310	7.647 #
39)	L8 AR-1262-4	0.000	7.688	0	22316	N.D.	5.630 #
40)	L8 AR-1262-5	0.000	8.187	0	8531	N.D.	4.762 #
41)	L9 AR-1268-1	8.775	7.626	46880	16120	5.370	2.642 #
42)	L9 AR-1268-2	0.000	7.688	0	22316	N.D.	4.065 #
43)	L9 AR-1268-3	0.000	7.868f	0	6478	N.D.	1.425 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
Data File : P0085998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2022 23:51
Operator : YP\AJ
Sample : N2771-06 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:14:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
44) L9	AR-1268-4	0.000	8.187	0	8531	N.D.	4.369 #
45) L9	AR-1268-5	0.000	8.484	0	14501	N.D.	0.989 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
Data File : P0085998.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2022 23:51
Operator : YP\AJ
Sample : N2771-06 10X
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:14:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

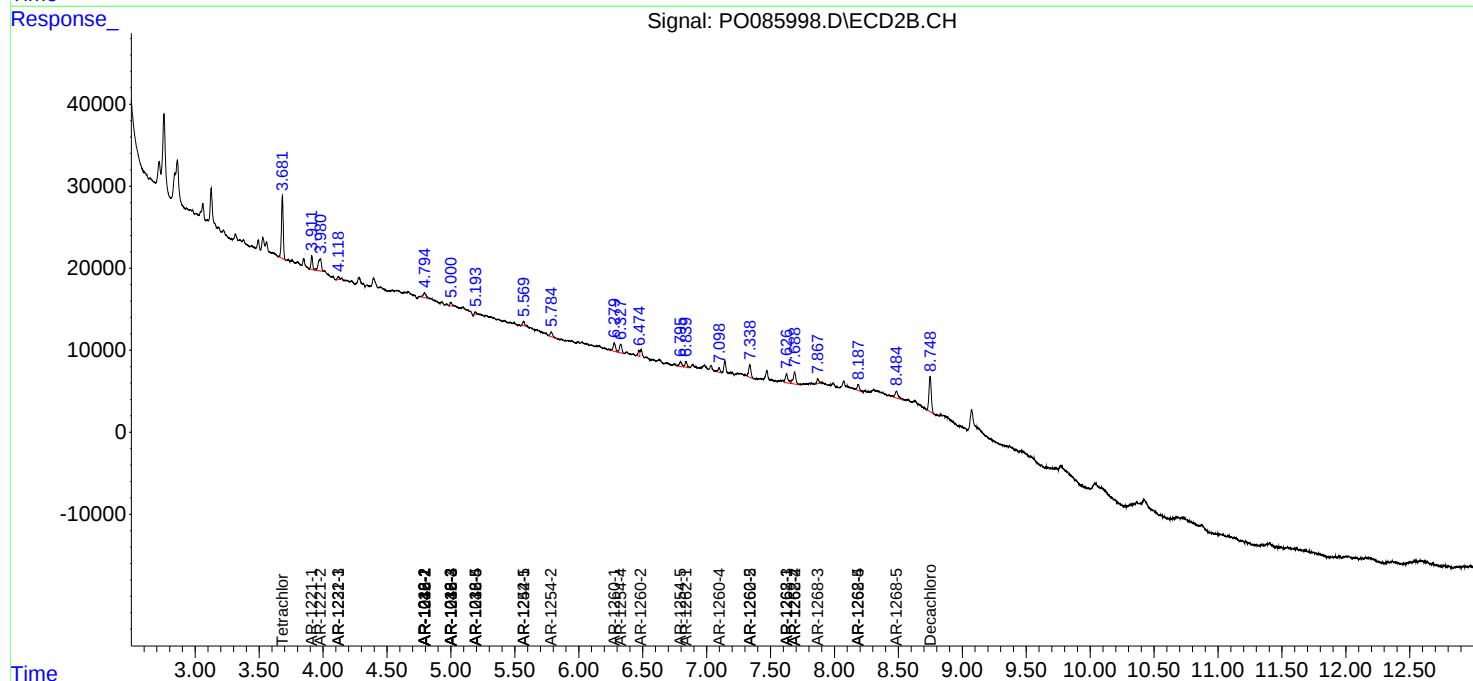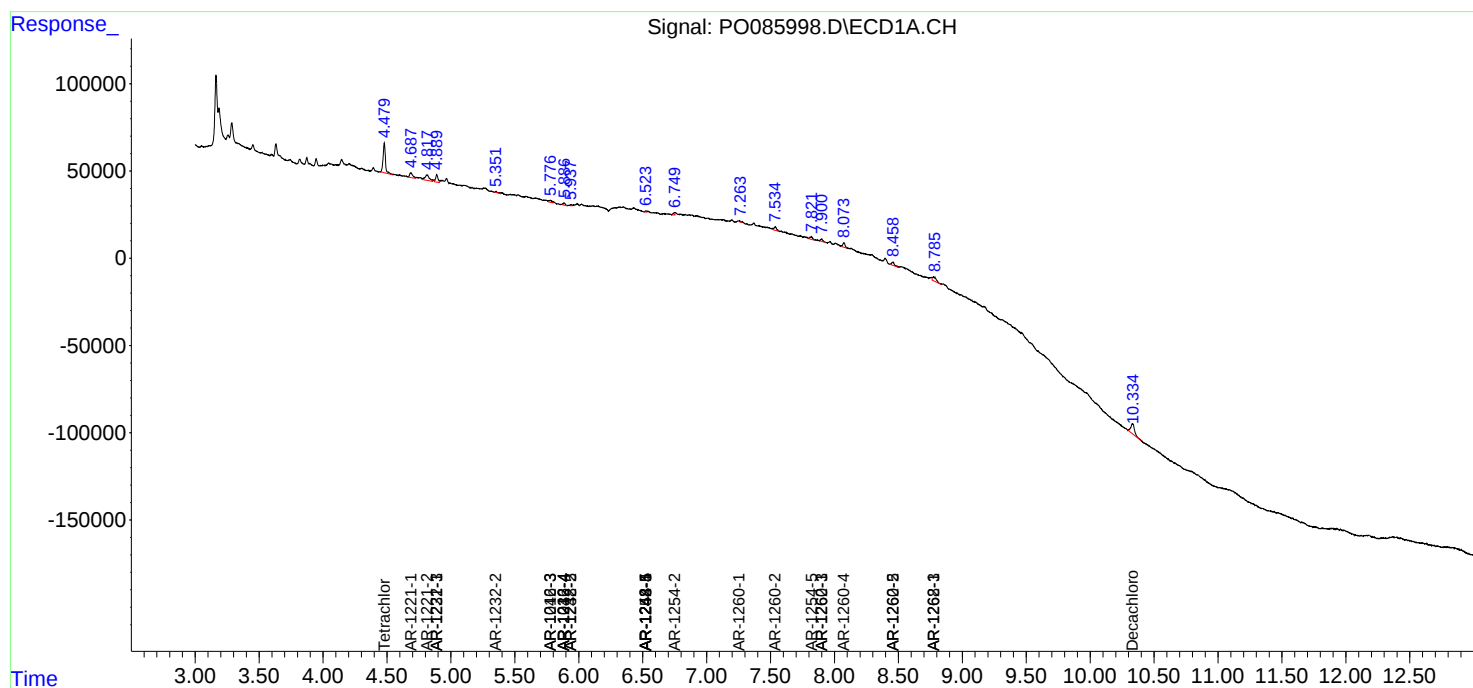


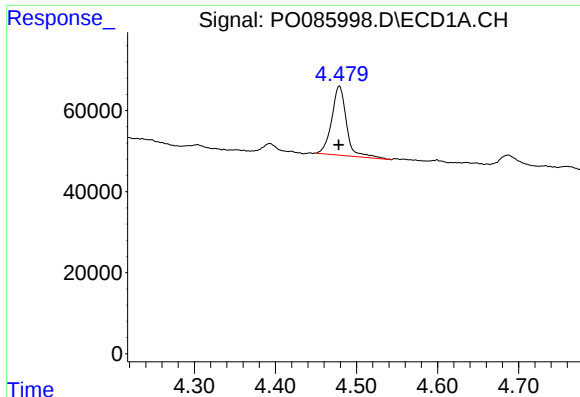

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 216376
Conc: 2.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

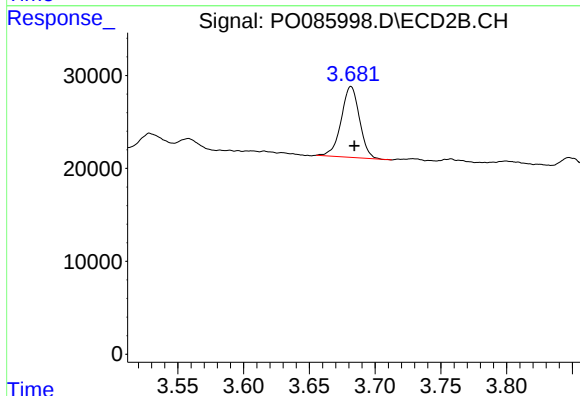


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.002 min
Response: 74002
Conc: 1.70 ng/ml

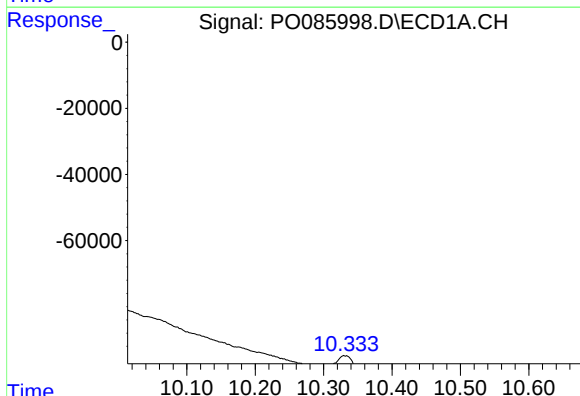


#2 Decachlorobiphenyl

R.T.: 10.330 min
Delta R.T.: 0.002 min
Response: 119445
Conc: 2.25 ng/ml

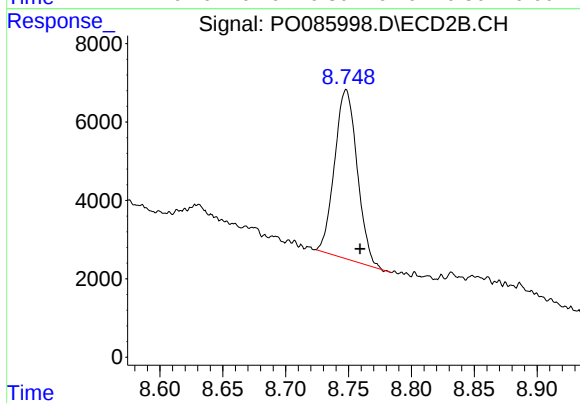

#2 Decachlorobiphenyl


R.T.: 8.748 min
Delta R.T.: -0.011 min
Response: 54056
Conc: 1.59 ng/ml

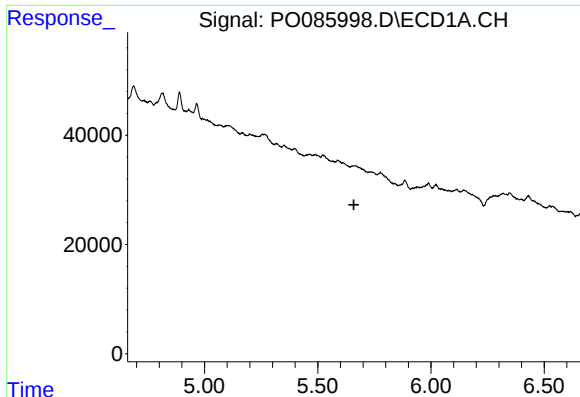

#3 AR-1016-1


R.T.: 0.000 min
Exp R.T.: 5.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

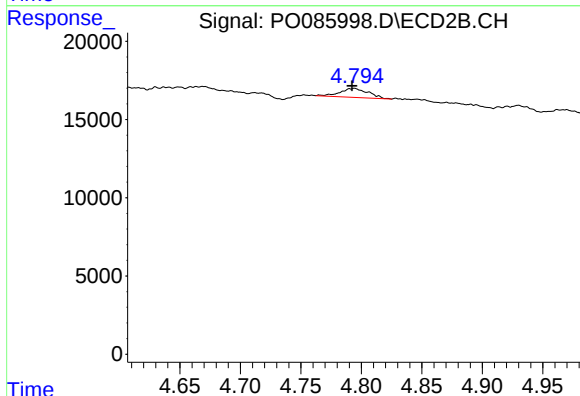


#3 AR-1016-1

R.T.: 4.795 min
Delta R.T.: 0.002 min
Response: 9380
Conc: 6.01 ng/ml

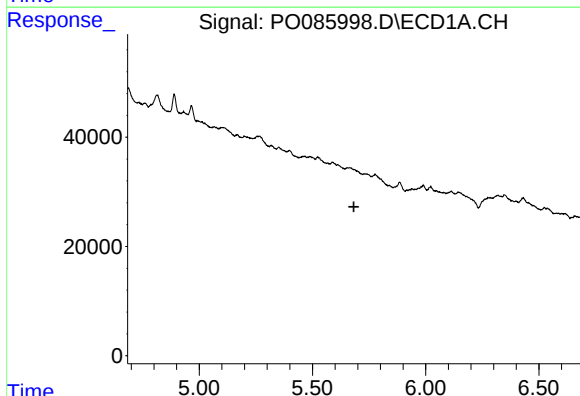


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T.: 5.683 min
Response: 0
Conc: N.D.

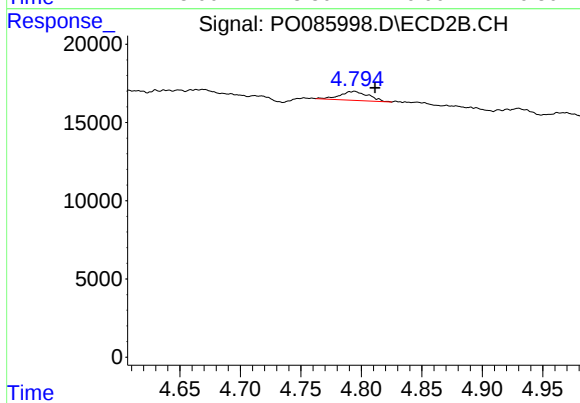

#4 AR-1016-2


R.T.: 4.795 min
Delta R.T.: -0.017 min
Response: 9380
Conc: 4.48 ng/ml

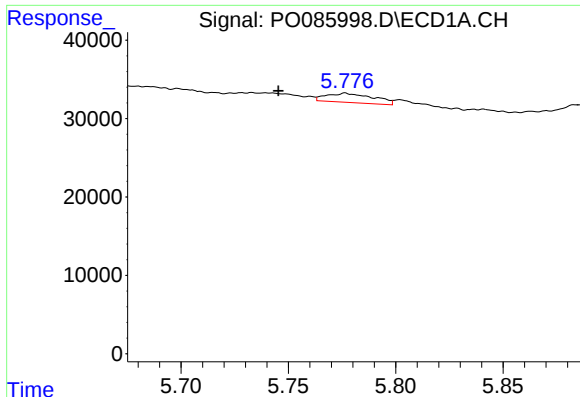

#5 AR-1016-3


R.T.: 5.777 min
Delta R.T.: 0.031 min
Response: 18084
Conc: 6.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

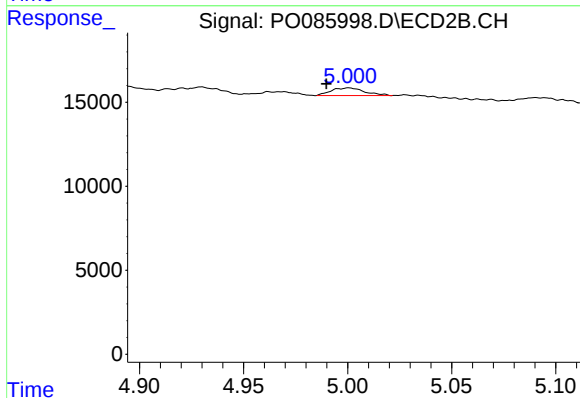


#5 AR-1016-3

R.T.: 5.001 min
Delta R.T.: 0.011 min
Response: 5135
Conc: 4.65 ng/ml

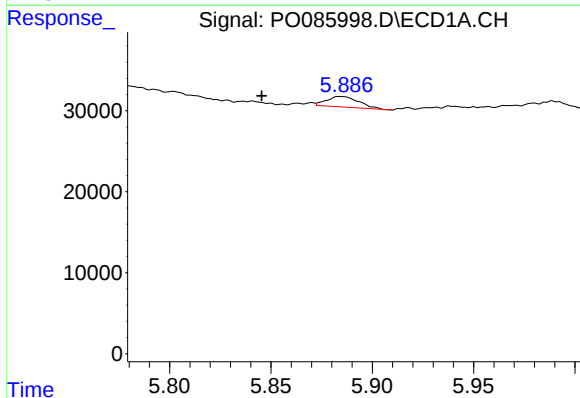


#6 AR-1016-4

R.T.: 5.884 min
Delta R.T.: 0.038 min
Response: 14468
Conc: 6.53 ng/ml

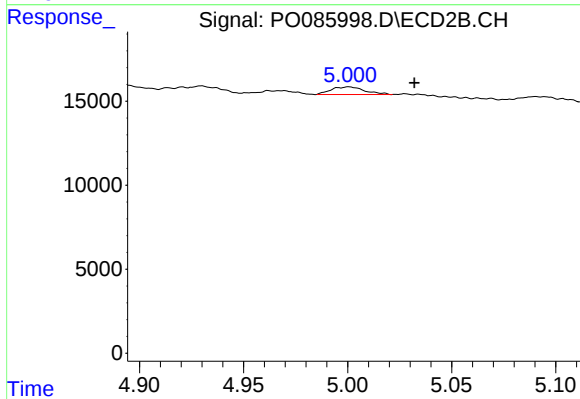

#6 AR-1016-4


R.T.: 5.001 min
Delta R.T.: -0.032 min
Response: 5135
Conc: 5.57 ng/ml

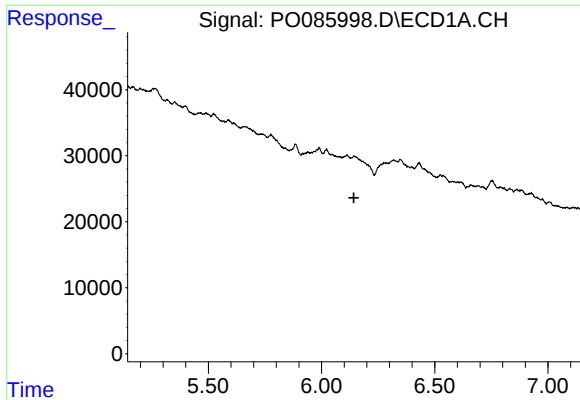

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

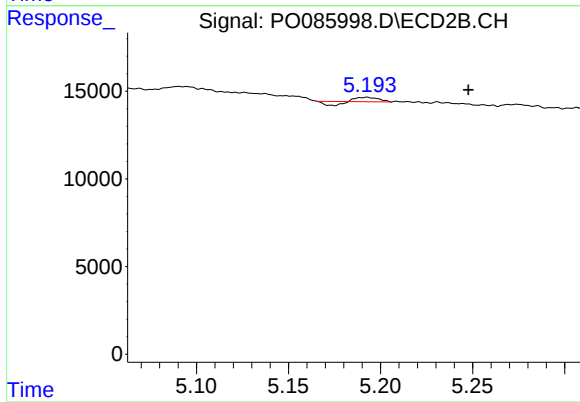


#7 AR-1016-5

R.T.: 5.193 min
Delta R.T.: -0.055 min
Response: 1131
Conc: 1.00 ng/ml

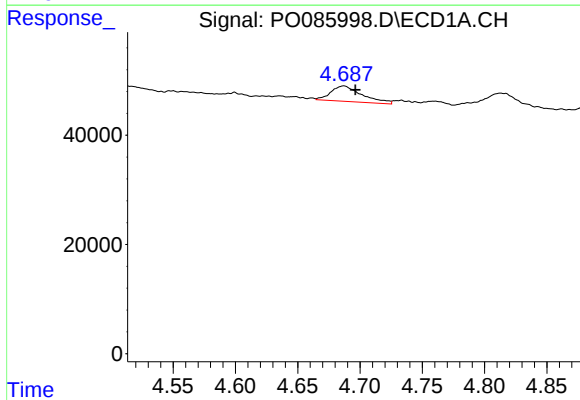


#8 AR-1221-1

R.T.: 4.687 min
Delta R.T.: -0.009 min
Response: 49180
Conc: 40.17 ng/ml

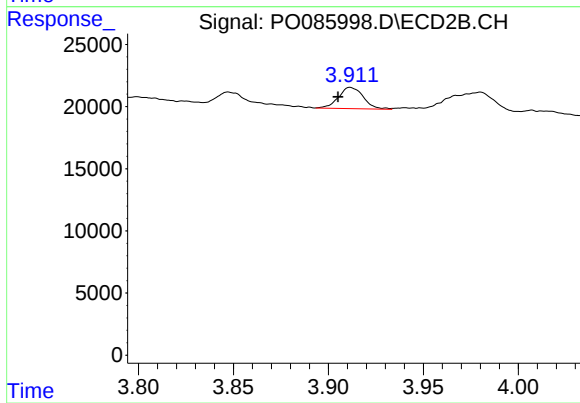

#8 AR-1221-1


R.T.: 3.911 min
Delta R.T.: 0.006 min
Response: 15485
Conc: 30.11 ng/ml

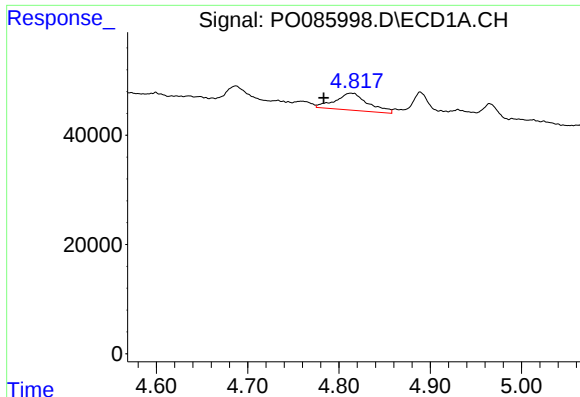

#9 AR-1221-2


R.T.: 4.813 min
Delta R.T.: 0.030 min
Response: 78208
Conc: 85.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

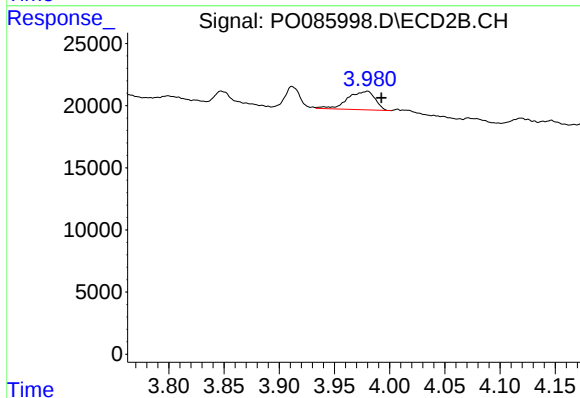


#9 AR-1221-2

R.T.: 3.980 min
Delta R.T.: -0.012 min
Response: 25561
Conc: 66.32 ng/ml

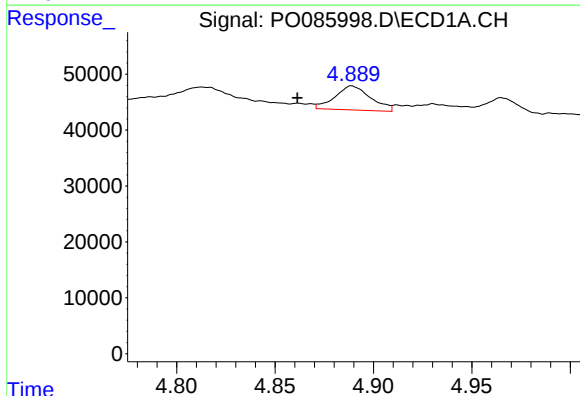


#10 AR-1221-3

R.T.: 4.889 min
Delta R.T.: 0.028 min
Response: 54403
Conc: 20.19 ng/ml

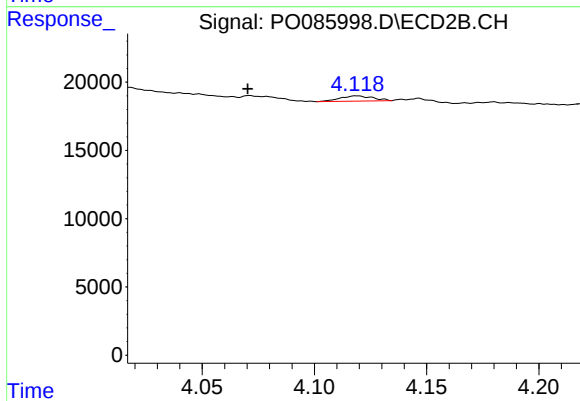

#10 AR-1221-3


R.T.: 4.119 min
Delta R.T.: 0.048 min
Response: 3853
Conc: 3.17 ng/ml

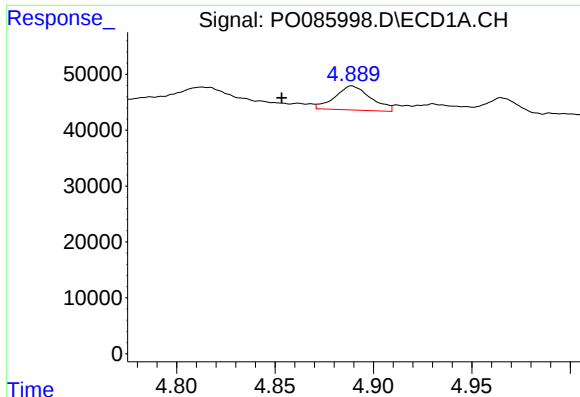

#11 AR-1232-1


R.T.: 4.889 min
Delta R.T.: 0.035 min
Response: 54403
Conc: 26.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

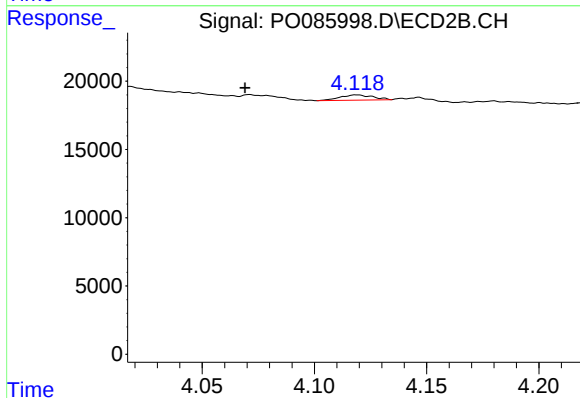


#11 AR-1232-1

R.T.: 4.119 min
Delta R.T.: 0.050 min
Response: 3853
Conc: 4.17 ng/ml

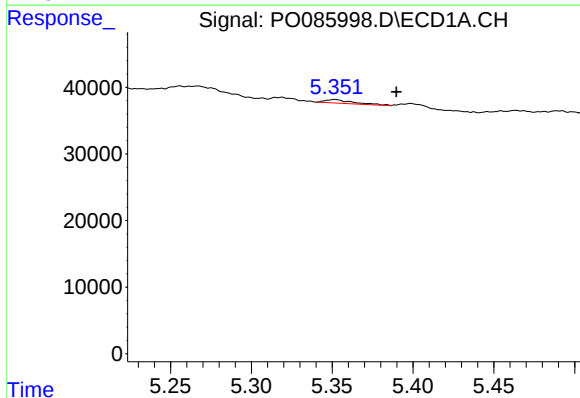


#12 AR-1232-2

R.T.: 5.352 min
Delta R.T.: -0.038 min
Response: 6644
Conc: 7.05 ng/ml

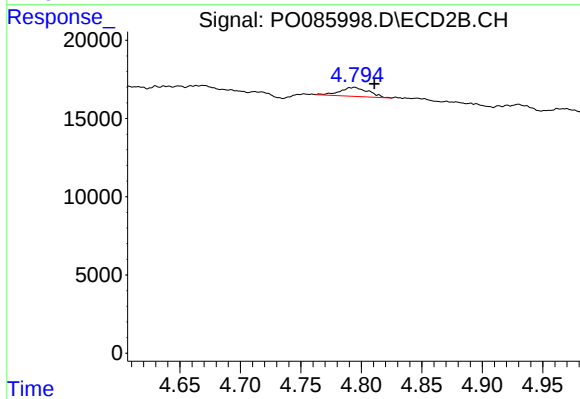

#12 AR-1232-2


R.T.: 4.795 min
Delta R.T.: -0.016 min
Response: 9380
Conc: 11.51 ng/ml

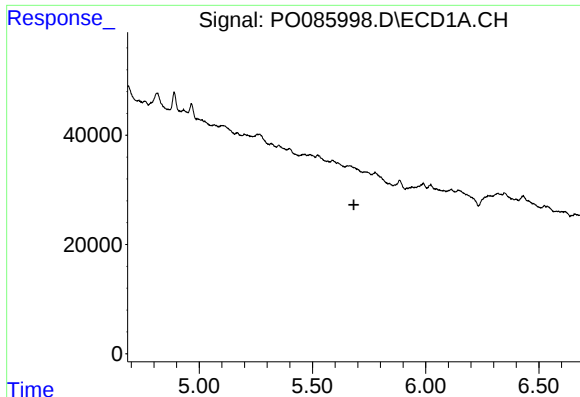

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.683 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

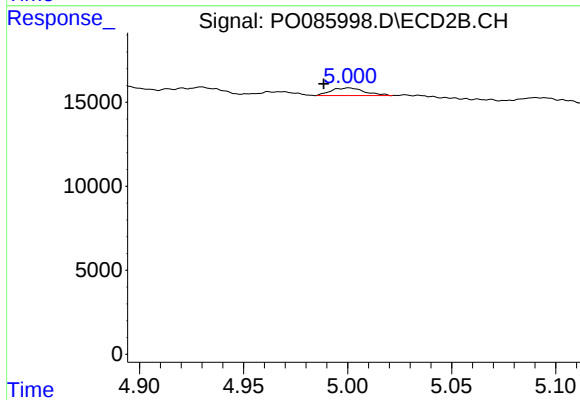


#13 AR-1232-3

R.T.: 5.001 min
Delta R.T.: 0.012 min
Response: 5135
Conc: 12.44 ng/ml

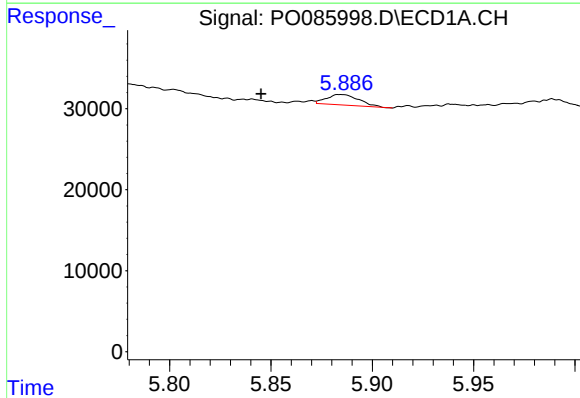


#14 AR-1232-4

R.T.: 5.884 min
Delta R.T.: 0.038 min
Response: 14468
Conc: 16.63 ng/ml

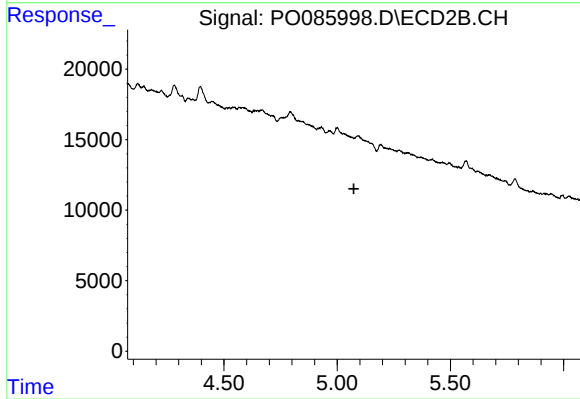

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T.: 5.073 min
Response: 0
Conc: N.D.

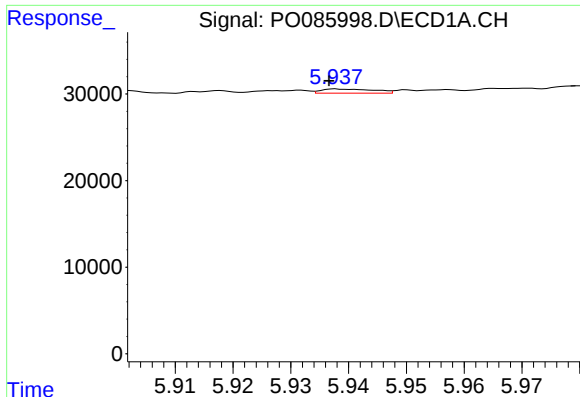

#15 AR-1232-5


R.T.: 5.938 min
Delta R.T.: 0.001 min
Response: 3091
Conc: 4.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

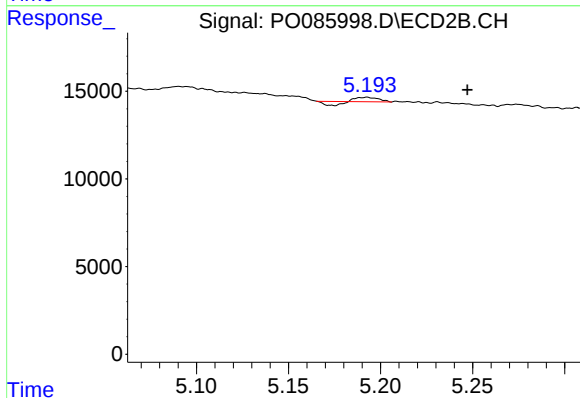


#15 AR-1232-5

R.T.: 5.193 min
Delta R.T.: -0.054 min
Response: 1131
Conc: 2.70 ng/ml

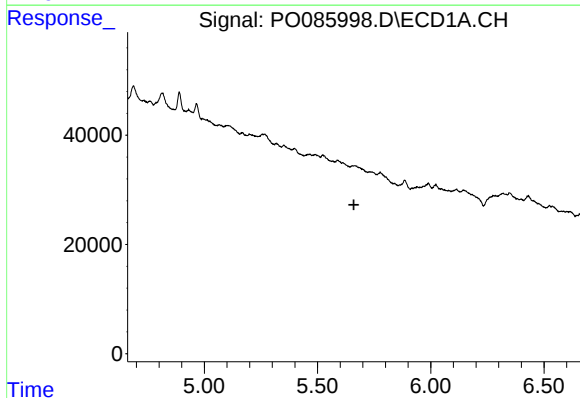


#16 AR-1242-1

R.T.: 0.000 min
Exp R.T. : 5.660 min
Response: 0
Conc: N.D.

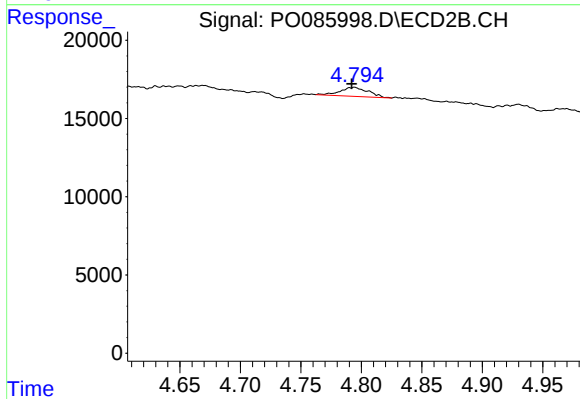

#16 AR-1242-1


R.T.: 4.795 min
Delta R.T.: 0.003 min
Response: 9380
Conc: 7.10 ng/ml

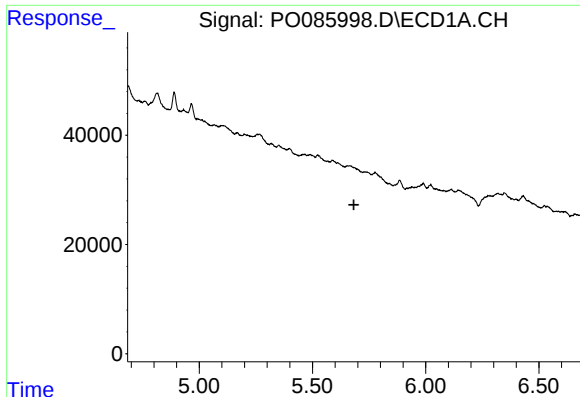

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.683 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

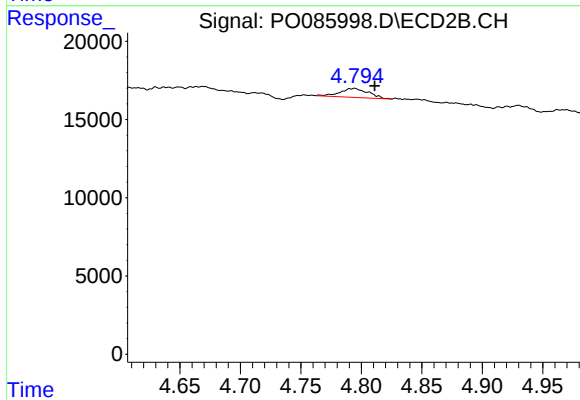


#17 AR-1242-2

R.T.: 4.795 min
Delta R.T.: -0.016 min
Response: 9380
Conc: 5.35 ng/ml

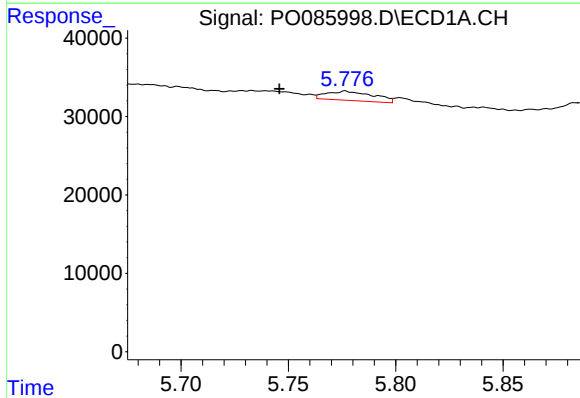


#18 AR-1242-3

R.T.: 5.777 min
Delta R.T.: 0.031 min
Response: 18084
Conc: 7.70 ng/ml

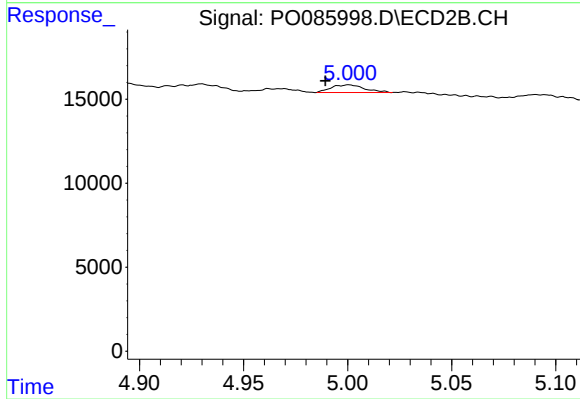

#18 AR-1242-3


R.T.: 5.001 min
Delta R.T.: 0.011 min
Response: 5135
Conc: 5.46 ng/ml

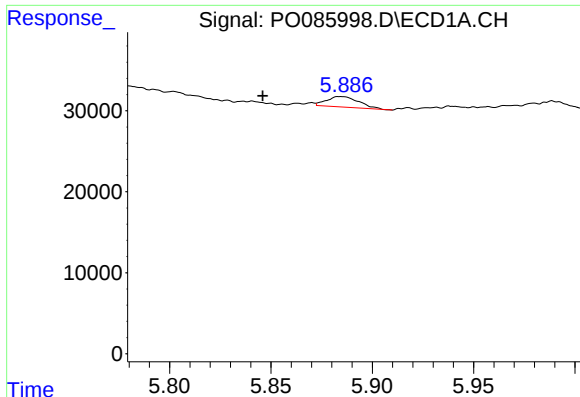

#19 AR-1242-4


R.T.: 5.884 min
Delta R.T.: 0.038 min
Response: 14468
Conc: 7.63 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

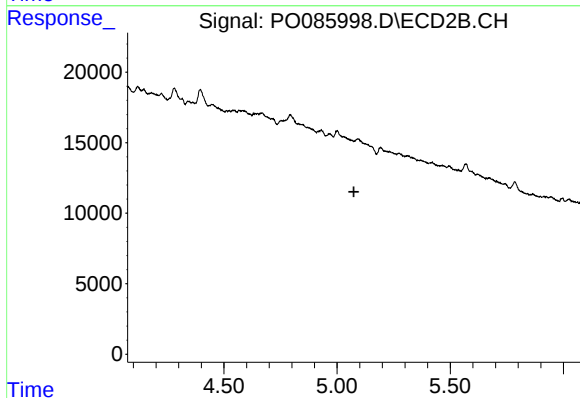


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.074 min
Response: 0
Conc: N.D.

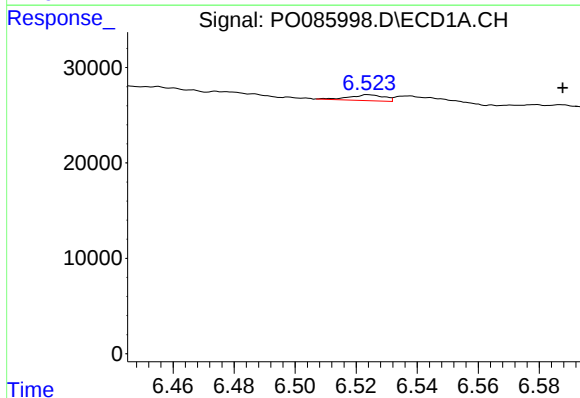


#20 AR-1242-5

R.T.: 6.524 min
Delta R.T.: -0.064 min
Response: 4839
Conc: 2.64 ng/ml

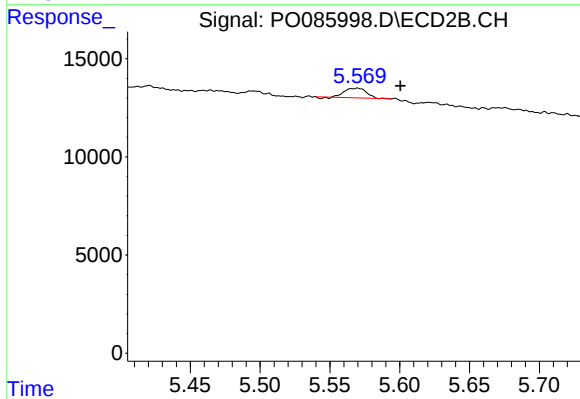

#20 AR-1242-5


R.T.: 5.570 min
Delta R.T.: -0.031 min
Response: 5180
Conc: 4.56 ng/ml

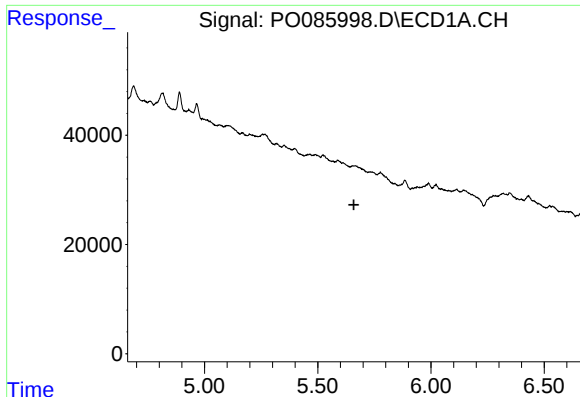

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.660 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

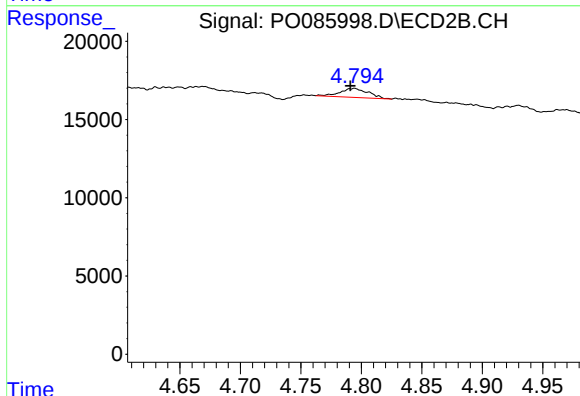


#21 AR-1248-1

R.T.: 4.795 min
Delta R.T.: 0.003 min
Response: 9380
Conc: 9.66 ng/ml

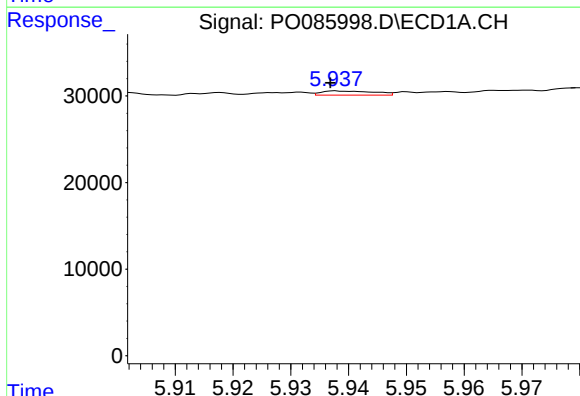


#22 AR-1248-2

R.T.: 5.938 min
Delta R.T.: 0.001 min
Response: 3091
Conc: 1.15 ng/ml

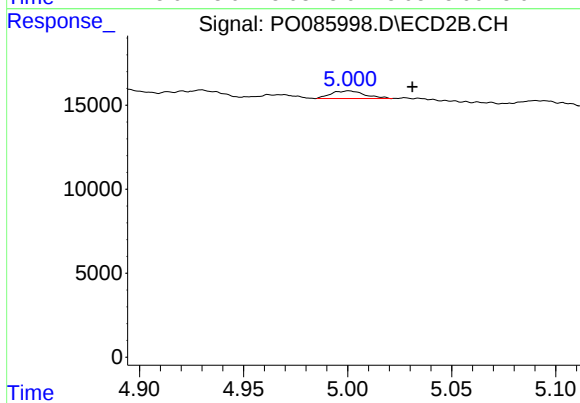

#22 AR-1248-2


R.T.: 5.001 min
Delta R.T.: -0.031 min
Response: 5135
Conc: 3.86 ng/ml

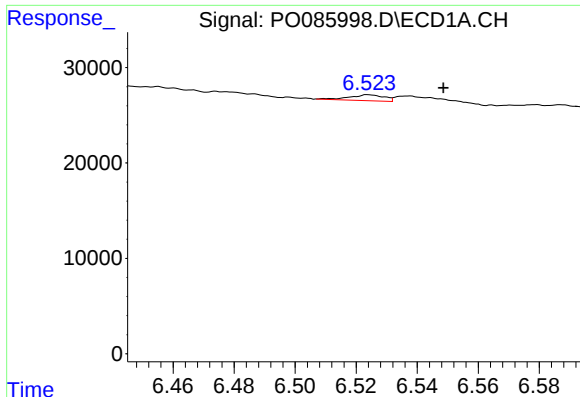

#24 AR-1248-4


R.T.: 6.524 min
Delta R.T.: -0.025 min
Response: 4839
Conc: 1.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

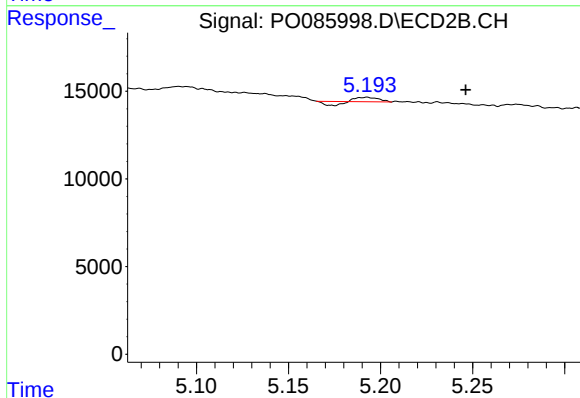


#24 AR-1248-4

R.T.: 5.193 min
Delta R.T.: -0.053 min
Response: 1131
Conc: 0.71 ng/ml

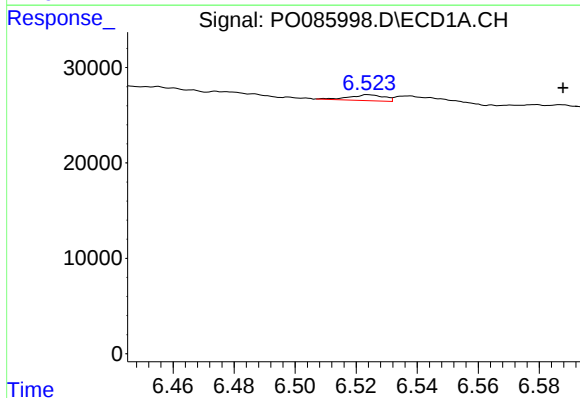


#25 AR-1248-5

R.T.: 6.524 min
Delta R.T.: -0.064 min
Response: 4839
Conc: 1.55 ng/ml

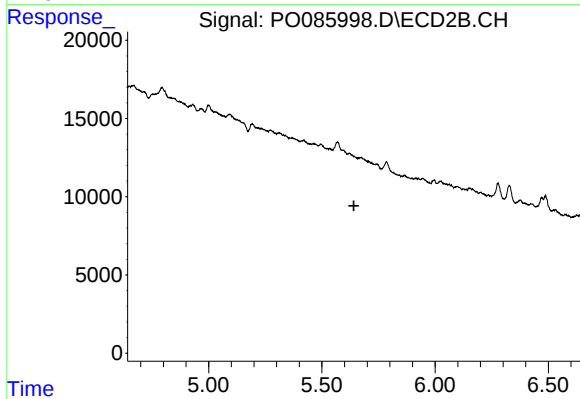

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 5.642 min
Response: 0
Conc: N.D.

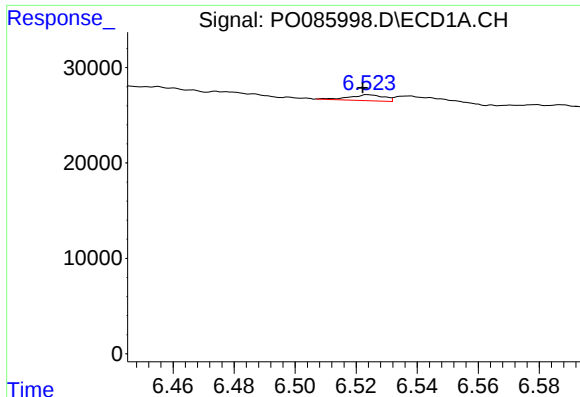

#26 AR-1254-1


R.T.: 6.524 min
Delta R.T.: 0.002 min
Response: 4839
Conc: 1.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

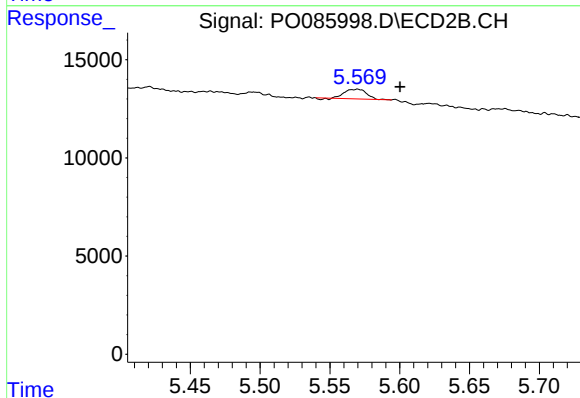


#26 AR-1254-1

R.T.: 5.570 min
Delta R.T.: -0.030 min
Response: 5180
Conc: 2.06 ng/ml

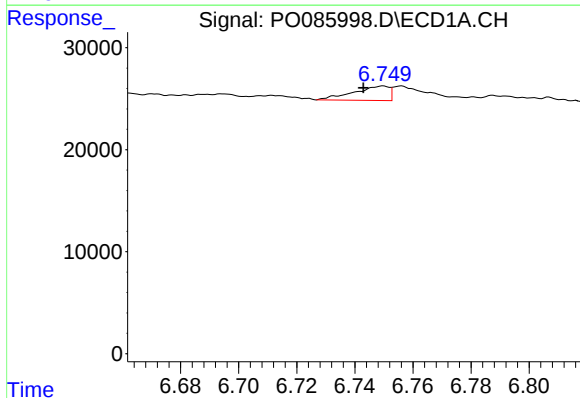


#27 AR-1254-2

R.T.: 6.750 min
Delta R.T.: 0.007 min
Response: 11995
Conc: 2.44 ng/ml

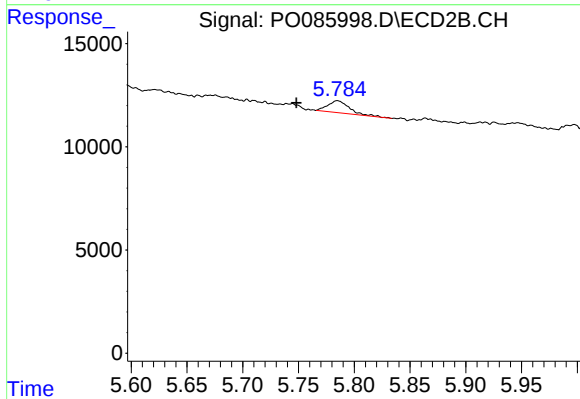

#27 AR-1254-2


R.T.: 5.785 min
Delta R.T.: 0.037 min
Response: 7987
Conc: 3.65 ng/ml

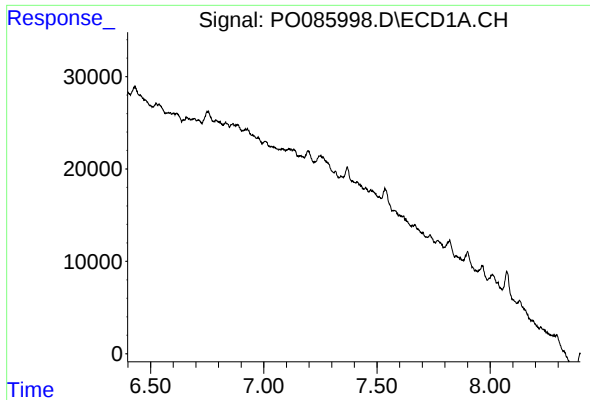

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

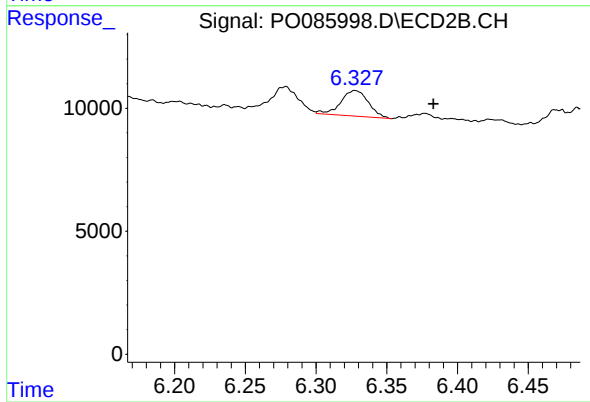


#29 AR-1254-4

R.T.: 6.328 min
Delta R.T.: -0.055 min
Response: 14169
Conc: 6.41 ng/ml

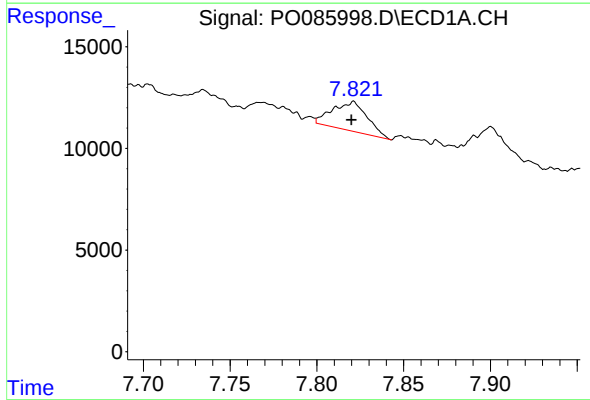


#30 AR-1254-5

R.T.: 7.821 min
Delta R.T.: 0.001 min
Response: 20093
Conc: 5.16 ng/ml

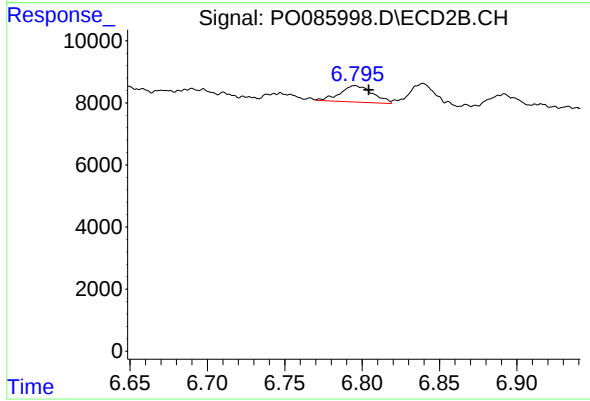

#30 AR-1254-5


R.T.: 6.796 min
Delta R.T.: -0.009 min
Response: 7826
Conc: 2.65 ng/ml

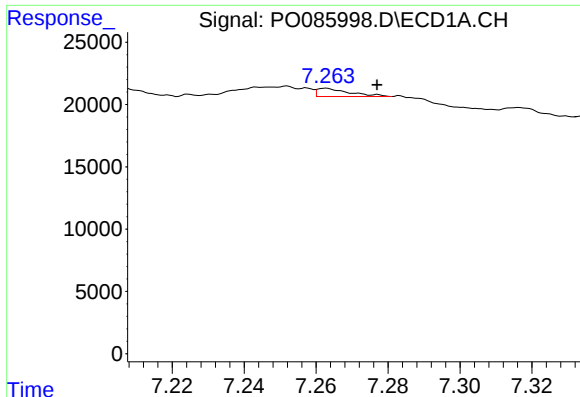

#31 AR-1260-1


R.T.: 7.263 min
Delta R.T.: -0.014 min
Response: 4041
Conc: 1.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

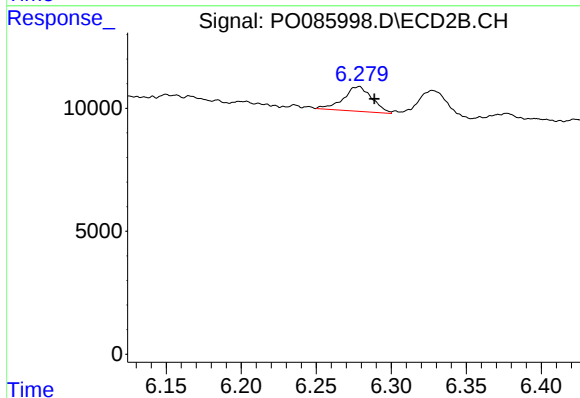


#31 AR-1260-1

R.T.: 6.279 min
Delta R.T.: -0.010 min
Response: 13353
Conc: 6.86 ng/ml

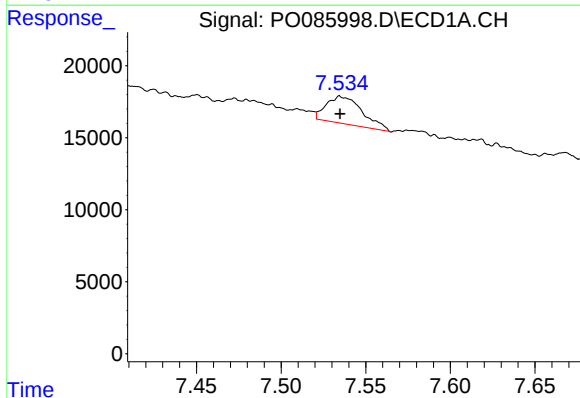


#32 AR-1260-2

R.T.: 7.535 min
Delta R.T.: 0.000 min
Response: 28261
Conc: 7.81 ng/ml

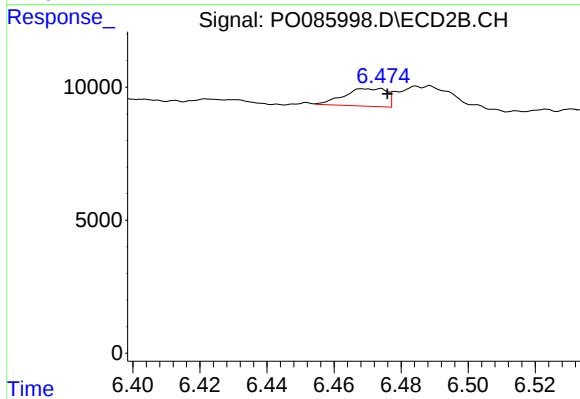

#32 AR-1260-2


R.T.: 6.474 min
Delta R.T.: -0.002 min
Response: 5830
Conc: 2.48 ng/ml

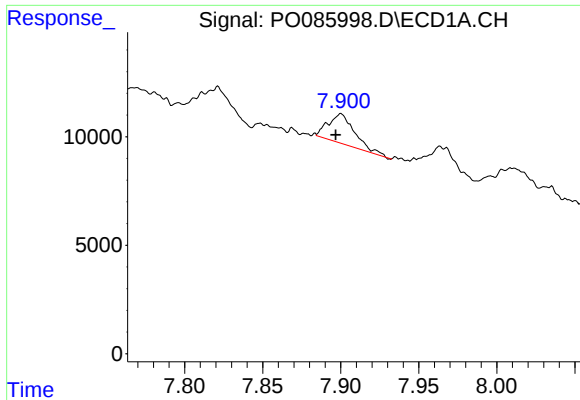

#33 AR-1260-3


R.T.: 7.900 min
Delta R.T.: 0.003 min
Response: 16134
Conc: 5.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

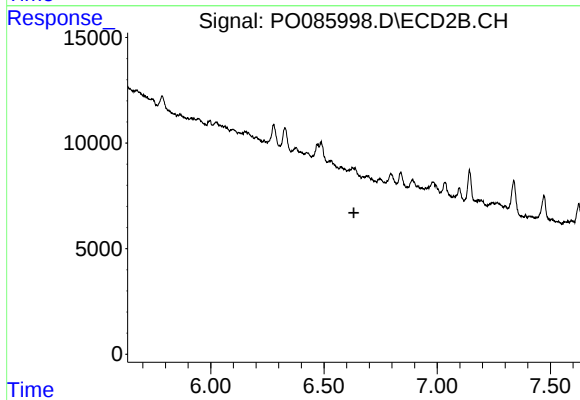


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.632 min
Response: 0
Conc: N.D.

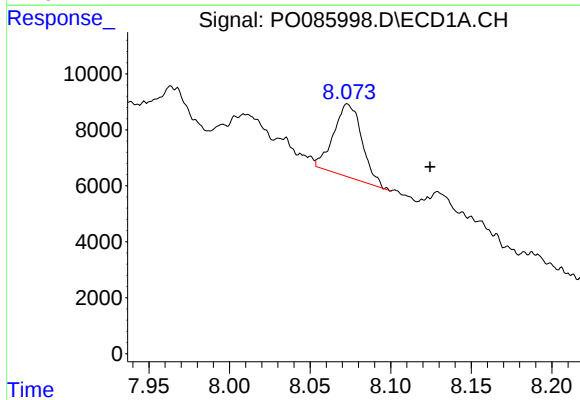


#34 AR-1260-4

R.T.: 8.073 min
Delta R.T.: -0.051 min
Response: 32092
Conc: 9.51 ng/ml

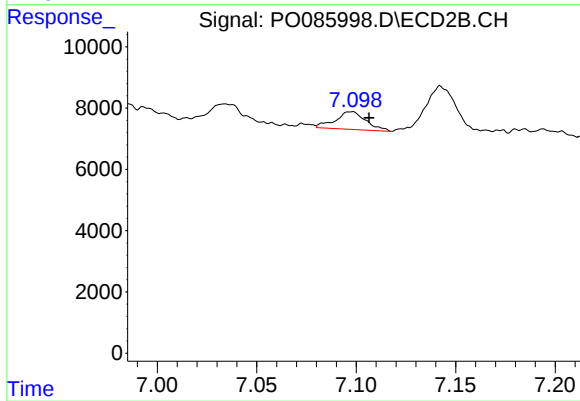

#34 AR-1260-4


R.T.: 7.098 min
Delta R.T.: -0.008 min
Response: 6238
Conc: 3.46 ng/ml

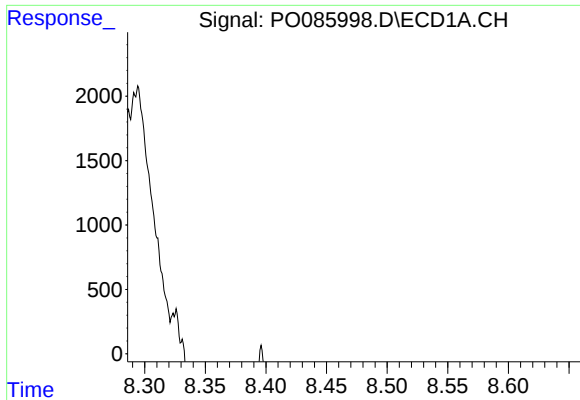

#35 AR-1260-5


R.T.: 8.459 min
Delta R.T.: 0.006 min
Response: 28742
Conc: 4.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

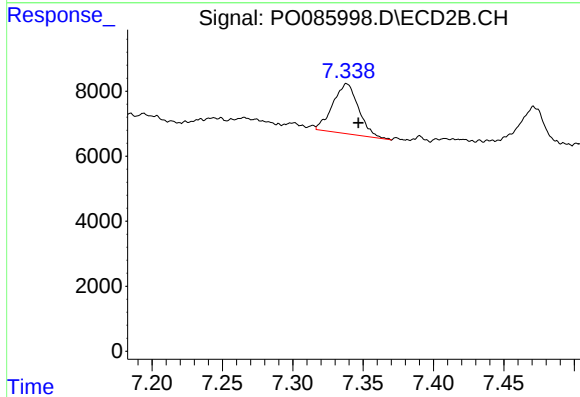


#35 AR-1260-5

R.T.: 7.338 min
Delta R.T.: -0.008 min
Response: 19701
Conc: 4.55 ng/ml

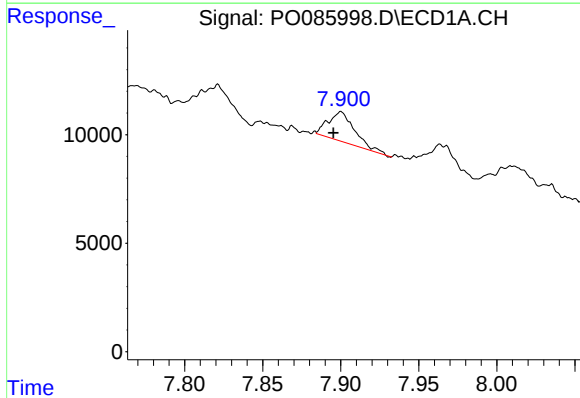


#36 AR-1262-1

R.T.: 7.900 min
Delta R.T.: 0.005 min
Response: 16134
Conc: 3.57 ng/ml

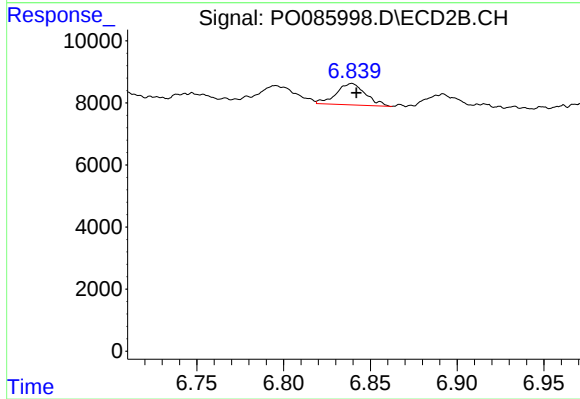

#36 AR-1262-1


R.T.: 6.839 min
Delta R.T.: -0.003 min
Response: 8105
Conc: 2.68 ng/ml

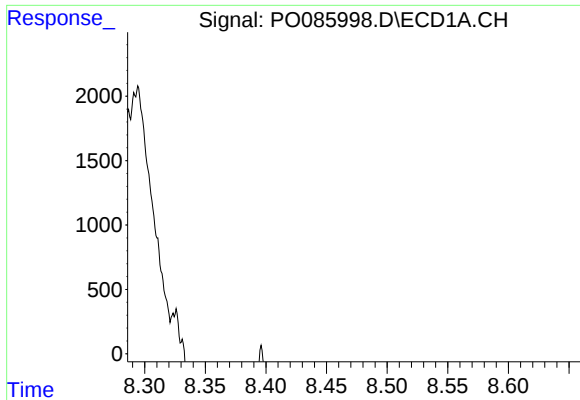

#37 AR-1262-2


R.T.: 8.459 min
Delta R.T.: 0.009 min
Response: 28742
Conc: 3.67 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

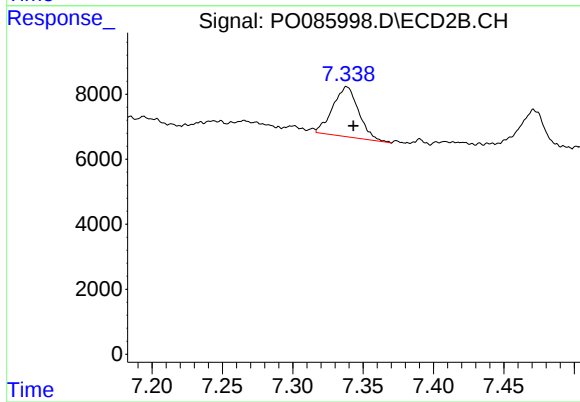


#37 AR-1262-2

R.T.: 7.338 min
Delta R.T.: -0.005 min
Response: 19701
Conc: 3.59 ng/ml

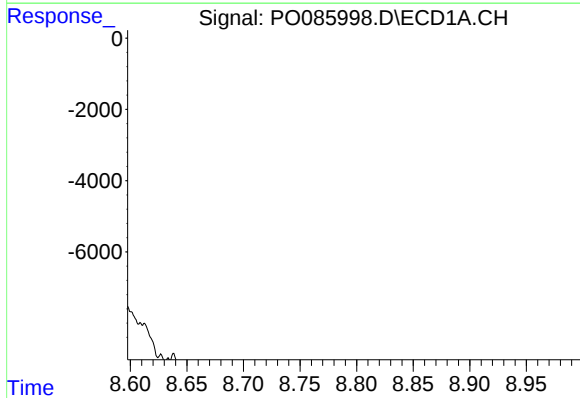


#38 AR-1262-3

R.T.: 8.775 min
Delta R.T.: 0.002 min
Response: 46880
Conc: 14.31 ng/ml

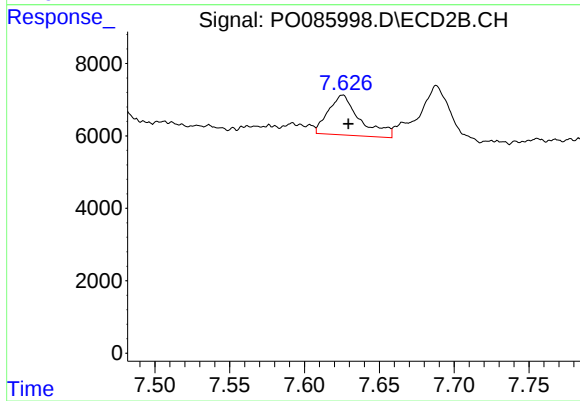

#38 AR-1262-3


R.T.: 7.626 min
Delta R.T.: -0.004 min
Response: 16120
Conc: 7.65 ng/ml

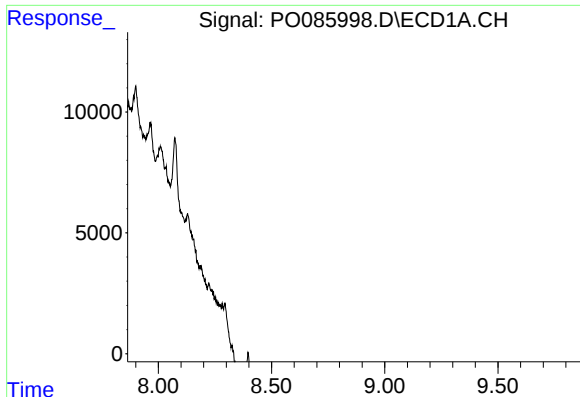

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.864 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

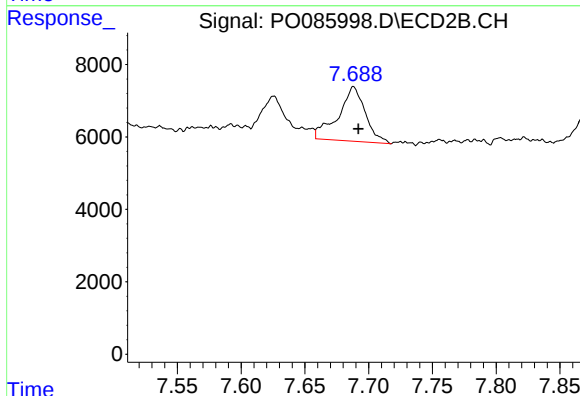


#39 AR-1262-4

R.T.: 7.688 min
Delta R.T.: -0.004 min
Response: 22316
Conc: 5.63 ng/ml

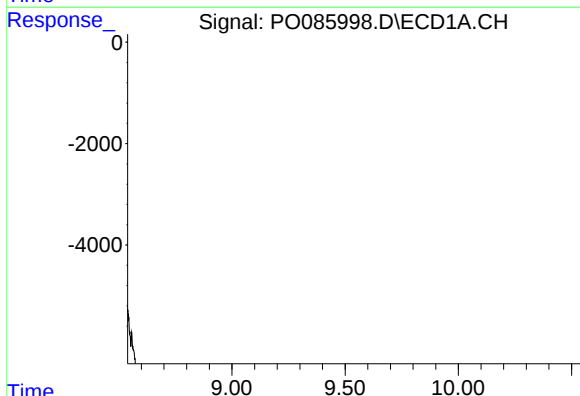


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.539 min
Response: 0
Conc: N.D.

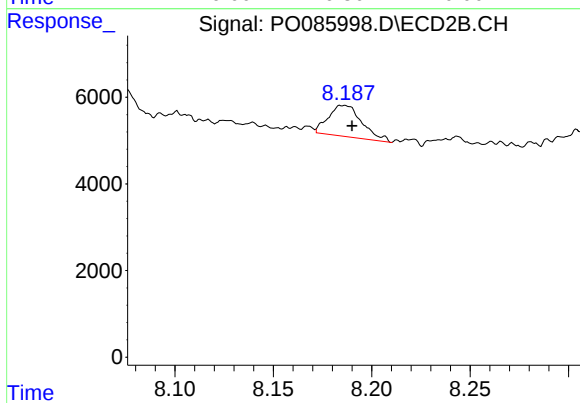

#40 AR-1262-5


R.T.: 8.187 min
Delta R.T.: -0.003 min
Response: 8531
Conc: 4.76 ng/ml

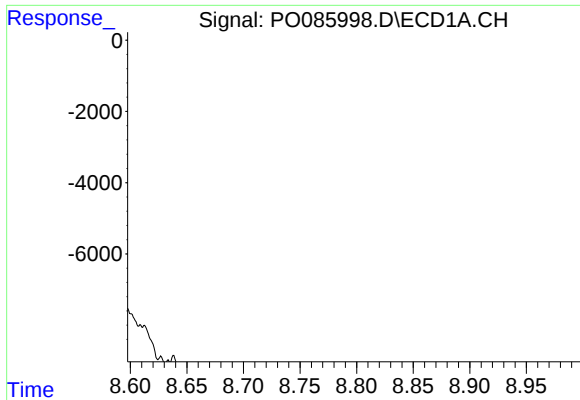

#41 AR-1268-1


R.T.: 8.775 min
Delta R.T.: 0.005 min
Response: 46880
Conc: 5.37 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

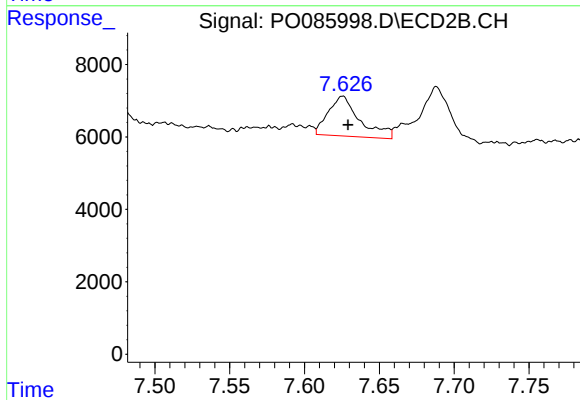


#41 AR-1268-1

R.T.: 7.626 min
Delta R.T.: -0.003 min
Response: 16120
Conc: 2.64 ng/ml

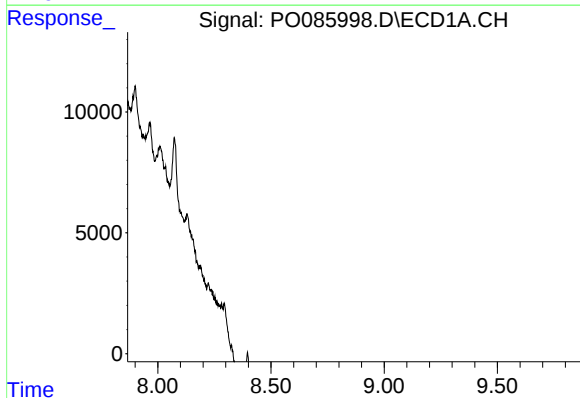


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.867 min
Response: 0
Conc: N.D.

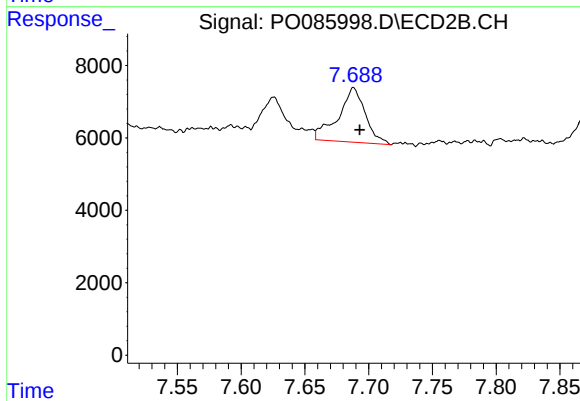

#42 AR-1268-2


R.T.: 7.688 min
Delta R.T.: -0.005 min
Response: 22316
Conc: 4.07 ng/ml

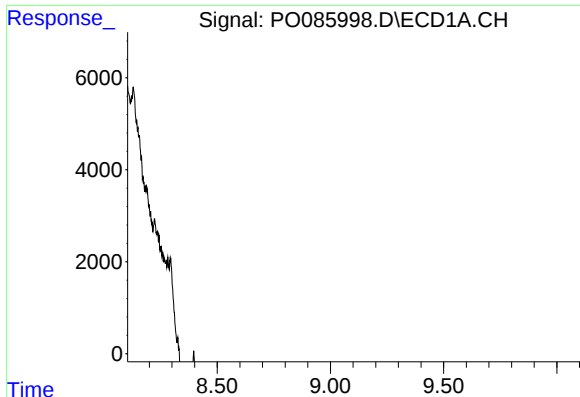

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T. : 9.104 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

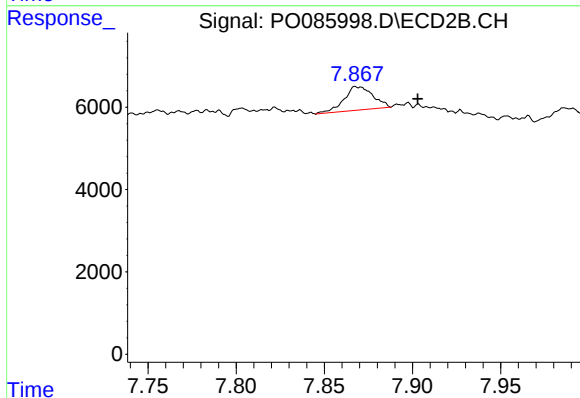


#43 AR-1268-3

R.T.: 7.868 min
Delta R.T.: -0.035 min
Response: 6478
Conc: 1.43 ng/ml

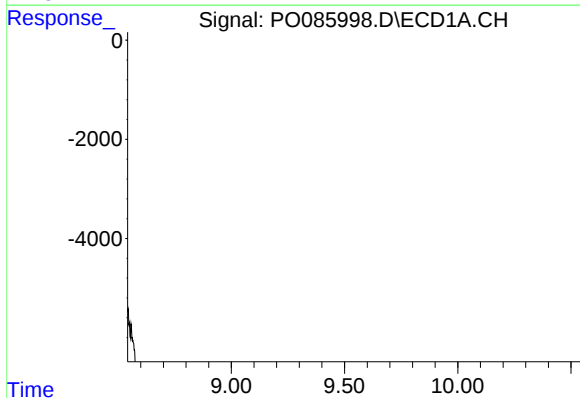


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.541 min
Response: 0
Conc: N.D.

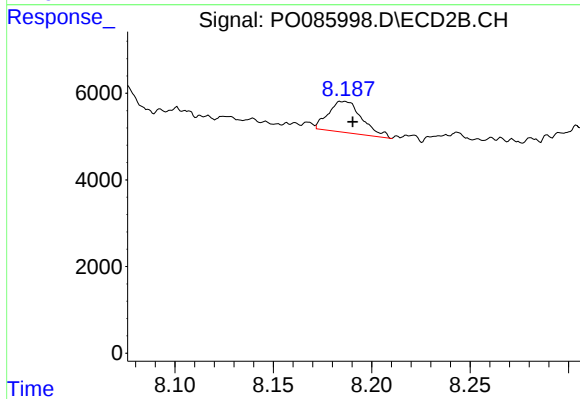

#44 AR-1268-4


R.T.: 8.187 min
Delta R.T.: -0.004 min
Response: 8531
Conc: 4.37 ng/ml

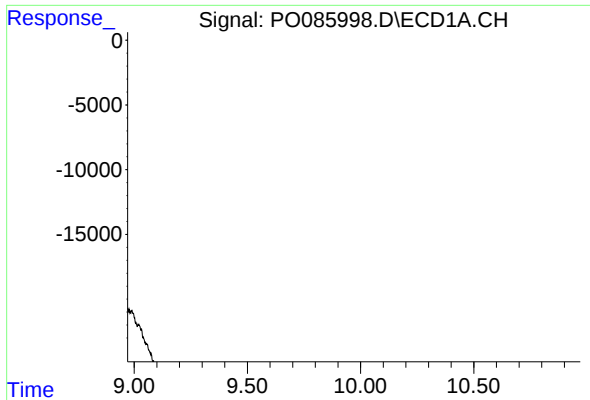

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-5

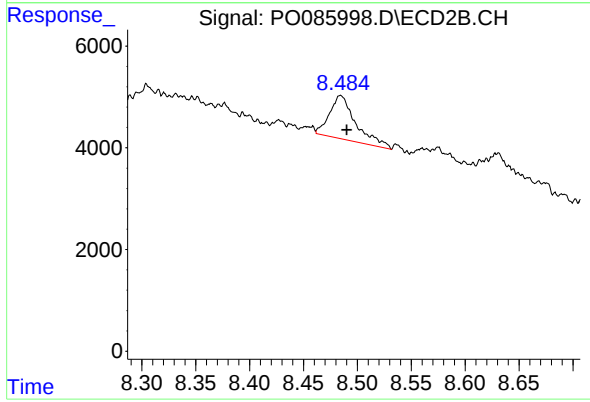

#45 AR-1268-5

R.T.: 8.484 min
Delta R.T.: -0.006 min
Response: 14501
Conc: 0.99 ng/ml