

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
 Data File : P0085999.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2022 00:08
 Operator : YP\AJ
 Sample : N2771-07 10X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-BC157517-1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 07:14:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	3.682	188164	80676	1.853	1.851
2)	SA Decachlor...	10.328	8.748	113294	58595	2.138	1.726
Target Compounds							
3)	L1 AR-1016-1	5.658	4.800	22485	8610	7.036	5.513
4)	L1 AR-1016-2	5.658	4.800	22485	8610	5.058	4.112
5)	L1 AR-1016-3	5.734	0.000	8390	0	3.060	N.D. #
6)	L1 AR-1016-4	5.802f	0.000	4029	0	1.818	N.D. #
7)	L1 AR-1016-5	0.000	5.221	0	2723	N.D.	2.411 #
8)	L2 AR-1221-1	4.692	0.000	3670	0	2.997	N.D. #
9)	L2 AR-1221-2	4.809	0.000	11184	0	12.252	N.D. #
10)	L2 AR-1221-3	4.832	0.000	914	0	0.339	N.D. #
11)	L3 AR-1232-1	4.832	0.000	914	0	0.447	N.D. #
12)	L3 AR-1232-2	5.378	4.800	26199	8610	27.819	10.562 #
13)	L3 AR-1232-3	5.658	0.000	22485	0	12.793	N.D. #
14)	L3 AR-1232-4	5.802f	0.000	4029	0	4.632	N.D. #
15)	L3 AR-1232-5	5.968	5.221	12419	2723	18.755	6.501 #
16)	L4 AR-1242-1	5.658	4.800	22485	8610	8.272	6.518
17)	L4 AR-1242-2	5.658	4.800	22485	8610	5.981	4.910
18)	L4 AR-1242-3	5.734	0.000	8390	0	3.571	N.D. #
19)	L4 AR-1242-4	5.802f	0.000	4029	0	2.126	N.D. #
21)	L5 AR-1248-1	5.658	4.800	22485	8610	11.132	8.867
22)	L5 AR-1248-2	5.968	0.000	12419	0	4.604	N.D. #
24)	L5 AR-1248-4	0.000	5.221	0	2723	N.D.	1.700 #
29)	L6 AR-1254-4	7.378	0.000	1497	0	0.402	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
Data File : P0085999.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2022 00:08
Operator : YP\AJ
Sample : N2771-07 10X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:14:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

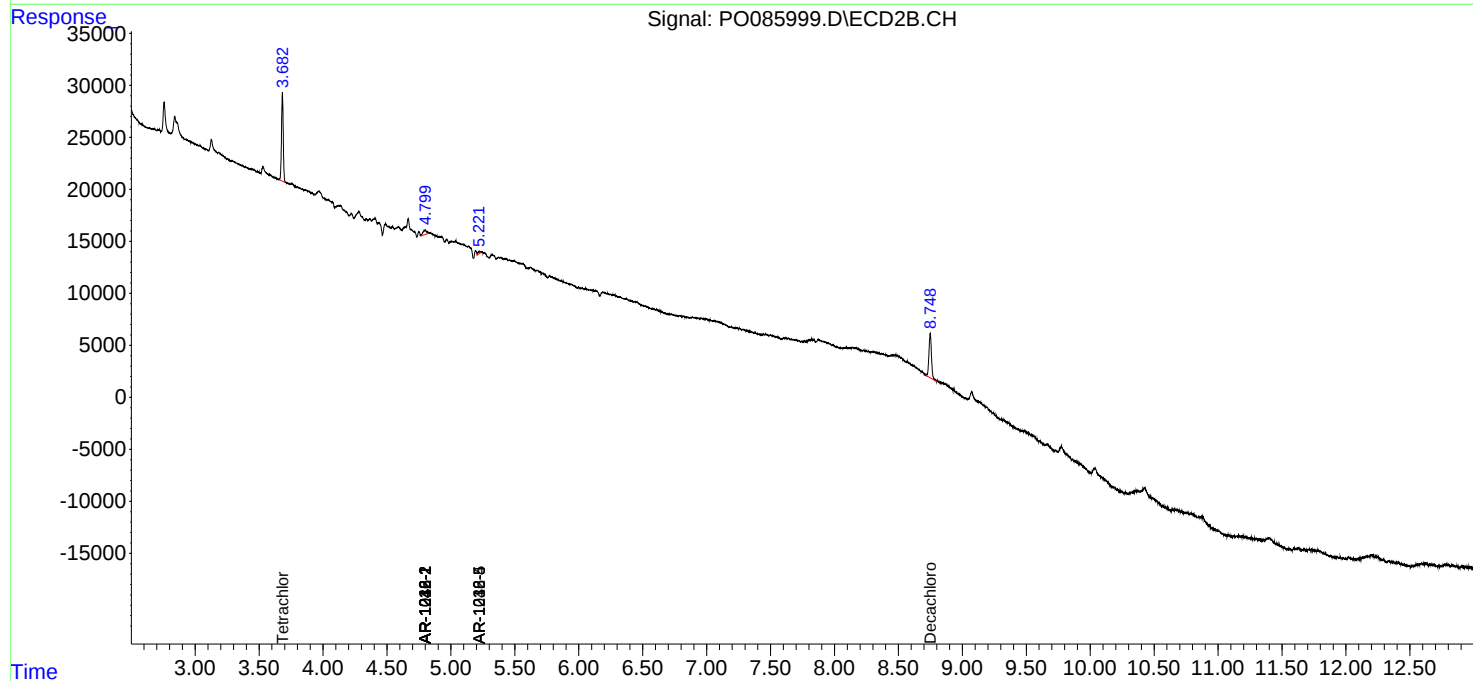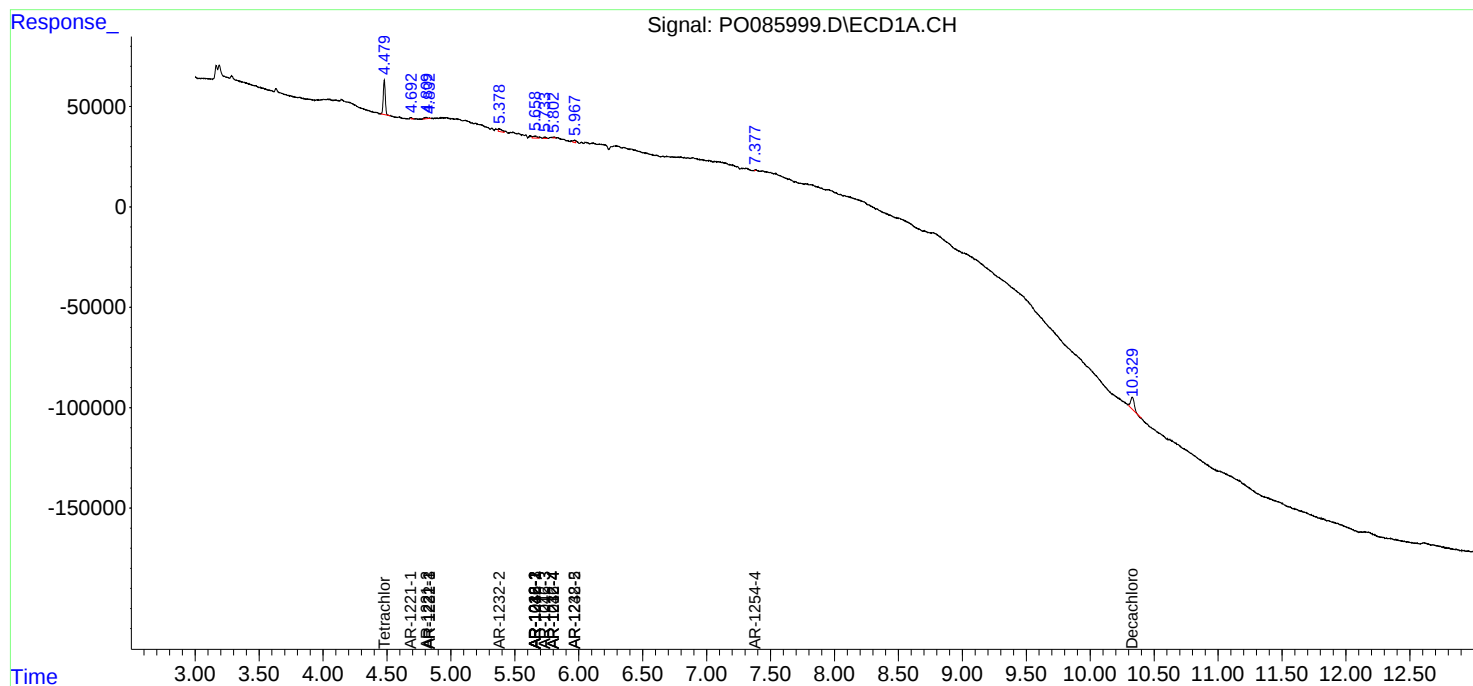


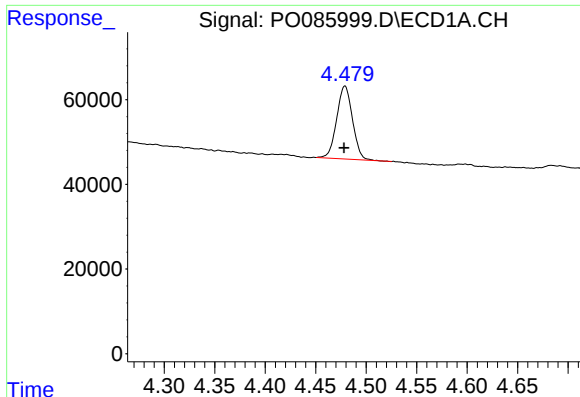

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: 0.001 min
Response: 188164
Conc: 1.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

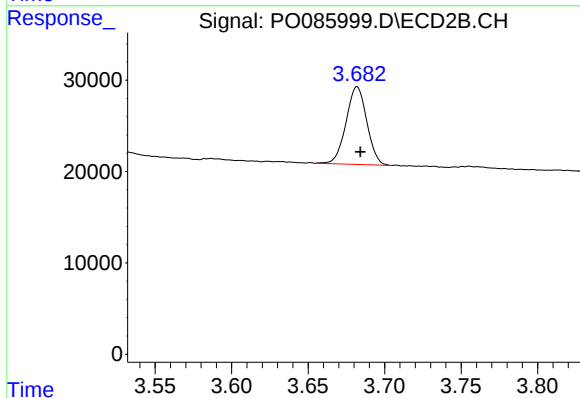


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.002 min
Response: 80676
Conc: 1.85 ng/ml

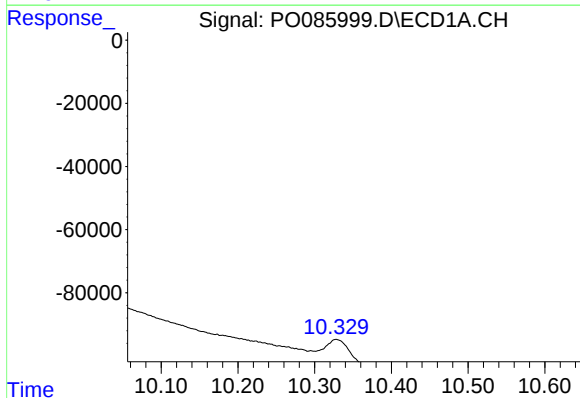


#2 Decachlorobiphenyl

R.T.: 10.328 min
Delta R.T.: 0.000 min
Response: 113294
Conc: 2.14 ng/ml

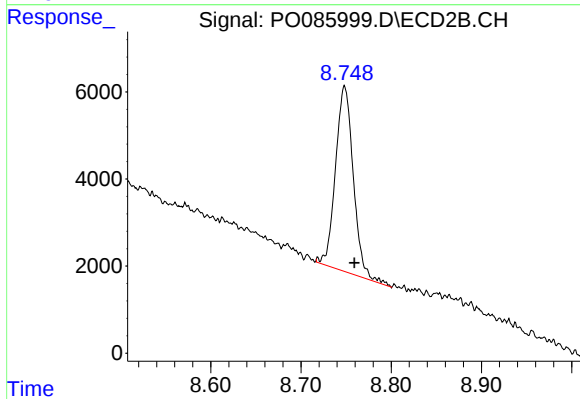

#2 Decachlorobiphenyl


R.T.: 8.748 min
Delta R.T.: -0.011 min
Response: 58595
Conc: 1.73 ng/ml

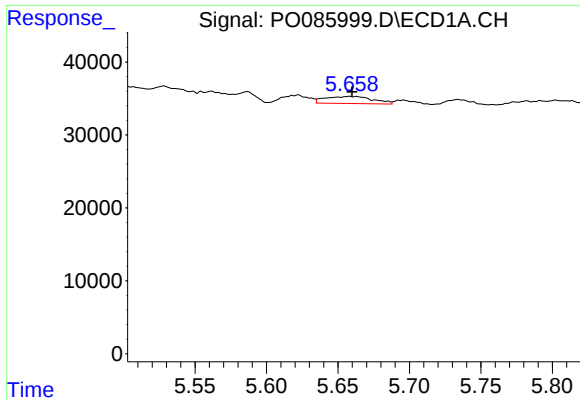

#3 AR-1016-1


R.T.: 5.658 min
Delta R.T.: -0.002 min
Response: 22485
Conc: 7.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

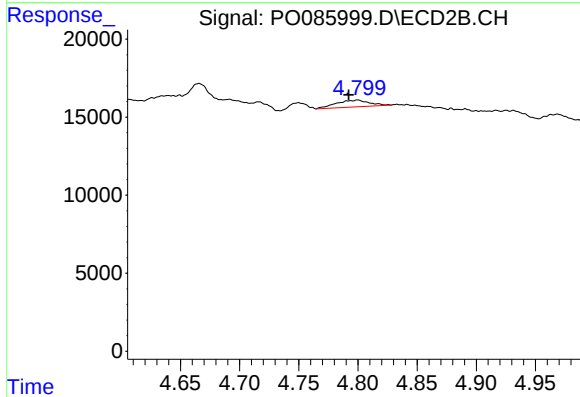


#3 AR-1016-1

R.T.: 4.800 min
Delta R.T.: 0.008 min
Response: 8610
Conc: 5.51 ng/ml

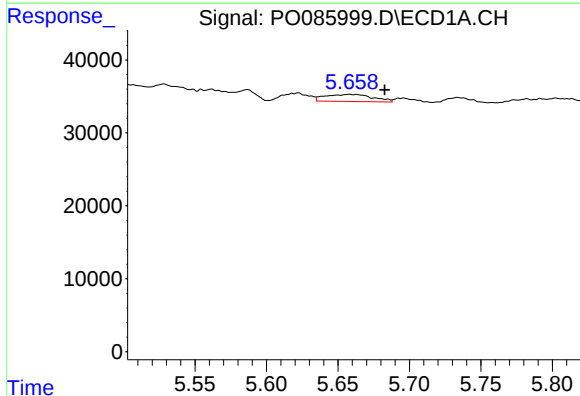


#4 AR-1016-2

R.T.: 5.658 min
Delta R.T.: -0.025 min
Response: 22485
Conc: 5.06 ng/ml

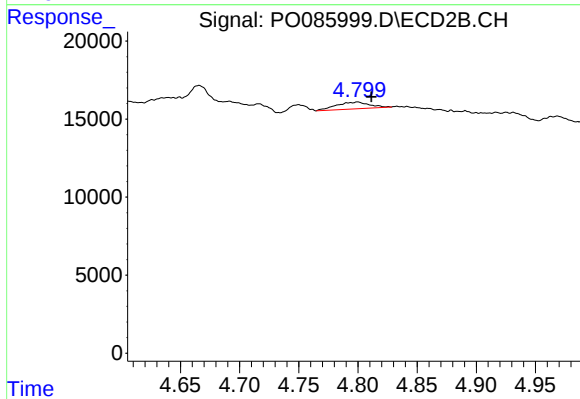

#4 AR-1016-2


R.T.: 4.800 min
Delta R.T.: -0.012 min
Response: 8610
Conc: 4.11 ng/ml

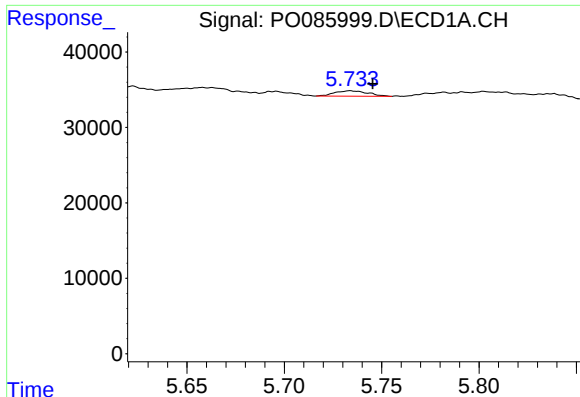

#5 AR-1016-3


R.T.: 5.734 min
Delta R.T.: -0.012 min
Response: 8390
Conc: 3.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

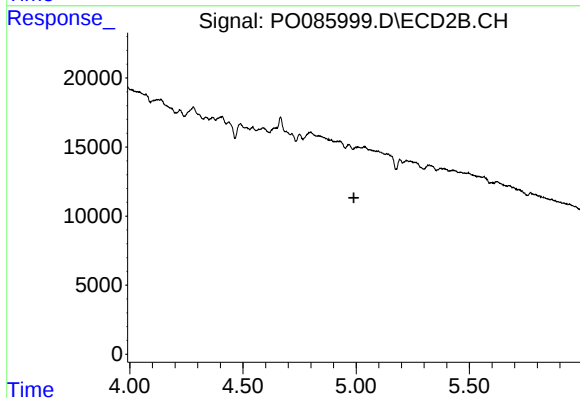


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.990 min
Response: 0
Conc: N.D.

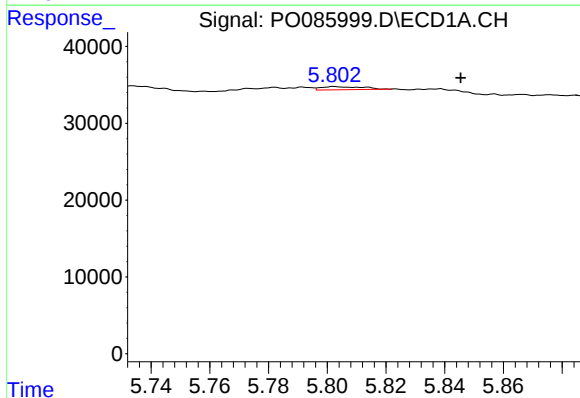


#6 AR-1016-4

R.T.: 5.802 min
Delta R.T.: -0.043 min
Response: 4029
Conc: 1.82 ng/ml

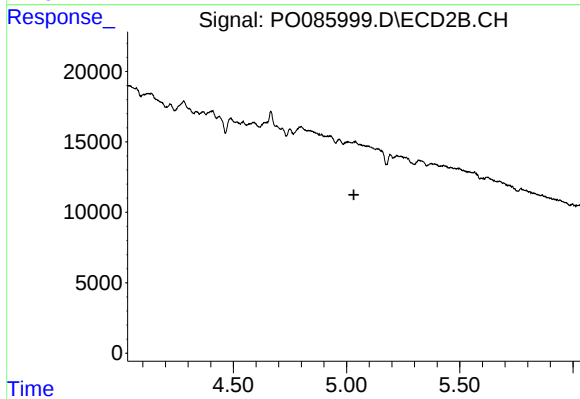

#6 AR-1016-4


R.T.: 0.000 min
Exp R.T. : 5.032 min
Response: 0
Conc: N.D.

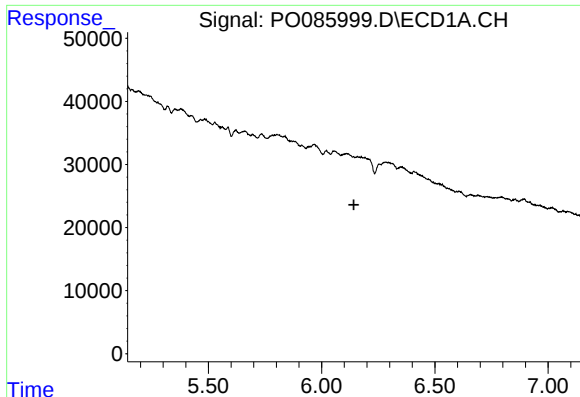

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

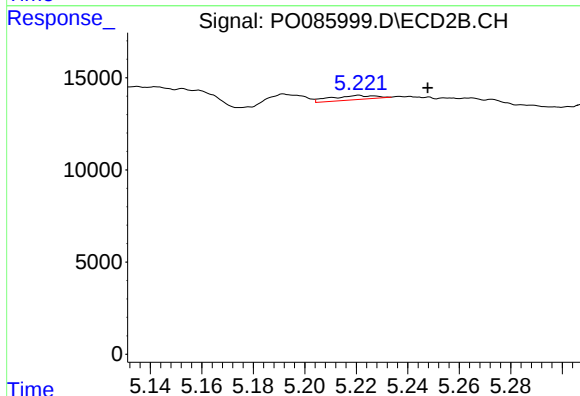


#7 AR-1016-5

R.T.: 5.221 min
Delta R.T.: -0.027 min
Response: 2723
Conc: 2.41 ng/ml

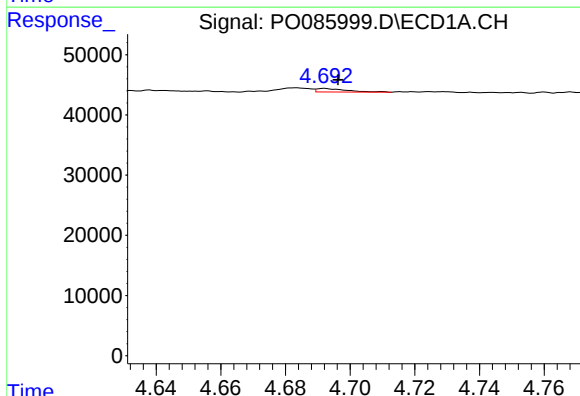


#8 AR-1221-1

R.T.: 4.692 min
Delta R.T.: -0.004 min
Response: 3670
Conc: 3.00 ng/ml

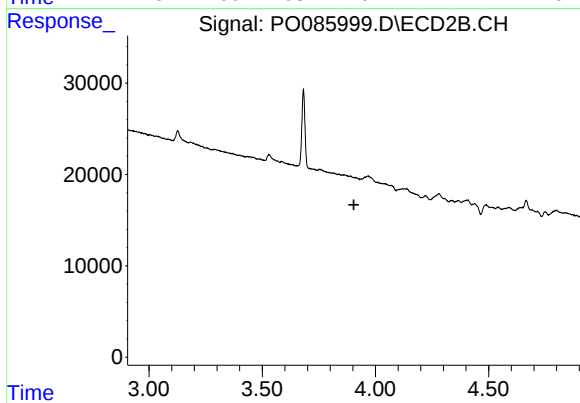

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 3.905 min
Response: 0
Conc: N.D.

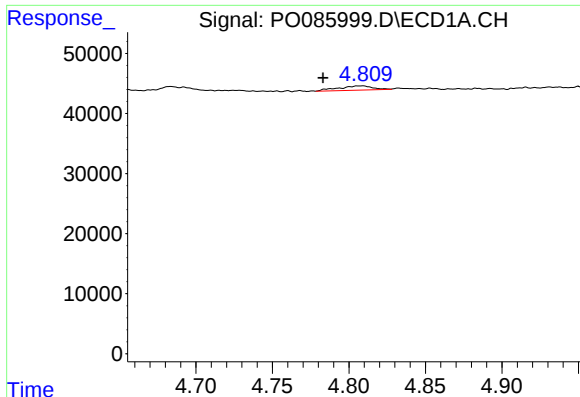

#9 AR-1221-2


R.T.: 4.809 min
Delta R.T.: 0.026 min
Response: 11184
Conc: 12.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

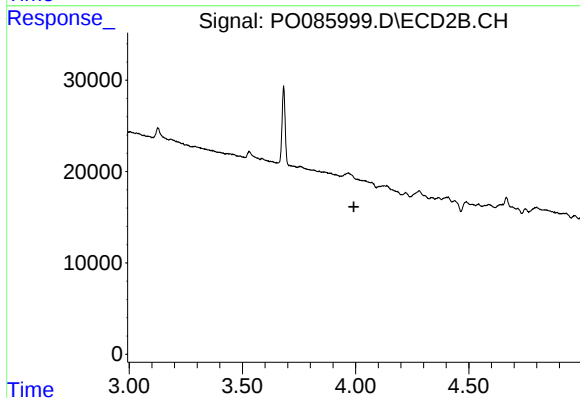


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 3.993 min
Response: 0
Conc: N.D.

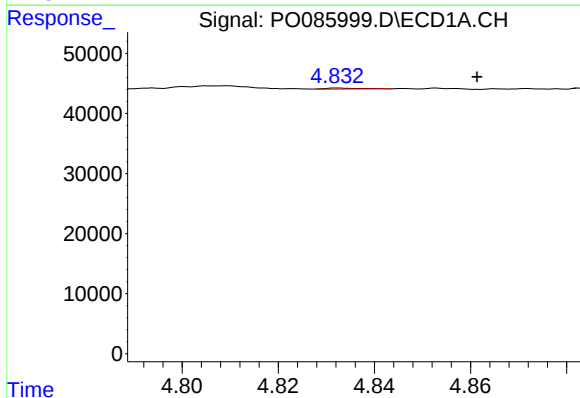


#10 AR-1221-3

R.T.: 4.832 min
Delta R.T.: -0.029 min
Response: 914
Conc: 0.34 ng/ml

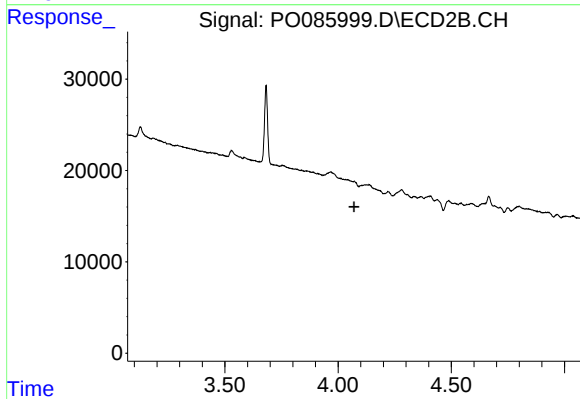

#10 AR-1221-3


R.T.: 0.000 min
Exp R.T. : 4.070 min
Response: 0
Conc: N.D.

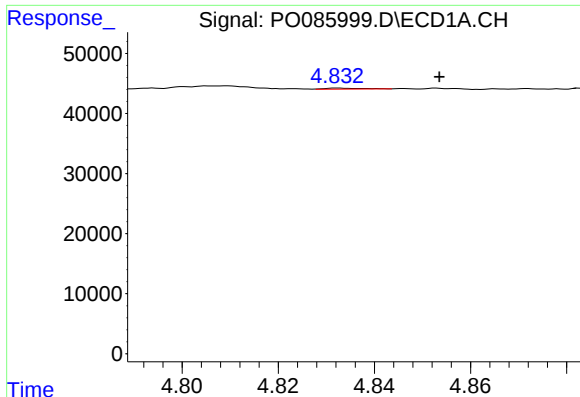

#11 AR-1232-1


R.T.: 4.832 min
Delta R.T.: -0.021 min
Response: 914
Conc: 0.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

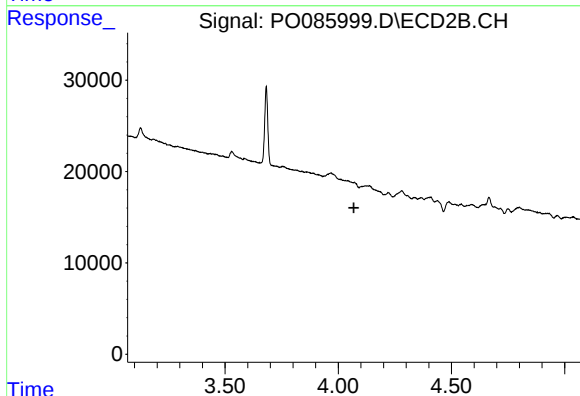


#11 AR-1232-1

R.T.: 0.000 min
Exp R.T. : 4.069 min
Response: 0
Conc: N.D.

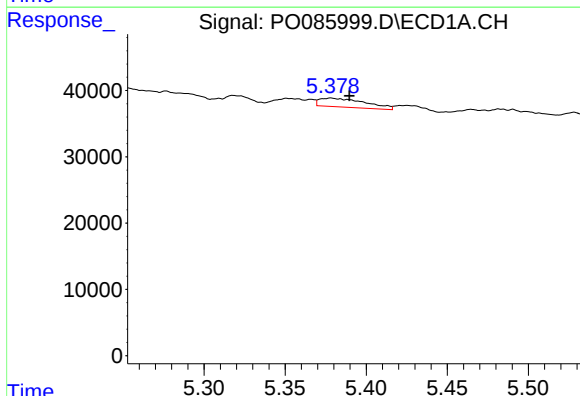


#12 AR-1232-2

R.T.: 5.378 min
Delta R.T.: -0.011 min
Response: 26199
Conc: 27.82 ng/ml

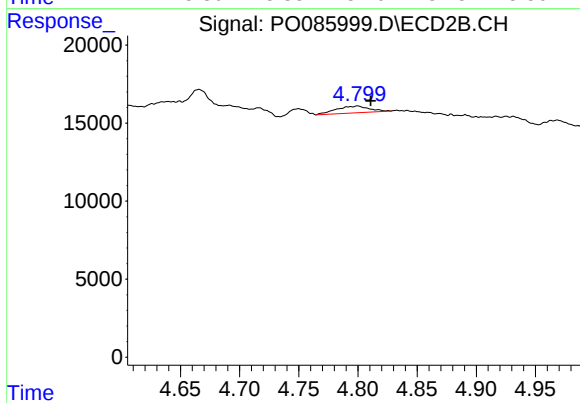

#12 AR-1232-2


R.T.: 4.800 min
Delta R.T.: -0.011 min
Response: 8610
Conc: 10.56 ng/ml

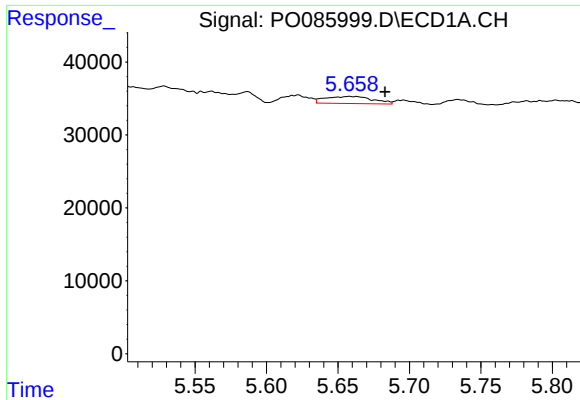

#13 AR-1232-3


R.T.: 5.658 min
Delta R.T.: -0.025 min
Response: 22485
Conc: 12.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

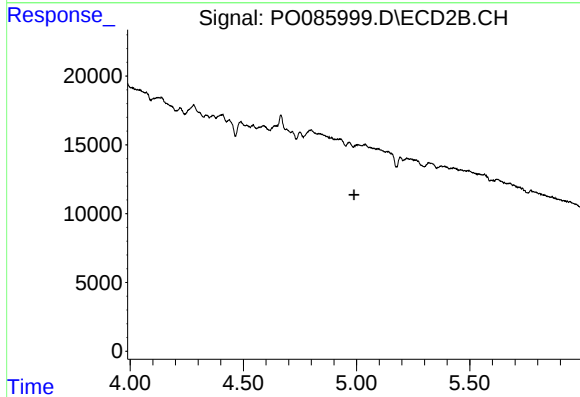


#13 AR-1232-3

R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

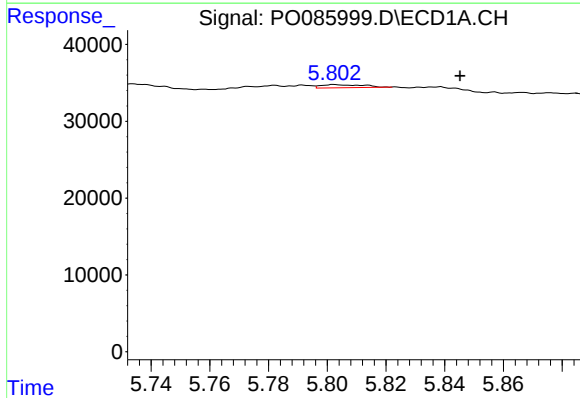


#14 AR-1232-4

R.T.: 5.802 min
Delta R.T.: -0.043 min
Response: 4029
Conc: 4.63 ng/ml

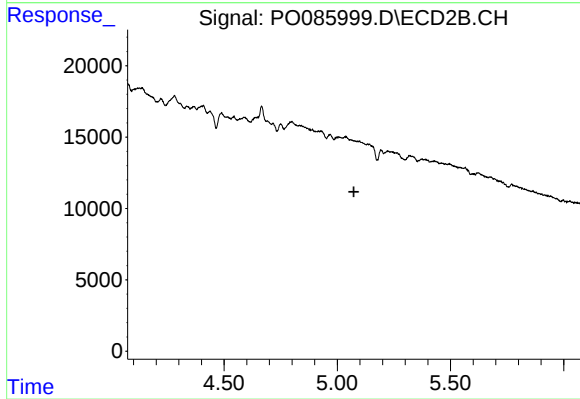

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.073 min
Response: 0
Conc: N.D.

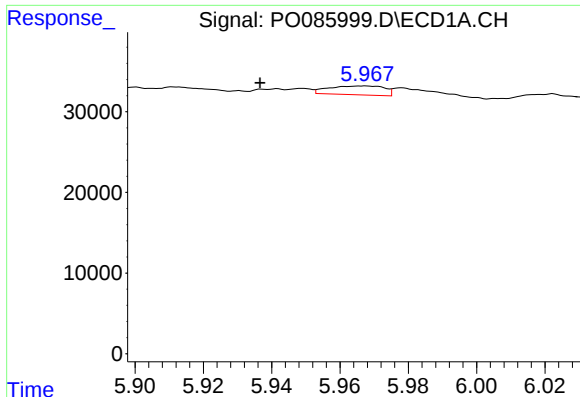

#15 AR-1232-5


R.T.: 5.968 min
Delta R.T.: 0.031 min
Response: 12419
Conc: 18.75 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

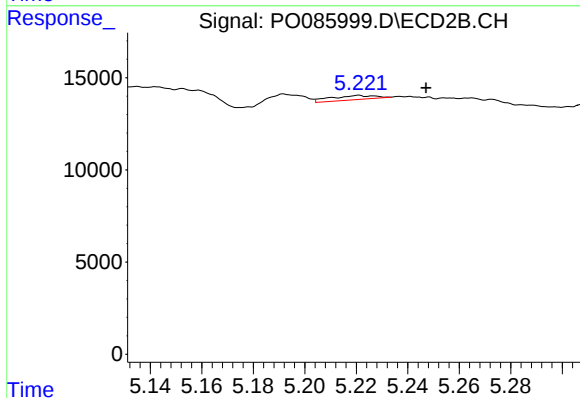


#15 AR-1232-5

R.T.: 5.221 min
Delta R.T.: -0.026 min
Response: 2723
Conc: 6.50 ng/ml

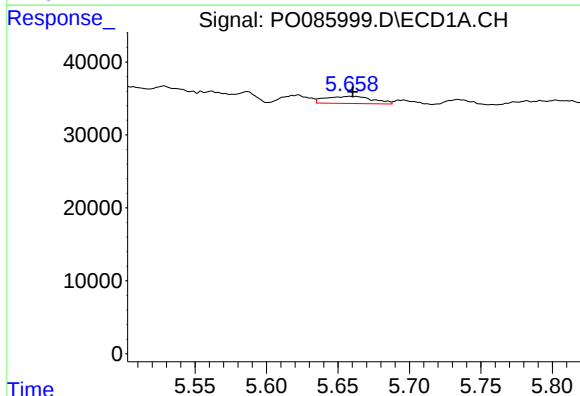


#16 AR-1242-1

R.T.: 5.658 min
Delta R.T.: -0.002 min
Response: 22485
Conc: 8.27 ng/ml

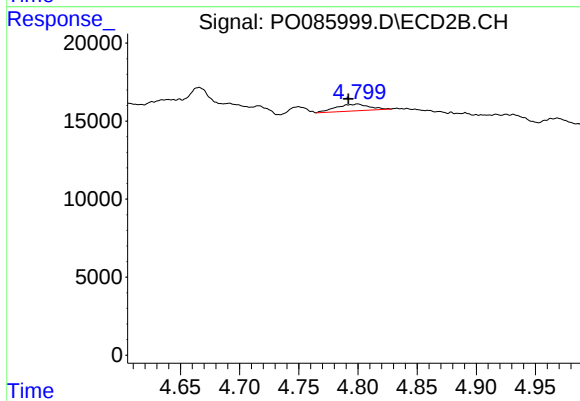

#16 AR-1242-1


R.T.: 4.800 min
Delta R.T.: 0.008 min
Response: 8610
Conc: 6.52 ng/ml

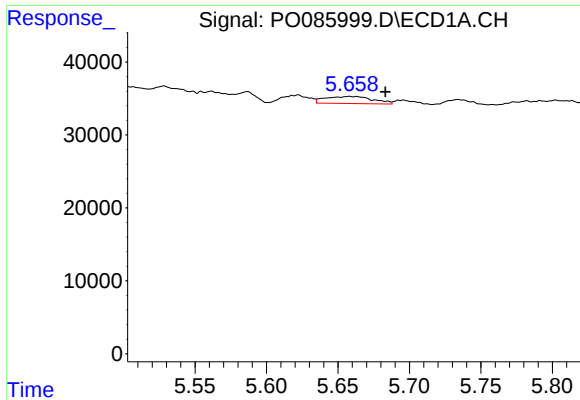

#17 AR-1242-2


R.T.: 5.658 min
Delta R.T.: -0.025 min
Response: 22485
Conc: 5.98 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

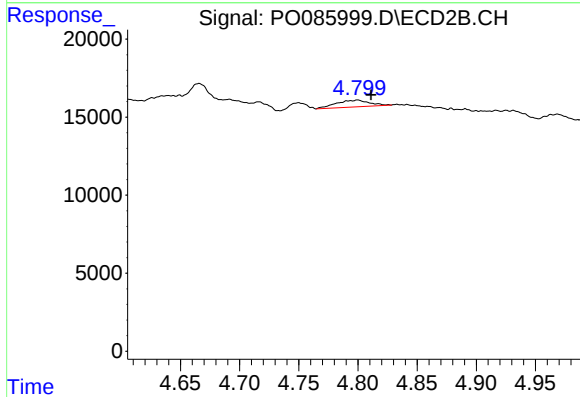


#17 AR-1242-2

R.T.: 4.800 min
Delta R.T.: -0.011 min
Response: 8610
Conc: 4.91 ng/ml

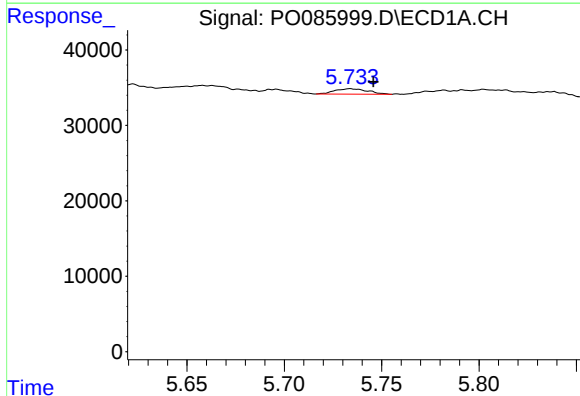


#18 AR-1242-3

R.T.: 5.734 min
Delta R.T.: -0.012 min
Response: 8390
Conc: 3.57 ng/ml

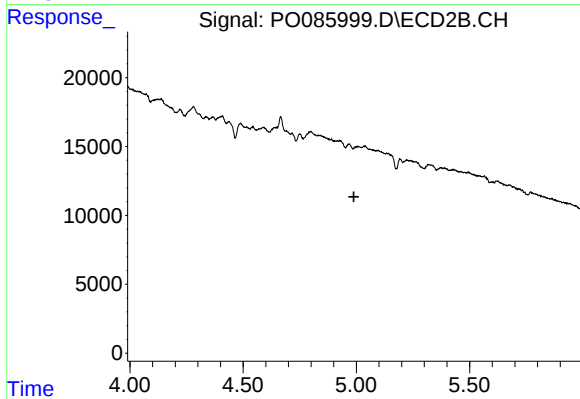

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.989 min
Response: 0
Conc: N.D.

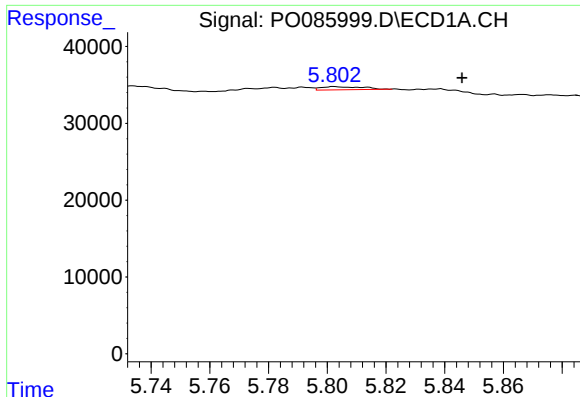

#19 AR-1242-4


R.T.: 5.802 min
Delta R.T.: -0.044 min
Response: 4029
Conc: 2.13 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

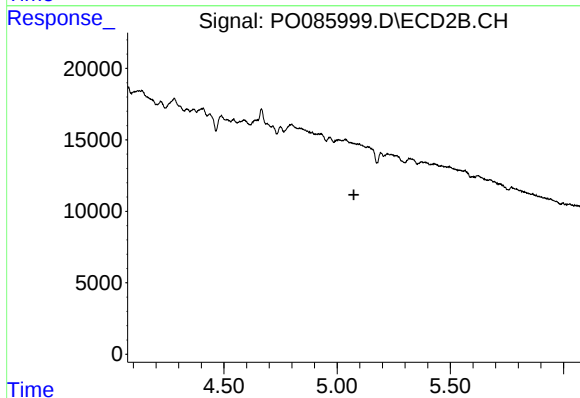


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.074 min
Response: 0
Conc: N.D.

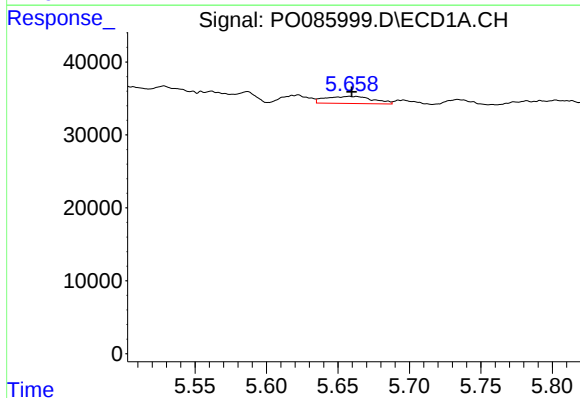


#21 AR-1248-1

R.T.: 5.658 min
Delta R.T.: -0.002 min
Response: 22485
Conc: 11.13 ng/ml

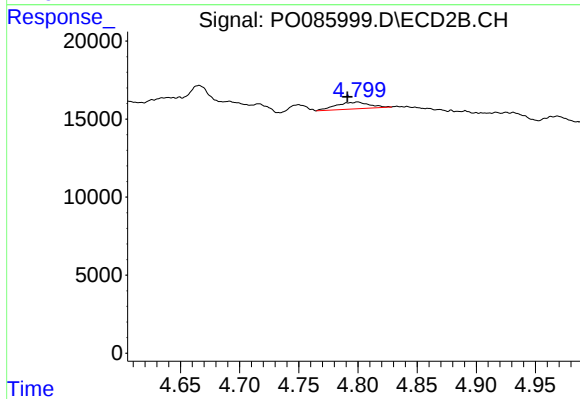

#21 AR-1248-1


R.T.: 4.800 min
Delta R.T.: 0.009 min
Response: 8610
Conc: 8.87 ng/ml

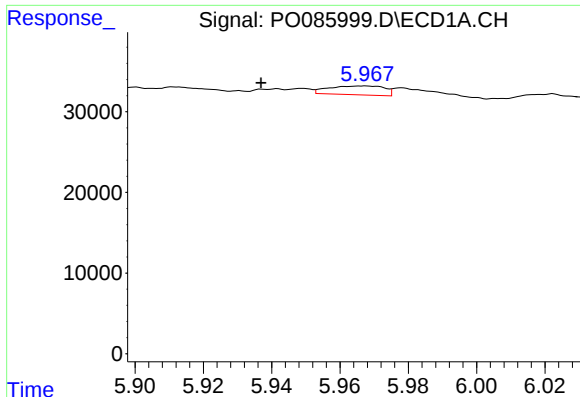

#22 AR-1248-2


R.T.: 5.968 min
Delta R.T.: 0.031 min
Response: 12419
Conc: 4.60 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

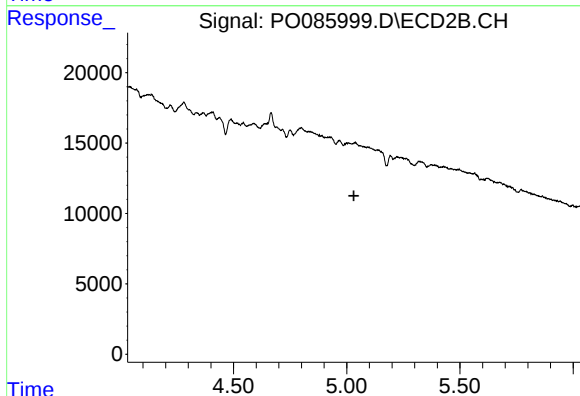


#22 AR-1248-2

R.T.: 0.000 min
Exp R.T. : 5.031 min
Response: 0
Conc: N.D.

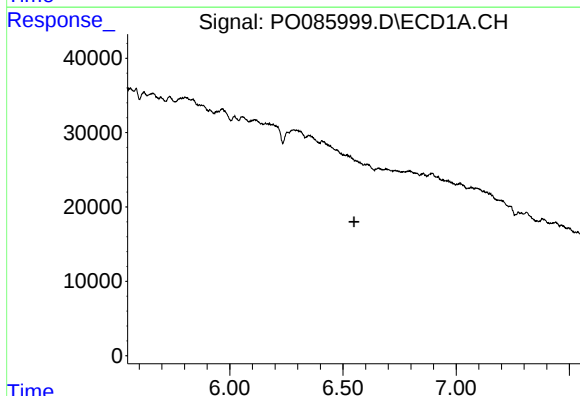


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 6.549 min
Response: 0
Conc: N.D.

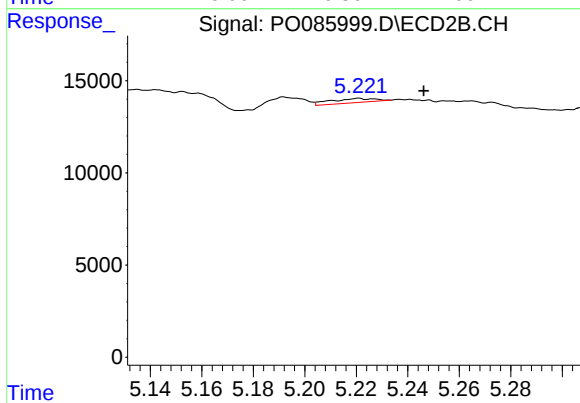

#24 AR-1248-4


R.T.: 5.221 min
Delta R.T.: -0.025 min
Response: 2723
Conc: 1.70 ng/ml

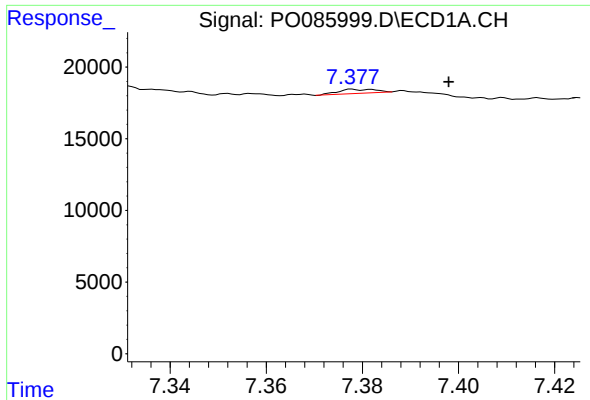

#29 AR-1254-4

R.T.: 7.378 min
Delta R.T.: -0.020 min
Response: 1497
Conc: 0.40 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC157517-1

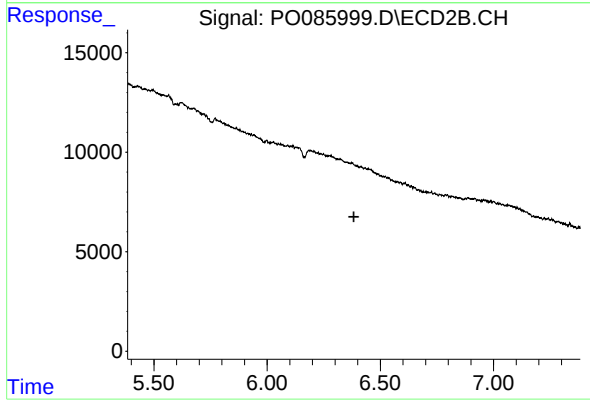

#29 AR-1254-4

R.T.: 0.000 min
Exp R.T. : 6.383 min
Response: 0
Conc: N.D.