

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
 Data File : P0085997.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 12 May 2022 23:35
 Operator : YP\AJ
 Sample : N2771-05 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CLI-2022-BC226656-4

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 13 07:13:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.480	3.682	181902	73366	1.791	1.683
2) SA Decachlor...	10.329	8.750	101981	55240	1.924	1.628

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051222\
Data File : P0085997.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 12 May 2022 23:35
Operator : YP\AJ
Sample : N2771-05 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 13 07:13:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

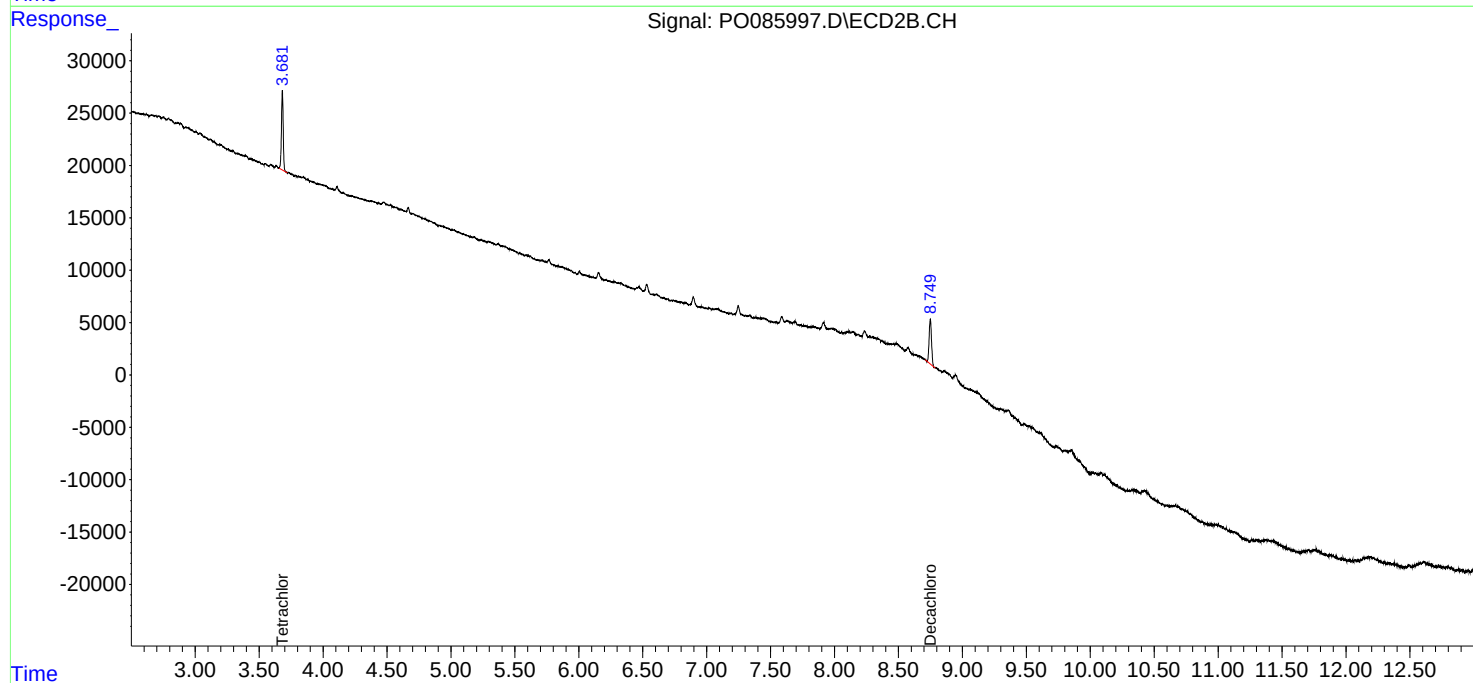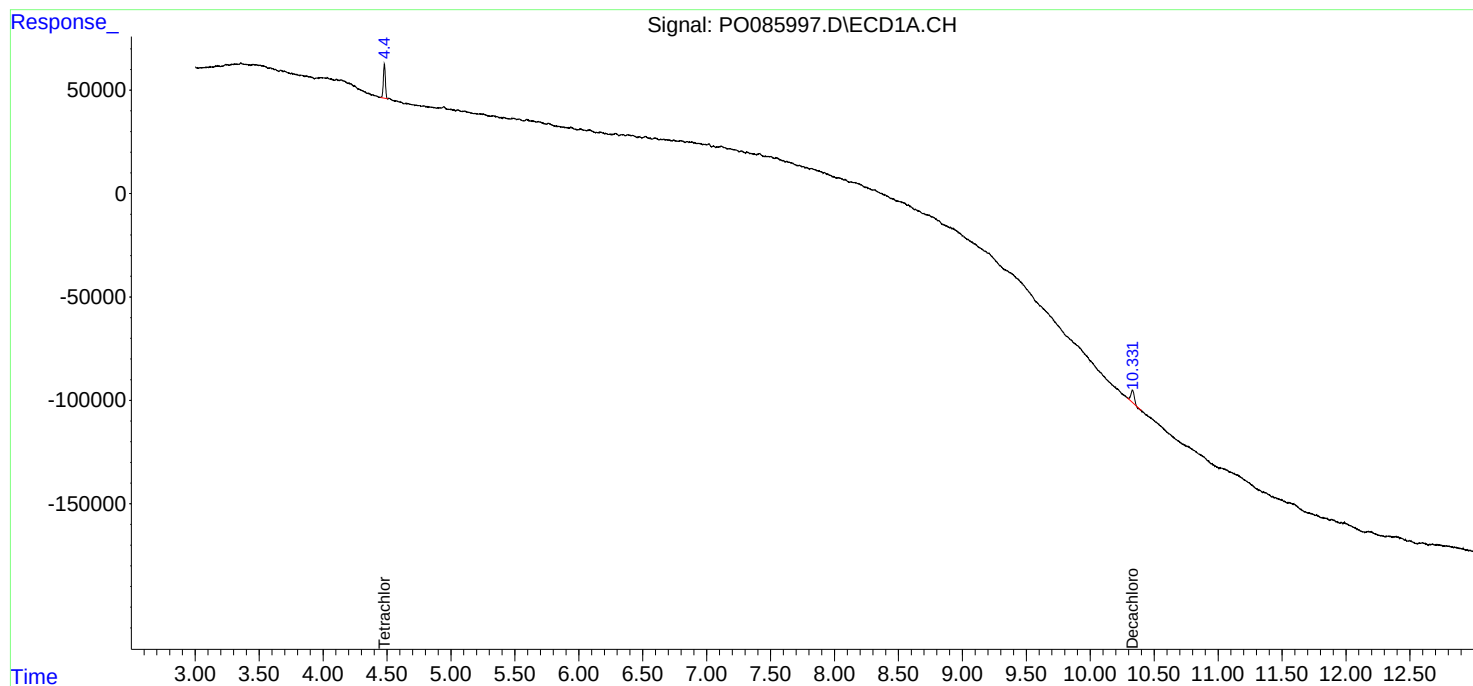


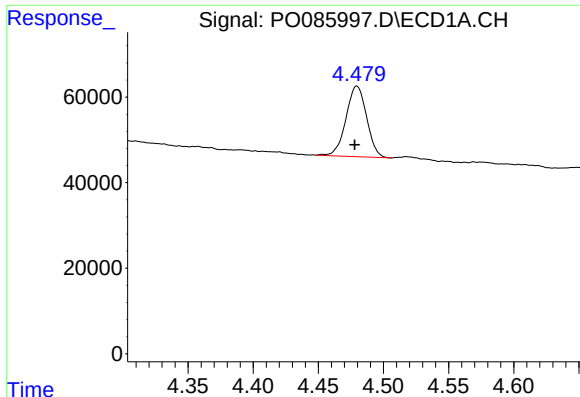

#1 Tetrachloro-m-xylene


R.T.: 4.480 min
Delta R.T.: 0.002 min
Response: 181902
Conc: 1.79 ng/ml

Instrument :
ECD_O
ClientSampleId :
CLI-2022-BC226656-4

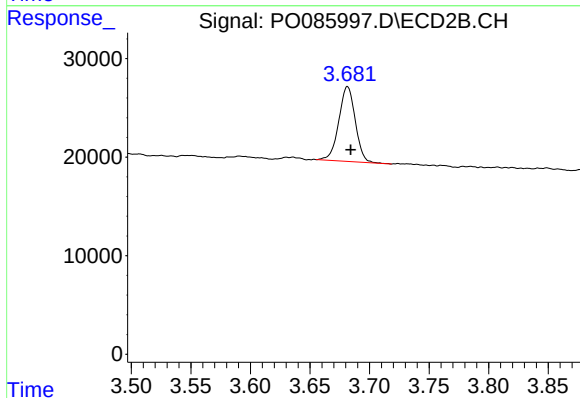


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.003 min
Response: 73366
Conc: 1.68 ng/ml

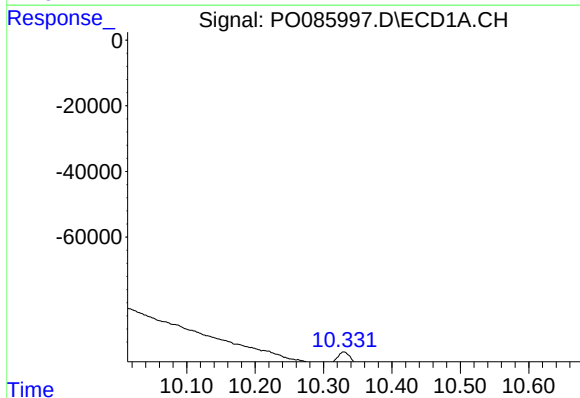

#2 Decachlorobiphenyl

R.T.: 10.329 min
Delta R.T.: 0.002 min
Response: 101981
Conc: 1.92 ng/ml

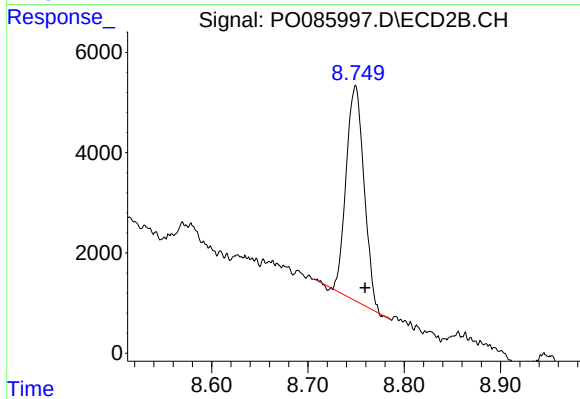

#2 Decachlorobiphenyl

R.T.: 8.750 min
Delta R.T.: -0.010 min
Response: 55240
Conc: 1.63 ng/ml