

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051223\
 Data File : P0095015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 May 2023 14:38
 Operator : YP/AJ
 Sample : 02750-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PAT-1-051123

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/15/2023
 Supervised By :Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 12 23:19:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.615	85678688	31475461	24.873m	23.523
2) SA Decachlor...	10.253	8.625	63458608	24567201	26.149	21.826

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051223\
Data File : P0095015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 May 2023 14:38
Operator : YP/AJ
Sample : 02750-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
PAT-1-051123


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/15/2023
Supervised By :Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 12 23:19:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

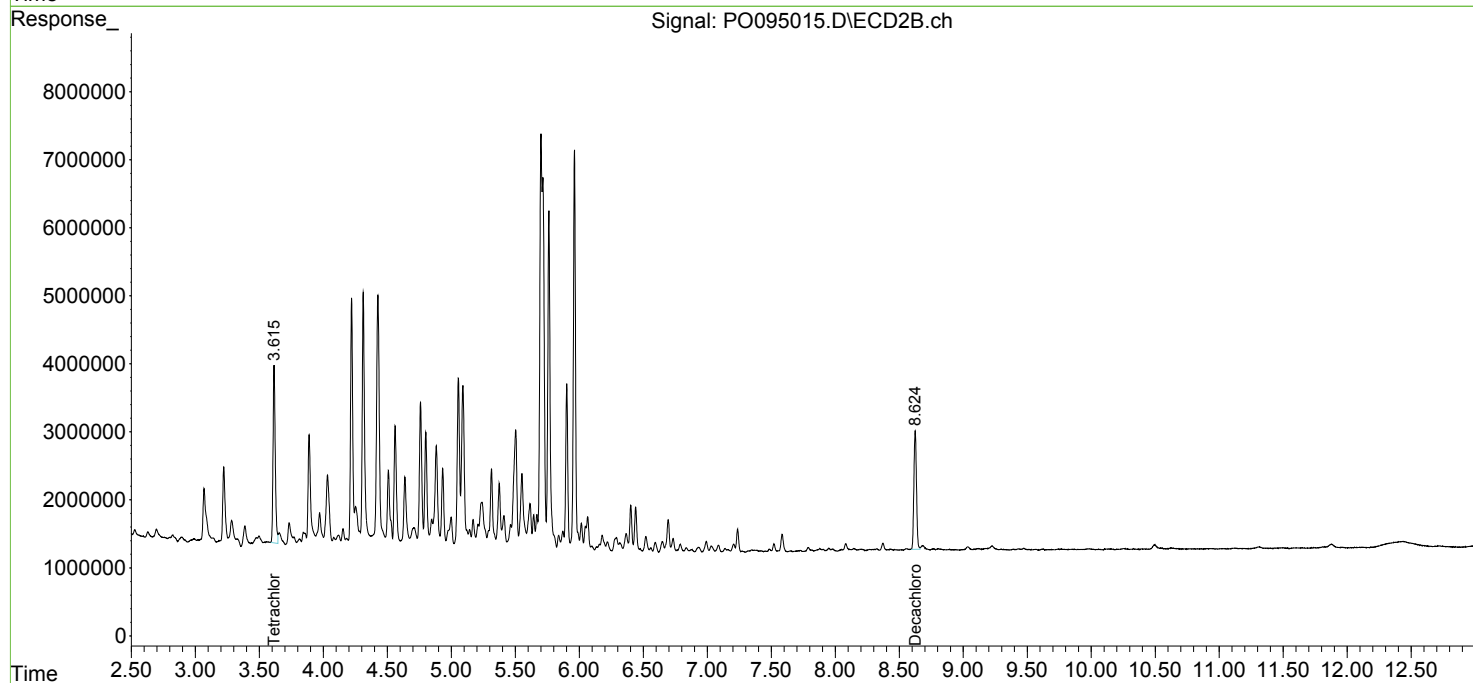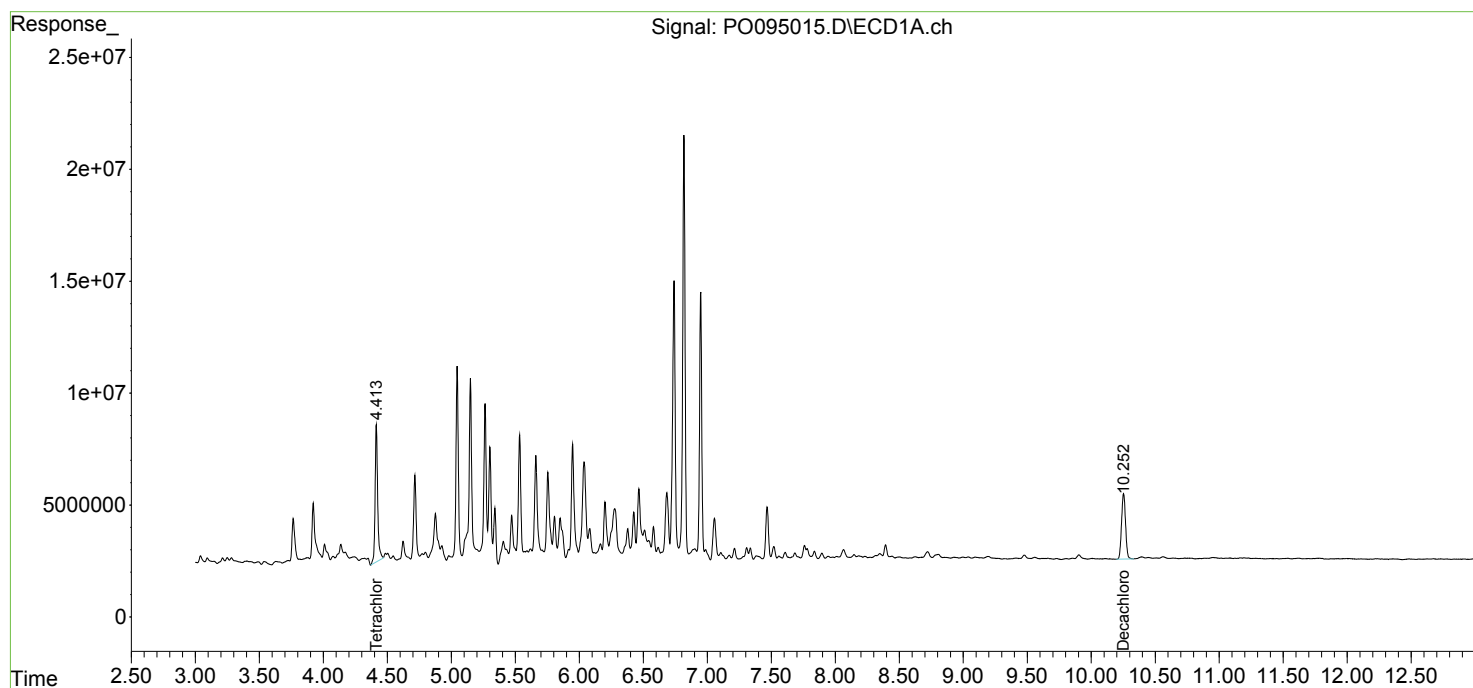

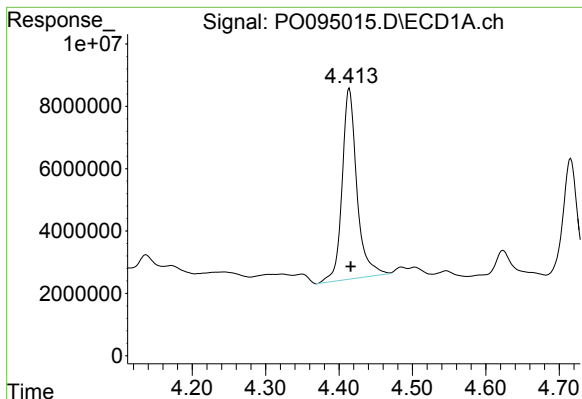

#1 Tetrachloro-m-xylene

R.T.: 4.413 min
Delta R.T.: -0.003 min
Response: 85678688
Conc: 24.87 ng/ml

Instrument :

ECD_O


ClientSampleId :

PAT-1-051123

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 05/15/2023
Supervised By :Ankita Jodhani 05/16/2023

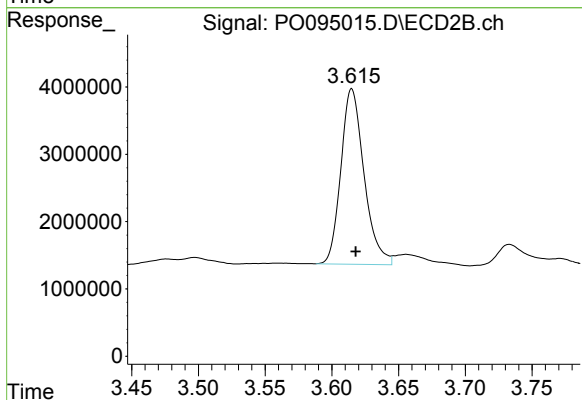


#1 Tetrachloro-m-xylene

R.T.: 3.615 min
Delta R.T.: -0.003 min
Response: 31475461
Conc: 23.52 ng/ml

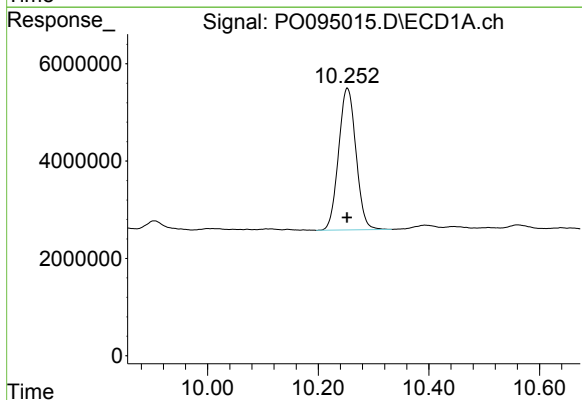

#2 Decachlorobiphenyl

R.T.: 10.253 min
Delta R.T.: 0.000 min
Response: 63458608
Conc: 26.15 ng/ml

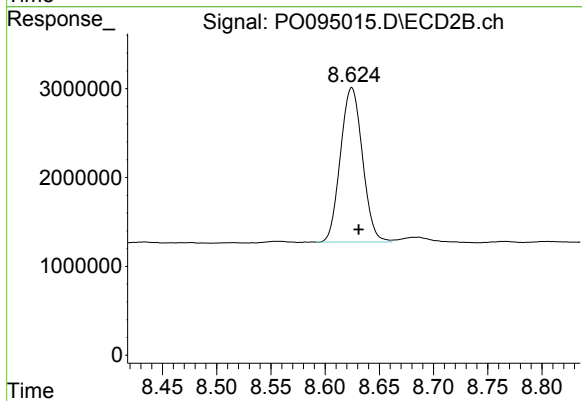

#2 Decachlorobiphenyl

R.T.: 8.625 min
Delta R.T.: -0.007 min
Response: 24567201
Conc: 21.83 ng/ml