

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
 Data File : PL066770.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 18:00
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 09:02:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 09:00:59 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.144	65861574	59243250	18.040	19.254
28)	SA Decachlor...	8.135	9.332	79431063	53361006	19.269	19.527
Target Compounds							
2)	A alpha-BHC	3.866	0.000	25338163	0	0.859	N.D. #
6)	B beta-BHC	0.000	5.030	0	45361149	N.D.	3.580 #
7)	B delta-BHC	0.000	5.266f	0	514343	N.D.	0.127 #
13)	MA Dieldrin	5.681	0.000	2132337	0	0.416	N.D. #
15)	B Endosulfa...	0.000	7.110	0	1463295	N.D.	0.504 #
23)	Chlordane-1	4.305f	0.000	456944	0	2.989	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
Data File : PL066770.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 18:00
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 09:02:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 09:00:59 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

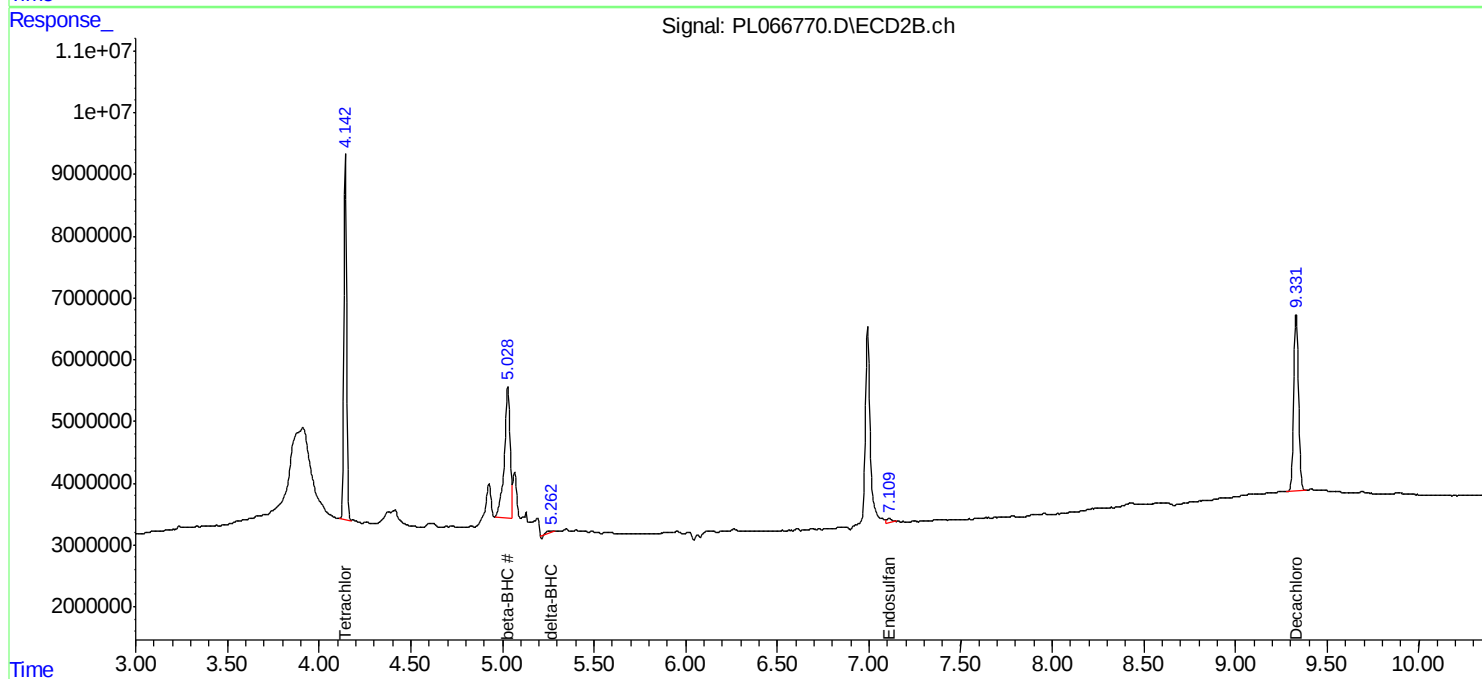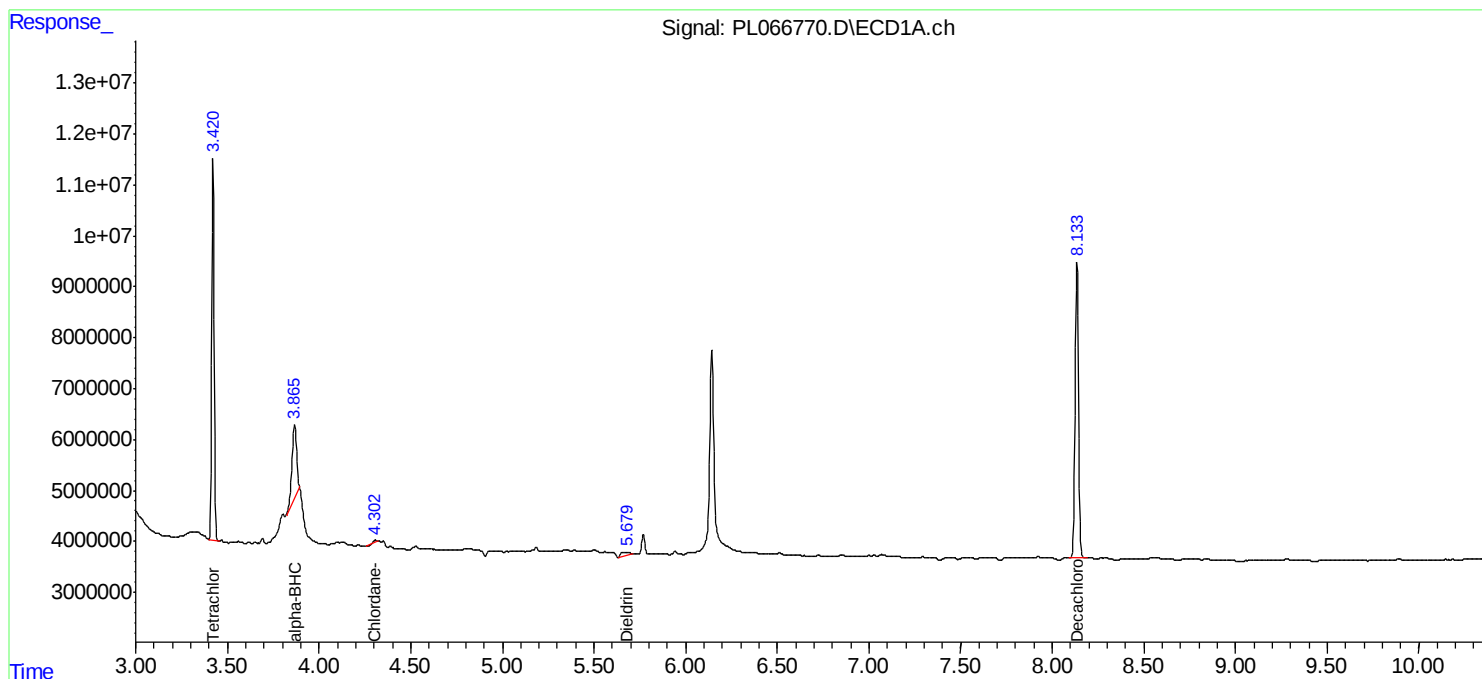


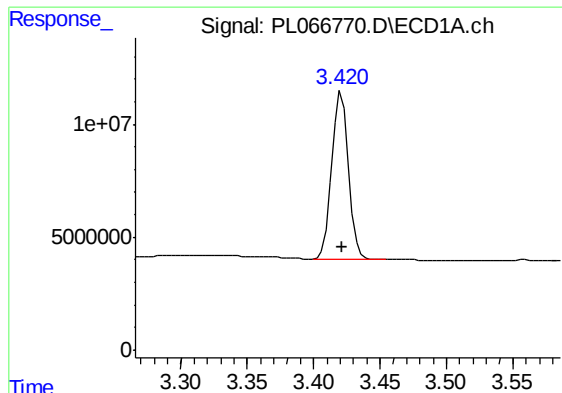

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 65861574
Conc: 18.04 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

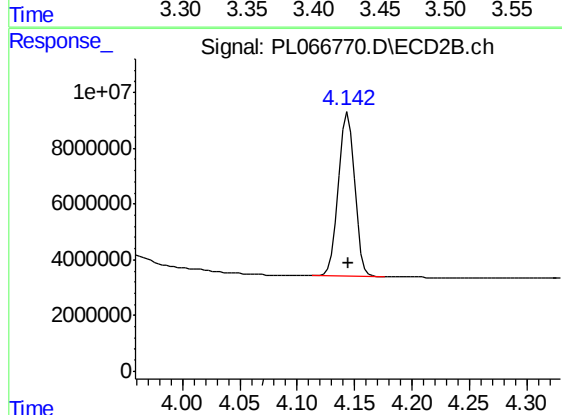


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 59243250
Conc: 19.25 ng/ml

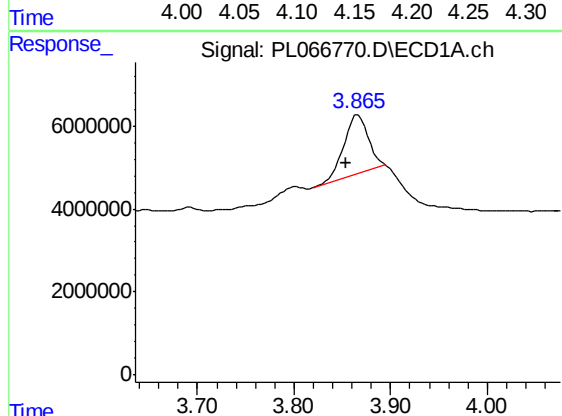


#2 alpha-BHC

R.T.: 3.866 min
Delta R.T.: 0.012 min
Response: 25338163
Conc: 0.86 ng/ml

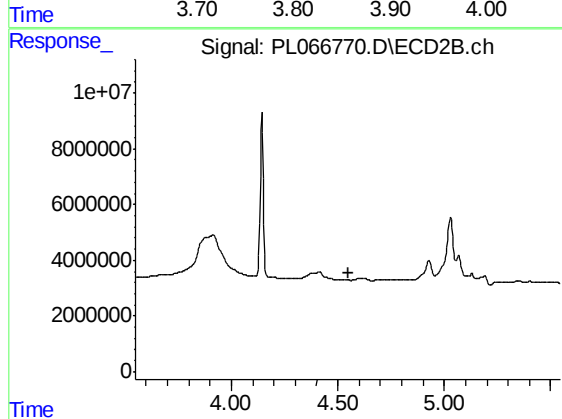

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.548 min
Response: 0
Conc: N.D.

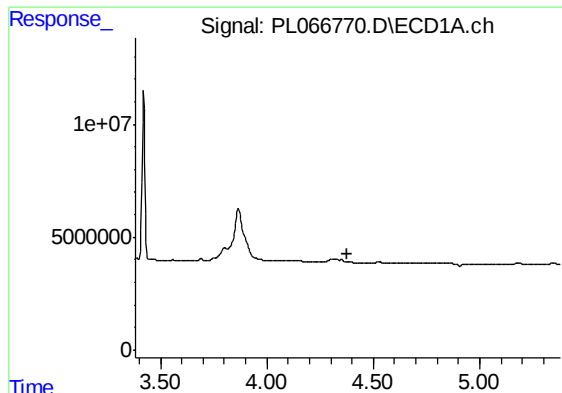

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.380 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :
I.BLK

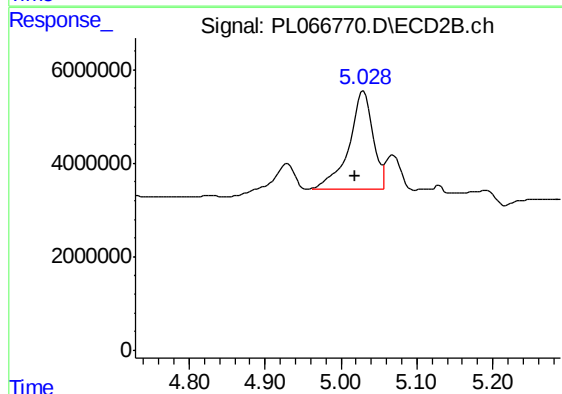


#6 beta-BHC

R.T.: 5.030 min
Delta R.T.: 0.012 min
Response: 45361149
Conc: 3.58 ng/ml

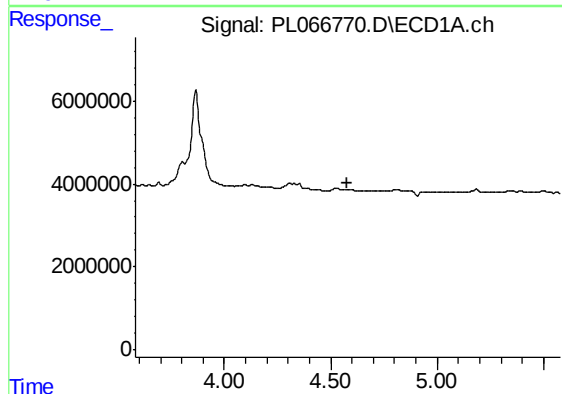


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.580 min
Response: 0
Conc: N.D.

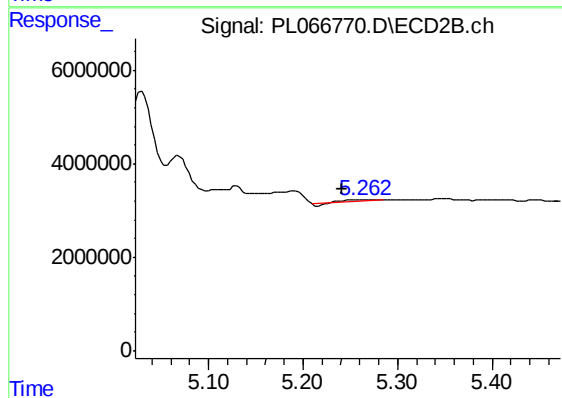

#7 delta-BHC


R.T.: 5.266 min
Delta R.T.: 0.025 min
Response: 514343
Conc: 0.13 ng/ml

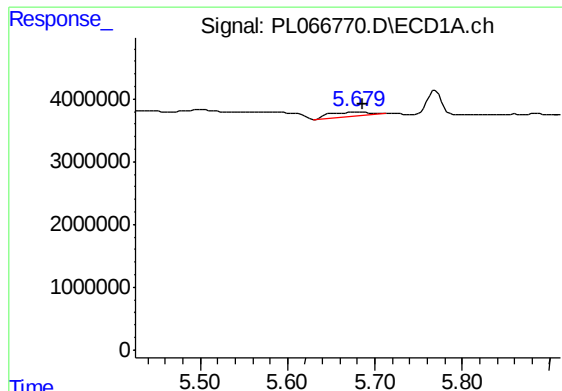

#13 Dieldrin


R.T.: 5.681 min
Delta R.T.: -0.004 min
Response: 2132337
Conc: 0.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

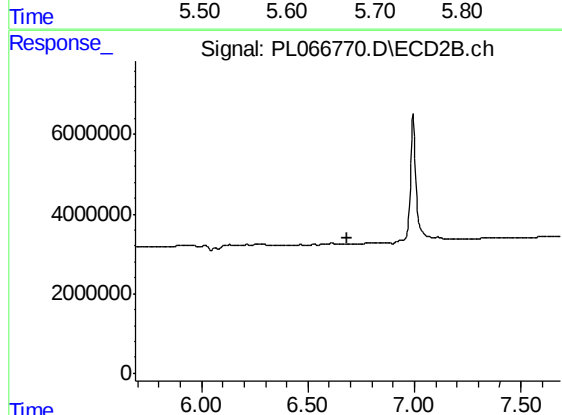


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.687 min
Response: 0
Conc: N.D.

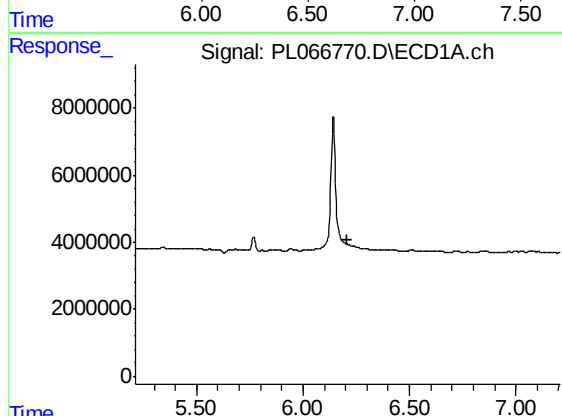


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 6.209 min
Response: 0
Conc: N.D.

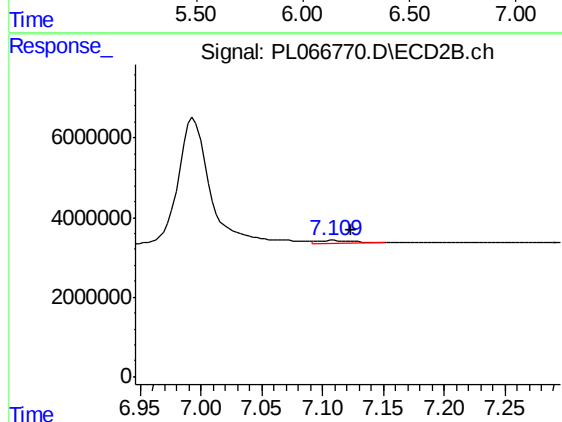

#15 Endosulfan II


R.T.: 7.110 min
Delta R.T.: -0.013 min
Response: 1463295
Conc: 0.50 ng/ml

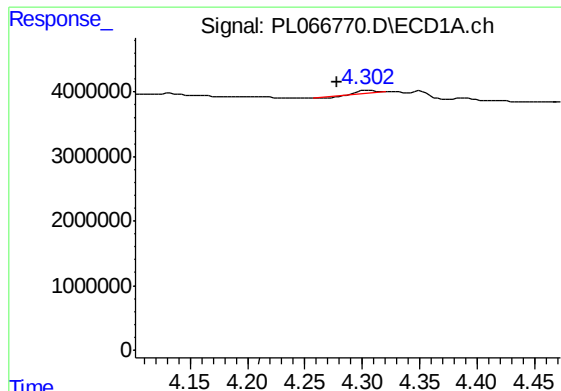

#23 Chlordane-1


R.T.: 4.305 min
Delta R.T.: 0.027 min
Response: 456944
Conc: 2.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

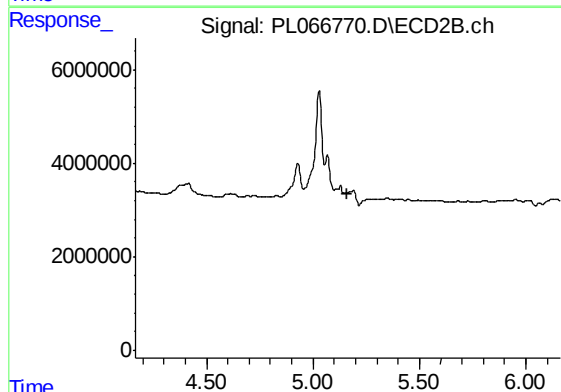


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.162 min
Response: 0
Conc: N.D.

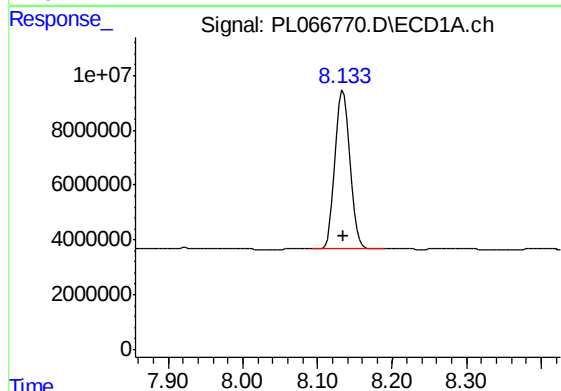

#28 Decachlorobiphenyl

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 79431063
Conc: 19.27 ng/ml

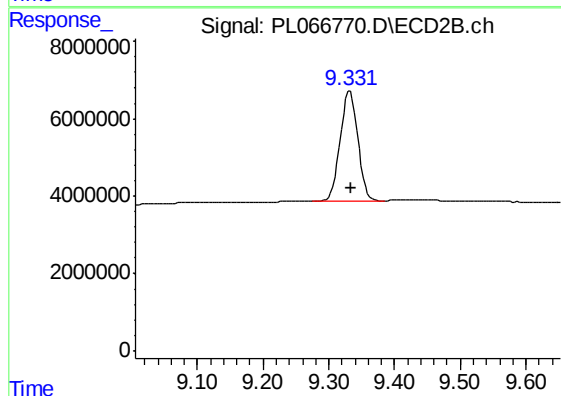

#28 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: 0.000 min
Response: 53361006
Conc: 19.53 ng/ml