

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
 Data File : PL066778.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 19:55
 Operator : AR\AJ
 Sample : PCHLORICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCHLORICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 08:47:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 08:46:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.144	436.4E6	328.4E6	99.853	98.888
28)	SA Decachlor...	8.135	9.332	380.6E6	280.1E6	94.046	94.087
Target Compounds							
23)	Chlordane-1	4.279	5.162	148.0E6	132.1E6	976.286	977.835
24)	Chlordane-2	4.774	5.639	160.4E6	148.6E6	945.679	969.353
25)	Chlordane-3	5.336	6.297	492.3E6	576.0E6	994.138	1016.196
26)	Chlordane-4	5.393	6.371	424.6E6	676.2E6	989.441	997.872
27)	Chlordane-5	6.218	7.193	178.3E6	102.7E6	988.669	1000.893



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
Data File : PL066778.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 19:55
Operator : AR\AJ
Sample : PCHLORICC1000
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCHLORICC1000

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 08:47:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 08:46:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

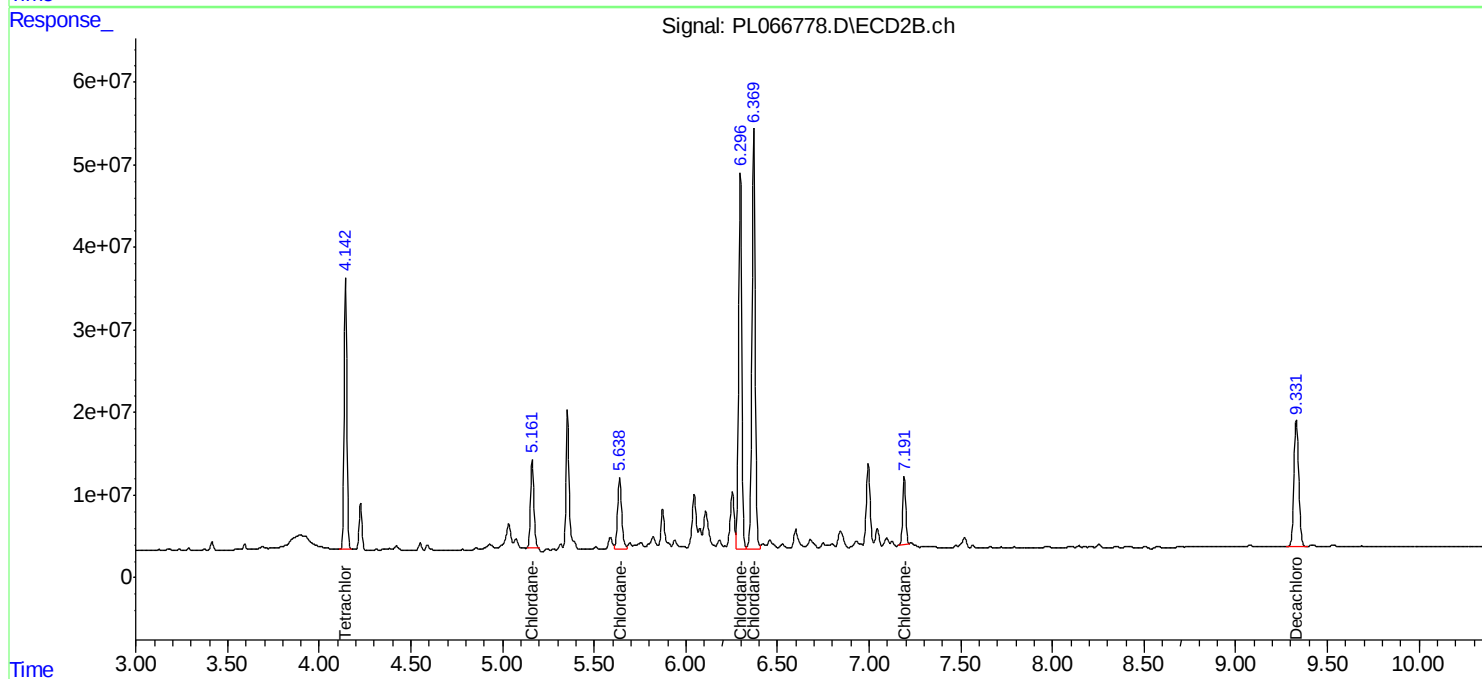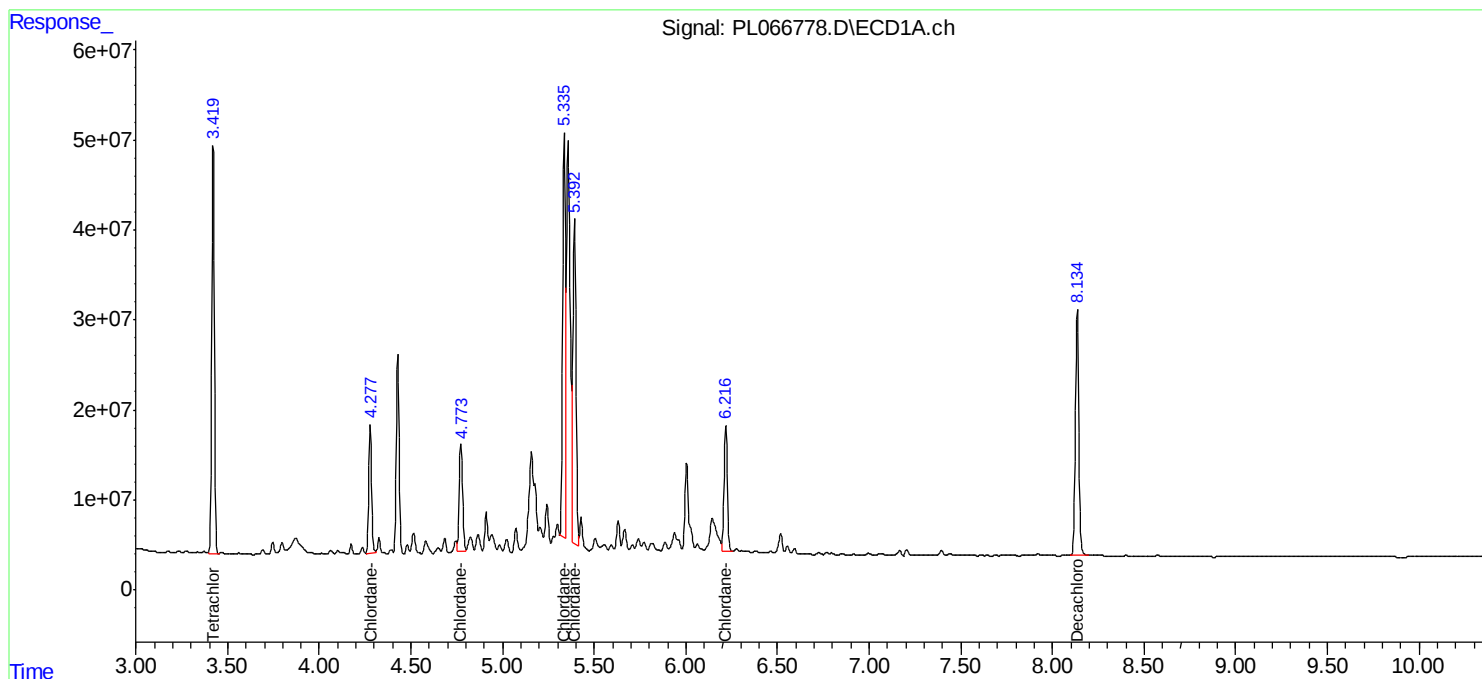


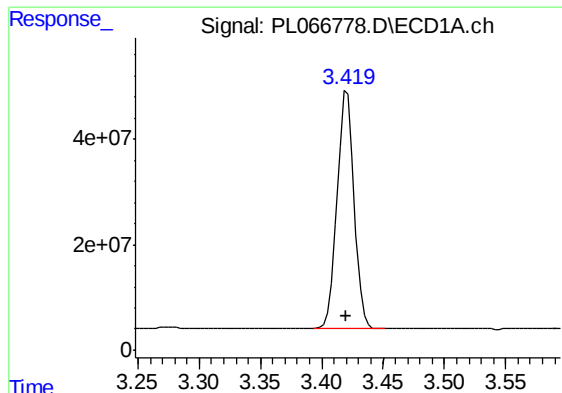

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 436382068
Conc: 99.85 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC1000

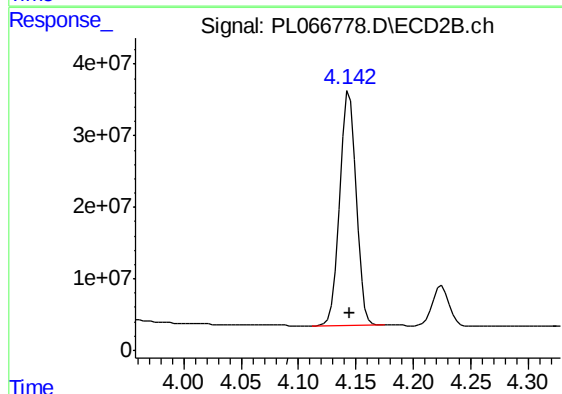


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 328412271
Conc: 98.89 ng/ml

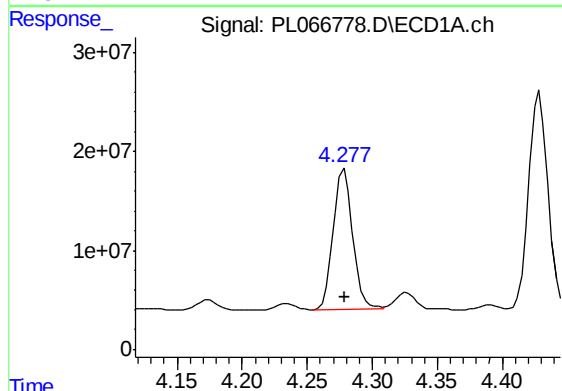


#23 Chlordane-1

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 148016027
Conc: 976.29 ng/ml

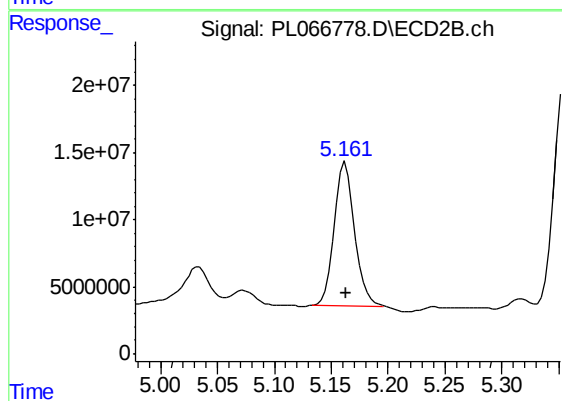

#23 Chlordane-1


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 132138460
Conc: 977.83 ng/ml

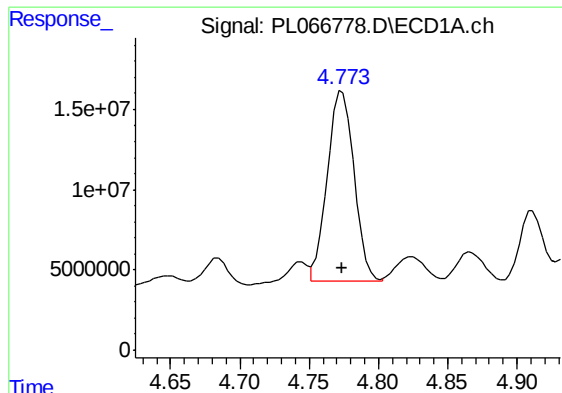

#24 Chlordane-2


R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 160431482
Conc: 945.68 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC1000

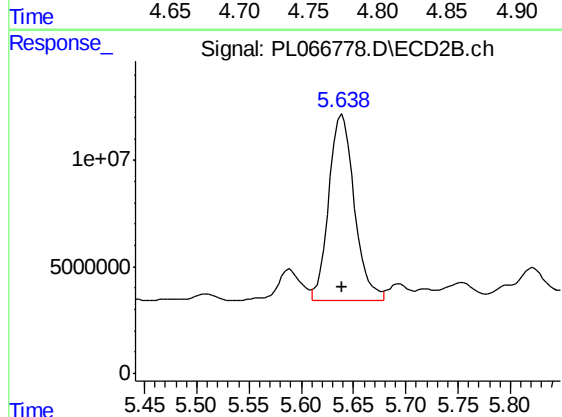


#24 Chlordane-2

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 148618183
Conc: 969.35 ng/ml

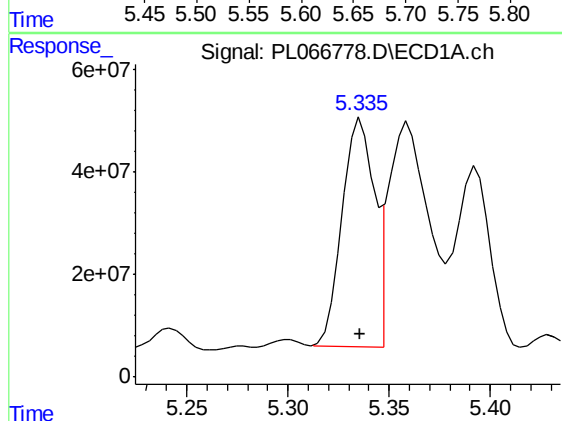


#25 Chlordane-3

R.T.: 5.336 min
Delta R.T.: 0.000 min
Response: 492282211
Conc: 994.14 ng/ml

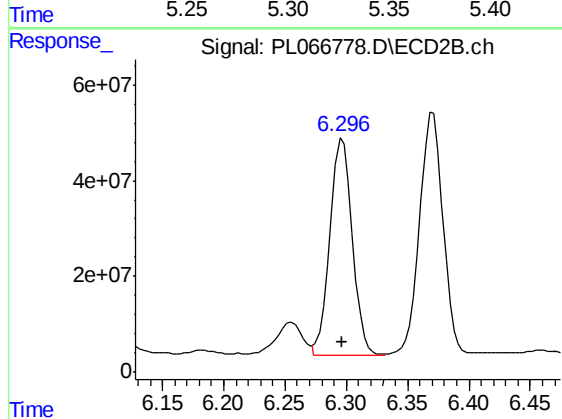

#25 Chlordane-3


R.T.: 6.297 min
Delta R.T.: 0.000 min
Response: 575999784
Conc: 1016.20 ng/ml

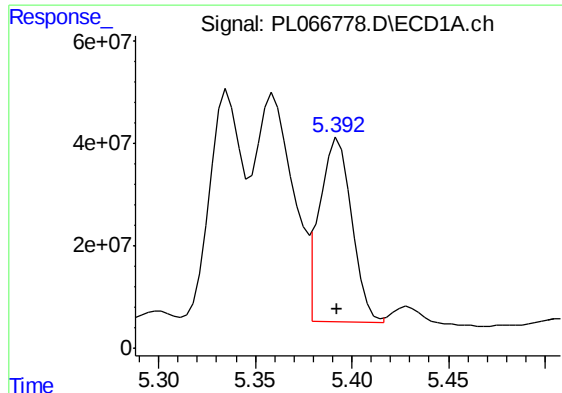

#26 Chlordane-4


R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 424628616
Conc: 989.44 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC1000

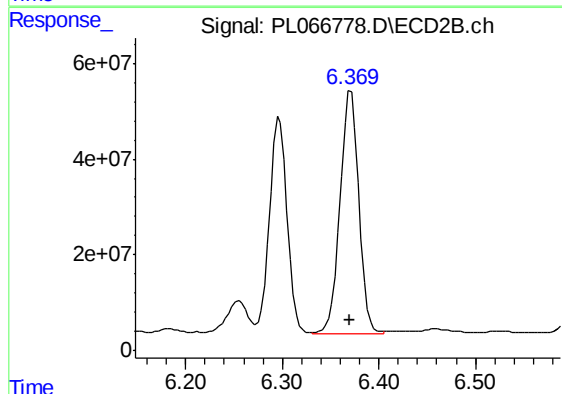


#26 Chlordane-4

R.T.: 6.371 min
Delta R.T.: 0.000 min
Response: 676234347
Conc: 997.87 ng/ml

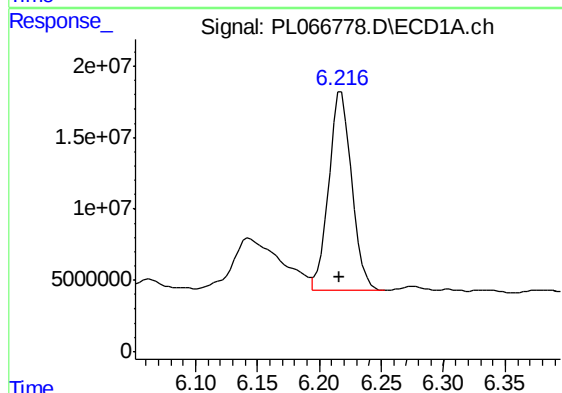


#27 Chlordane-5

R.T.: 6.218 min
Delta R.T.: 0.001 min
Response: 178290476
Conc: 988.67 ng/ml

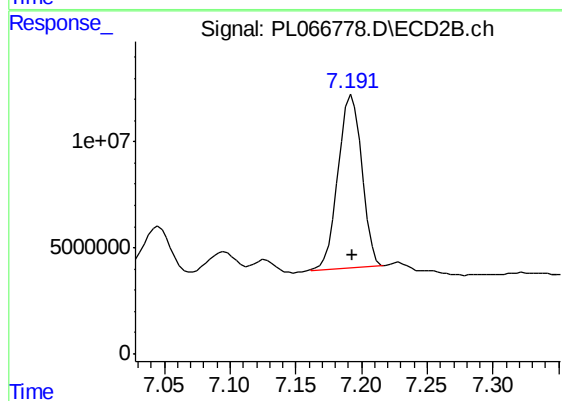

#27 Chlordane-5


R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 102687212
Conc: 1000.89 ng/ml

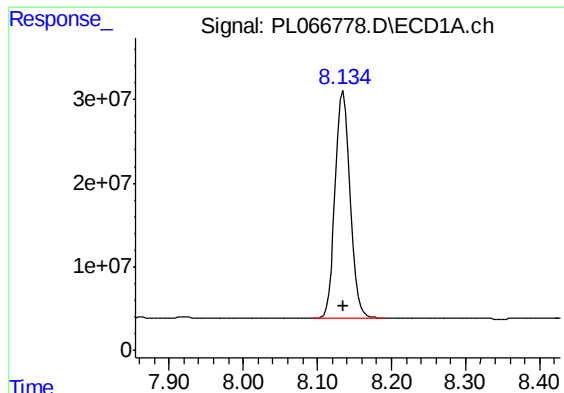

#28 Decachlorobiphenyl

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 380632379
Conc: 94.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC1000

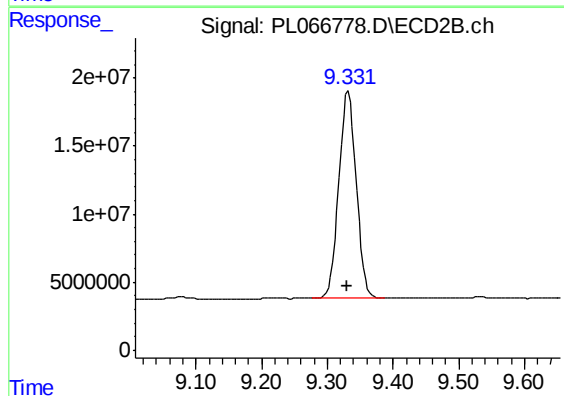

#28 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: 0.000 min
Response: 280146606
Conc: 94.09 ng/ml