

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
 Data File : PL066779.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 20:10
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCHLORICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 08:47:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 08:46:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	4.144	326.3E6	246.9E6	74.655	74.345
28)	SA Decachlor...	8.135	9.331	295.7E6	212.0E6	73.053	71.214
Target Compounds							
23)	Chlordane-1	4.279	5.163	112.3E6	99535498	740.901	736.570
24)	Chlordane-2	4.774	5.639	124.4E6	112.5E6	733.082	733.634
25)	Chlordane-3	5.335	6.297	373.6E6	428.8E6	754.522	756.467
26)	Chlordane-4	5.392	6.370	322.5E6	507.4E6	751.576	748.725
27)	Chlordane-5	6.217	7.192	135.0E6	76918407	748.407	749.725



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
Data File : PL066779.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 20:10
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCHLORICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 08:47:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 08:46:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

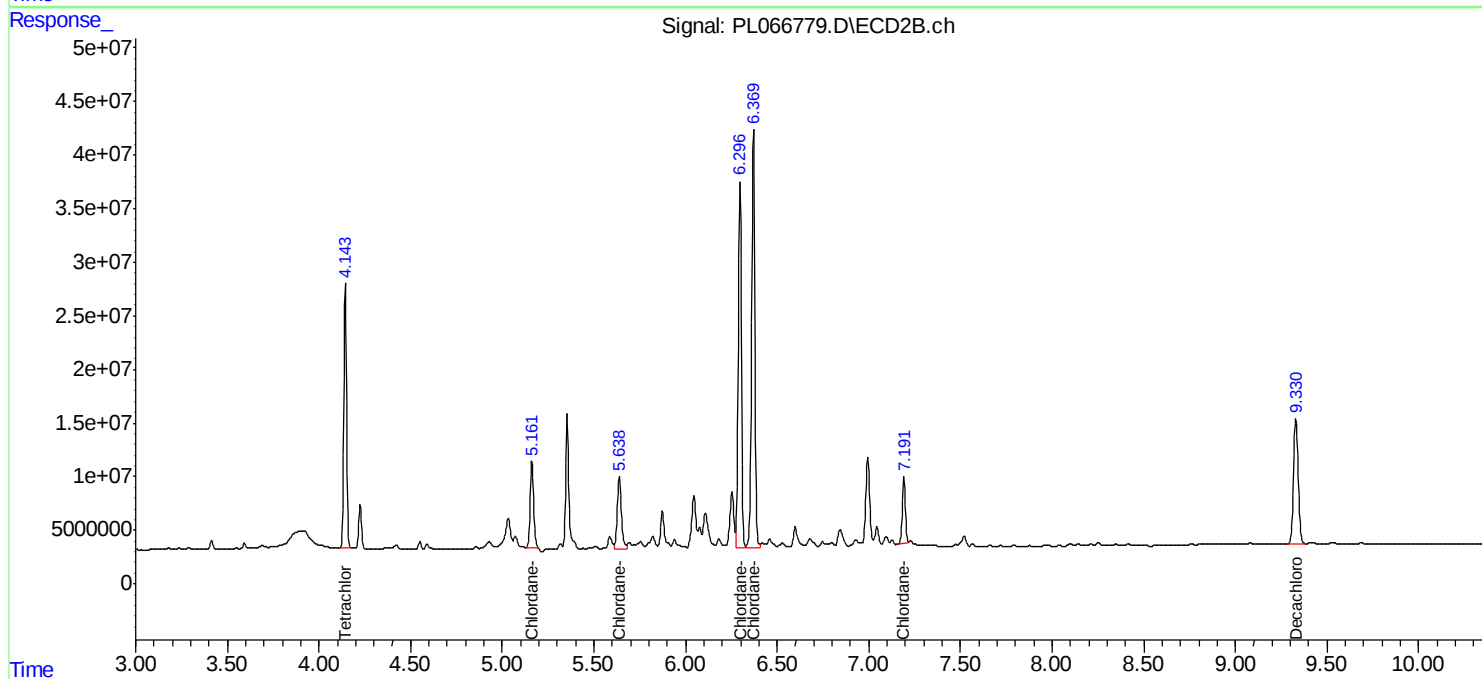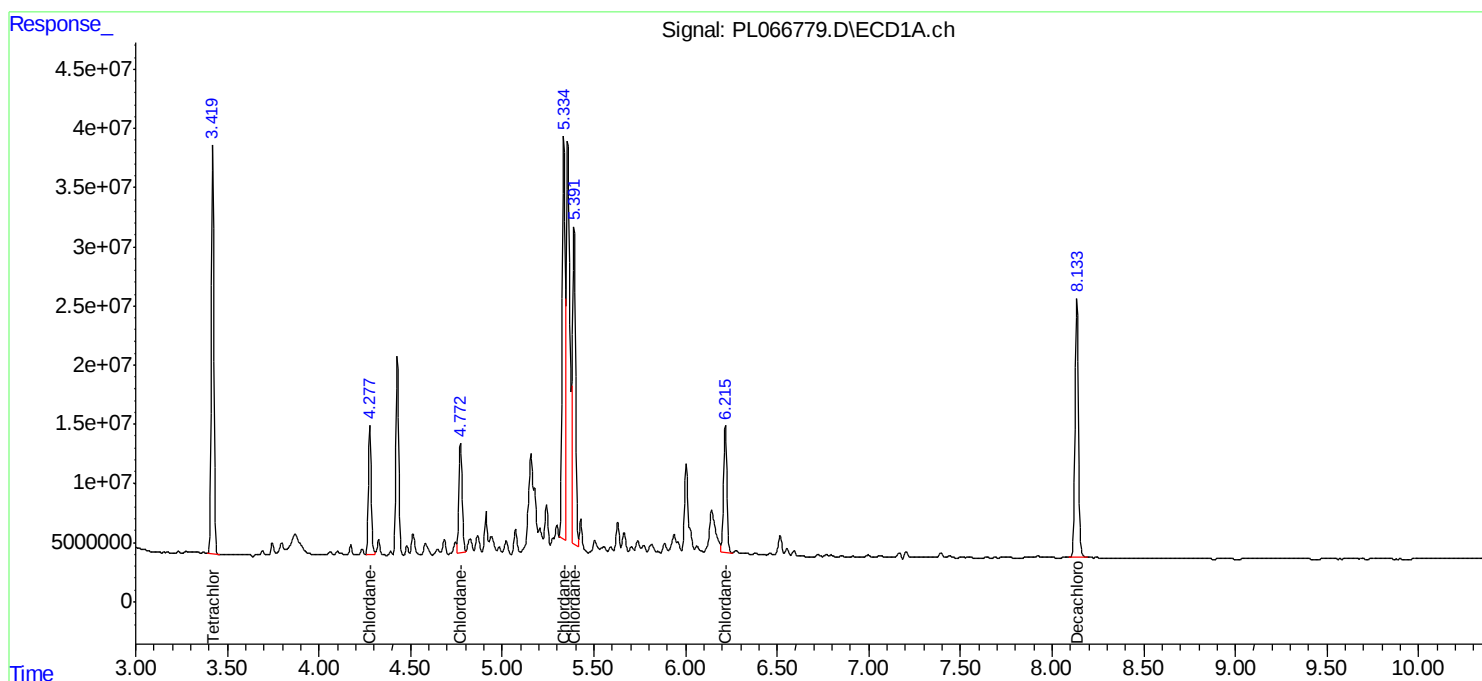


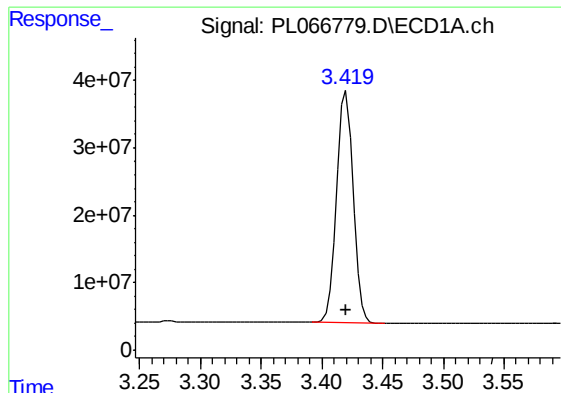

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 326258691
Conc: 74.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC750

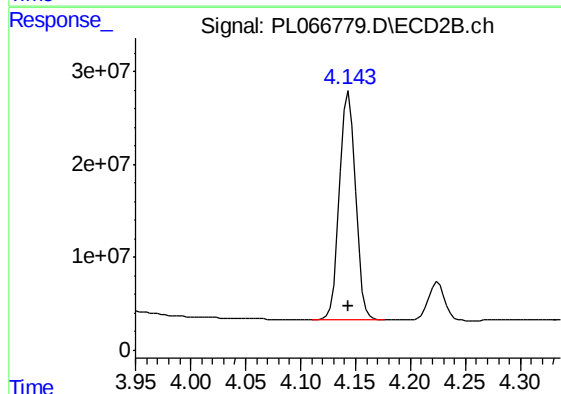


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 246901645
Conc: 74.34 ng/ml

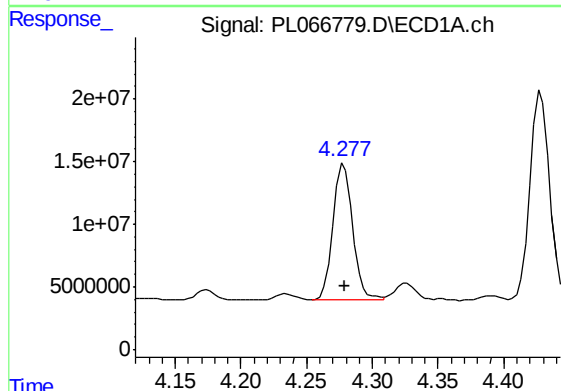


#23 Chlordane-1

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 112328960
Conc: 740.90 ng/ml

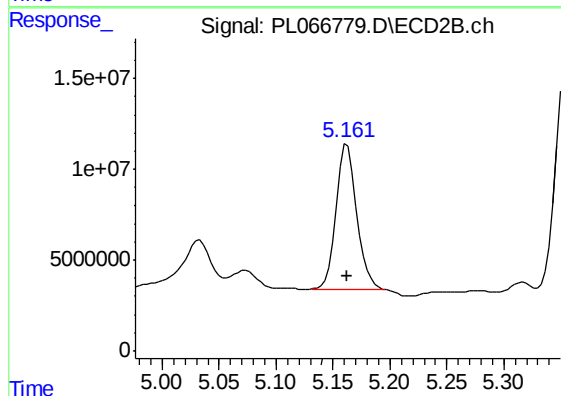

#23 Chlordane-1


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 99535498
Conc: 736.57 ng/ml

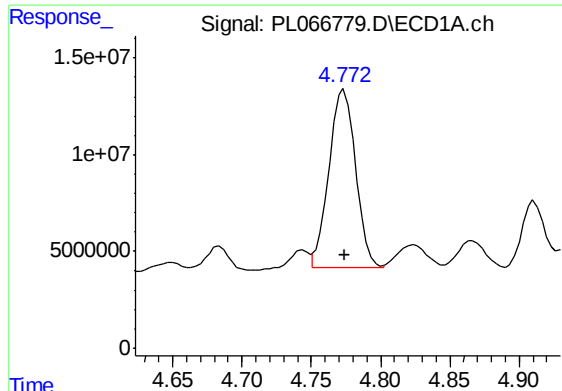

#24 Chlordane-2


R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 124365102
Conc: 733.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC750

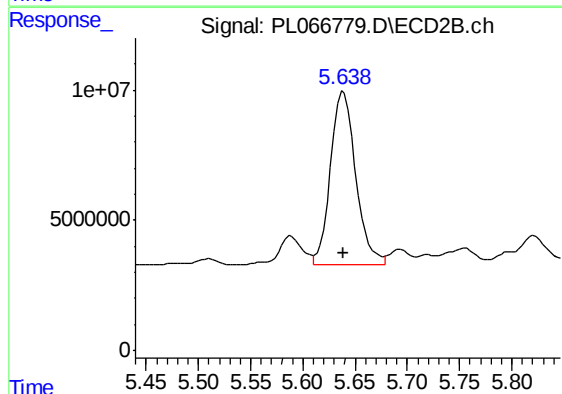


#24 Chlordane-2

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 112478570
Conc: 733.63 ng/ml

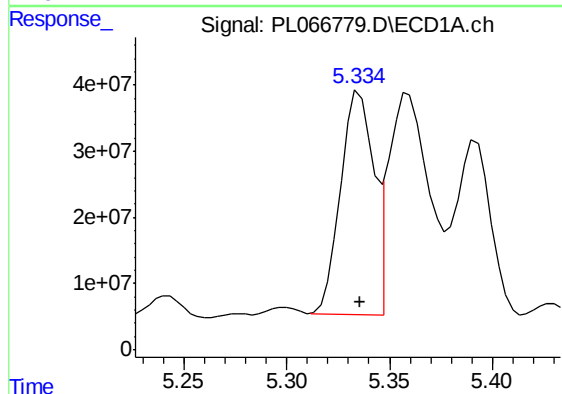


#25 Chlordane-3

R.T.: 5.335 min
Delta R.T.: 0.000 min
Response: 373627927
Conc: 754.52 ng/ml

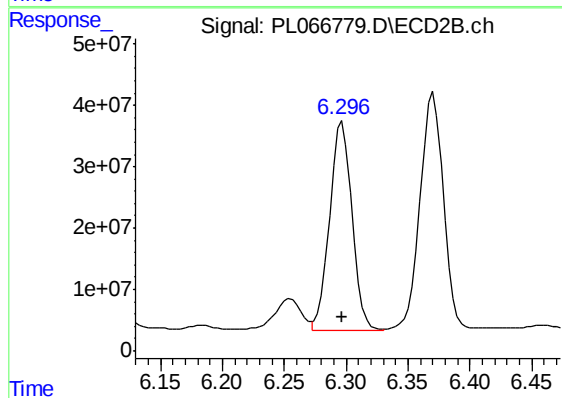

#25 Chlordane-3


R.T.: 6.297 min
Delta R.T.: 0.000 min
Response: 428780193
Conc: 756.47 ng/ml

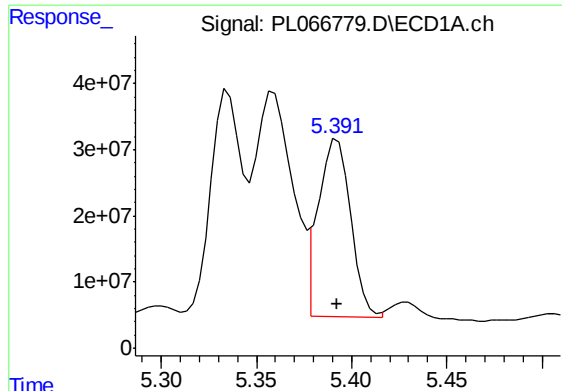

#26 Chlordane-4


R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 322546455
Conc: 751.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC750

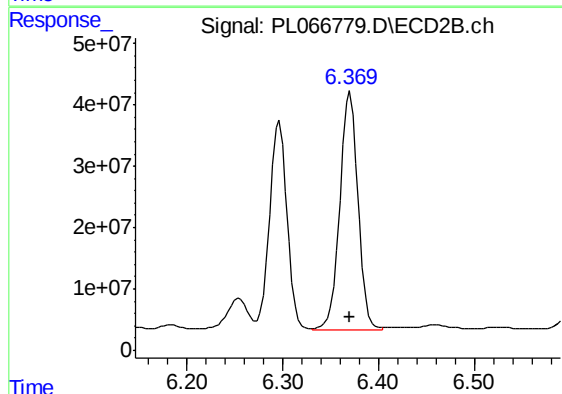


#26 Chlordane-4

R.T.: 6.370 min
Delta R.T.: 0.000 min
Response: 507393403
Conc: 748.72 ng/ml

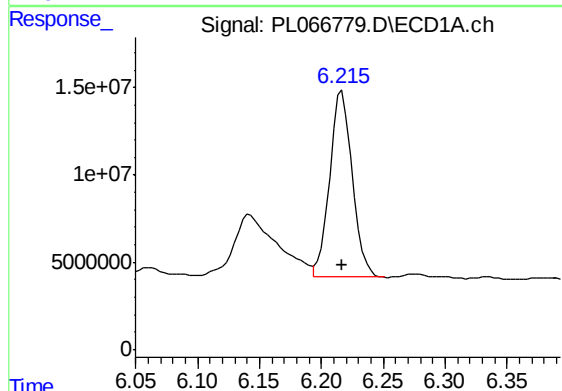


#27 Chlordane-5

R.T.: 6.217 min
Delta R.T.: 0.000 min
Response: 134963106
Conc: 748.41 ng/ml

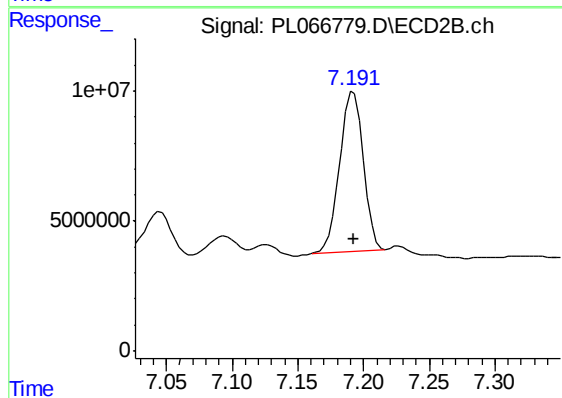

#27 Chlordane-5


R.T.: 7.192 min
Delta R.T.: 0.000 min
Response: 76918407
Conc: 749.72 ng/ml

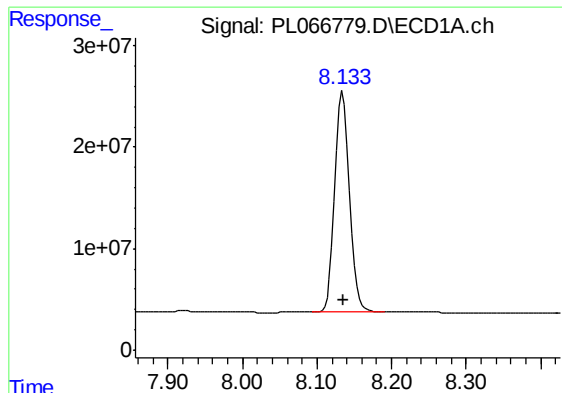

#28 Decachlorobiphenyl

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 295665439
Conc: 73.05 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC750

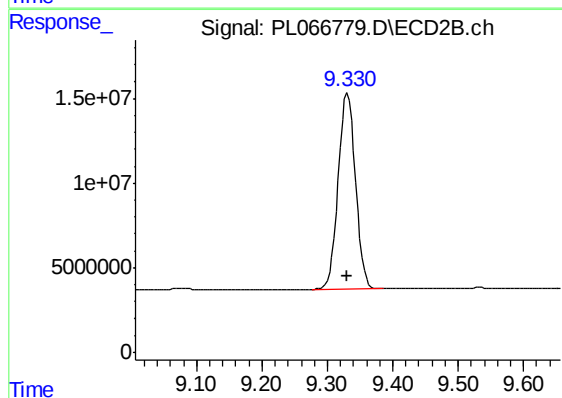

#28 Decachlorobiphenyl

R.T.: 9.331 min
Delta R.T.: 0.000 min
Response: 212041715
Conc: 71.21 ng/ml