

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
 Data File : PL066780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 20:24
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 08:47:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 08:46:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	4.144	218.5E6	166.1E6	50.000	50.000
28)	SA Decachlor...	8.135	9.331	202.4E6	148.9E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.279	5.163	75805640	67566861	500.000	500.000
24)	Chlordane-2	4.774	5.639	84823427	76658480	500.000	500.000
25)	Chlordane-3	5.336	6.297	247.6E6	283.4E6	500.000	500.000
26)	Chlordane-4	5.392	6.371	214.6E6	338.8E6	500.000	500.000
27)	Chlordane-5	6.217	7.193	90166901	51297780	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
Data File : PL066780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 20:24
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 08:47:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 08:46:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

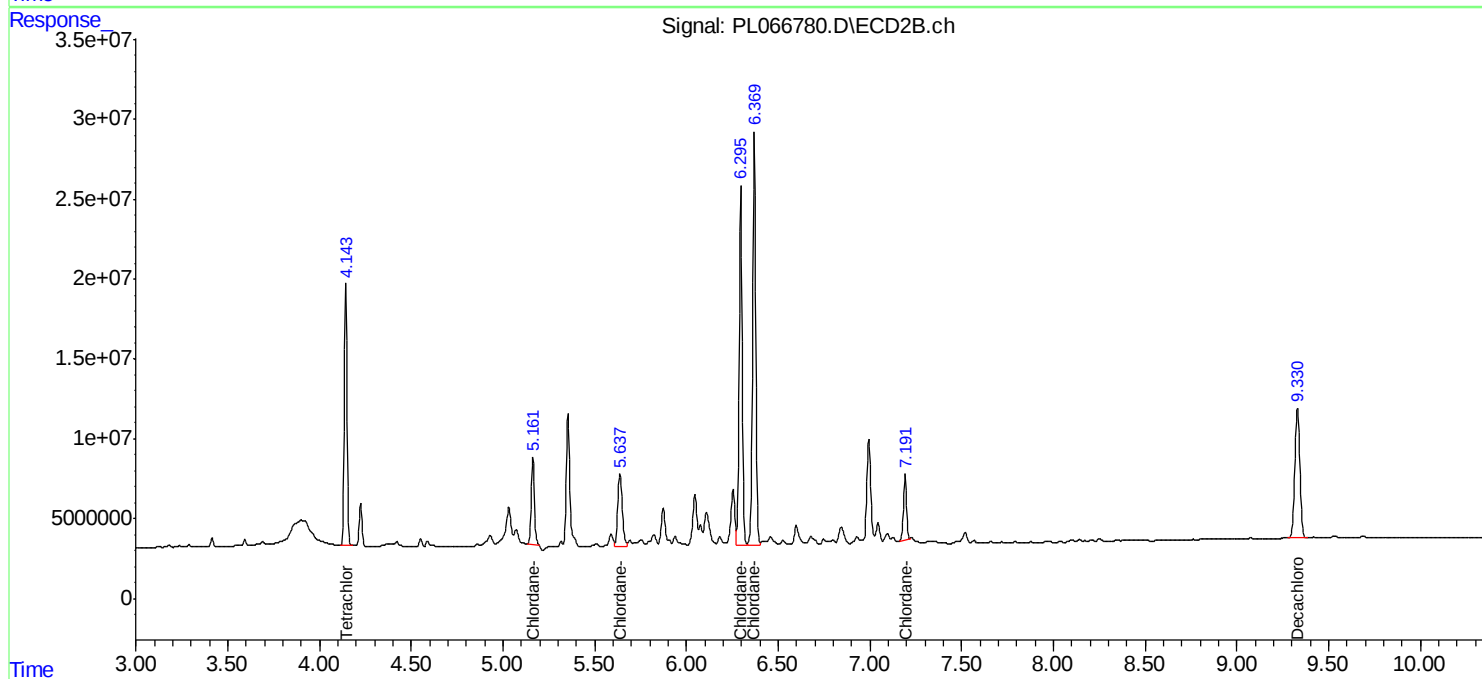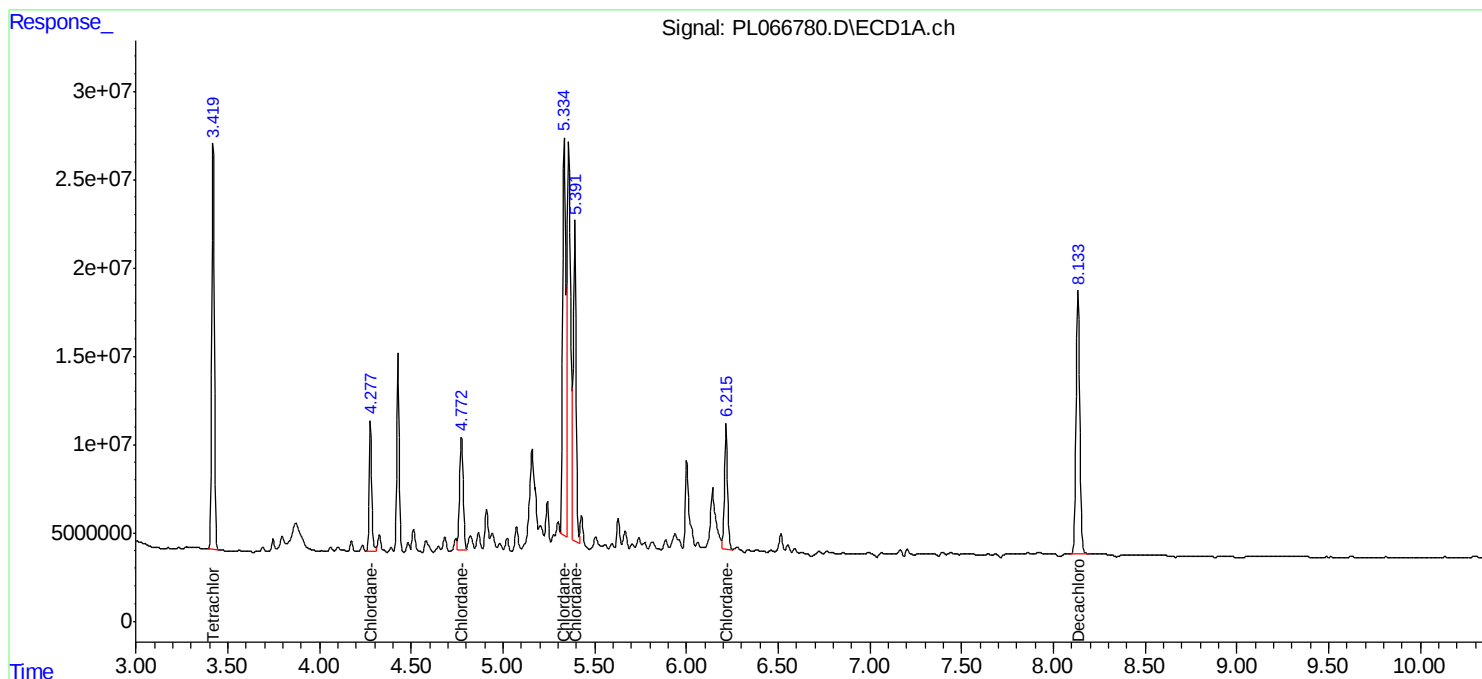


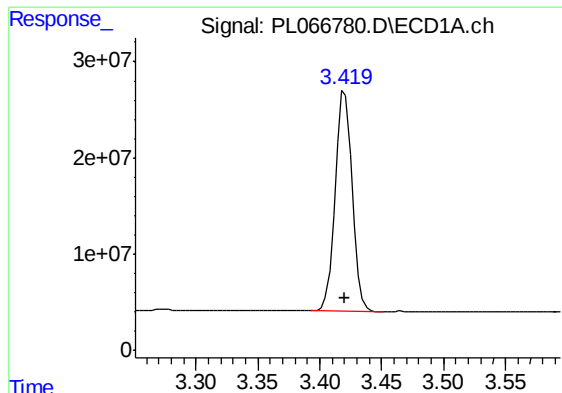

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 218511292
Conc: 50.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC500

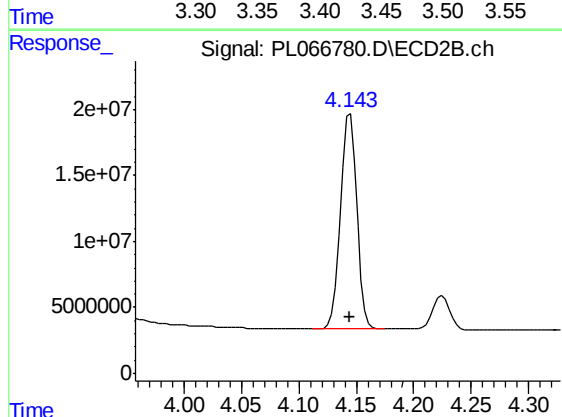


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 166052383
Conc: 50.00 ng/ml

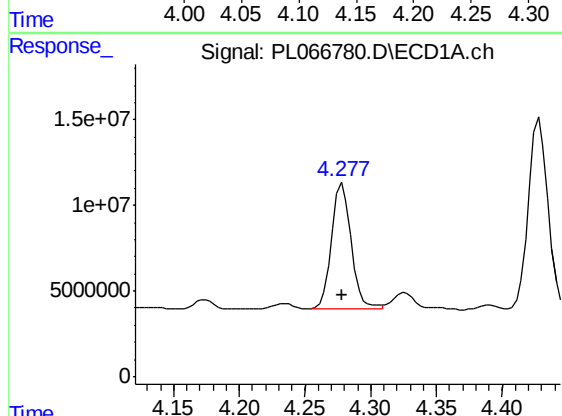


#23 Chlordane-1

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 75805640
Conc: 500.00 ng/ml

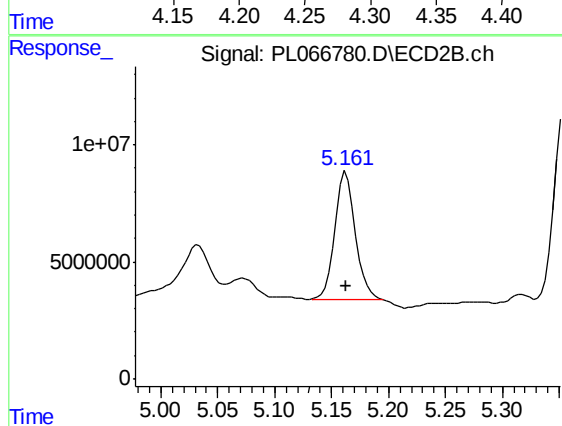

#23 Chlordane-1


R.T.: 5.163 min
Delta R.T.: 0.000 min
Response: 67566861
Conc: 500.00 ng/ml

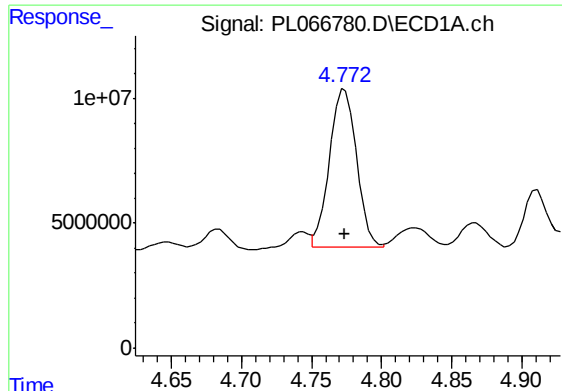

#24 Chlordane-2


R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 84823427
Conc: 500.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC500

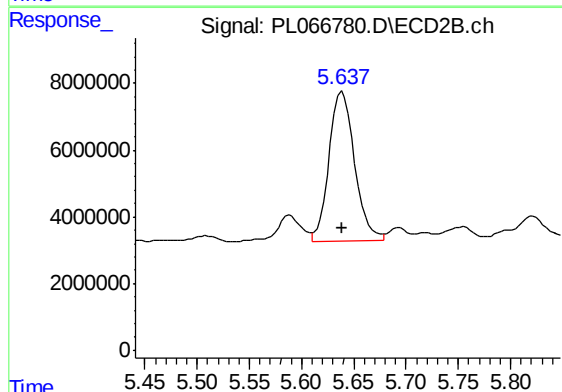


#24 Chlordane-2

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 76658480
Conc: 500.00 ng/ml

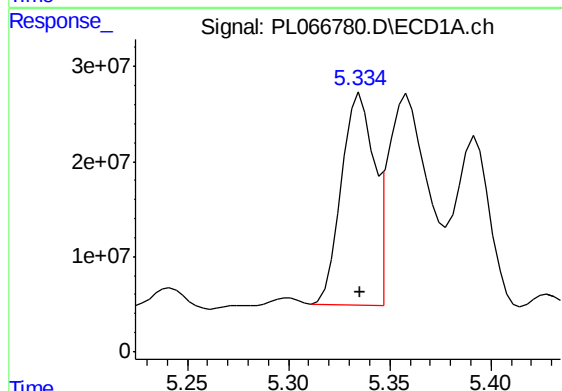


#25 Chlordane-3

R.T.: 5.336 min
Delta R.T.: 0.000 min
Response: 247592510
Conc: 500.00 ng/ml

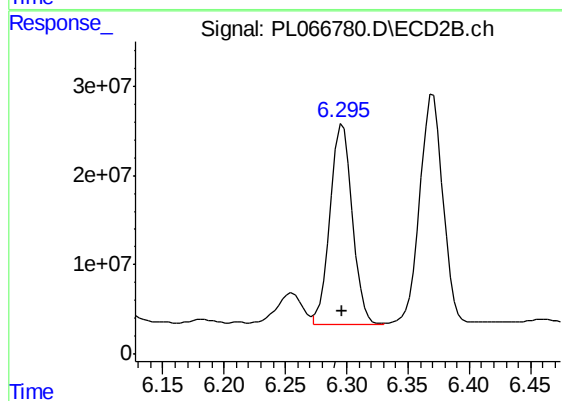

#25 Chlordane-3


R.T.: 6.297 min
Delta R.T.: 0.000 min
Response: 283409830
Conc: 500.00 ng/ml

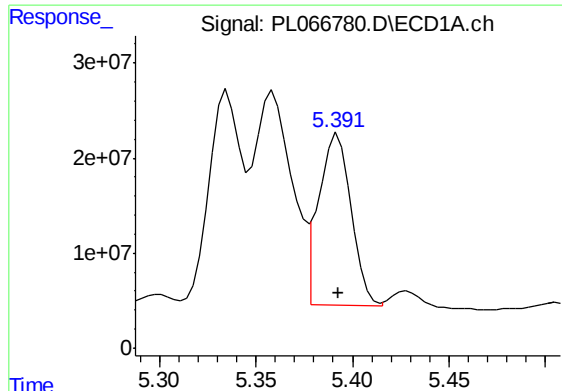

#26 Chlordane-4


R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 214580059
Conc: 500.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC500

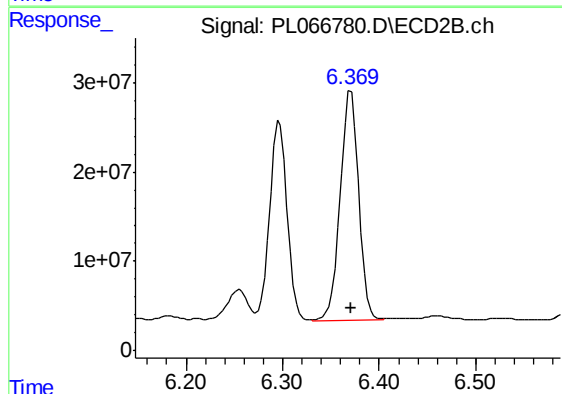


#26 Chlordane-4

R.T.: 6.371 min
Delta R.T.: 0.000 min
Response: 338838305
Conc: 500.00 ng/ml

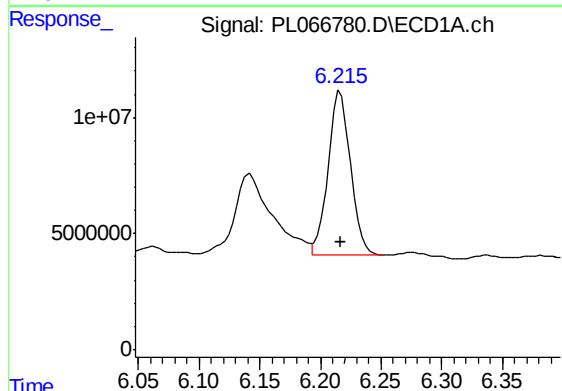


#27 Chlordane-5

R.T.: 6.217 min
Delta R.T.: 0.000 min
Response: 90166901
Conc: 500.00 ng/ml

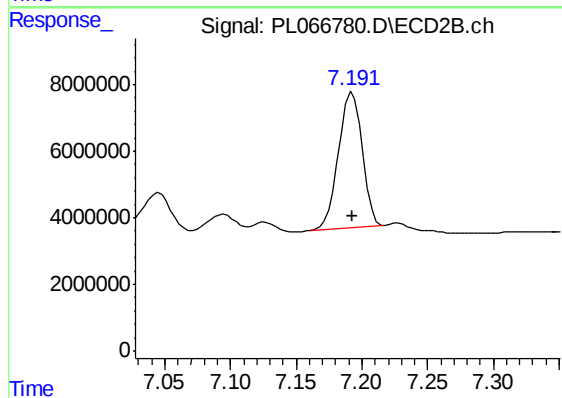

#27 Chlordane-5


R.T.: 7.193 min
Delta R.T.: 0.000 min
Response: 51297780
Conc: 500.00 ng/ml

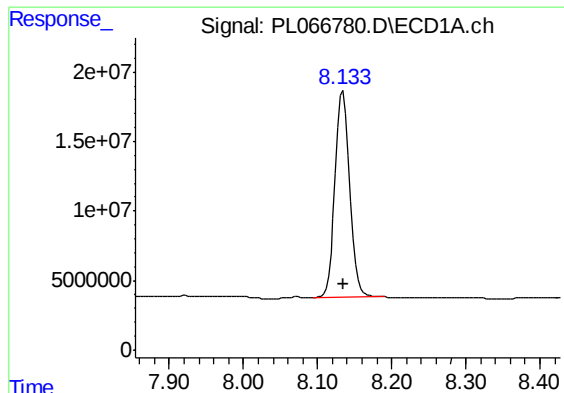

#28 Decachlorobiphenyl

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 202364899
Conc: 50.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC500

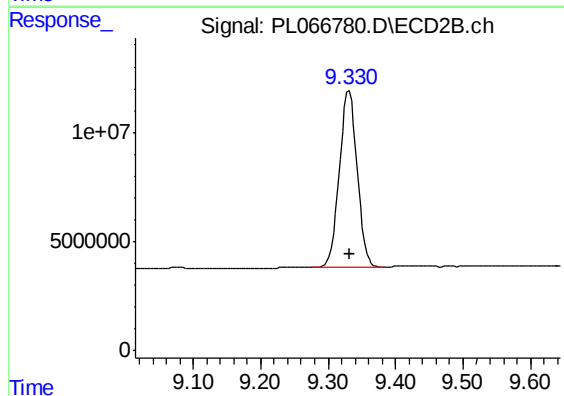

#28 Decachlorobiphenyl

R.T.: 9.331 min
Delta R.T.: 0.000 min
Response: 148876050
Conc: 50.00 ng/ml