

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
 Data File : PL066781.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 20:38
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 08:47:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 08:46:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	4.144	105.7E6	82579532	24.195	24.866
28)	SA Decachlor...	8.134	9.331	105.5E6	76928985	26.077	25.837
Target Compounds							
23)	Chlordane-1	4.278	5.162	38631643	33738053	254.807	249.664
24)	Chlordane-2	4.773	5.639	44105720	39913540	259.985	260.333
25)	Chlordane-3	5.335	6.297	121.3E6	139.2E6	245.043	245.522
26)	Chlordane-4	5.392	6.370	106.1E6	168.4E6	247.214	248.516
27)	Chlordane-5	6.216	7.192	45539389	25626249	252.528	249.779



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
Data File : PL066781.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 20:38
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 08:47:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 08:46:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

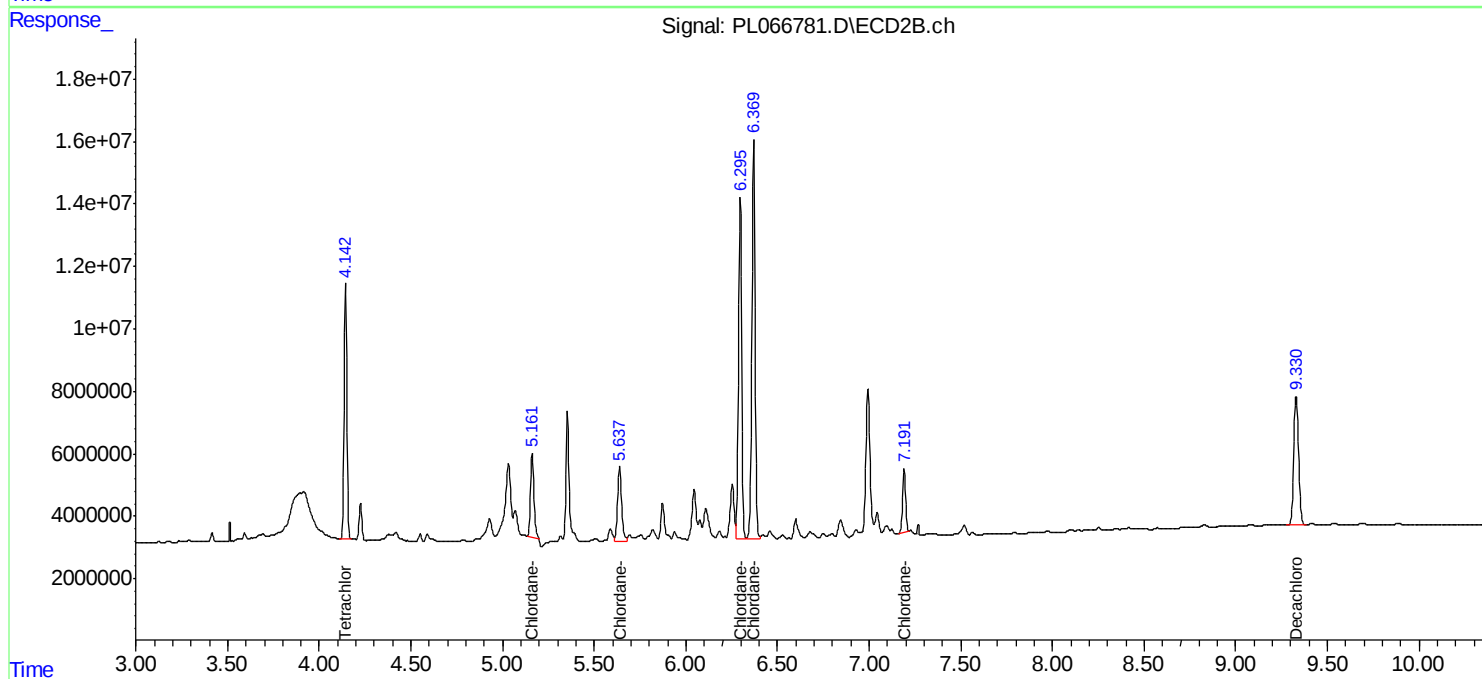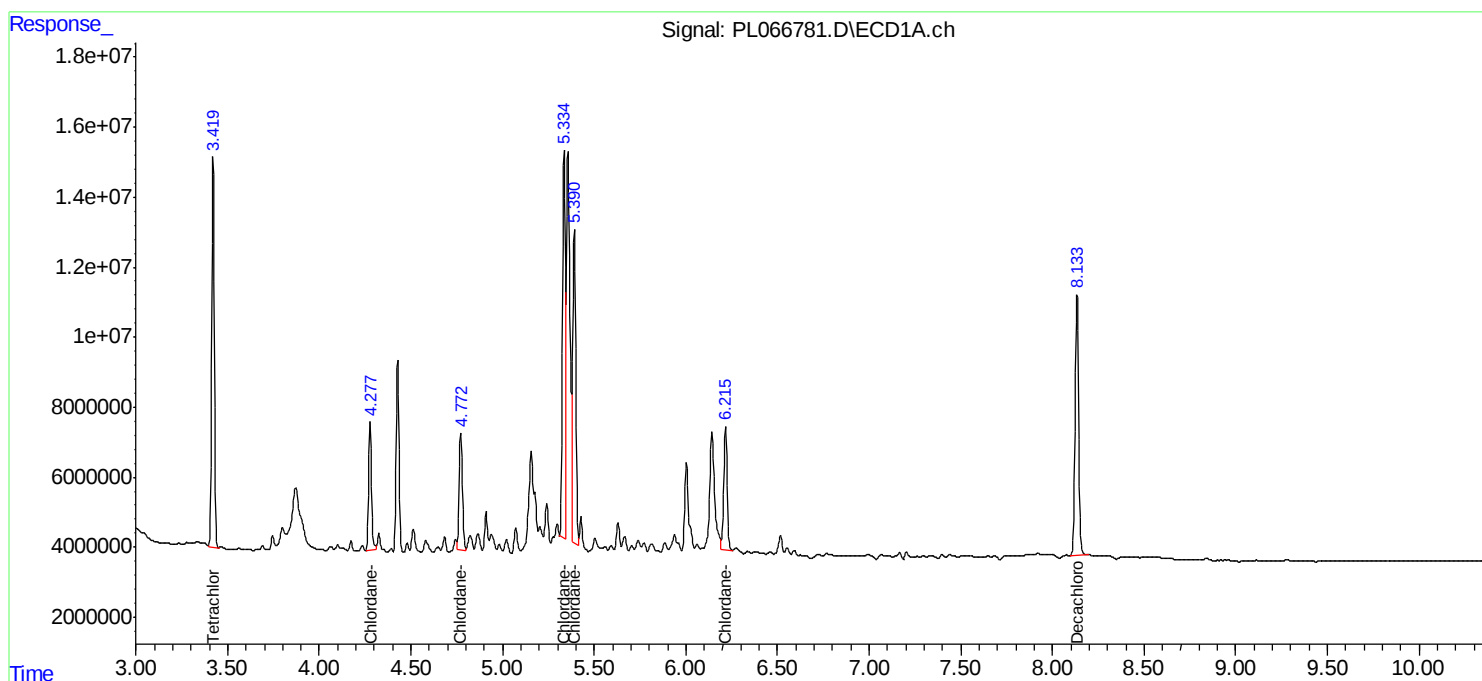


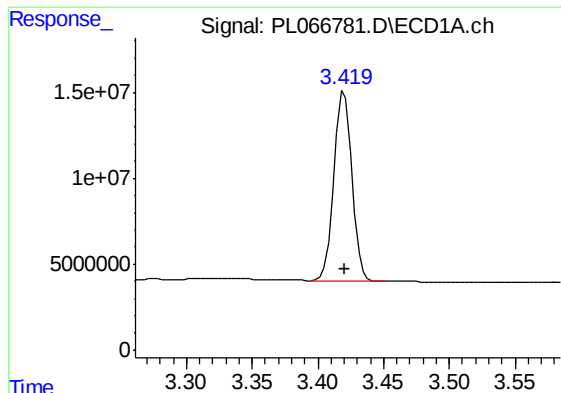

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 105738919
Conc: 24.20 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC250

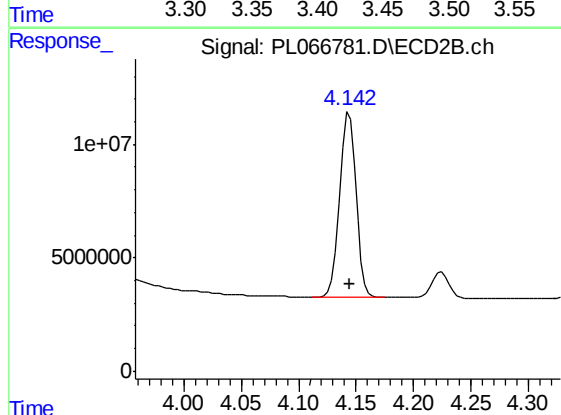


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 82579532
Conc: 24.87 ng/ml

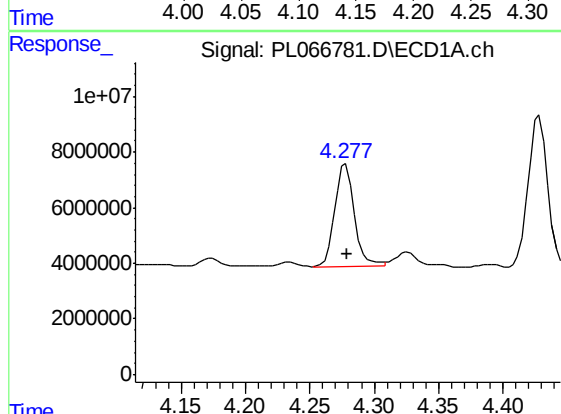


#23 Chlordane-1

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 38631643
Conc: 254.81 ng/ml

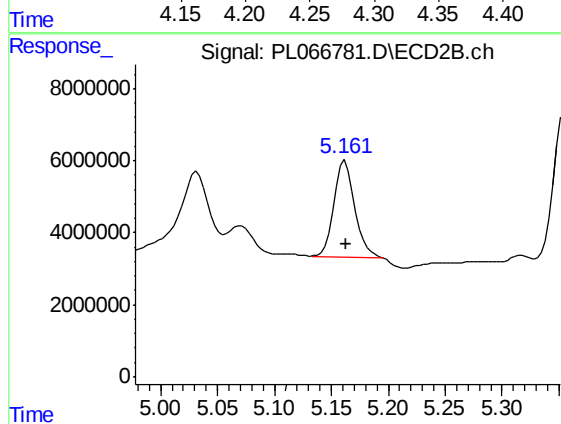

#23 Chlordane-1


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 33738053
Conc: 249.66 ng/ml

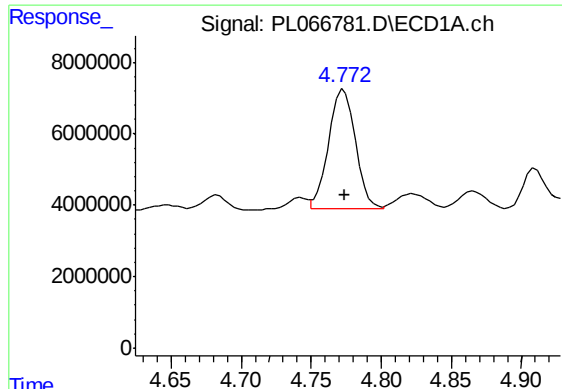

#24 Chlordane-2


R.T.: 4.773 min
Delta R.T.: 0.000 min
Response: 44105720
Conc: 259.99 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC250

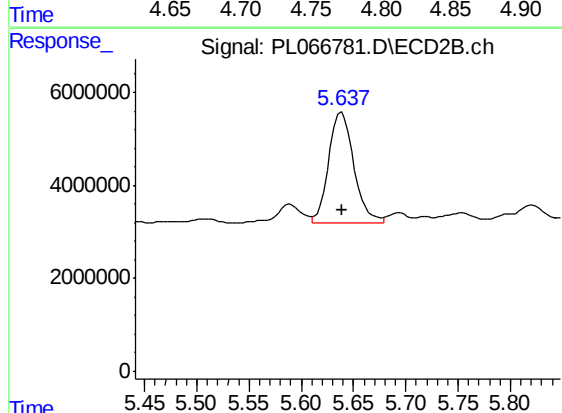


#24 Chlordane-2

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 39913540
Conc: 260.33 ng/ml

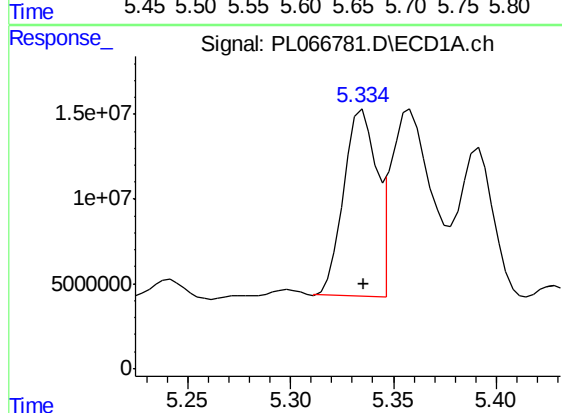


#25 Chlordane-3

R.T.: 5.335 min
Delta R.T.: 0.000 min
Response: 121341677
Conc: 245.04 ng/ml

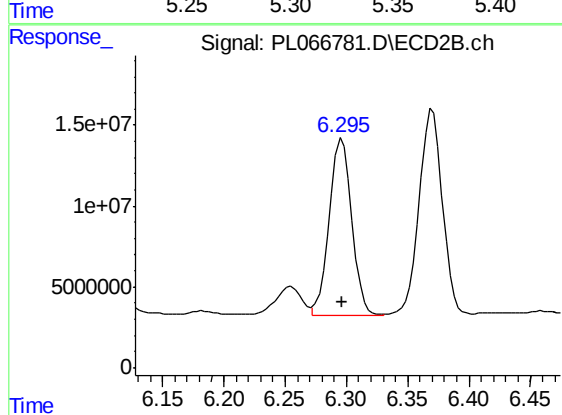

#25 Chlordane-3


R.T.: 6.297 min
Delta R.T.: 0.000 min
Response: 139166693
Conc: 245.52 ng/ml

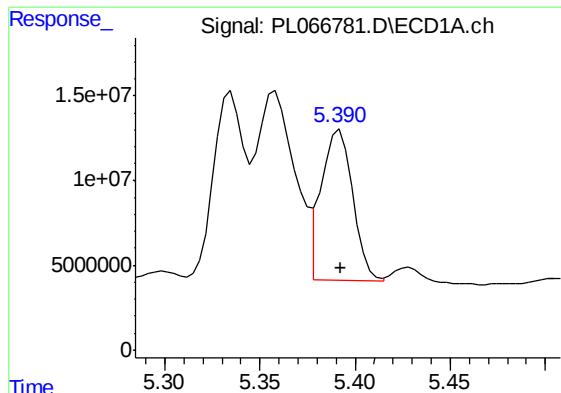

#26 Chlordane-4


R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 106094450
Conc: 247.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC250

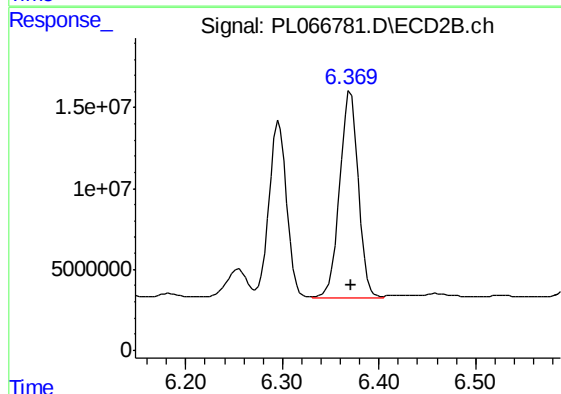


#26 Chlordane-4

R.T.: 6.370 min
Delta R.T.: 0.000 min
Response: 168413308
Conc: 248.52 ng/ml

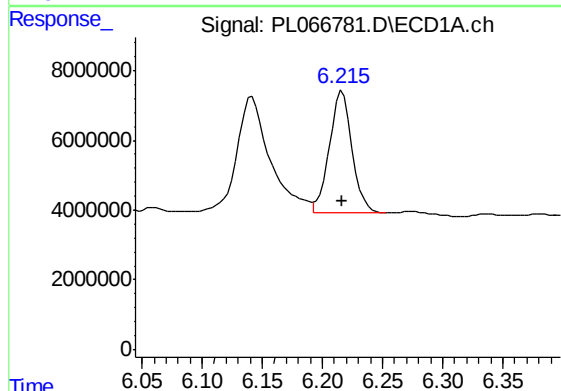


#27 Chlordane-5

R.T.: 6.216 min
Delta R.T.: 0.000 min
Response: 45539389
Conc: 252.53 ng/ml

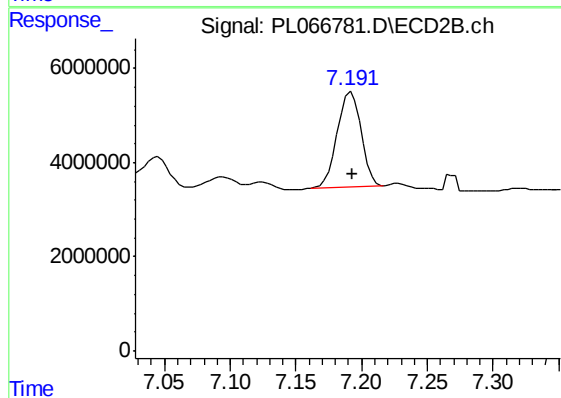

#27 Chlordane-5


R.T.: 7.192 min
Delta R.T.: 0.000 min
Response: 25626249
Conc: 249.78 ng/ml

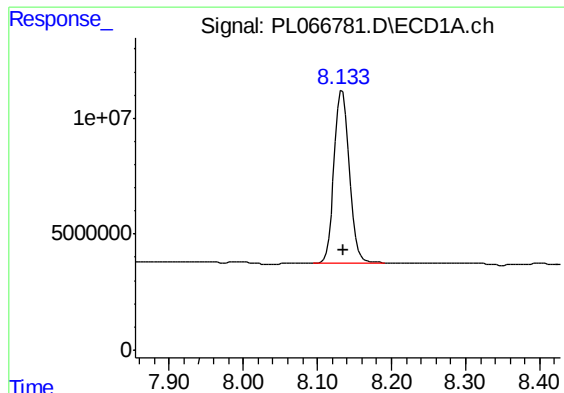

#28 Decachlorobiphenyl

R.T.: 8.134 min
Delta R.T.: 0.000 min
Response: 105543094
Conc: 26.08 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC250

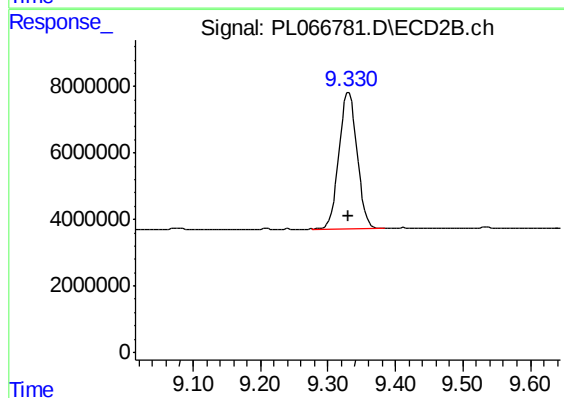

#28 Decachlorobiphenyl

R.T.: 9.331 min
Delta R.T.: 0.000 min
Response: 76928985
Conc: 25.84 ng/ml