

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
 Data File : PL066782.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 20:53
 Operator : AR\AJ
 Sample : PCHLORICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCHLORICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 08:48:18 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 08:46:31 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.144	19459405	15527595	4.453	4.676
28)	SA Decachlor...	8.135	9.332	22275921	15825667	5.504	5.315
Target Compounds							
23)	Chlordane-1	4.279	5.162	8021181	6285931	52.906	46.516
24)	Chlordane-2	4.774	5.638	9761503	7162460	57.540	46.717
25)	Chlordane-3	5.335	6.297	22660067	25467249	45.761	44.930
26)	Chlordane-4	5.393	6.370	20291736	31852769	47.282	47.003
27)	Chlordane-5	6.217	7.191	9407215	4693578	52.166	45.748



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
Data File : PL066782.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 20:53
Operator : AR\AJ
Sample : PCHLORICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCHLORICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 08:48:18 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 08:46:31 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

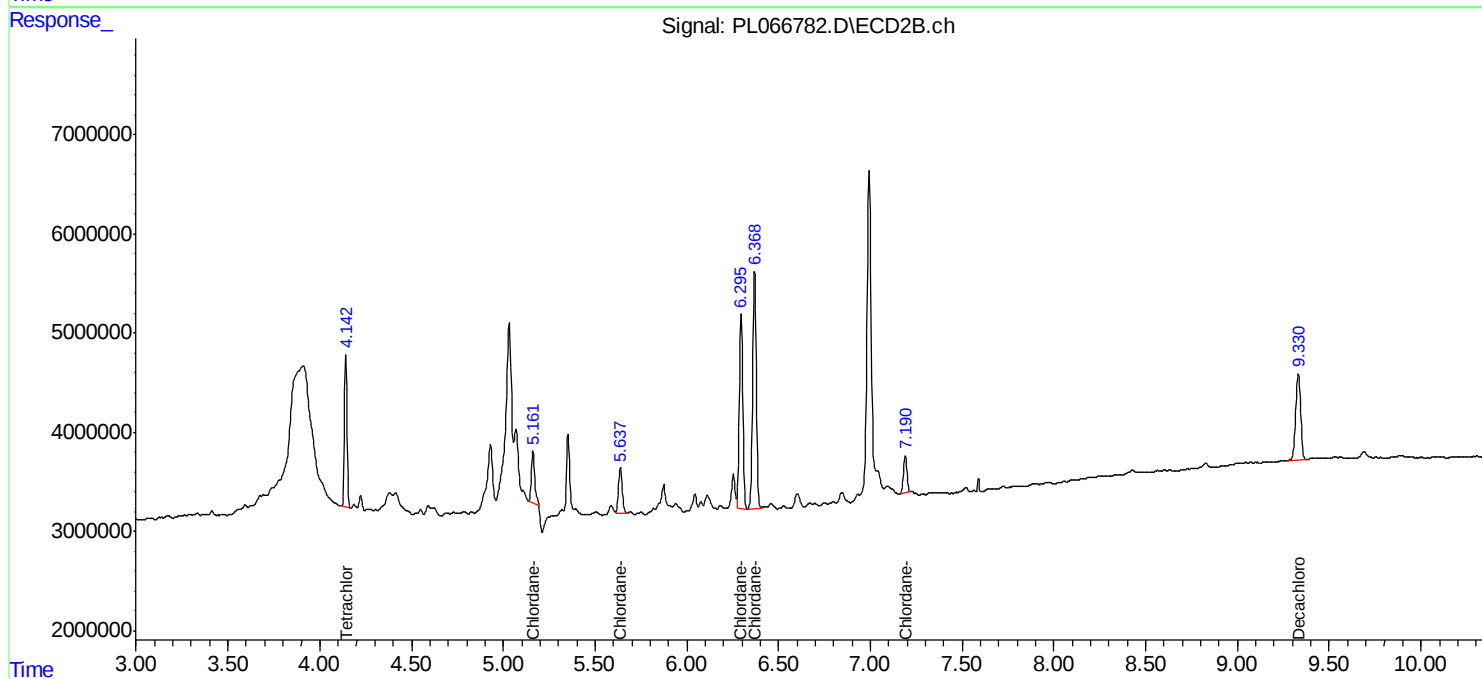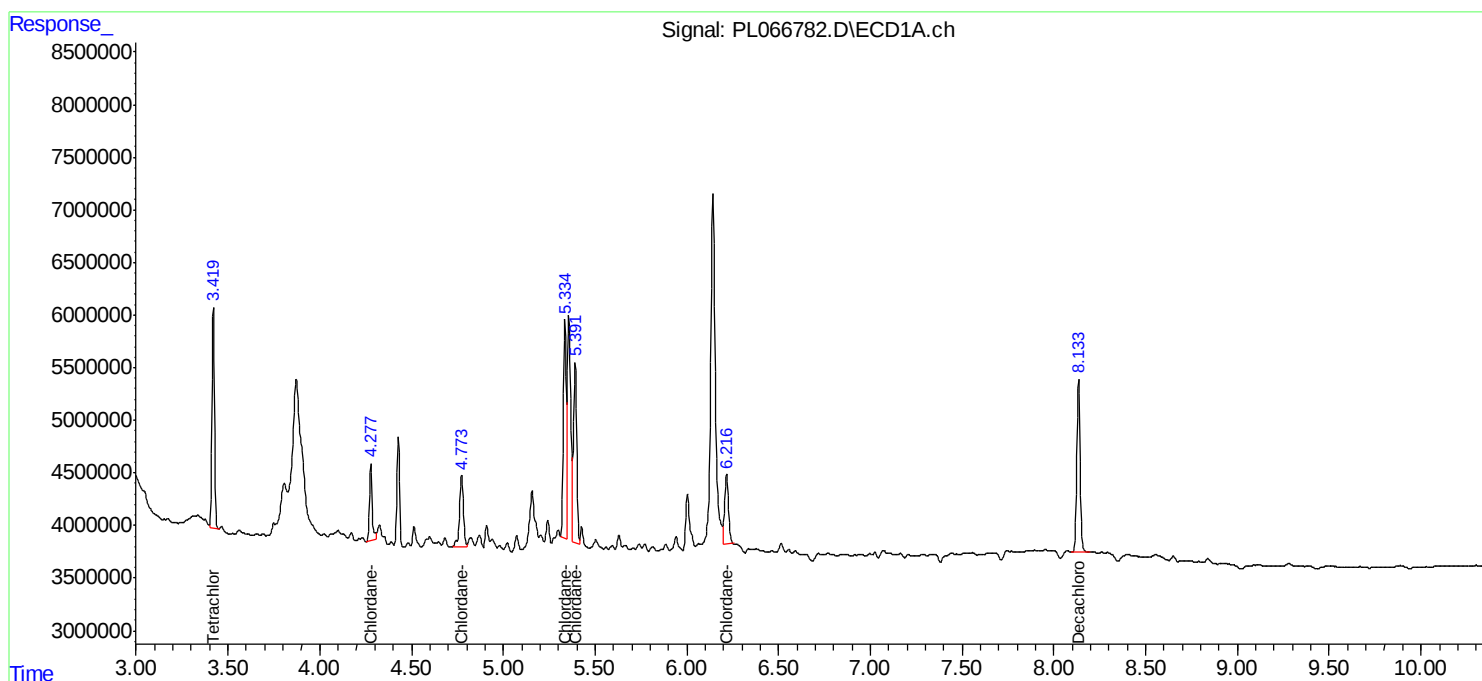


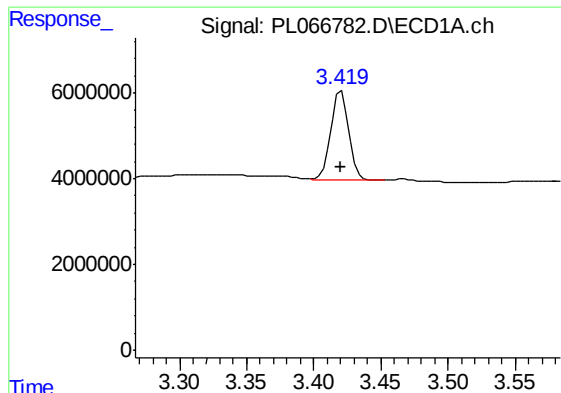

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: 0.000 min
Response: 19459405
Conc: 4.45 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC050

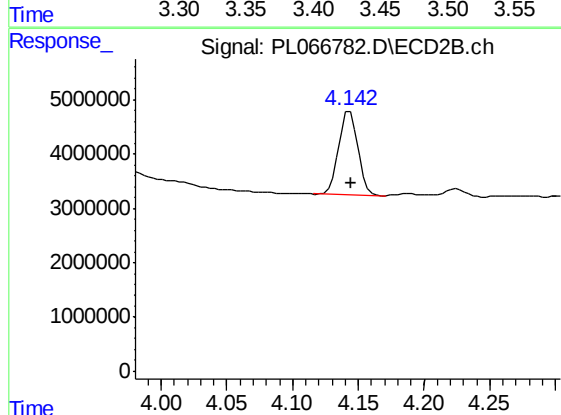


#1 Tetrachloro-m-xylene

R.T.: 4.144 min
Delta R.T.: 0.000 min
Response: 15527595
Conc: 4.68 ng/ml

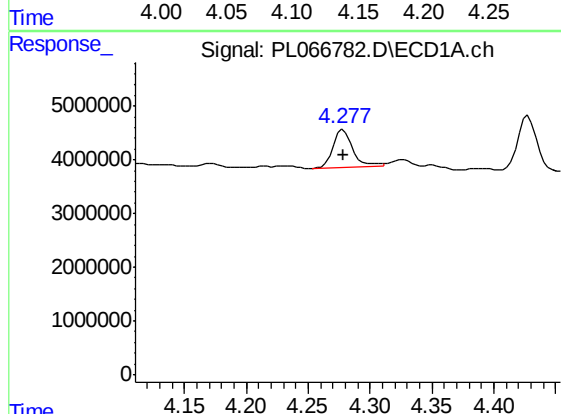


#23 Chlordane-1

R.T.: 4.279 min
Delta R.T.: 0.000 min
Response: 8021181
Conc: 52.91 ng/ml

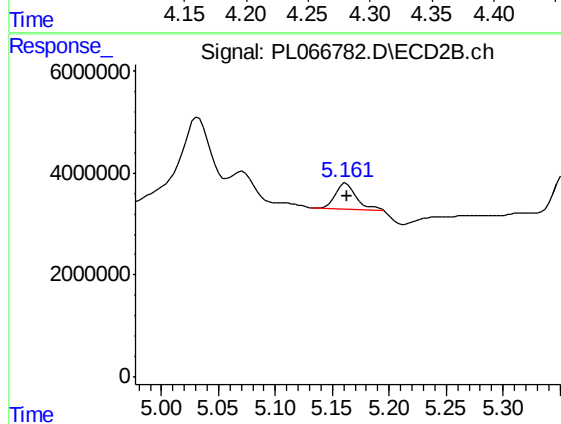

#23 Chlordane-1


R.T.: 5.162 min
Delta R.T.: 0.000 min
Response: 6285931
Conc: 46.52 ng/ml

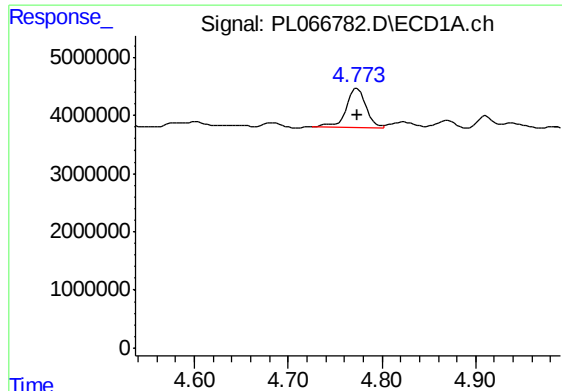

#24 Chlordane-2


R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 9761503
Conc: 57.54 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC050

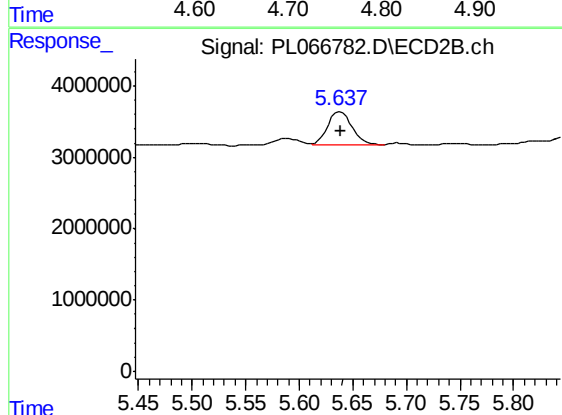


#24 Chlordane-2

R.T.: 5.638 min
Delta R.T.: 0.000 min
Response: 7162460
Conc: 46.72 ng/ml

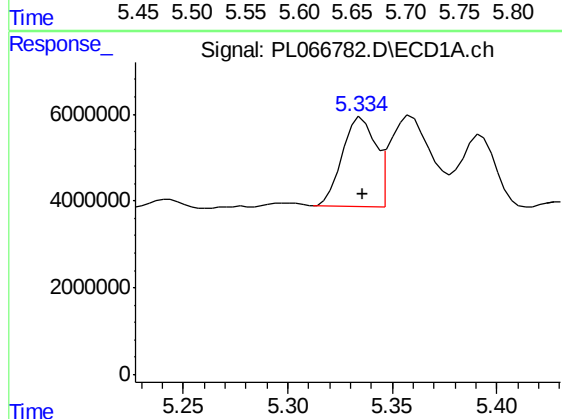


#25 Chlordane-3

R.T.: 5.335 min
Delta R.T.: 0.000 min
Response: 22660067
Conc: 45.76 ng/ml

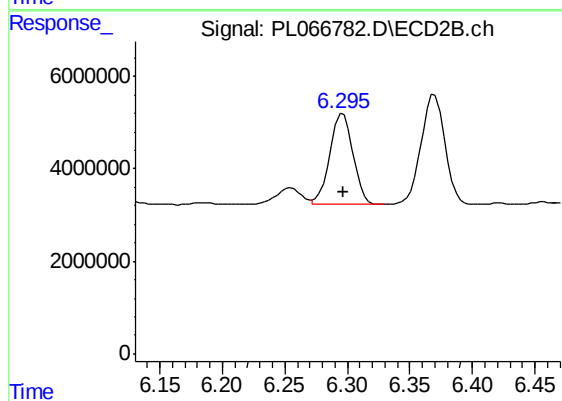

#25 Chlordane-3


R.T.: 6.297 min
Delta R.T.: 0.000 min
Response: 25467249
Conc: 44.93 ng/ml

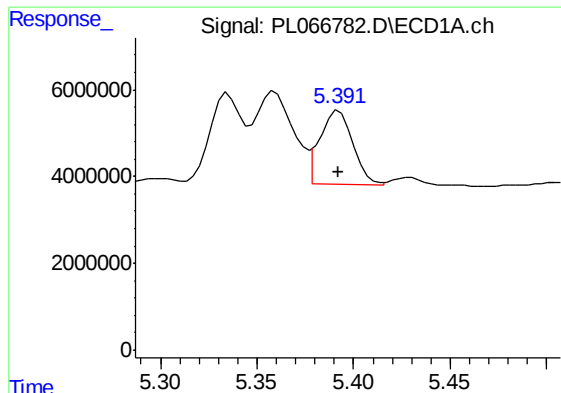

#26 Chlordane-4


R.T.: 5.393 min
Delta R.T.: 0.000 min
Response: 20291736
Conc: 47.28 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC050

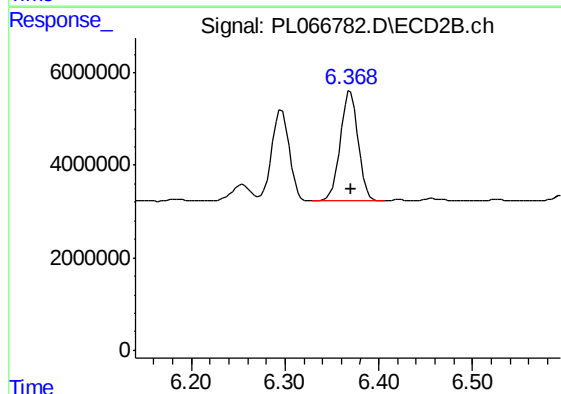


#26 Chlordane-4

R.T.: 6.370 min
Delta R.T.: 0.000 min
Response: 31852769
Conc: 47.00 ng/ml

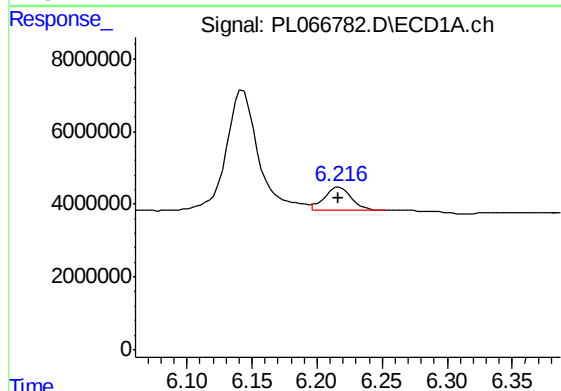


#27 Chlordane-5

R.T.: 6.217 min
Delta R.T.: 0.000 min
Response: 9407215
Conc: 52.17 ng/ml

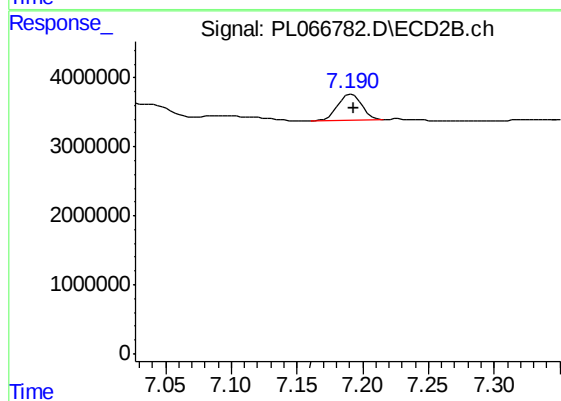

#27 Chlordane-5


R.T.: 7.191 min
Delta R.T.: -0.001 min
Response: 4693578
Conc: 45.75 ng/ml

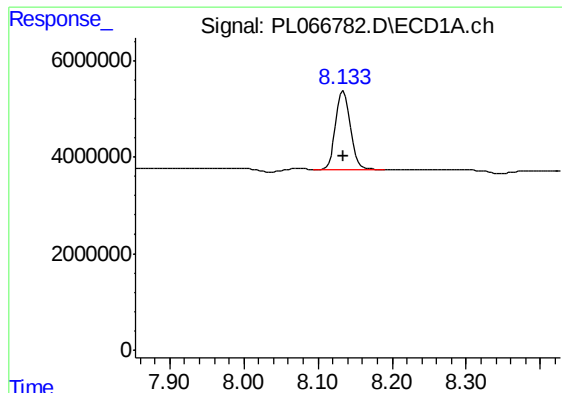

#28 Decachlorobiphenyl

R.T.: 8.135 min
Delta R.T.: 0.000 min
Response: 22275921
Conc: 5.50 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCHLORICC050

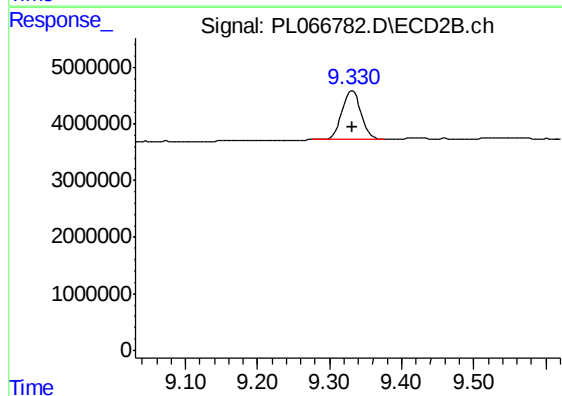

#28 Decachlorobiphenyl

R.T.: 9.332 min
Delta R.T.: 0.000 min
Response: 15825667
Conc: 5.32 ng/ml