

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
 Data File : PL066789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 May 2021 22:33
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 ICVPL051321CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 08:56:22 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
 Quant Title : GC Extractables
 QLast Update : Fri May 14 08:55:43 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.420	4.143	218.3E6	160.7E6	51.471	49.276
28)	SA Decachlor...	8.134	9.330	204.2E6	145.5E6	49.875	49.005
Target Compounds							
23)	Chlordane-1	4.278	5.162	75998118	65314625	497.142	505.316
24)	Chlordane-2	4.774	5.639	85217666	75367528	502.250	499.248
25)	Chlordane-3	5.335	6.297	249.5E6	278.7E6	514.616	501.219
26)	Chlordane-4	5.392	6.370	215.3E6	331.9E6	509.182	496.635
27)	Chlordane-5	6.216	7.192	90044170	50066652	495.360	496.479



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL051321\
Data File : PL066789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 May 2021 22:33
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPL051321CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 08:56:22 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL051321.M
Quant Title : GC Extractables
QLast Update : Fri May 14 08:55:43 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

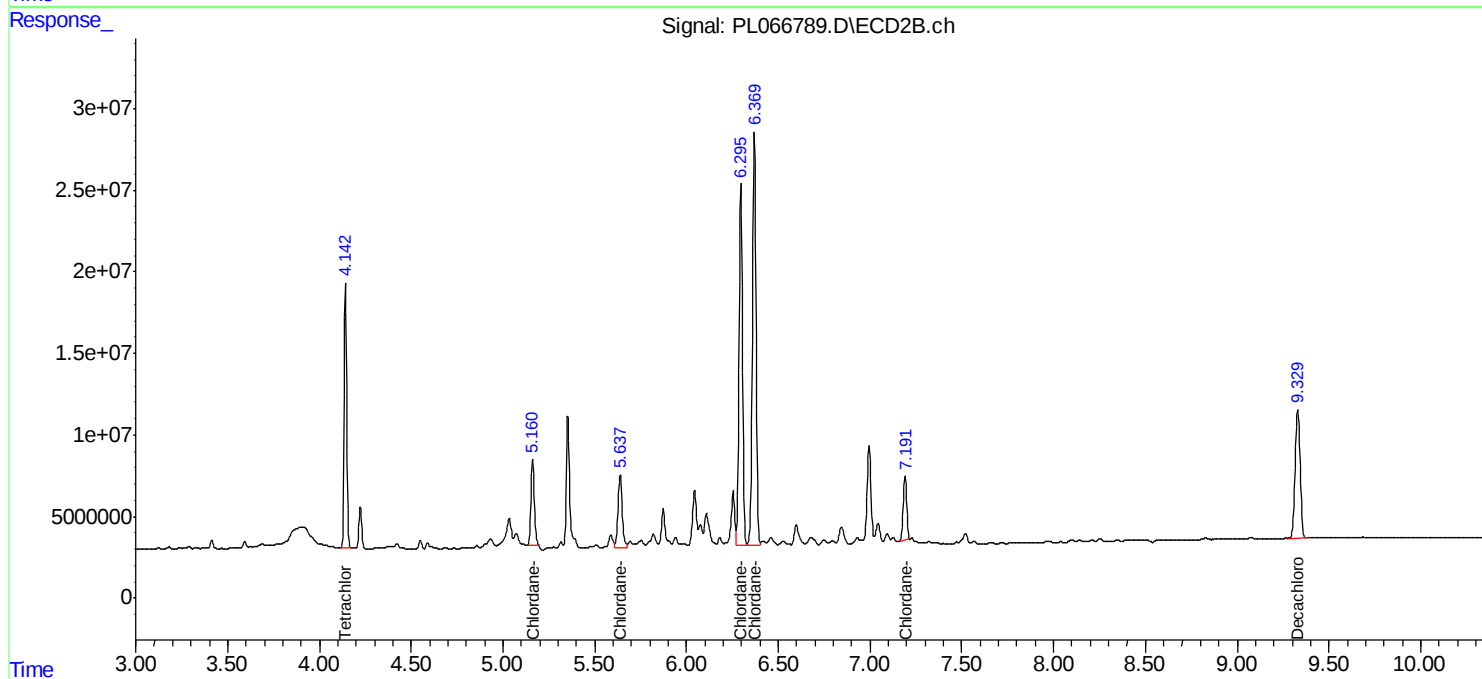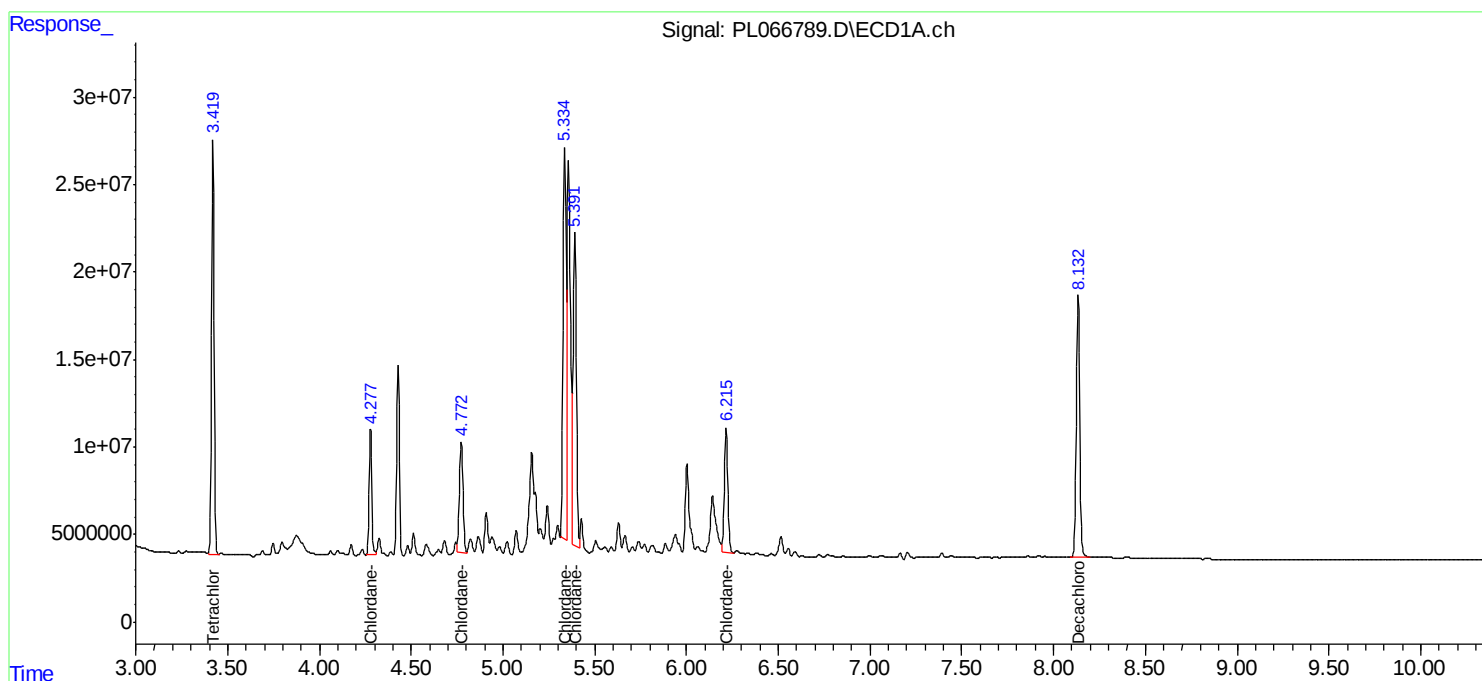


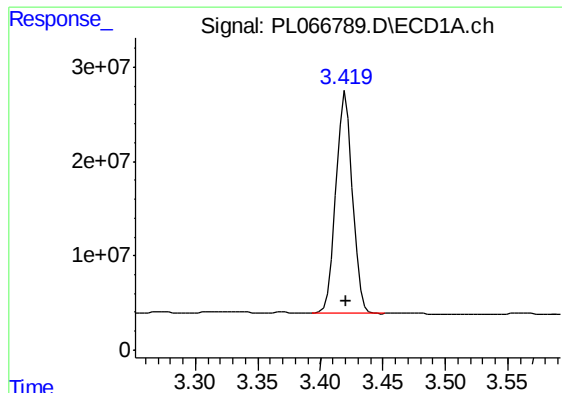

#1 Tetrachloro-m-xylene


R.T.: 3.420 min
Delta R.T.: 0.000 min
Response: 218294003
Conc: 51.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPL051321CHLOR

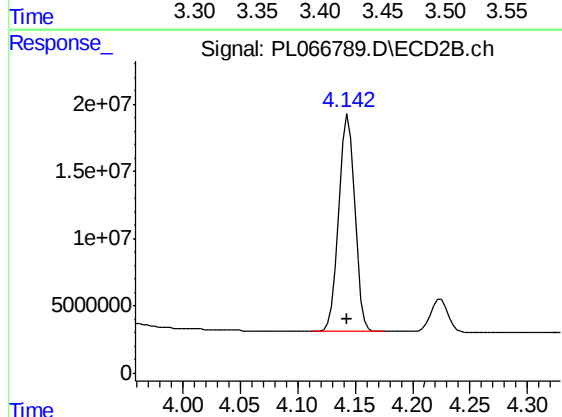


#1 Tetrachloro-m-xylene

R.T.: 4.143 min
Delta R.T.: 0.000 min
Response: 160698545
Conc: 49.28 ng/ml

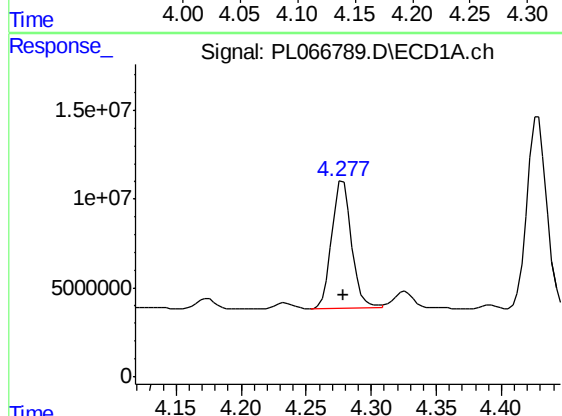


#23 Chlordane-1

R.T.: 4.278 min
Delta R.T.: 0.000 min
Response: 75998118
Conc: 497.14 ng/ml

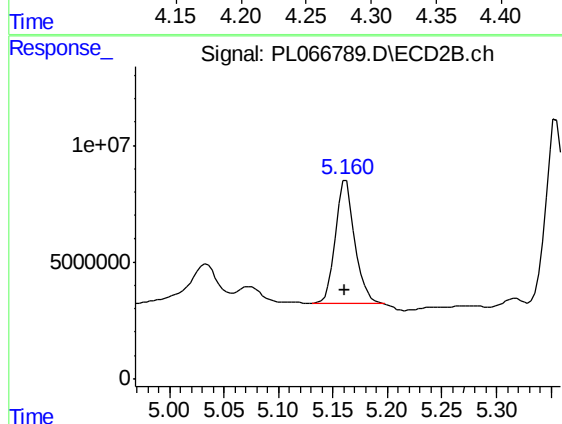

#23 Chlordane-1


R.T.: 5.162 min
Delta R.T.: 0.001 min
Response: 65314625
Conc: 505.32 ng/ml

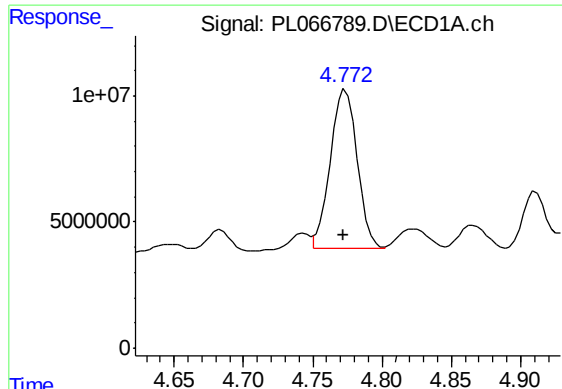

#24 Chlordane-2


R.T.: 4.774 min
Delta R.T.: 0.001 min
Response: 85217666
Conc: 502.25 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPL051321CHLOR

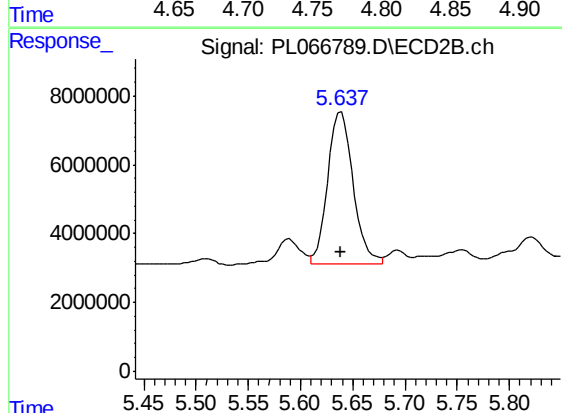


#24 Chlordane-2

R.T.: 5.639 min
Delta R.T.: 0.000 min
Response: 75367528
Conc: 499.25 ng/ml

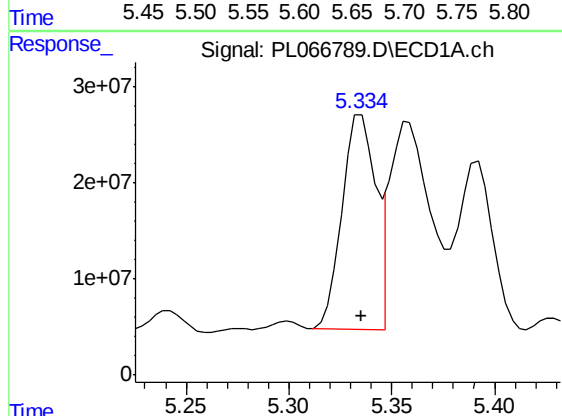


#25 Chlordane-3

R.T.: 5.335 min
Delta R.T.: 0.000 min
Response: 249507199
Conc: 514.62 ng/ml

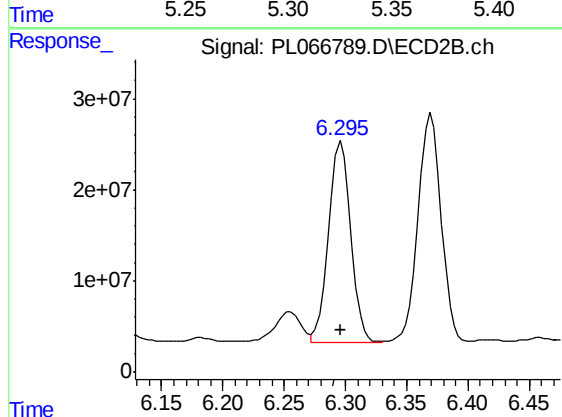

#25 Chlordane-3


R.T.: 6.297 min
Delta R.T.: 0.000 min
Response: 278731778
Conc: 501.22 ng/ml

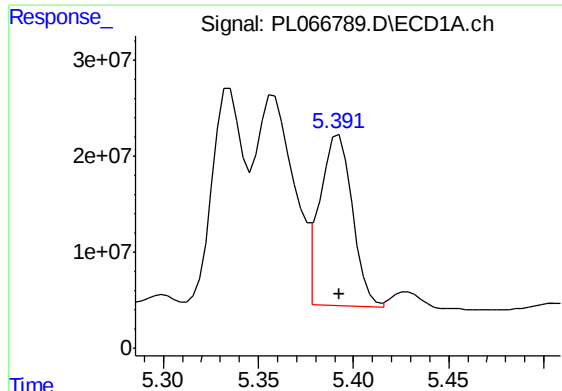

#26 Chlordane-4


R.T.: 5.392 min
Delta R.T.: 0.000 min
Response: 215288783
Conc: 509.18 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPL051321CHLOR

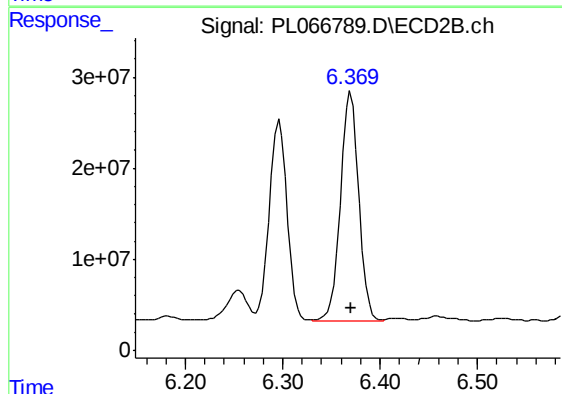


#26 Chlordane-4

R.T.: 6.370 min
Delta R.T.: 0.000 min
Response: 331865719
Conc: 496.63 ng/ml

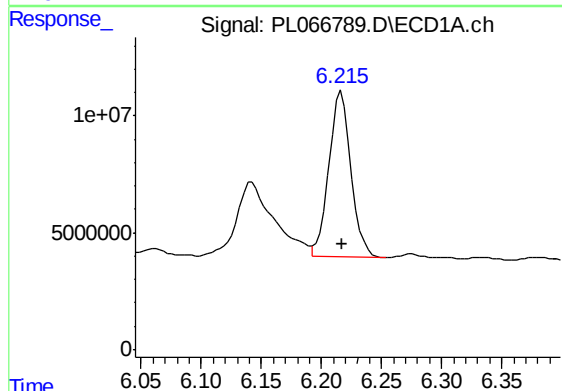


#27 Chlordane-5

R.T.: 6.216 min
Delta R.T.: 0.000 min
Response: 90044170
Conc: 495.36 ng/ml

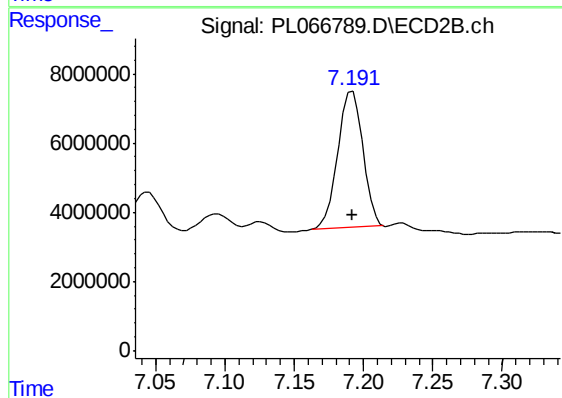

#27 Chlordane-5


R.T.: 7.192 min
Delta R.T.: 0.000 min
Response: 50066652
Conc: 496.48 ng/ml

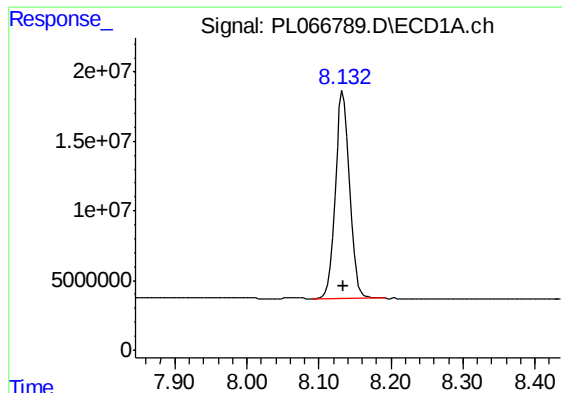

#28 Decachlorobiphenyl

R.T.: 8.134 min
Delta R.T.: 0.000 min
Response: 204215874
Conc: 49.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
ICVPL051321CHLOR

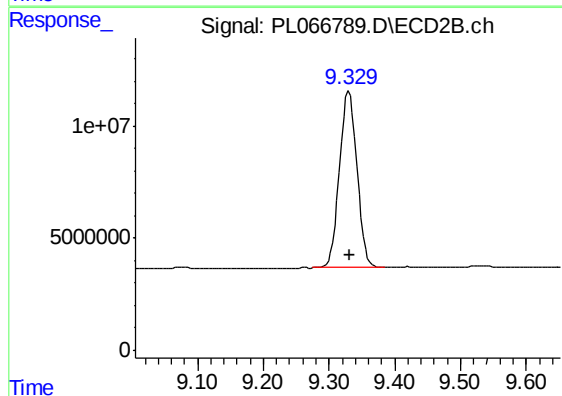

#28 Decachlorobiphenyl

R.T.: 9.330 min
Delta R.T.: -0.002 min
Response: 145531396
Conc: 49.01 ng/ml