

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077823.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 17:09
 Operator : DD\AJ
 Sample : M2262-09
 Misc : AR1248 MDL 25 PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 17:31:59 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.352	3.632	1431108	629413	24.380	24.736
2)	SA Decachlor...	9.970	8.827	1030014	648396	24.915	26.980
Target Compounds							
21)	L5 AR-1248-1	5.648	4.862	28603	22408	24.929	39.769 #
22)	L5 AR-1248-2	5.939	5.122	45290	24843	28.524	31.122
23)	L5 AR-1248-3	6.151	5.164	54039	26330	29.324	32.622
24)	L5 AR-1248-4	6.573	5.346	55685	28281	28.422	29.487
25)	L5 AR-1248-5	6.610	5.762	51372	25449	26.894	27.544



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077823.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 17:09
Operator : DD\AJ
Sample : M2262-09
Misc : AR1248 MDL 25 PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 17:31:59 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

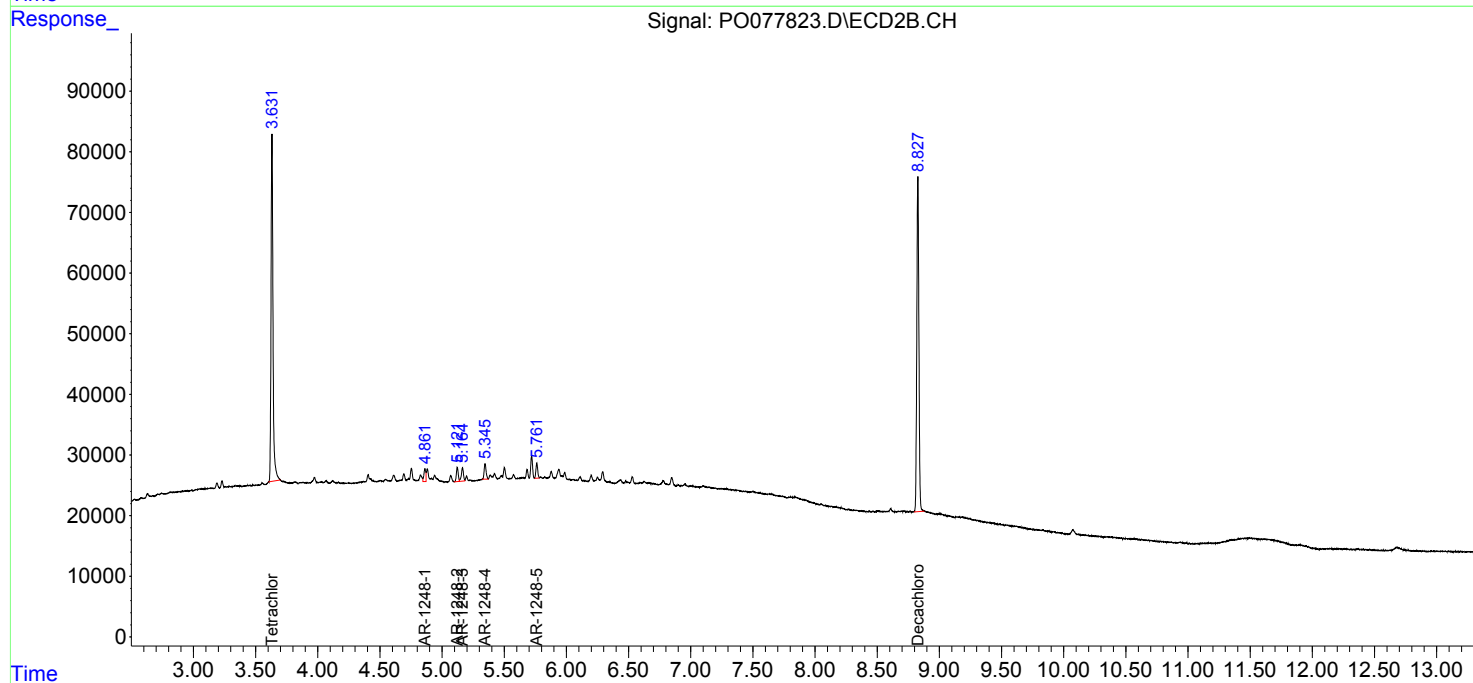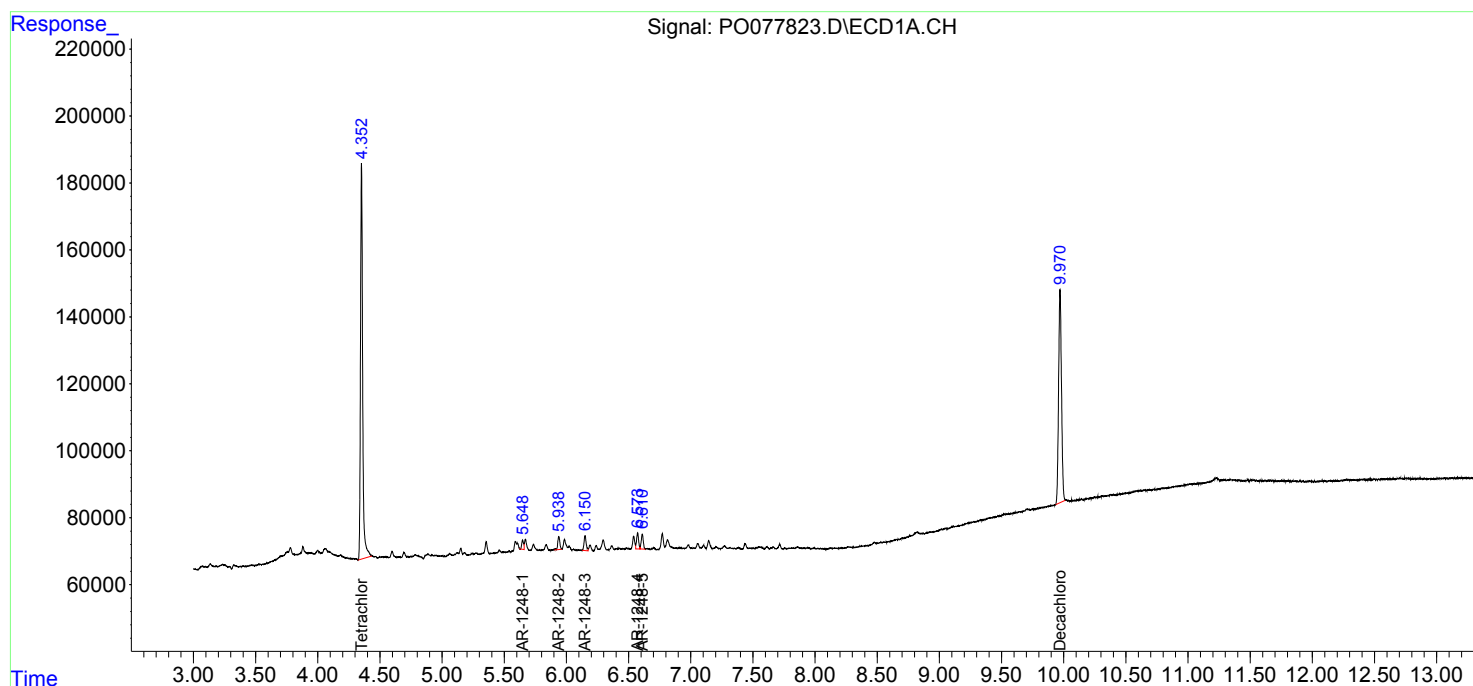


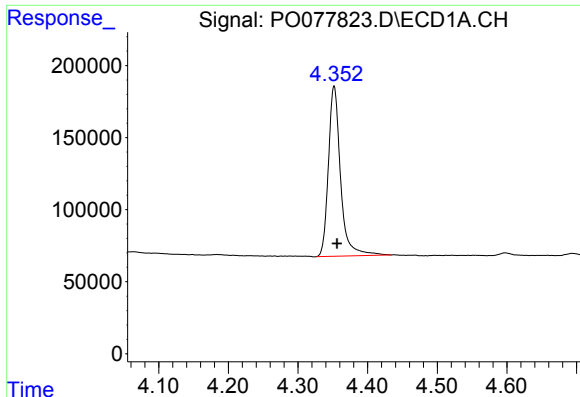

#1 Tetrachloro-m-xylene


R.T.: 4.352 min
Delta R.T.: -0.004 min
Response: 1431108
Conc: 24.38 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

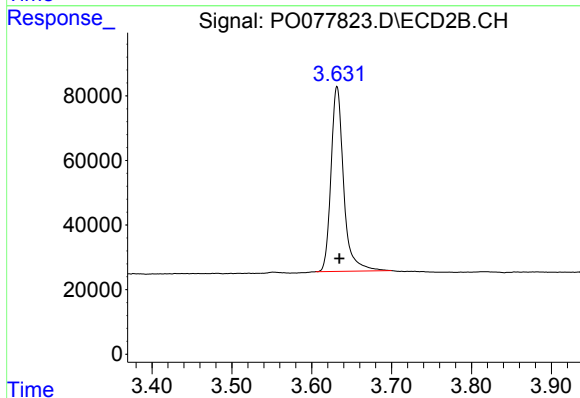


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.003 min
Response: 629413
Conc: 24.74 ng/ml

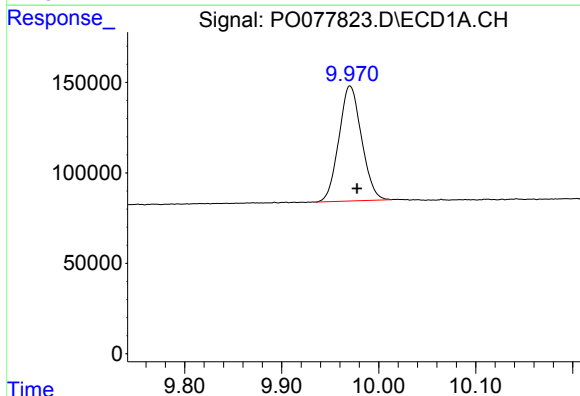


#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.007 min
Response: 1030014
Conc: 24.92 ng/ml

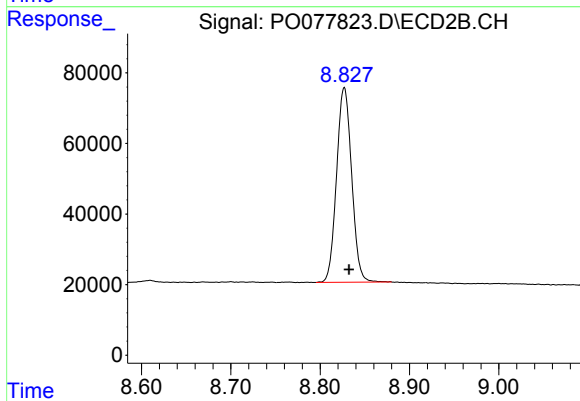

#2 Decachlorobiphenyl


R.T.: 8.827 min
Delta R.T.: -0.005 min
Response: 648396
Conc: 26.98 ng/ml

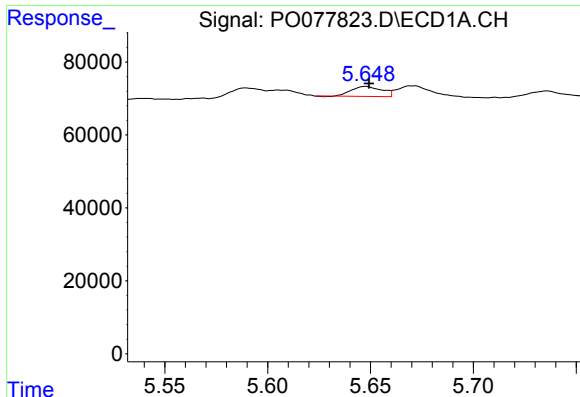

#21 AR-1248-1


R.T.: 5.648 min
Delta R.T.: -0.001 min
Response: 28603
Conc: 24.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

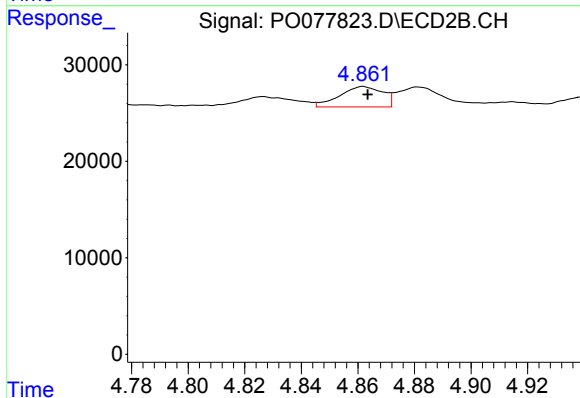


#21 AR-1248-1

R.T.: 4.862 min
Delta R.T.: -0.001 min
Response: 22408
Conc: 39.77 ng/ml

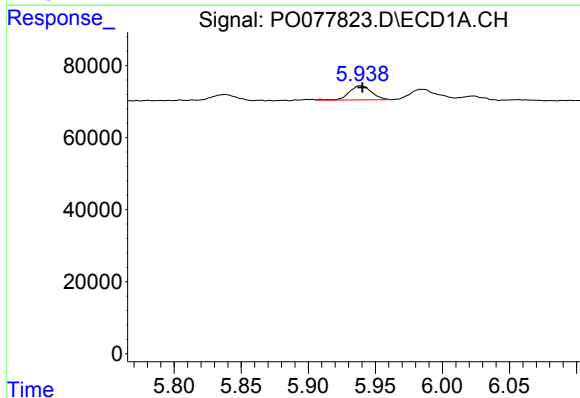


#22 AR-1248-2

R.T.: 5.939 min
Delta R.T.: -0.002 min
Response: 45290
Conc: 28.52 ng/ml

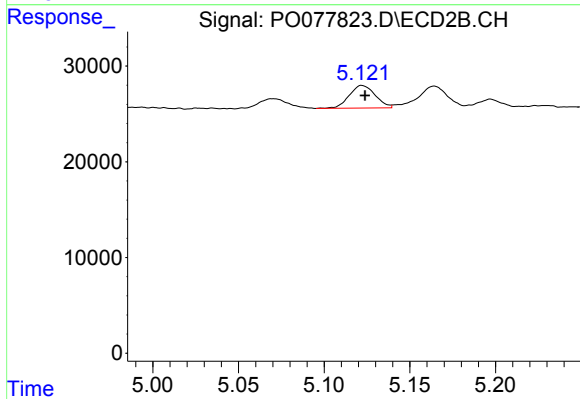

#22 AR-1248-2


R.T.: 5.122 min
Delta R.T.: -0.002 min
Response: 24843
Conc: 31.12 ng/ml

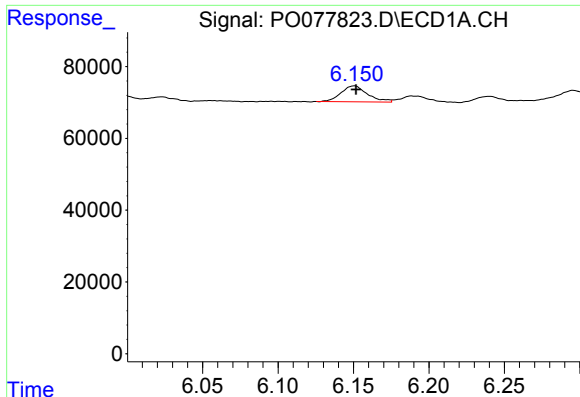

#23 AR-1248-3


R.T.: 6.151 min
Delta R.T.: 0.000 min
Response: 54039
Conc: 29.32 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

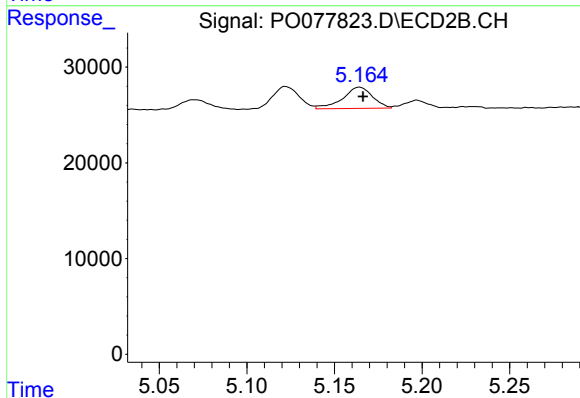


#23 AR-1248-3

R.T.: 5.164 min
Delta R.T.: -0.002 min
Response: 26330
Conc: 32.62 ng/ml

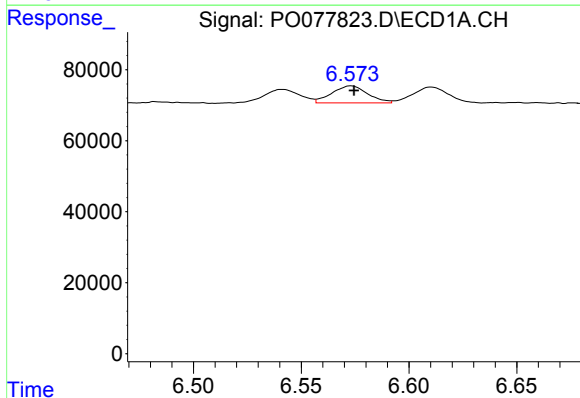


#24 AR-1248-4

R.T.: 6.573 min
Delta R.T.: -0.002 min
Response: 55685
Conc: 28.42 ng/ml

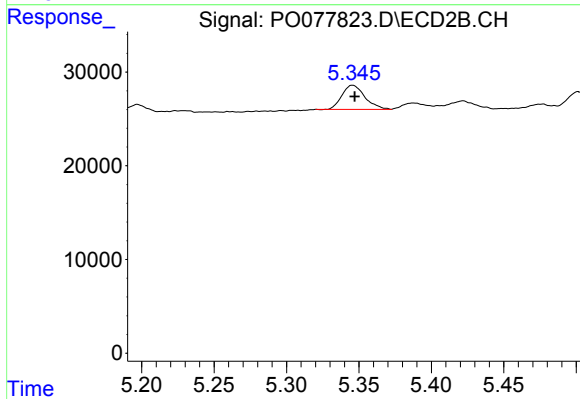

#24 AR-1248-4


R.T.: 5.346 min
Delta R.T.: -0.001 min
Response: 28281
Conc: 29.49 ng/ml

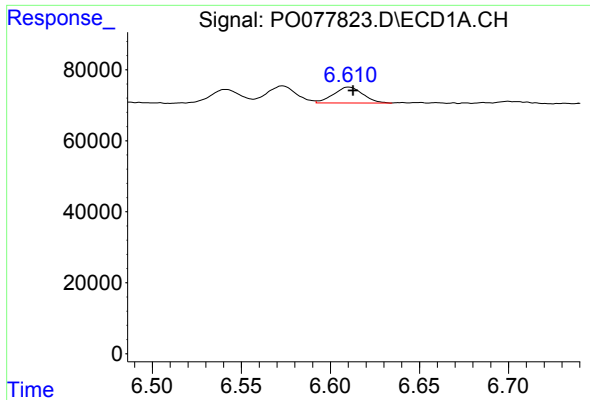

#25 AR-1248-5

R.T.: 6.610 min
Delta R.T.: -0.002 min
Response: 51372
Conc: 26.89 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

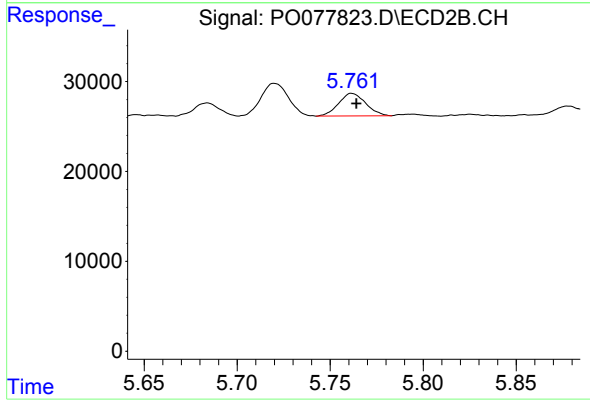

#25 AR-1248-5

R.T.: 5.762 min
Delta R.T.: -0.002 min
Response: 25449
Conc: 27.54 ng/ml