

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077824.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 17:26
 Operator : DD\AJ
 Sample : M2262-09
 Misc : AR1254 MDL 25 PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 17:47:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.351	3.630	1107850	489900	18.873	19.253
2)	SA Decachlor...	9.970	8.826	805776	516683	19.491	21.499
Target Compounds							
26)	L6 AR-1254-1	6.541	5.719	48495	37987	22.858	25.813
27)	L6 AR-1254-2	6.768	5.877	72003	41305	22.151	30.608 #
28)	L6 AR-1254-3	7.143	6.291	73163	61554	22.194	30.384 #
29)	L6 AR-1254-4	7.437	6.529	55072	29280	23.716	23.388
30)	L6 AR-1254-5	7.859	6.951	49109	46476	18.815	24.525 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077824.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 17:26
Operator : DD\AJ
Sample : M2262-09
Misc : AR1254 MDL 25 PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 17:47:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

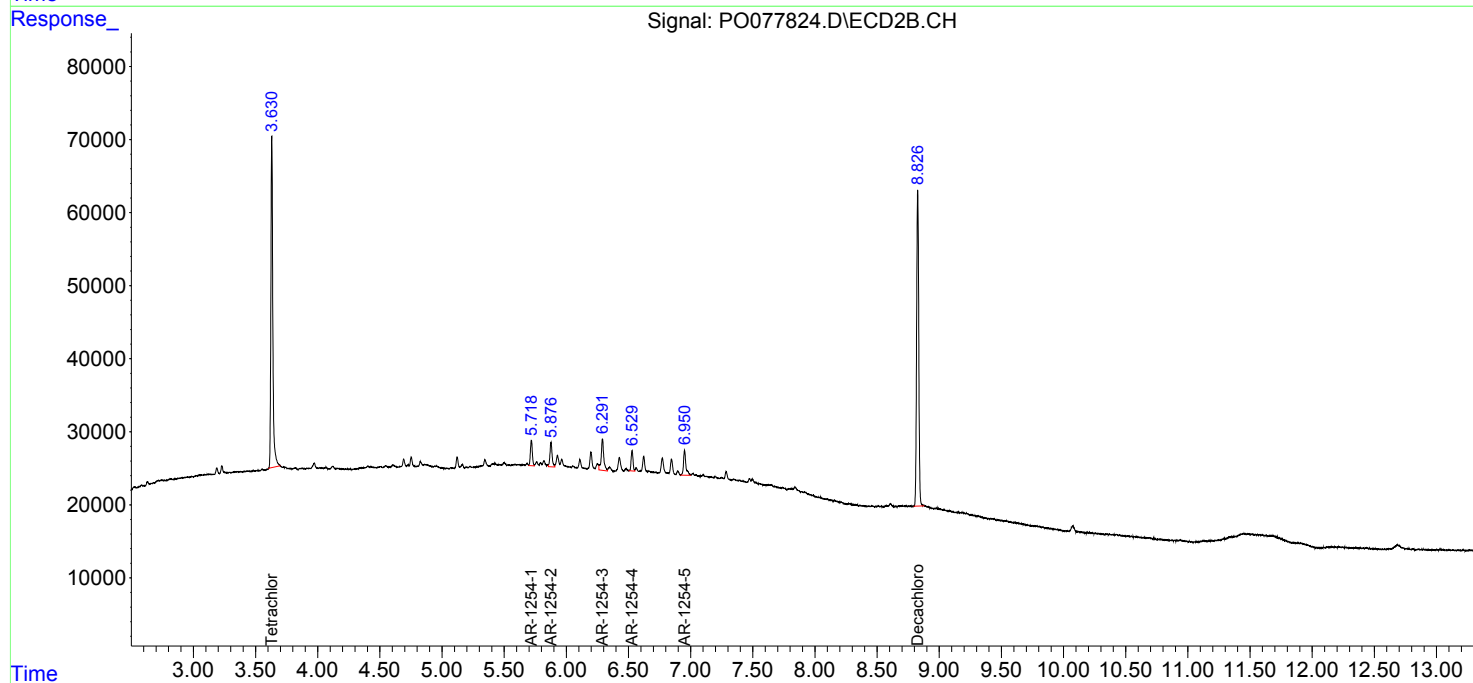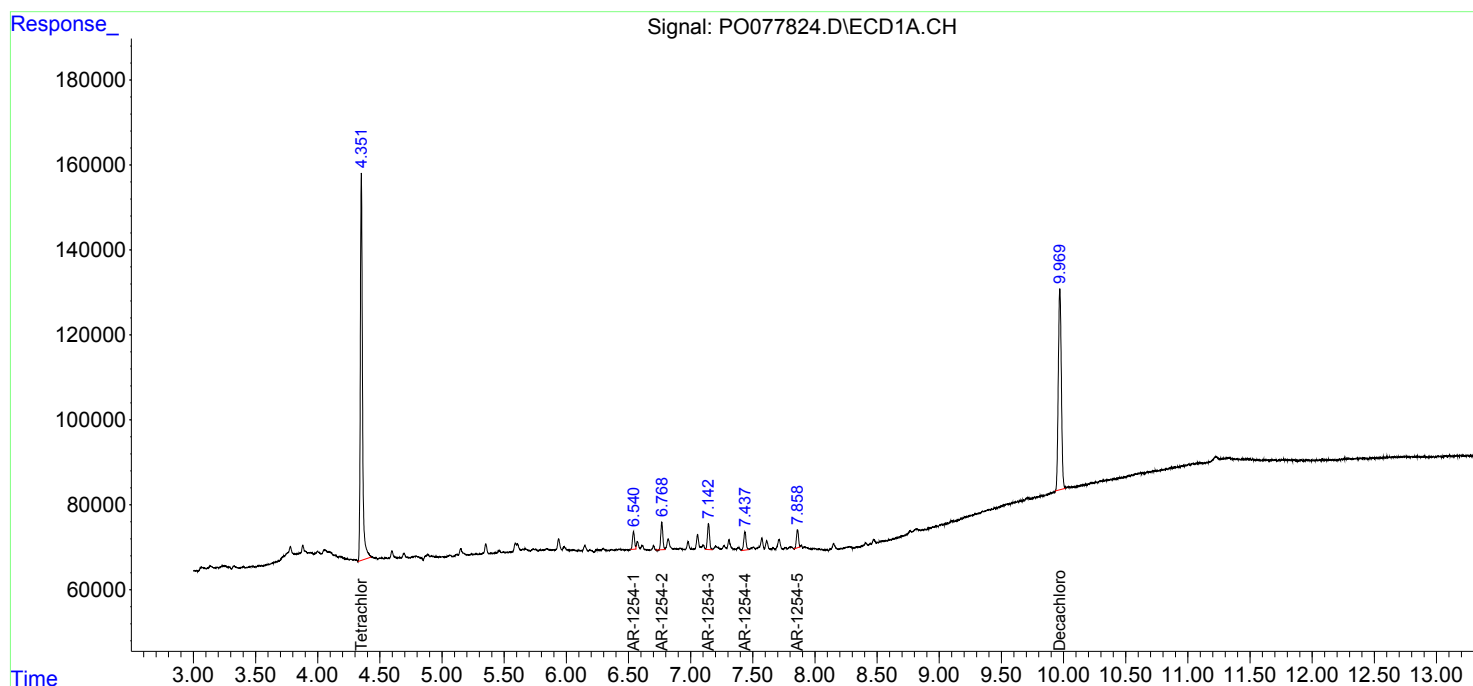


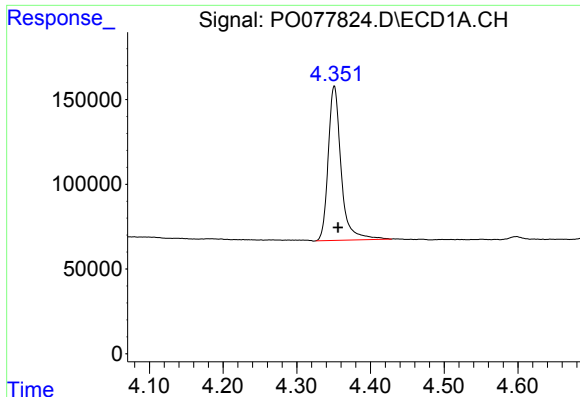

#1 Tetrachloro-m-xylene


R.T.: 4.351 min
Delta R.T.: -0.005 min
Response: 1107850
Conc: 18.87 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

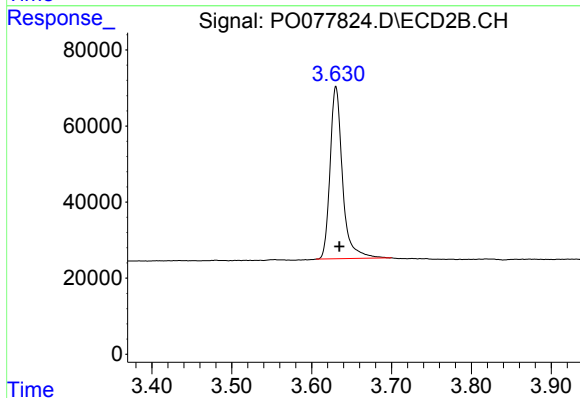


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.004 min
Response: 489900
Conc: 19.25 ng/ml

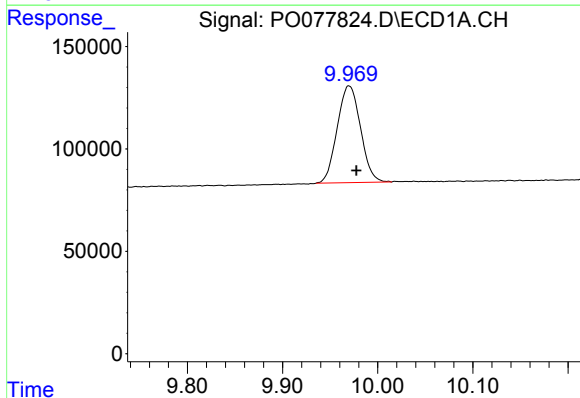


#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.008 min
Response: 805776
Conc: 19.49 ng/ml

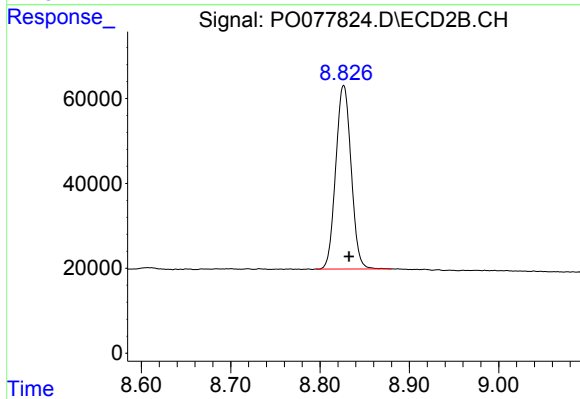

#2 Decachlorobiphenyl


R.T.: 8.826 min
Delta R.T.: -0.006 min
Response: 516683
Conc: 21.50 ng/ml

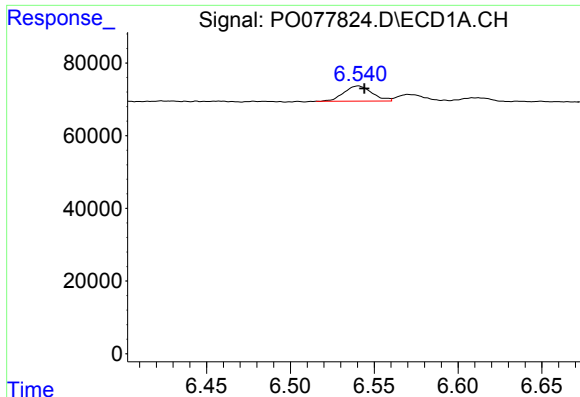

#26 AR-1254-1


R.T.: 6.541 min
Delta R.T.: -0.004 min
Response: 48495
Conc: 22.86 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

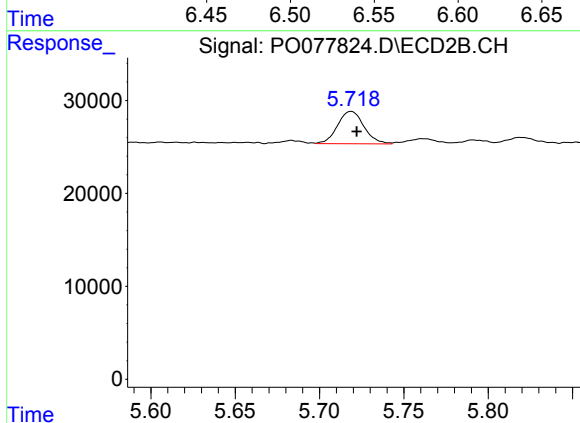


#26 AR-1254-1

R.T.: 5.719 min
Delta R.T.: -0.003 min
Response: 37987
Conc: 25.81 ng/ml

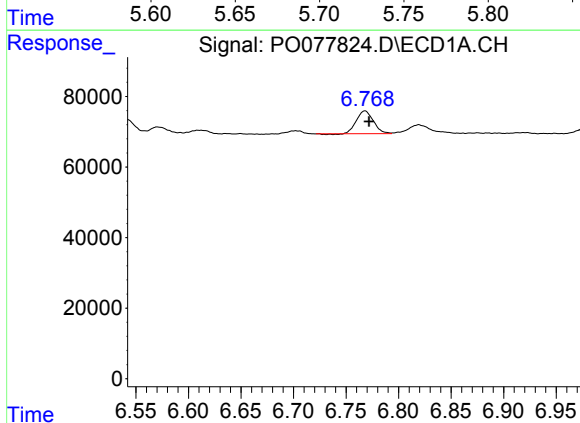


#27 AR-1254-2

R.T.: 6.768 min
Delta R.T.: -0.004 min
Response: 72003
Conc: 22.15 ng/ml

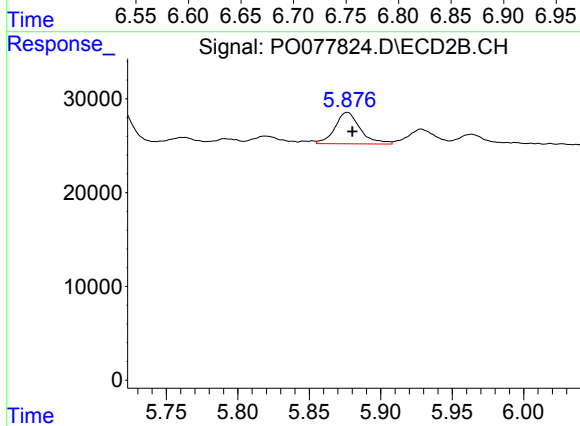

#27 AR-1254-2


R.T.: 5.877 min
Delta R.T.: -0.003 min
Response: 41305
Conc: 30.61 ng/ml

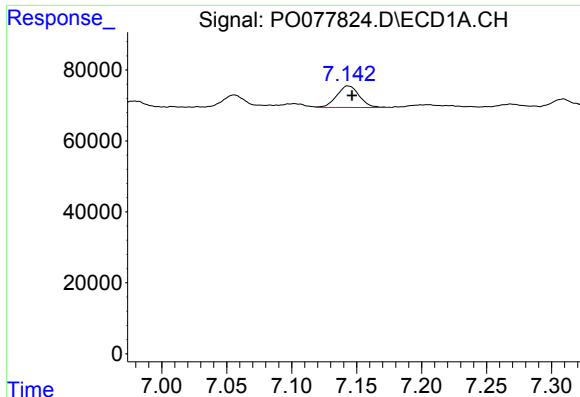

#28 AR-1254-3


R.T.: 7.143 min
Delta R.T.: -0.003 min
Response: 73163
Conc: 22.19 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

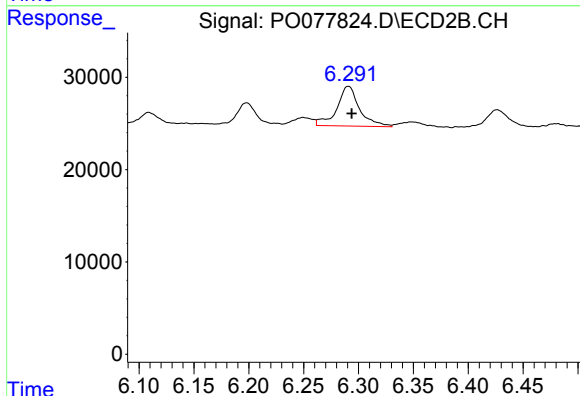


#28 AR-1254-3

R.T.: 6.291 min
Delta R.T.: -0.003 min
Response: 61554
Conc: 30.38 ng/ml

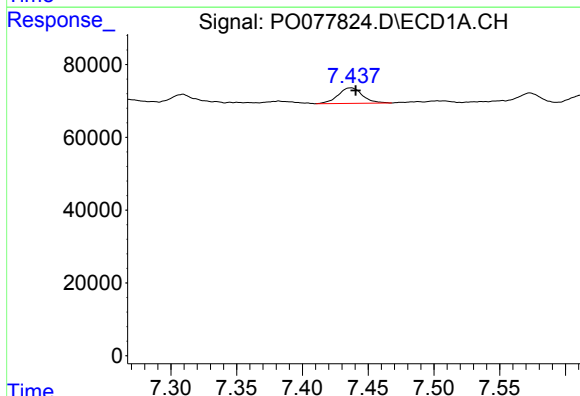


#29 AR-1254-4

R.T.: 7.437 min
Delta R.T.: -0.003 min
Response: 55072
Conc: 23.72 ng/ml

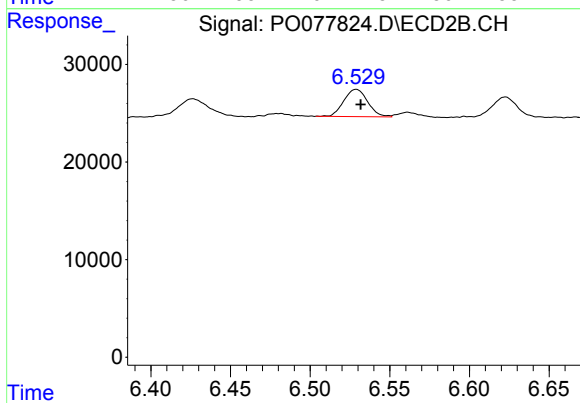

#29 AR-1254-4


R.T.: 6.529 min
Delta R.T.: -0.003 min
Response: 29280
Conc: 23.39 ng/ml

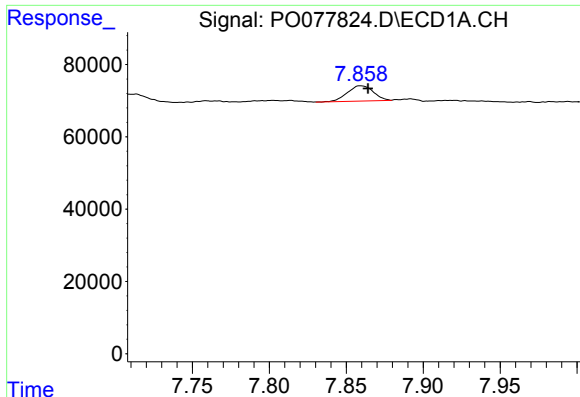

#30 AR-1254-5

R.T.: 7.859 min
Delta R.T.: -0.005 min
Response: 49109
Conc: 18.82 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

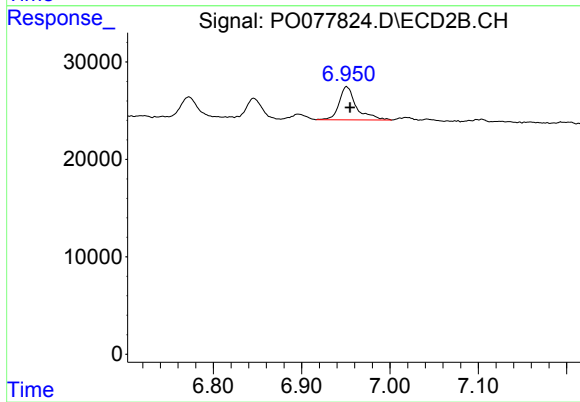

#30 AR-1254-5

R.T.: 6.951 min
Delta R.T.: -0.004 min
Response: 46476
Conc: 24.52 ng/ml