

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077826.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 18:01
 Operator : DD\AJ
 Sample : M2262-09
 Misc : AR1268 MDL 25 PPB
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:01:40 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.353	3.632	1273769	560308	21.699	22.020
2) SA Decachlor...	9.973	8.828	987231	624394	23.880	25.981
Target Compounds						
41) L9 AR-1268-1	8.746	7.783	161383	111400	27.613	30.666
42) L9 AR-1268-2	8.827	7.847	161407	101136	29.246	30.676
43) L9 AR-1268-3	9.010	8.051	124231	89949	27.351	31.416
44) L9 AR-1268-4	9.376	8.341	45864	35539	24.826	29.083
45) L9 AR-1268-5	9.707	8.610	387099	264209	26.312	30.769



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077826.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 18:01
Operator : DD\AJ
Sample : M2262-09
Misc : AR1268 MDL 25 PPB
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:01:40 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

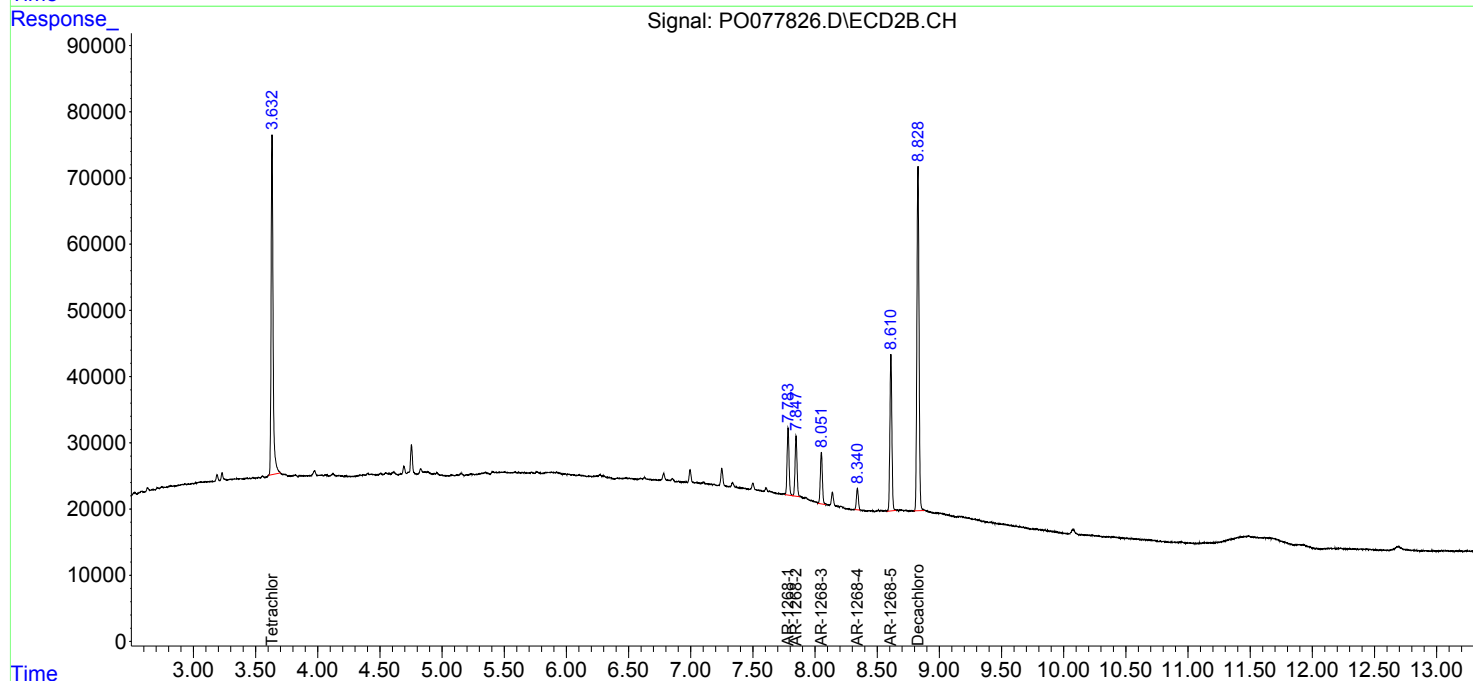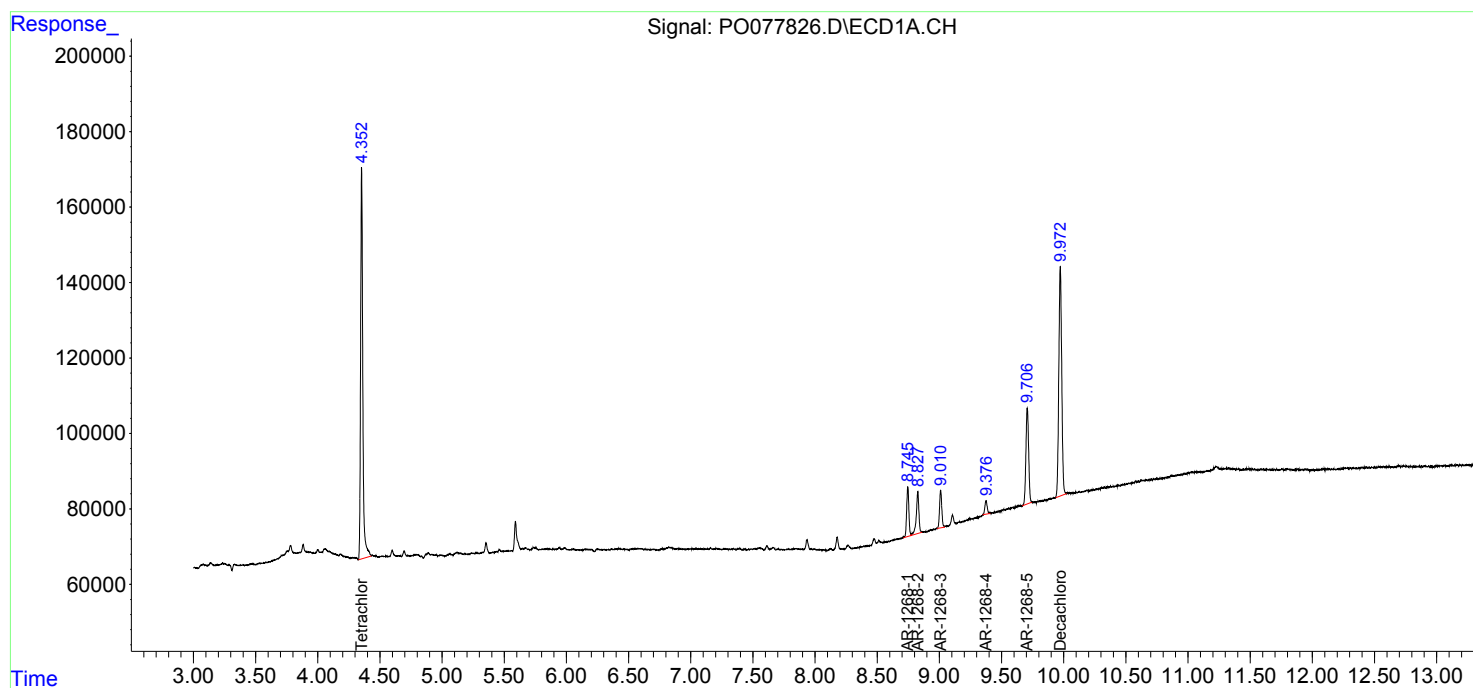


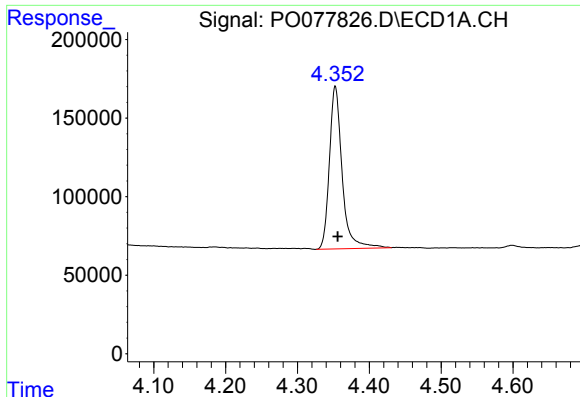

#1 Tetrachloro-m-xylene


R.T.: 4.353 min
Delta R.T.: -0.003 min
Response: 1273769
Conc: 21.70 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

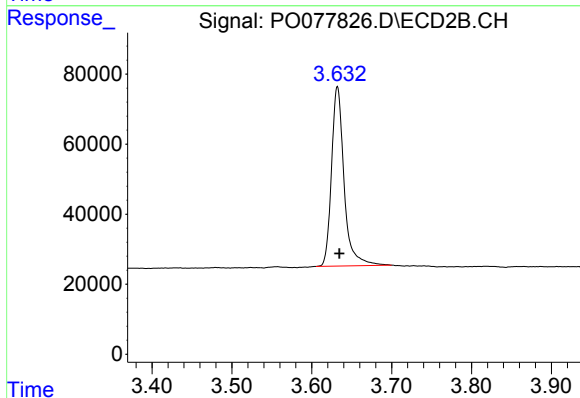


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.002 min
Response: 560308
Conc: 22.02 ng/ml

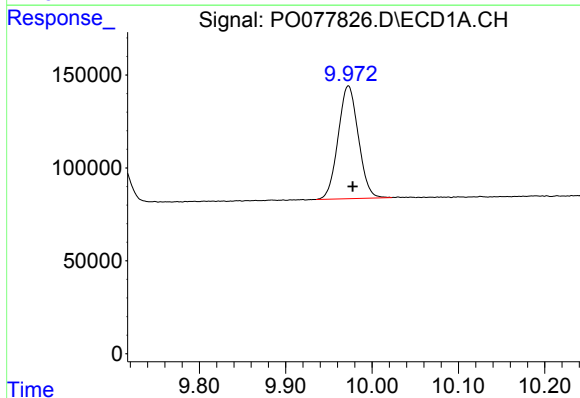


#2 Decachlorobiphenyl

R.T.: 9.973 min
Delta R.T.: -0.005 min
Response: 987231
Conc: 23.88 ng/ml

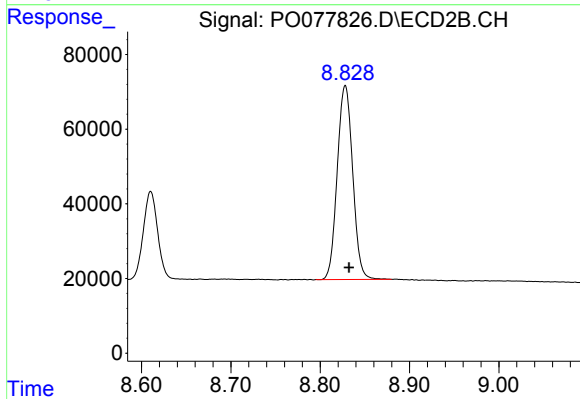

#2 Decachlorobiphenyl


R.T.: 8.828 min
Delta R.T.: -0.004 min
Response: 624394
Conc: 25.98 ng/ml

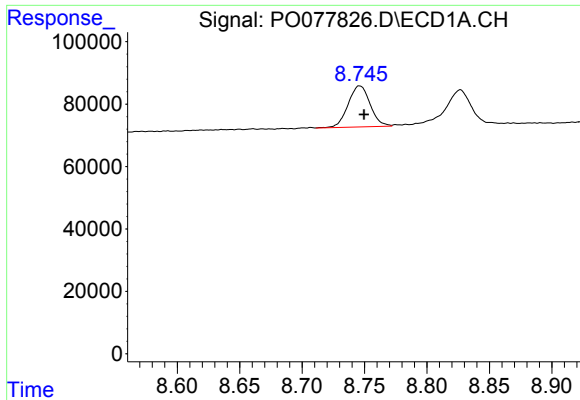

#41 AR-1268-1


R.T.: 8.746 min
Delta R.T.: -0.004 min
Response: 161383
Conc: 27.61 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

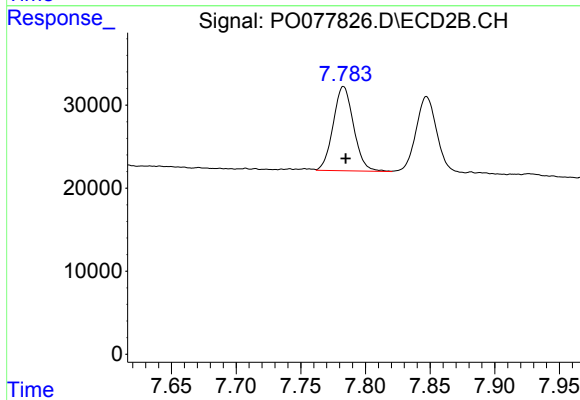


#41 AR-1268-1

R.T.: 7.783 min
Delta R.T.: -0.002 min
Response: 111400
Conc: 30.67 ng/ml

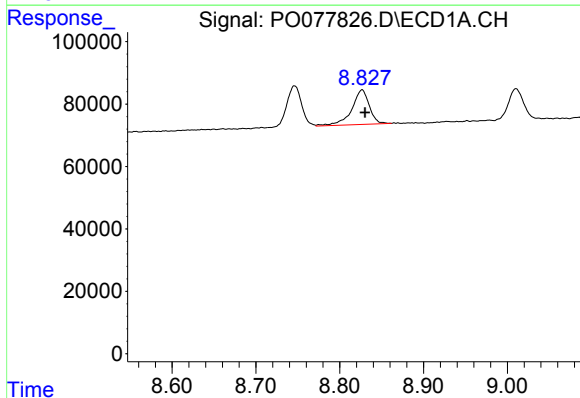


#42 AR-1268-2

R.T.: 8.827 min
Delta R.T.: -0.003 min
Response: 161407
Conc: 29.25 ng/ml

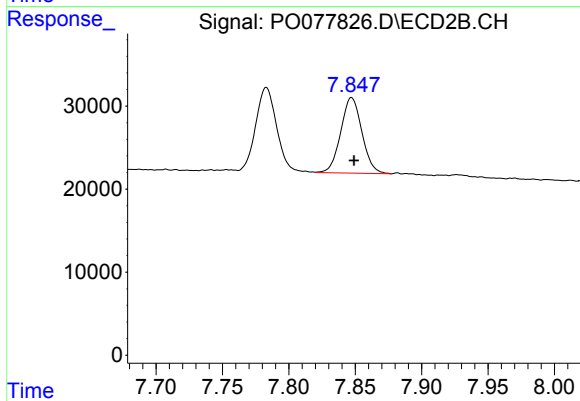

#42 AR-1268-2


R.T.: 7.847 min
Delta R.T.: -0.002 min
Response: 101136
Conc: 30.68 ng/ml

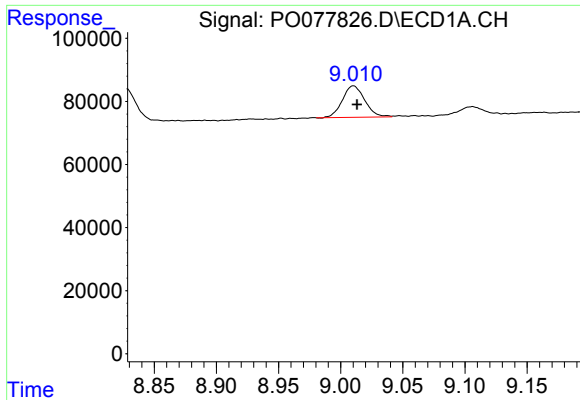

#43 AR-1268-3


R.T.: 9.010 min
Delta R.T.: -0.003 min
Response: 124231
Conc: 27.35 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

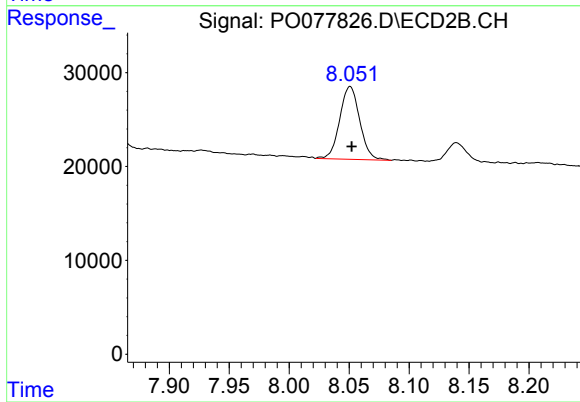


#43 AR-1268-3

R.T.: 8.051 min
Delta R.T.: -0.001 min
Response: 89949
Conc: 31.42 ng/ml

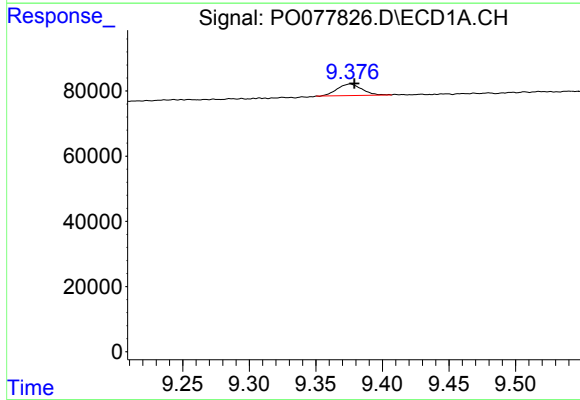


#44 AR-1268-4

R.T.: 9.376 min
Delta R.T.: -0.003 min
Response: 45864
Conc: 24.83 ng/ml

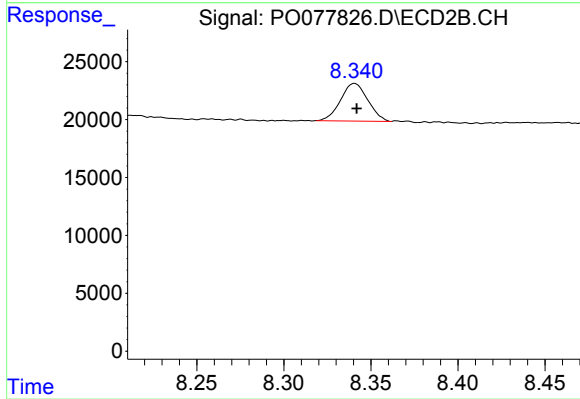

#44 AR-1268-4


R.T.: 8.341 min
Delta R.T.: -0.001 min
Response: 35539
Conc: 29.08 ng/ml

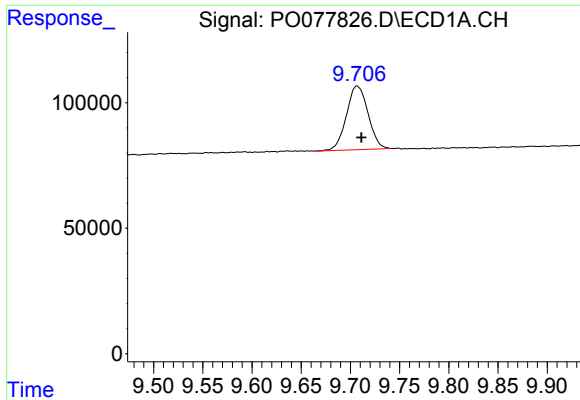

#45 AR-1268-5

R.T.: 9.707 min
Delta R.T.: -0.004 min
Response: 387099
Conc: 26.31 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2021

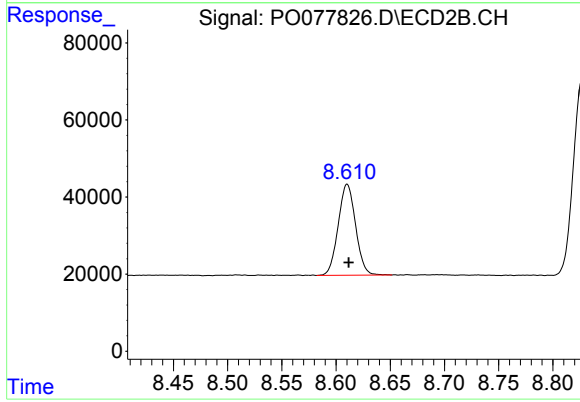

#45 AR-1268-5

R.T.: 8.610 min
Delta R.T.: -0.001 min
Response: 264209
Conc: 30.77 ng/ml