

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077829.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 18:52
 Operator : DD\AJ
 Sample : M2383-07
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KTW-01

Manual Integrations
 APPROVED

Ankita
 5/18/2021 8:55:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:02:55 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.352	3.632	1384617	593328	23.588m	23.318
2) SA Decachlor...	9.972	8.828	911983	575873	22.060	23.962

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077829.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 18:52
Operator : DD\AJ
Sample : M2383-07
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampled :
KTW-01


Manual Integrations
APPROVED

Ankita
5/18/2021 8:55:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:02:55 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

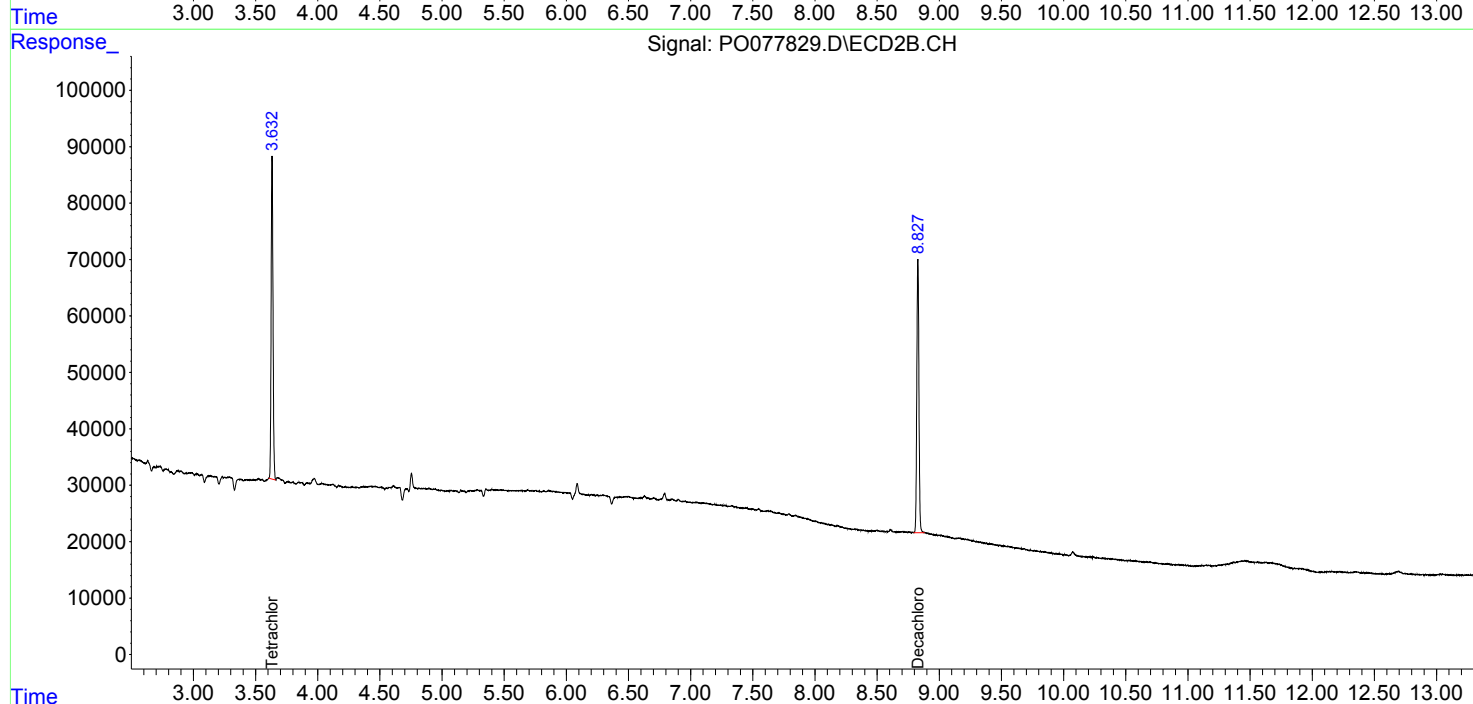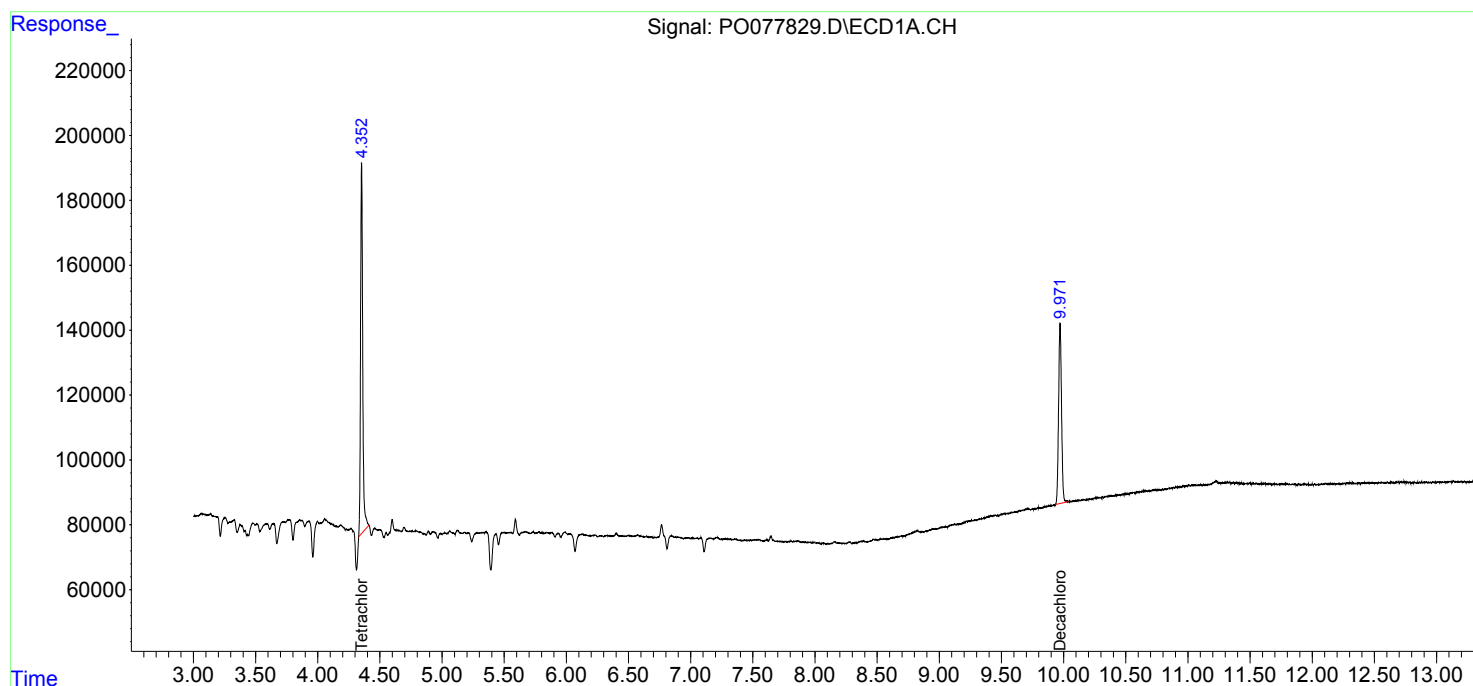

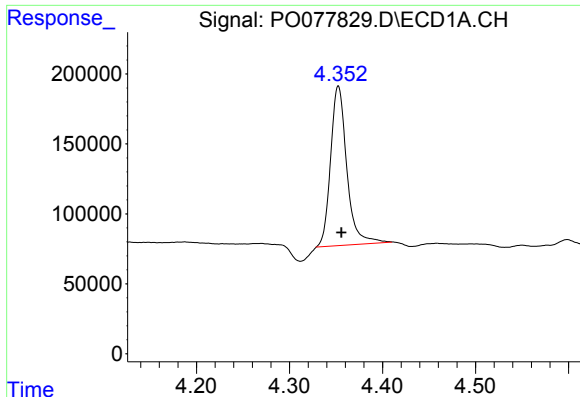


#1 Tetrachloro-m-xylene

R.T.: 4.352 min
Delta R.T.: -0.004 min
Response: 1384617
Conc: 23.59 ng/ml m

Instrument :
ECD_O
ClientSampleId :
KTW-01


Manual Integrations
APPROVED

Ankita
5/18/2021 8:55:48 AM

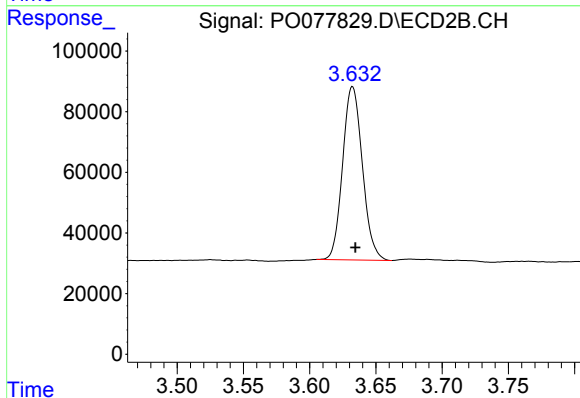


#1 Tetrachloro-m-xylene

R.T.: 3.632 min
Delta R.T.: -0.002 min
Response: 593328
Conc: 23.32 ng/ml

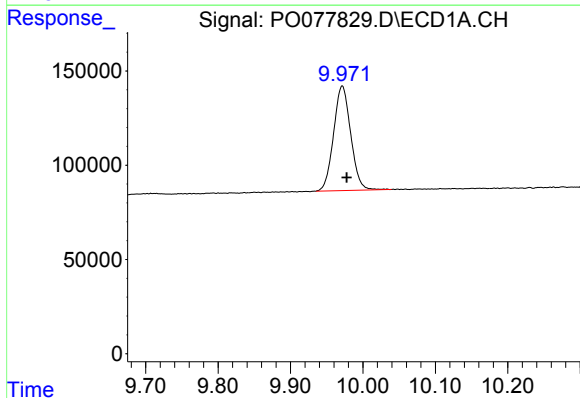

#2 Decachlorobiphenyl

R.T.: 9.972 min
Delta R.T.: -0.006 min
Response: 911983
Conc: 22.06 ng/ml

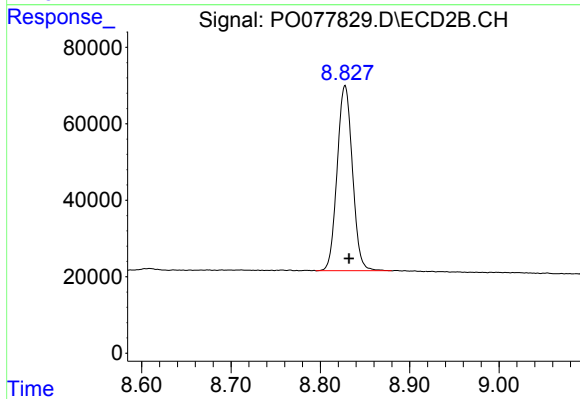

#2 Decachlorobiphenyl

R.T.: 8.828 min
Delta R.T.: -0.005 min
Response: 575873
Conc: 23.96 ng/ml