

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077843.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 14 May 2021 22:53
 Operator : DD\AJ
 Sample : M2383-06
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 DUP-01-05112021

Manual Integrations
 APPROVED

Ankita
 5/18/2021 8:55:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:09:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.365	3.634	5684304	633357	96.836m	24.891 #
2) SA Decachlor...	9.968	8.824	362631	244169	8.772	10.160

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077843.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 14 May 2021 22:53
Operator : DD\AJ
Sample : M2383-06
Misc :
ALS Vial : 37 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
DUP-01-05112021


Manual Integrations
APPROVED

Ankita
5/18/2021 8:55:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:09:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

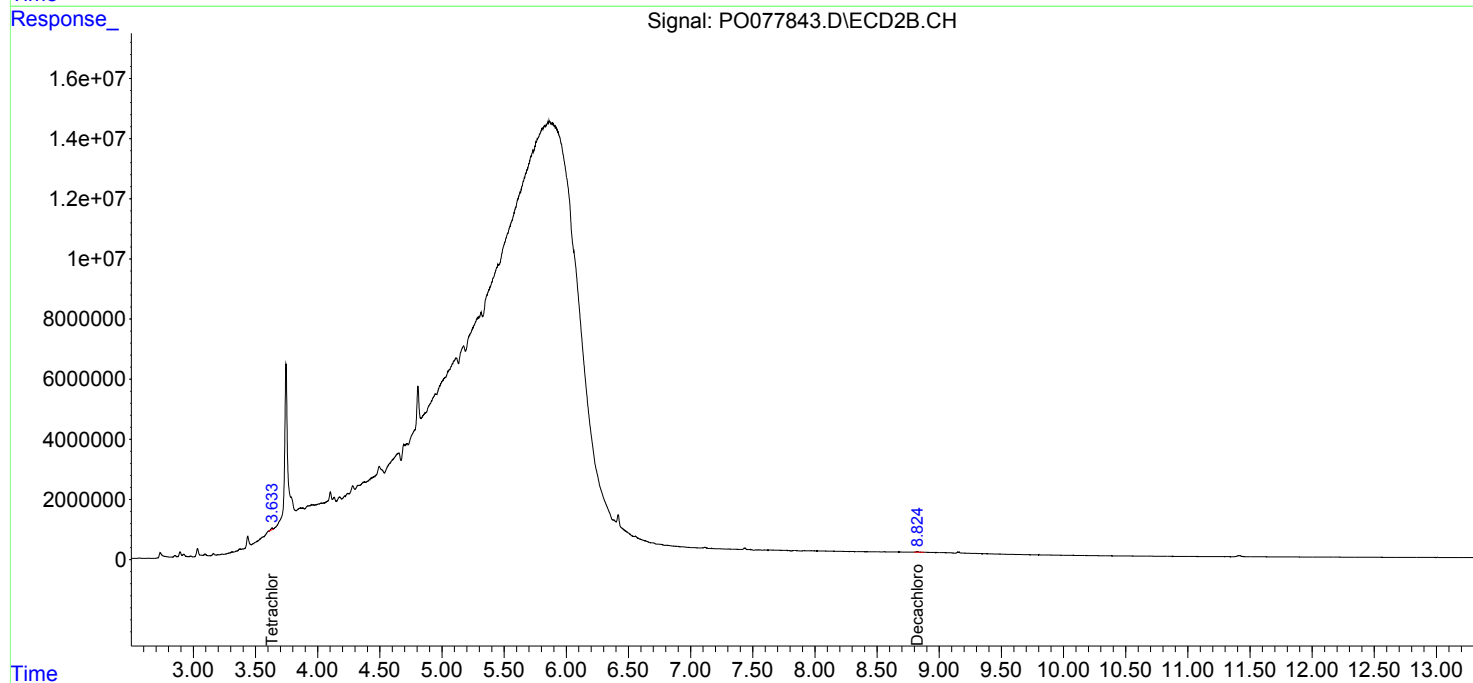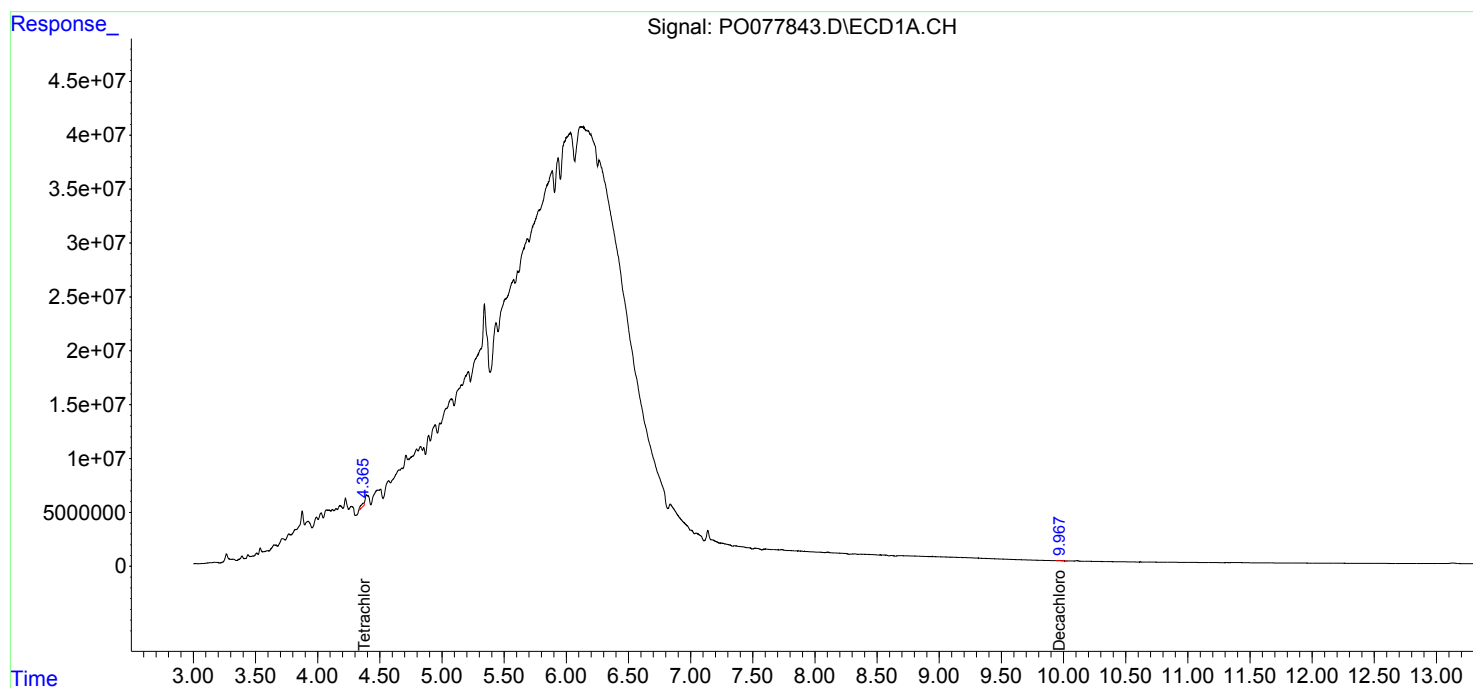

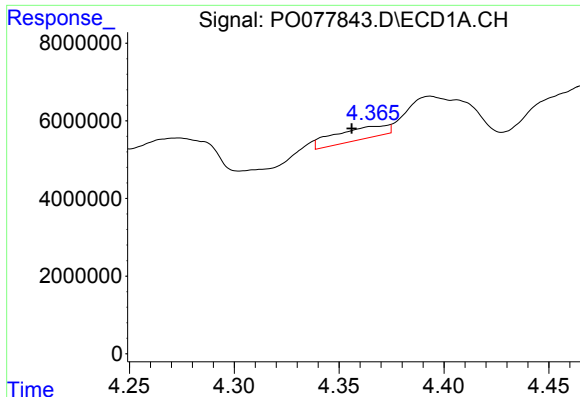


#1 Tetrachloro-m-xylene

R.T.: 4.365 min
Delta R.T.: 0.009 min
Response: 5684304
Conc: 96.84 ng/ml m

Instrument :
ECD_O
ClientSampleId :
DUP-01-05112021


Manual Integrations
APPROVED

Ankita
5/18/2021 8:55:54 AM

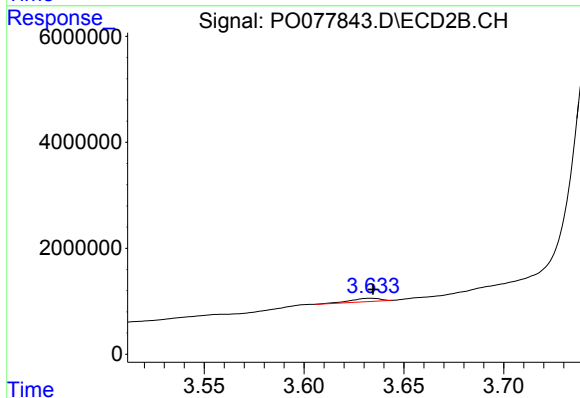


#1 Tetrachloro-m-xylene

R.T.: 3.634 min
Delta R.T.: -0.001 min
Response: 633357
Conc: 24.89 ng/ml

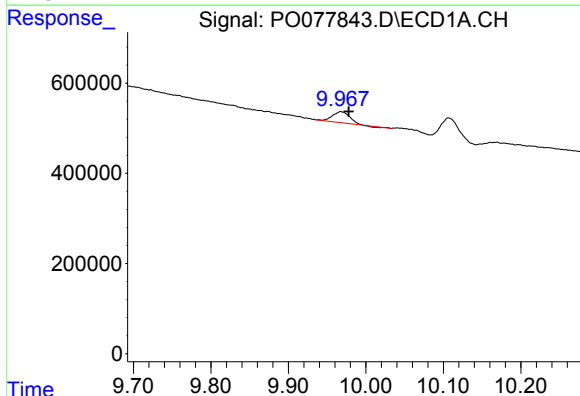

#2 Decachlorobiphenyl

R.T.: 9.968 min
Delta R.T.: -0.010 min
Response: 362631
Conc: 8.77 ng/ml

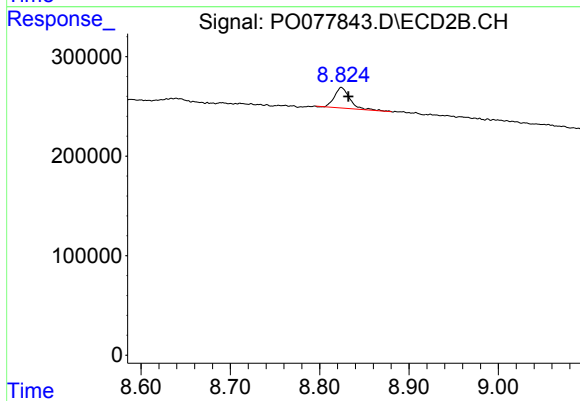

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: -0.008 min
Response: 244169
Conc: 10.16 ng/ml