

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077853.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 May 2021 1:45
 Operator : DD\AJ
 Sample : M2387-10
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 30795

Manual Integrations
 APPROVED

Ankita
 5/18/2021 8:56:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 02:13:54 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.629	973105	369984	16.577	14.540m
2) SA Decachlor...	9.967	8.824	402133	245115	9.727	10.199

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077853.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 May 2021 1:45
Operator : DD\AJ
Sample : M2387-10
Misc :
ALS Vial : 45 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
30795


Manual Integrations
APPROVED

Ankita
5/18/2021 8:56:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 02:13:54 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

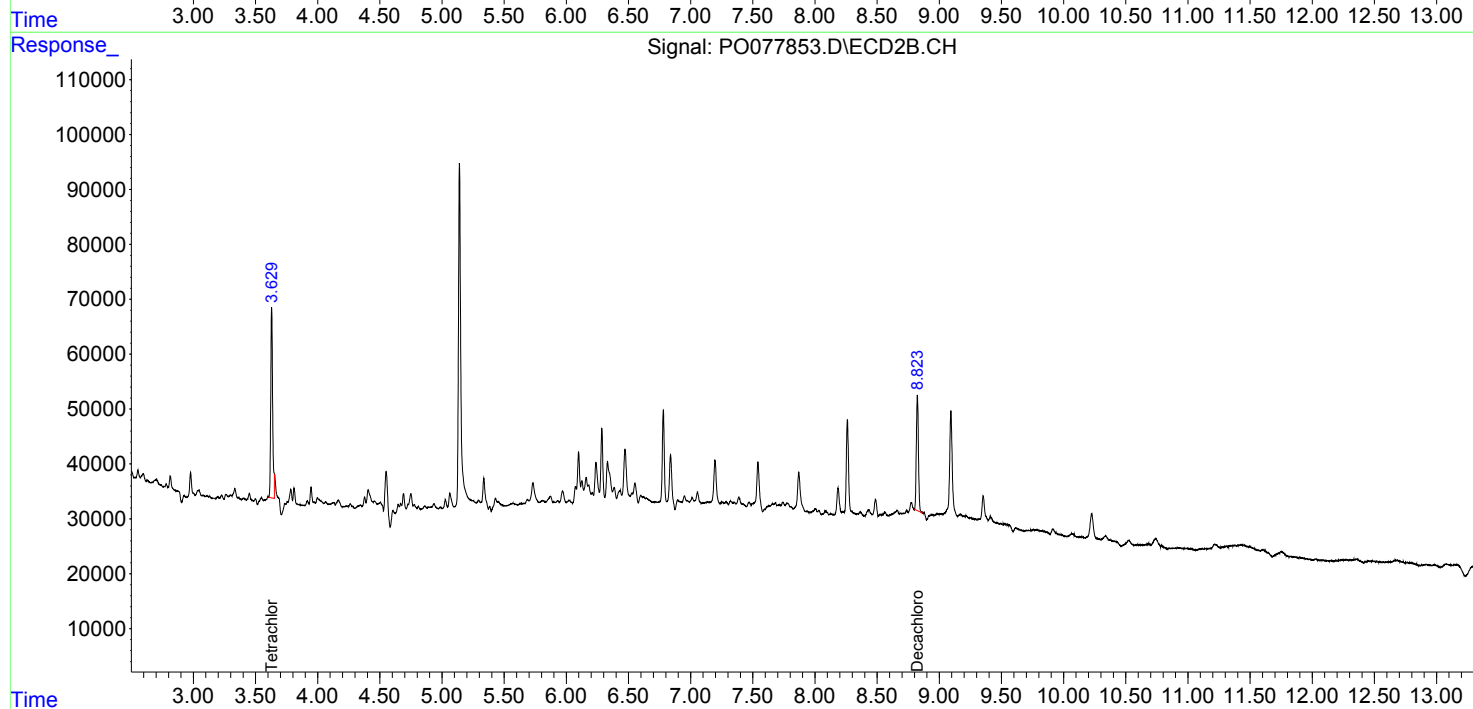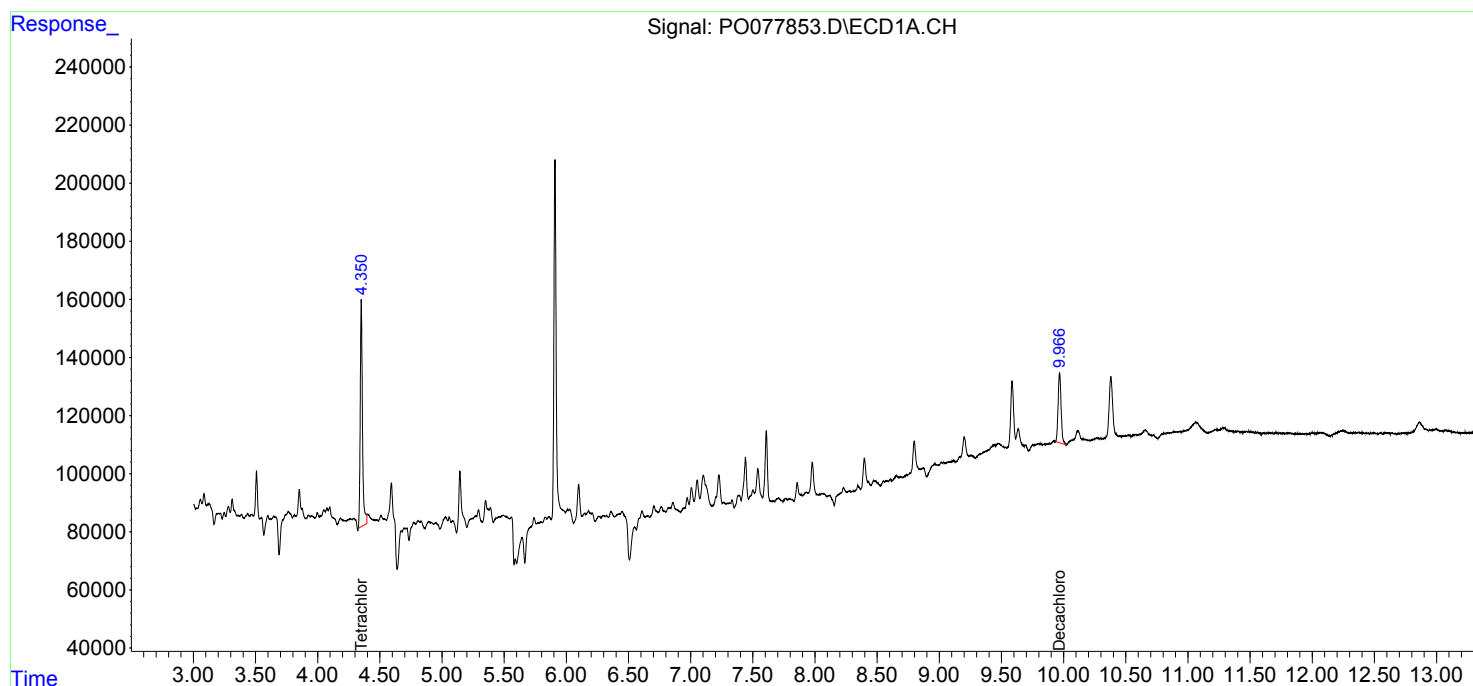

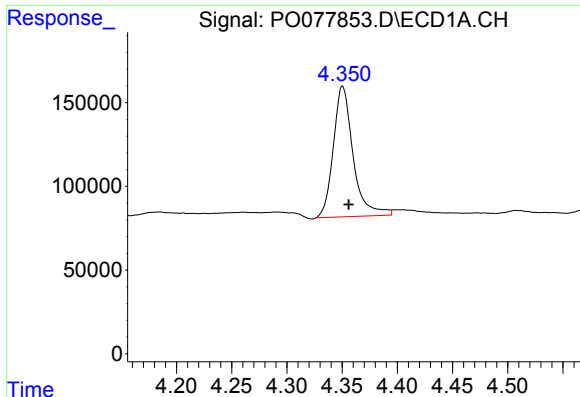


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: -0.006 min
Response: 973105
Conc: 16.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
30795


Manual Integrations
APPROVED

Ankita
5/18/2021 8:56:04 AM

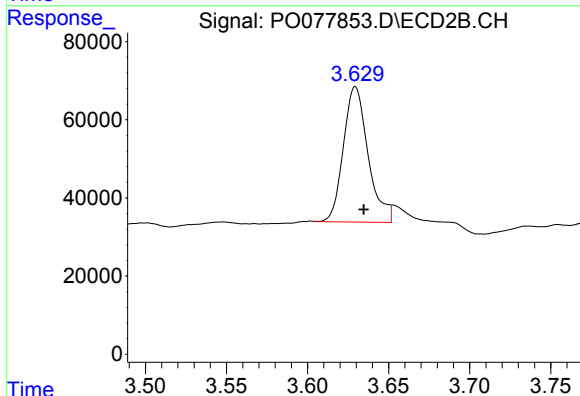


#1 Tetrachloro-m-xylene

R.T.: 3.629 min
Delta R.T.: -0.006 min
Response: 369984
Conc: 14.54 ng/ml m

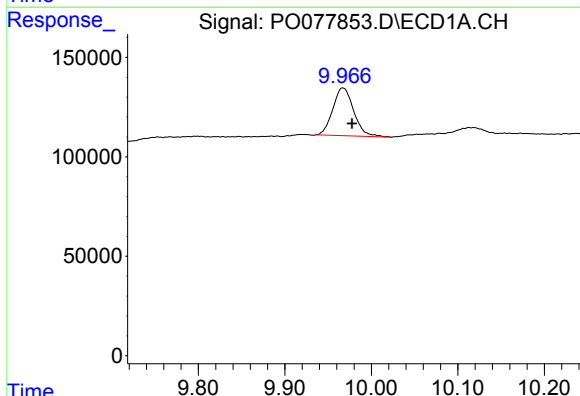

#2 Decachlorobiphenyl

R.T.: 9.967 min
Delta R.T.: -0.010 min
Response: 402133
Conc: 9.73 ng/ml

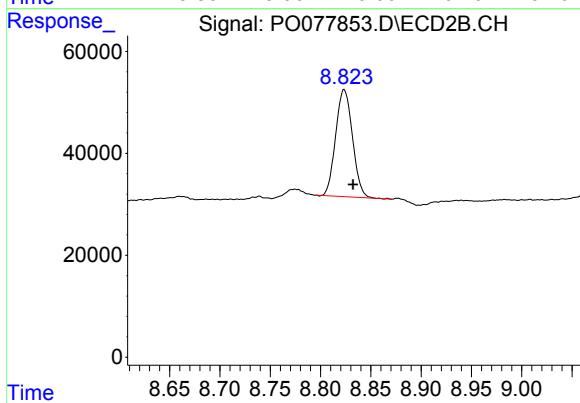

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: -0.009 min
Response: 245115
Conc: 10.20 ng/ml