

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077855.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 May 2021 2:20
 Operator : DD\AJ
 Sample : M2388-12
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 41769

Manual Integrations
 APPROVED

Ankita
 5/18/2021 8:56:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 02:55:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.351	3.631	1523904	683390	25.961m	26.857
2) SA Decachlor...	9.970	8.825	875300	522644	21.173	21.747

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077855.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 May 2021 2:20
Operator : DD\AJ
Sample : M2388-12
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
41769


Manual Integrations
APPROVED

Ankita
5/18/2021 8:56:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 02:55:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

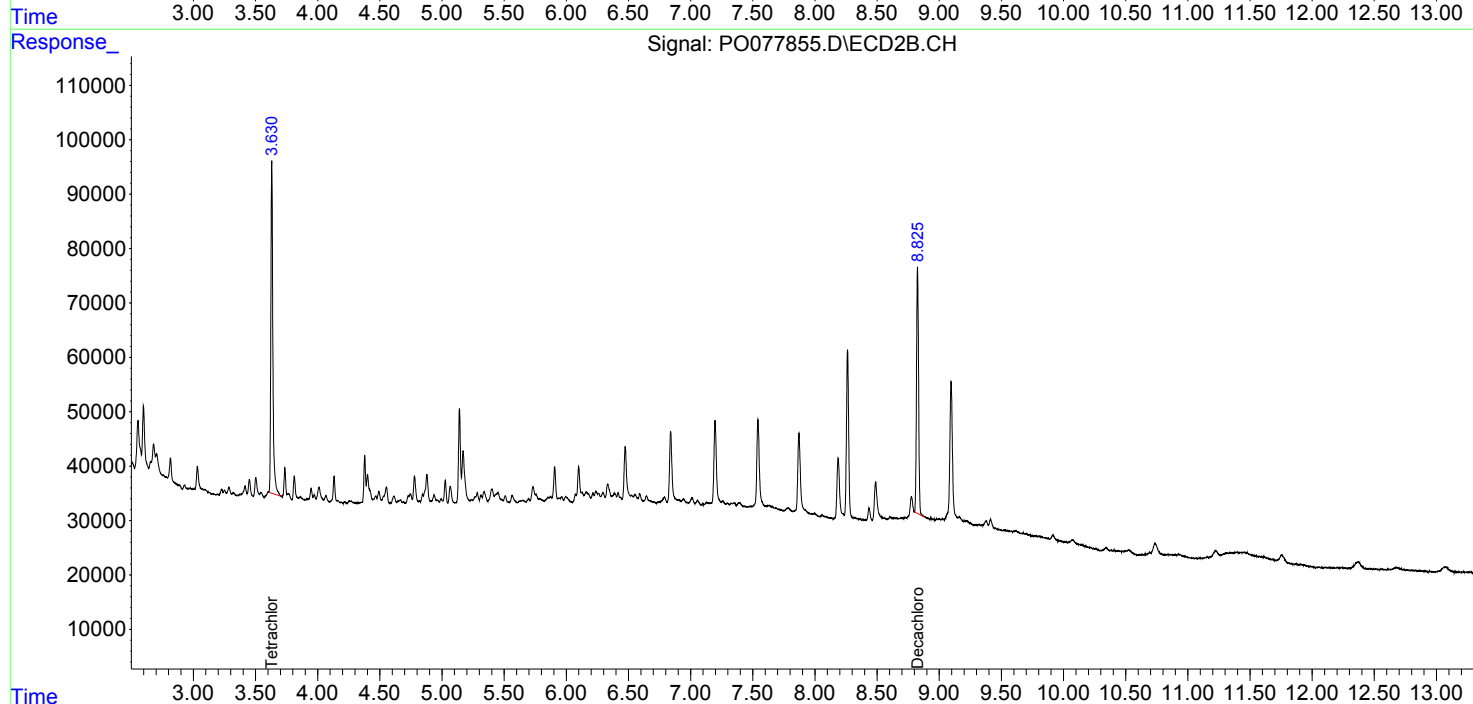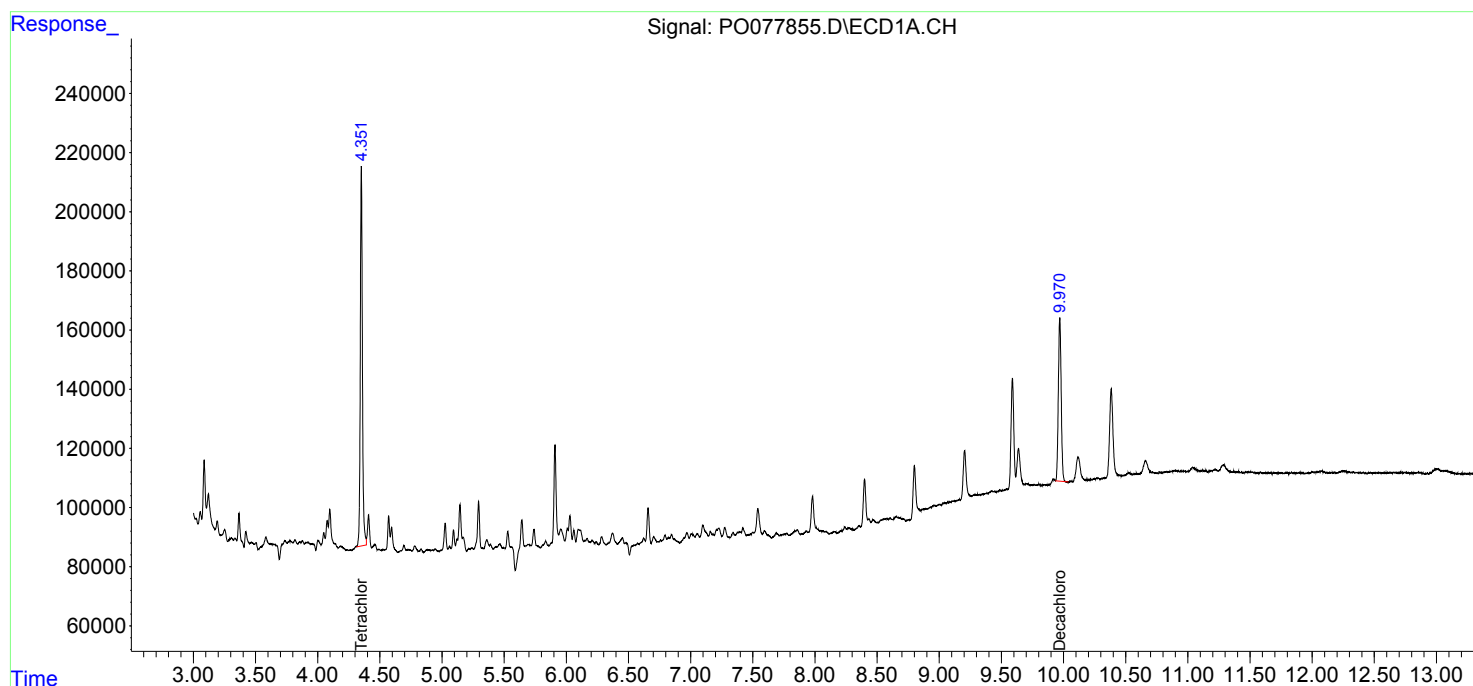

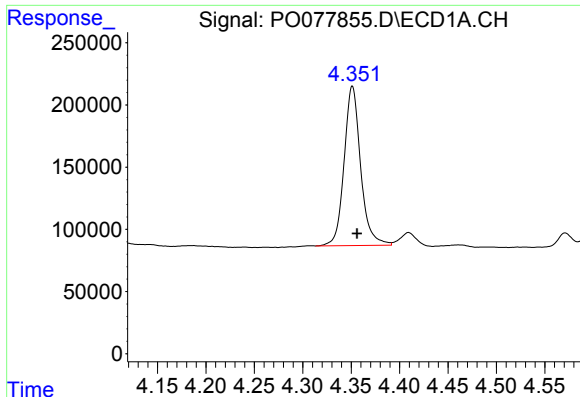


#1 Tetrachloro-m-xylene

R.T.: 4.351 min
Delta R.T.: -0.005 min
Response: 1523904
Conc: 25.96 ng/ml m

Instrument :
ECD_O
ClientSampleId :
41769


Manual Integrations
APPROVED

Ankita
5/18/2021 8:56:08 AM

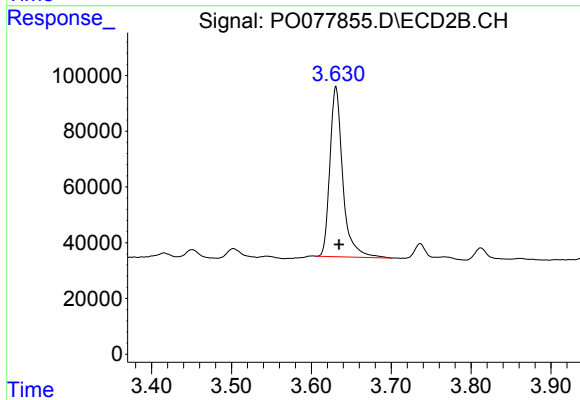


#1 Tetrachloro-m-xylene

R.T.: 3.631 min
Delta R.T.: -0.004 min
Response: 683390
Conc: 26.86 ng/ml

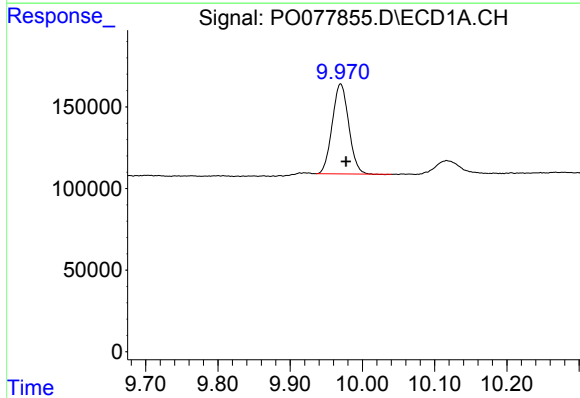

#2 Decachlorobiphenyl

R.T.: 9.970 min
Delta R.T.: -0.008 min
Response: 875300
Conc: 21.17 ng/ml

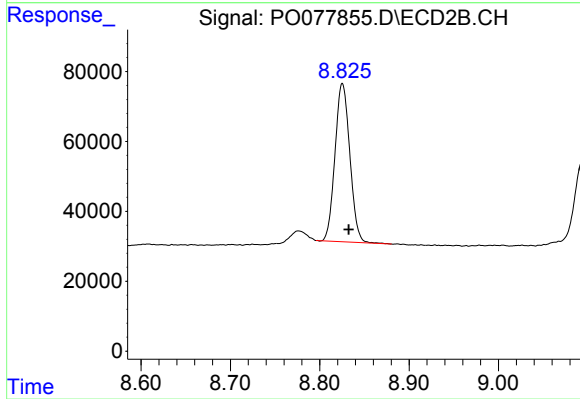

#2 Decachlorobiphenyl

R.T.: 8.825 min
Delta R.T.: -0.007 min
Response: 522644
Conc: 21.75 ng/ml