

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
 Data File : P0077858.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 May 2021 3:12
 Operator : DD\AJ
 Sample : 200 PPB SURR
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 200 PPB SURR

Manual Integrations
 APPROVED

Ankita
 5/18/2021 8:56:36 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 02:57:07 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.350	3.630	13915525	6008825	237.060	236.148
2) SA Decachlor...	9.967	8.824	9077019	5080373	219.565m	211.395

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051421\
Data File : P0077858.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 May 2021 3:12
Operator : DD\AJ
Sample : 200 PPB SURR
Misc :
ALS Vial : 48 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
200 PPB SURR


Manual Integrations
APPROVED

Ankita
5/18/2021 8:56:36 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 02:57:07 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

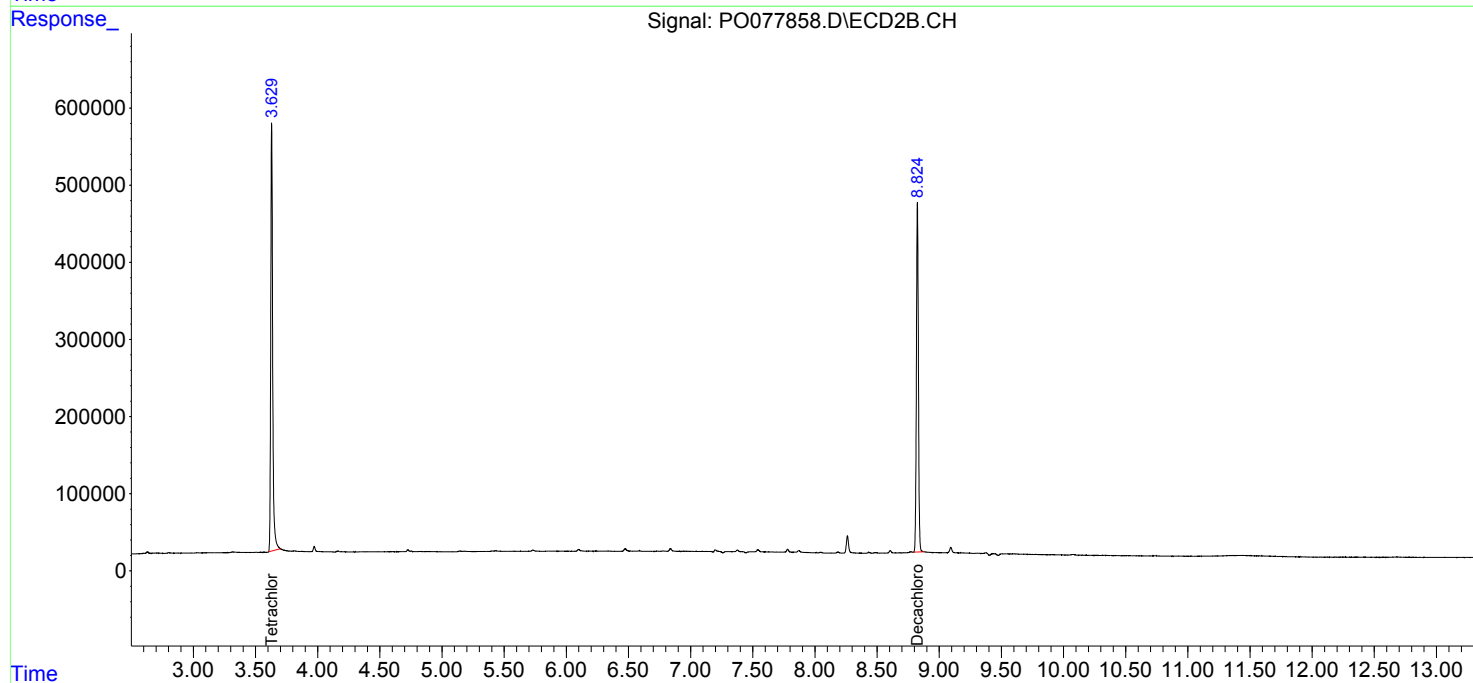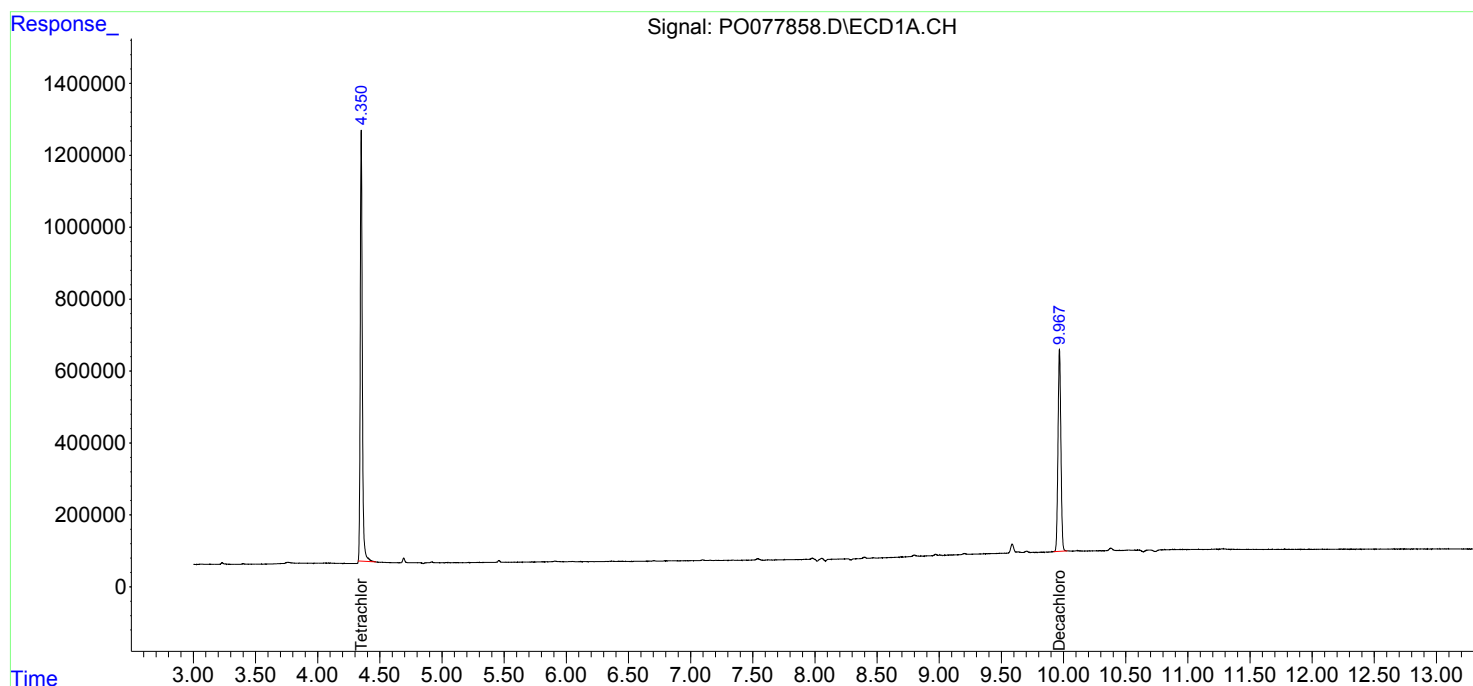

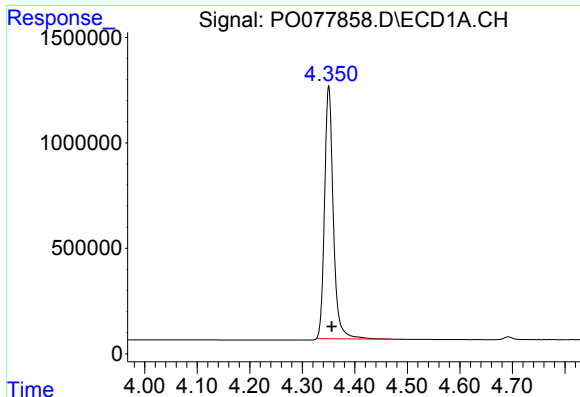


#1 Tetrachloro-m-xylene

R.T.: 4.350 min
Delta R.T.: -0.006 min
Response: 13915525
Conc: 237.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
200 PPB SURR


Manual Integrations
APPROVED

Ankita
5/18/2021 8:56:36 AM

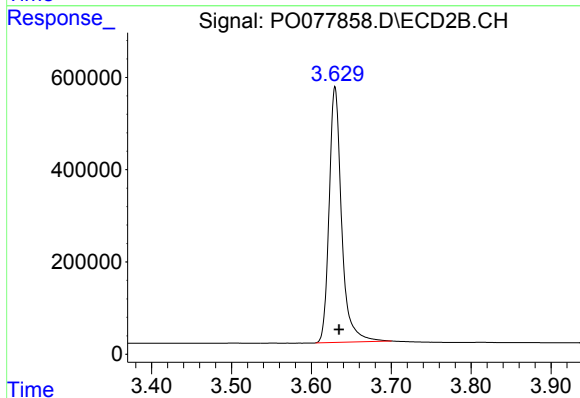


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.005 min
Response: 6008825
Conc: 236.15 ng/ml

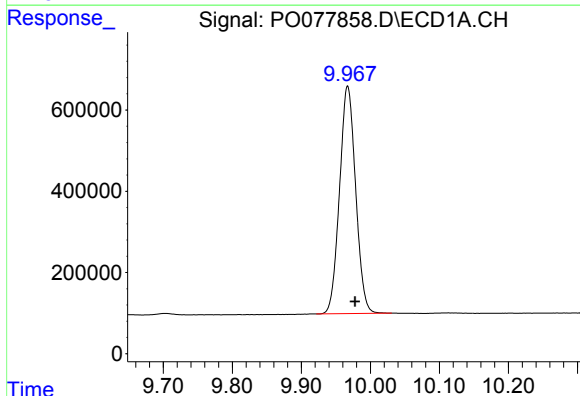

#2 Decachlorobiphenyl

R.T.: 9.967 min
Delta R.T.: -0.011 min
Response: 9077019
Conc: 219.57 ng/ml m

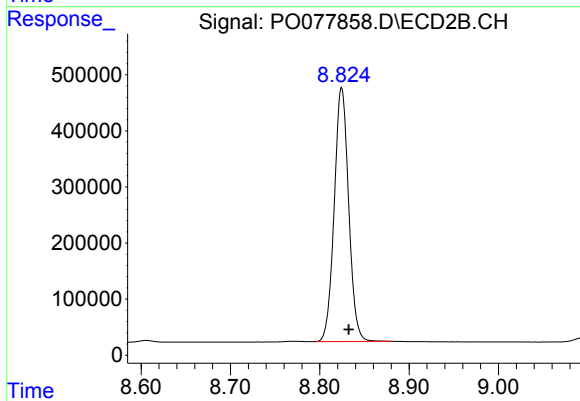

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: -0.008 min
Response: 5080373
Conc: 211.40 ng/ml