

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051422\
 Data File : P0086044.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 May 2022 23:54
 Operator : YP\AJ
 Sample : N2814-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PIPE-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 14 02:16:53 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.479	3.679	2461765	960594	24.242	22.041
2)	SA Decachlor...	10.331	8.742	1521925	821357	28.719	24.199

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051422\
Data File : P0086044.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 May 2022 23:54
Operator : YP\AJ
Sample : N2814-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PIPE-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 14 02:16:53 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

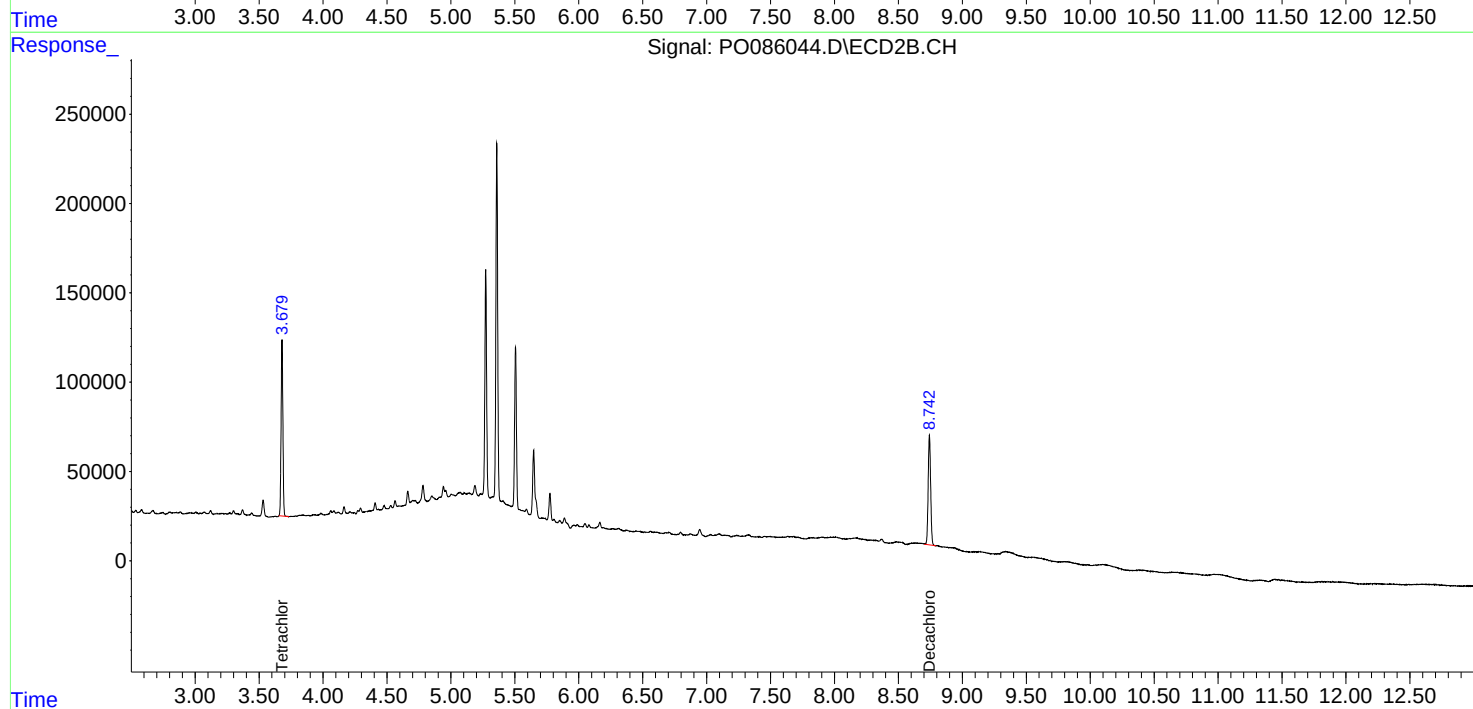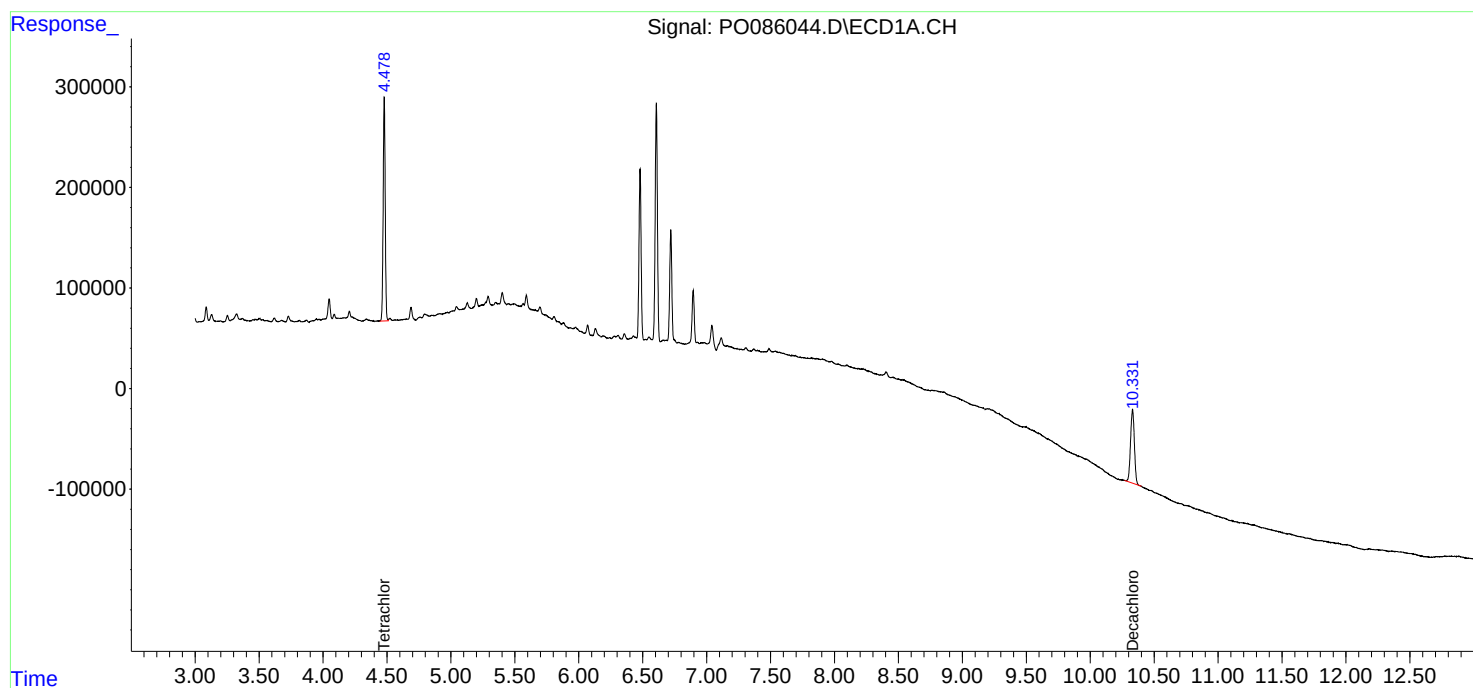


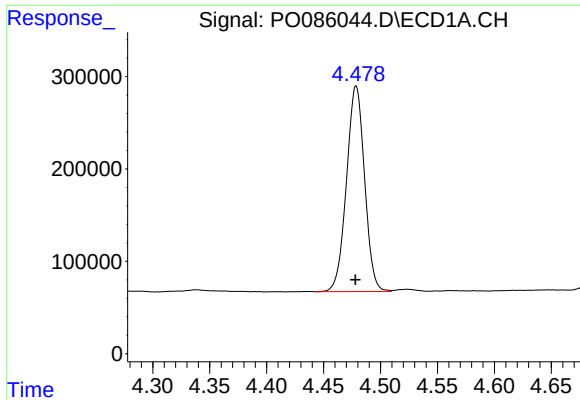

#1 Tetrachloro-m-xylene


R.T.: 4.479 min
Delta R.T.: 0.000 min
Response: 2461765
Conc: 24.24 ng/ml

Instrument :
ECD_O
ClientSampleId :
PIPE-10

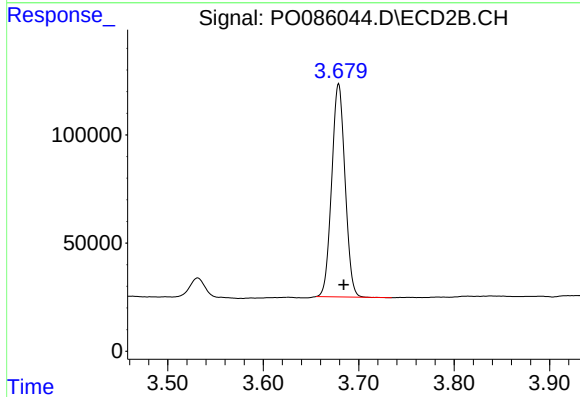


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: -0.005 min
Response: 960594
Conc: 22.04 ng/ml

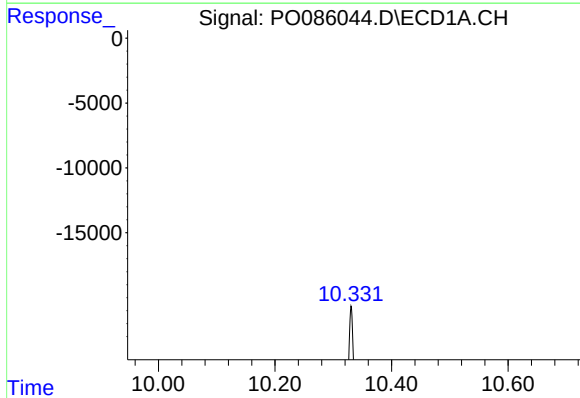

#2 Decachlorobiphenyl

R.T.: 10.331 min
Delta R.T.: 0.004 min
Response: 1521925
Conc: 28.72 ng/ml

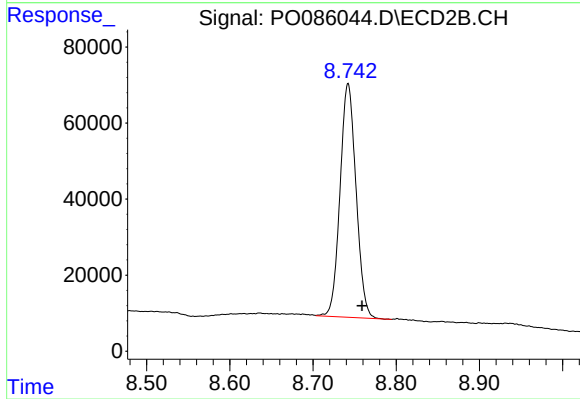

#2 Decachlorobiphenyl

R.T.: 8.742 min
Delta R.T.: -0.017 min
Response: 821357
Conc: 24.20 ng/ml