

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051519\
 Data File : P0056259.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 15 May 2019 15:15
 Operator : SM/SJ
 Sample : K2746-01RE
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 COMP-5.8.19RE

Manual Integrations
 APPROVED

Ankita
 5/16/2019 8:36:11 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 16:02:24 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.261	3.577	922650	866347	30.831	30.674
2) SA Decachlor...	9.848	8.522	1188489	911588	31.763	33.709
Target Compounds						
31) L7 AR-1260-1	7.012	6.114	177228	160632	82.069m	72.909
32) L7 AR-1260-2	7.269	6.300	210841	199698	80.508	65.398m
33) L7 AR-1260-3	7.625	6.453	103313	142507	51.657	57.185m
34) L7 AR-1260-4	7.848	6.921	143386	84231	62.002	40.820m#
35) L7 AR-1260-5	8.159	7.163	204579	244053	48.223	48.594m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051519\
Data File : P0056259.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 May 2019 15:15
Operator : SM/SJ
Sample : K2746-01RE
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19RE


Manual Integrations
APPROVED

Ankita
5/16/2019 8:36:11 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 16:02:24 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

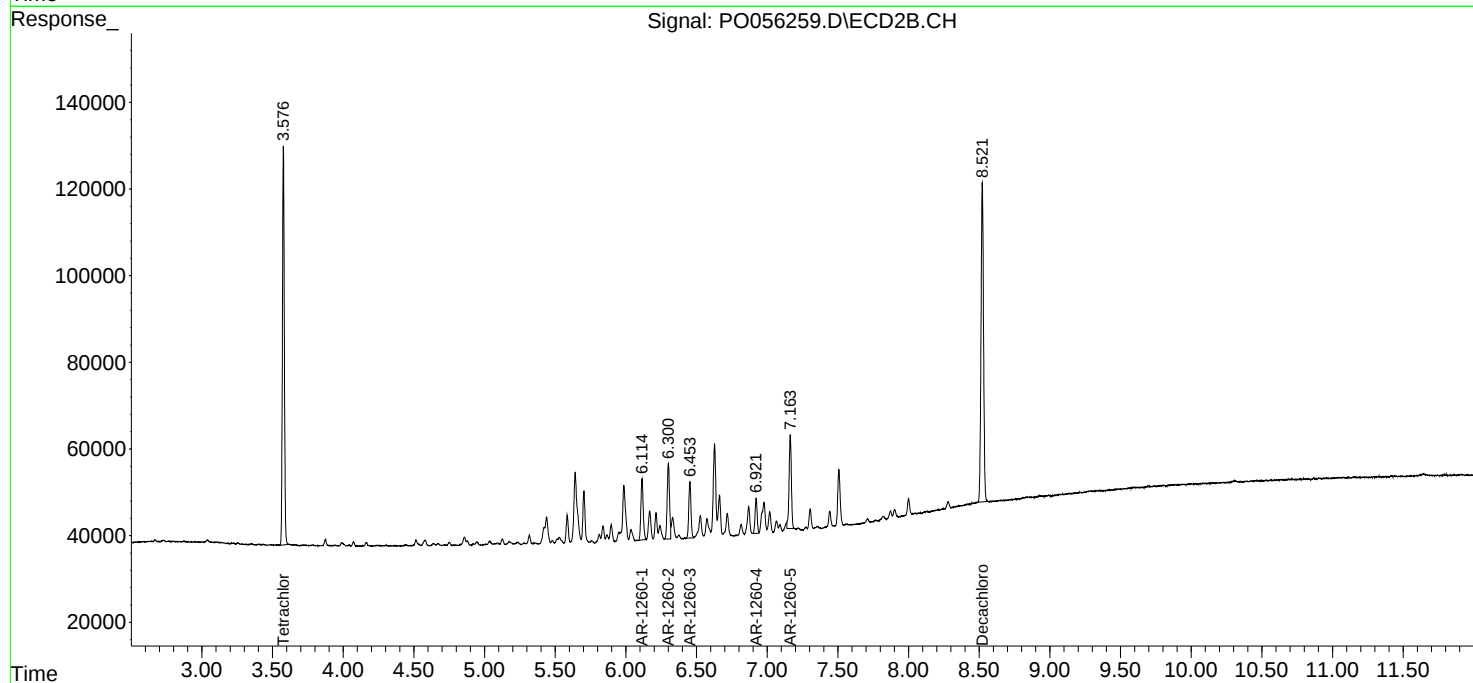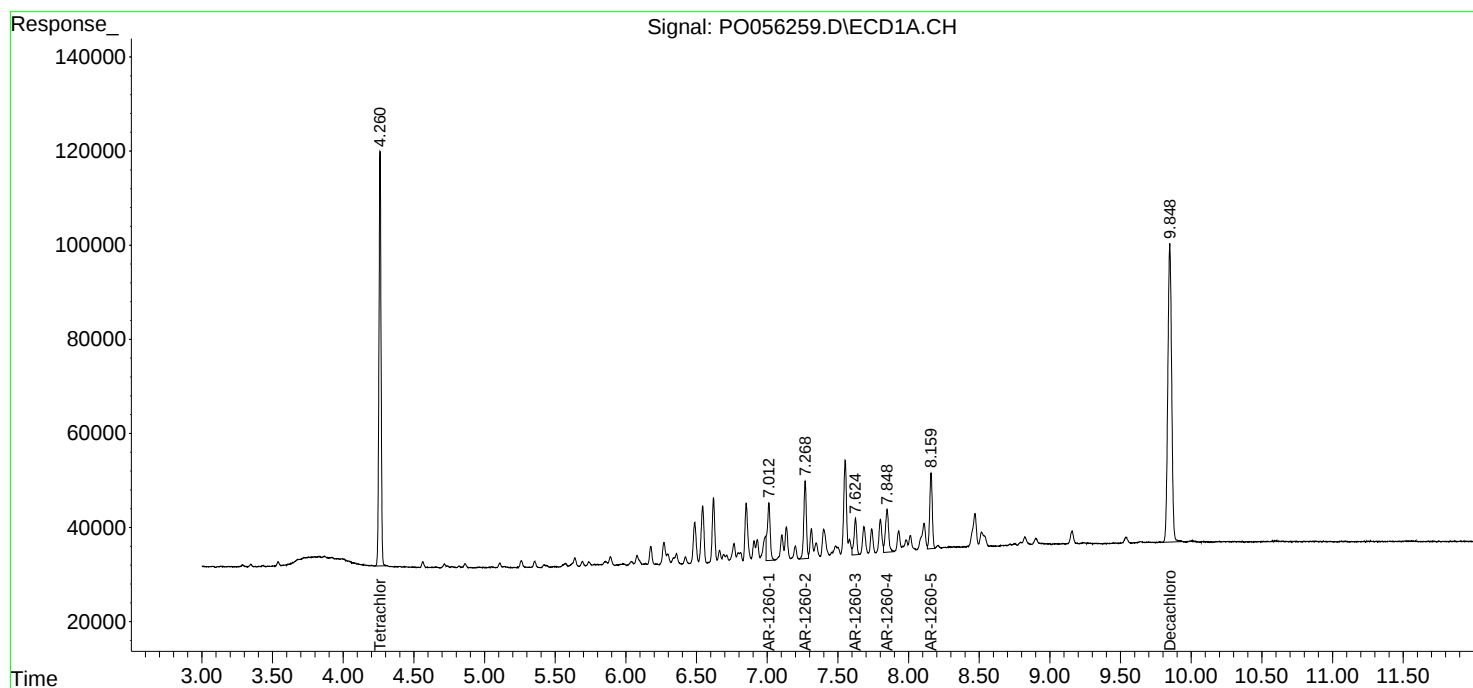

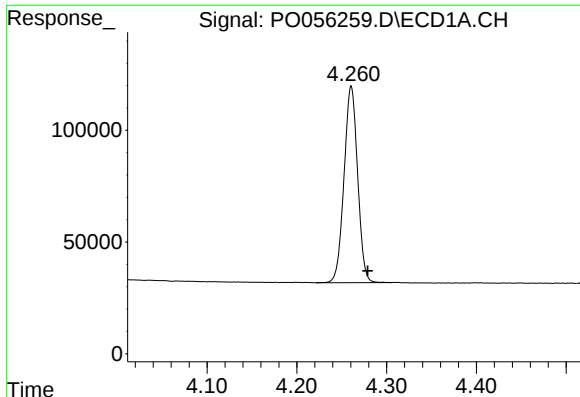


#1 Tetrachloro-m-xylene

R.T.: 4.261 min
Delta R.T.: -0.018 min
Response: 922650
Conc: 30.83 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19RE


Manual Integrations
APPROVED

Ankita
5/16/2019 8:36:11 AM

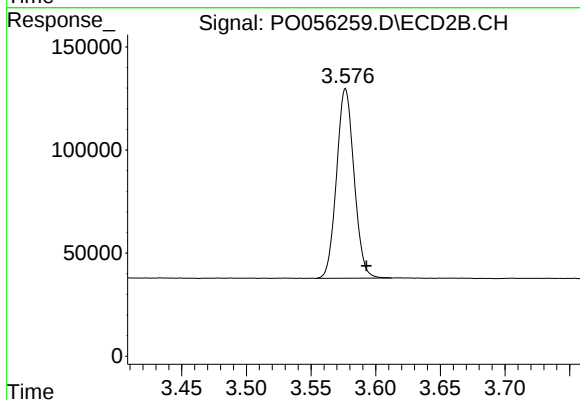


#1 Tetrachloro-m-xylene

R.T.: 3.577 min
Delta R.T.: -0.016 min
Response: 866347
Conc: 30.67 ng/ml

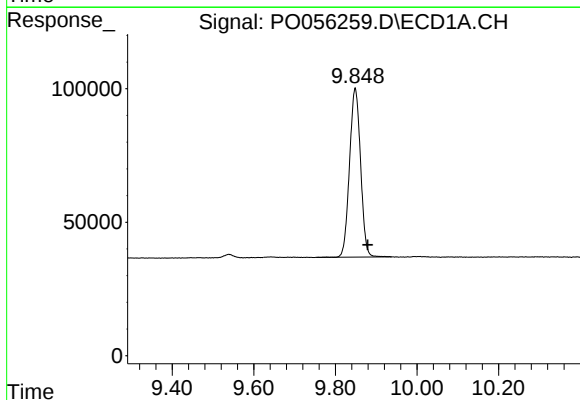


#2 Decachlorobiphenyl

R.T.: 9.848 min
Delta R.T.: -0.031 min
Response: 1188489
Conc: 31.76 ng/ml

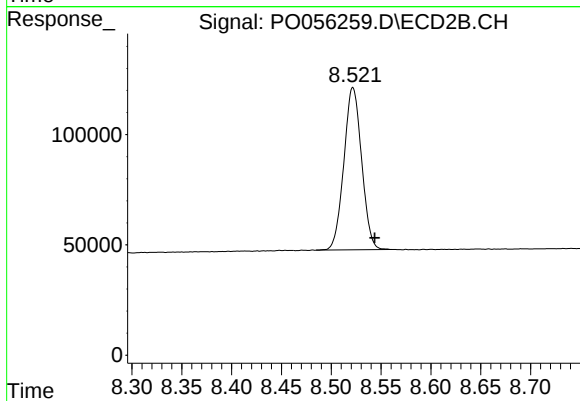

#2 Decachlorobiphenyl

R.T.: 8.522 min
Delta R.T.: -0.022 min
Response: 911588
Conc: 33.71 ng/ml

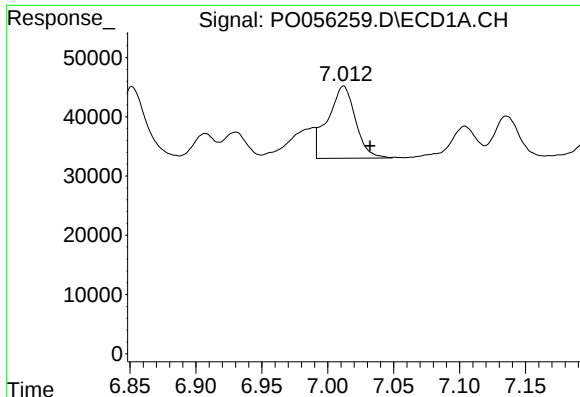


#31 AR-1260-1

R.T.: 7.012 min
Delta R.T.: -0.021 min
Response: 177228
Conc: 82.07 ng/ml m

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19RE


Manual Integrations
APPROVED

Ankita
5/16/2019 8:36:11 AM

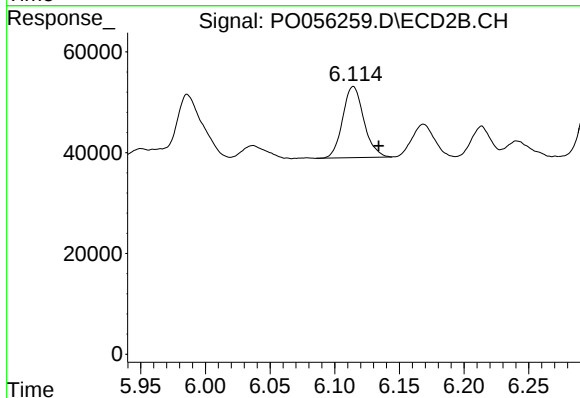


#31 AR-1260-1

R.T.: 6.114 min
Delta R.T.: -0.020 min
Response: 160632
Conc: 72.91 ng/ml

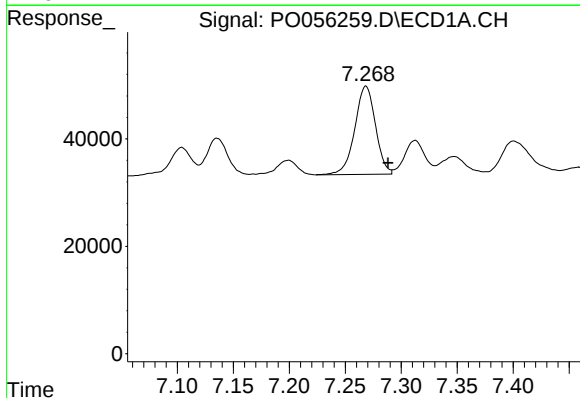


#32 AR-1260-2

R.T.: 7.269 min
Delta R.T.: -0.020 min
Response: 210841
Conc: 80.51 ng/ml

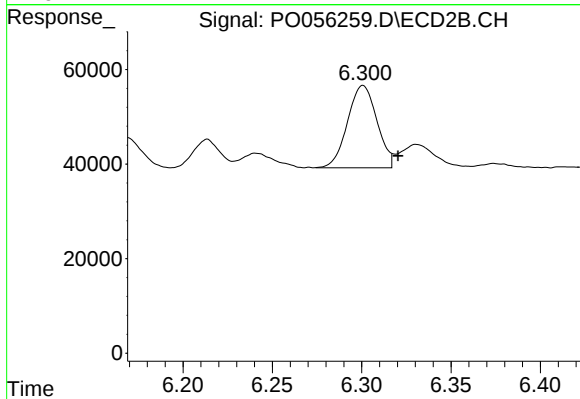

#32 AR-1260-2

R.T.: 6.300 min
Delta R.T.: -0.020 min
Response: 199698
Conc: 65.40 ng/ml m

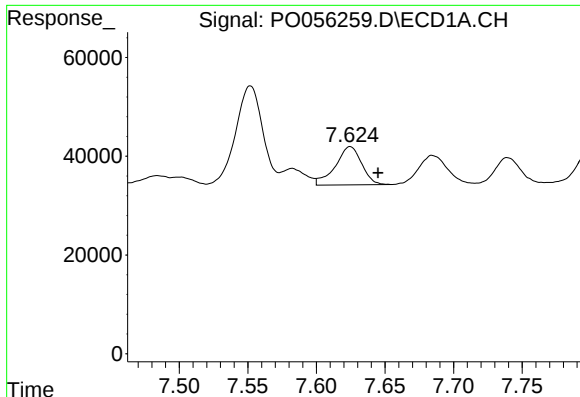


#33 AR-1260-3

R.T.: 7.625 min
Delta R.T.: -0.020 min
Response: 103313
Conc: 51.66 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19RE


Manual Integrations
APPROVED

Ankita
5/16/2019 8:36:11 AM

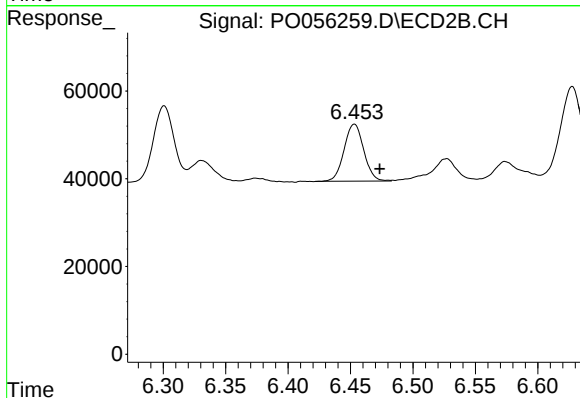


#33 AR-1260-3

R.T.: 6.453 min
Delta R.T.: -0.020 min
Response: 142507
Conc: 57.19 ng/ml m

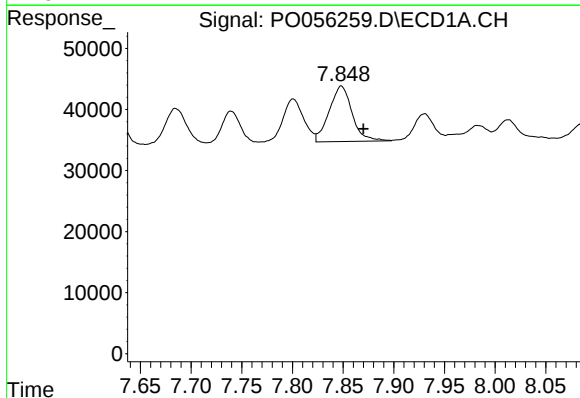


#34 AR-1260-4

R.T.: 7.848 min
Delta R.T.: -0.022 min
Response: 143386
Conc: 62.00 ng/ml

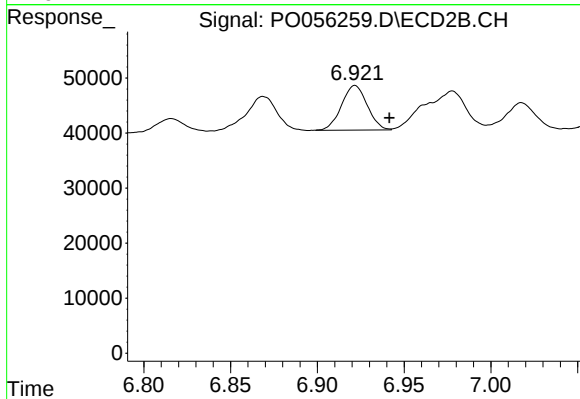

#34 AR-1260-4

R.T.: 6.921 min
Delta R.T.: -0.020 min
Response: 84231
Conc: 40.82 ng/ml m

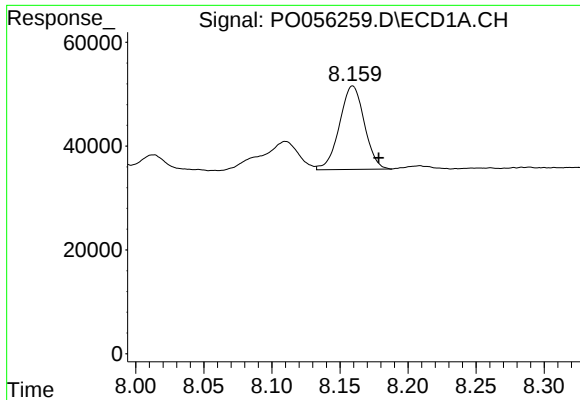


#35 AR-1260-5

R.T.: 8.159 min
Delta R.T.: -0.019 min
Response: 204579
Conc: 48.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
COMP-5.8.19RE

Manual Integrations
APPROVED

Ankita
5/16/2019 8:36:11 AM

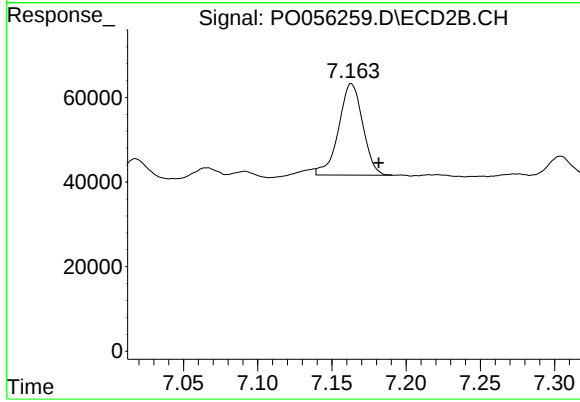

#35 AR-1260-5

R.T.: 7.163 min
Delta R.T.: -0.019 min
Response: 244053
Conc: 48.59 ng/ml m