

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051519\
Data File : P0056277.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 May 2019 23:34
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 02:21:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.260	3.578	713435	663552	23.840	23.494
2) SA Decachlor...	9.843	8.522	865262	681962	23.125	25.218

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051519\
Data File : P0056277.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 15 May 2019 23:34
Operator : SM/SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 02:21:09 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

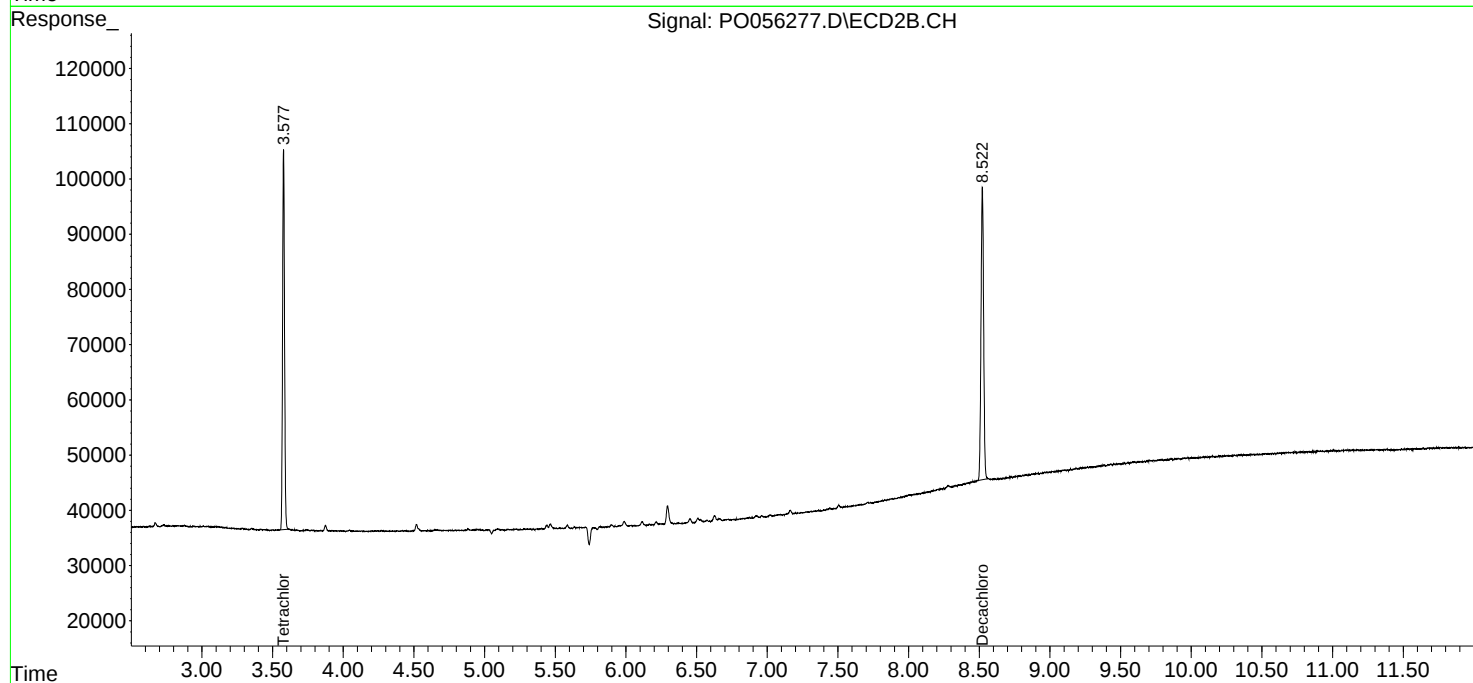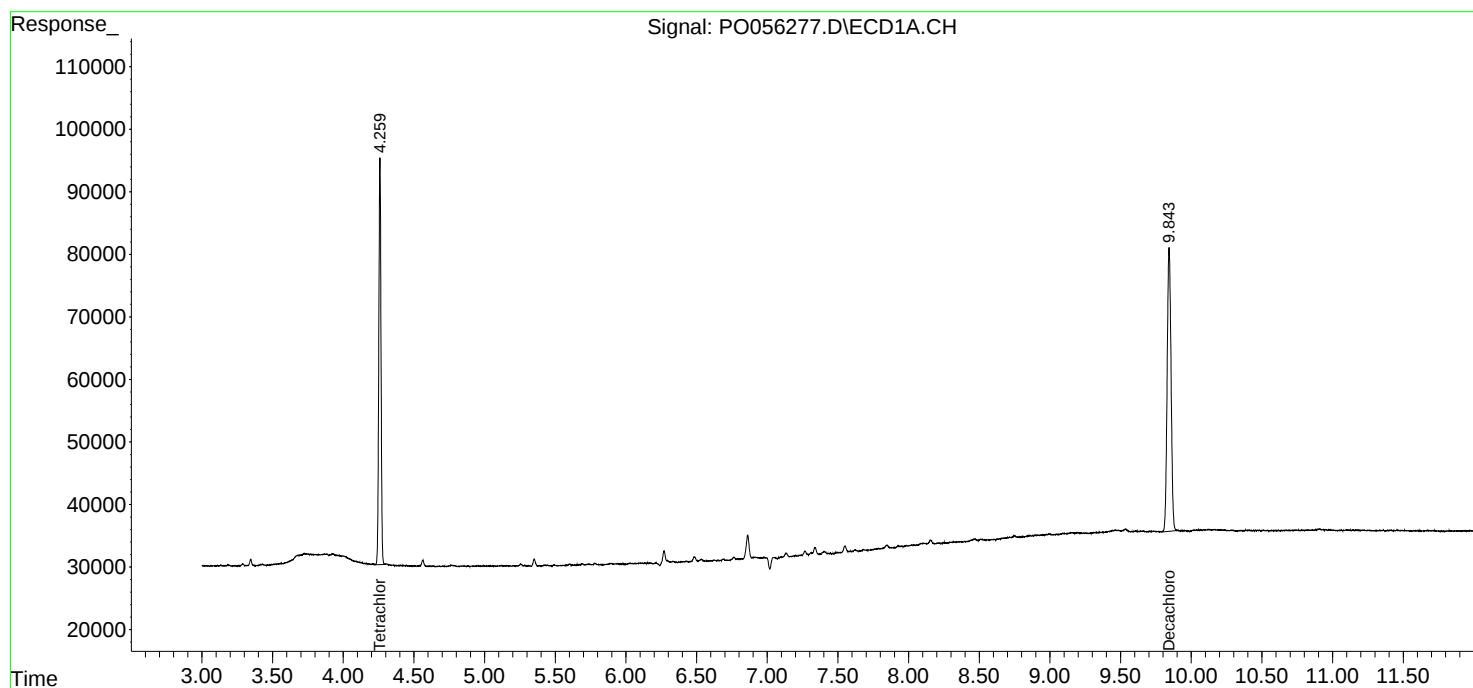


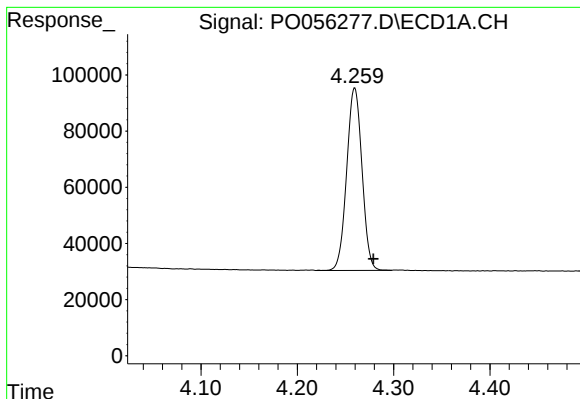

#1 Tetrachloro-m-xylene


R.T.: 4.260 min
Delta R.T.: -0.019 min
Response: 713435
Conc: 23.84 ng/ml

Instrument :
ECD_O
ClientSampleId :
I.BLK

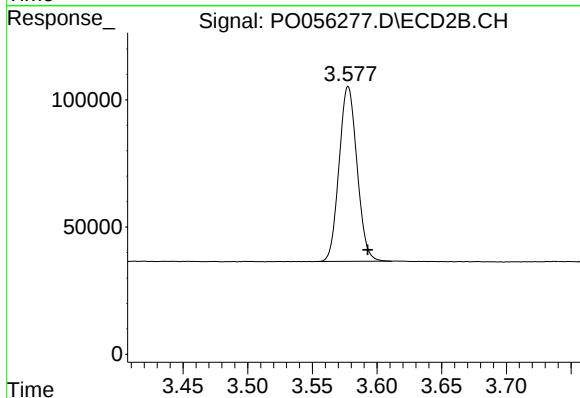


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: -0.015 min
Response: 663552
Conc: 23.49 ng/ml

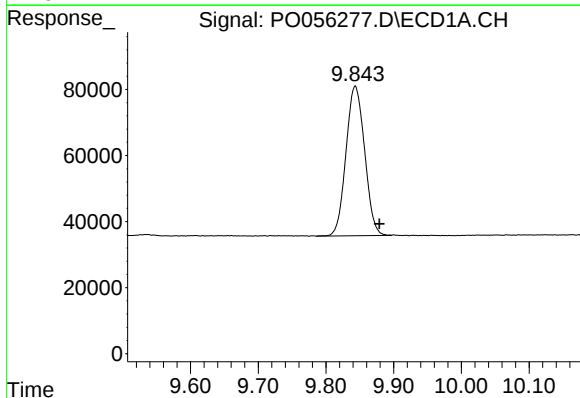

#2 Decachlorobiphenyl

R.T.: 9.843 min
Delta R.T.: -0.035 min
Response: 865262
Conc: 23.12 ng/ml

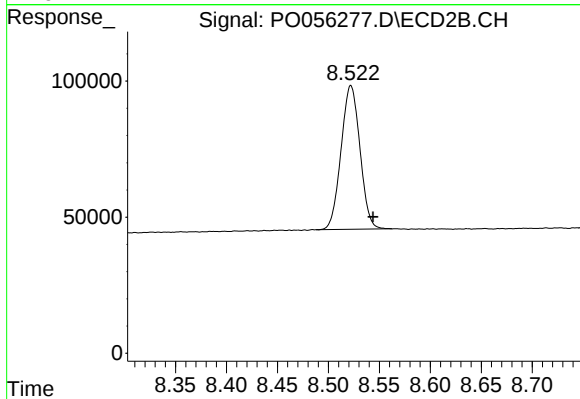

#2 Decachlorobiphenyl

R.T.: 8.522 min
Delta R.T.: -0.022 min
Response: 681962
Conc: 25.22 ng/ml