

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051523\
 Data File : P0095044.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2023 13:58
 Operator : YP/AJ
 Sample : 02782-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 D3034

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2023
 Supervised By :Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 17:29:57 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.421	3.619	51549786	20426928	14.965	15.266
2) SA Decachlor...	10.232	8.651	272.8E6	15351175	112.400m	13.638m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO051523\
Data File : PO095044.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2023 13:58
Operator : YP/AJ
Sample : 02782-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
D3034


Manual Integrations
APPROVED

Reviewed By : Yogesh Patel 05/16/2023
Supervised By : Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 17:29:57 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

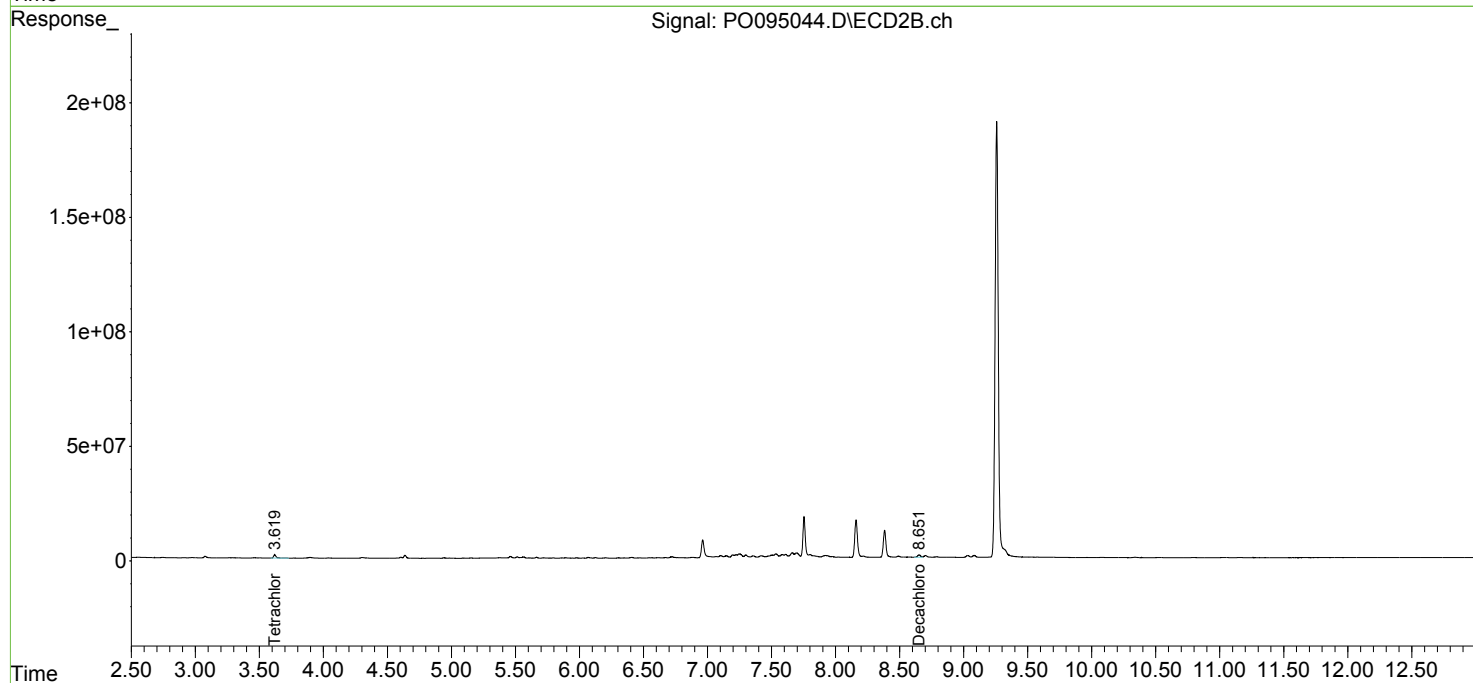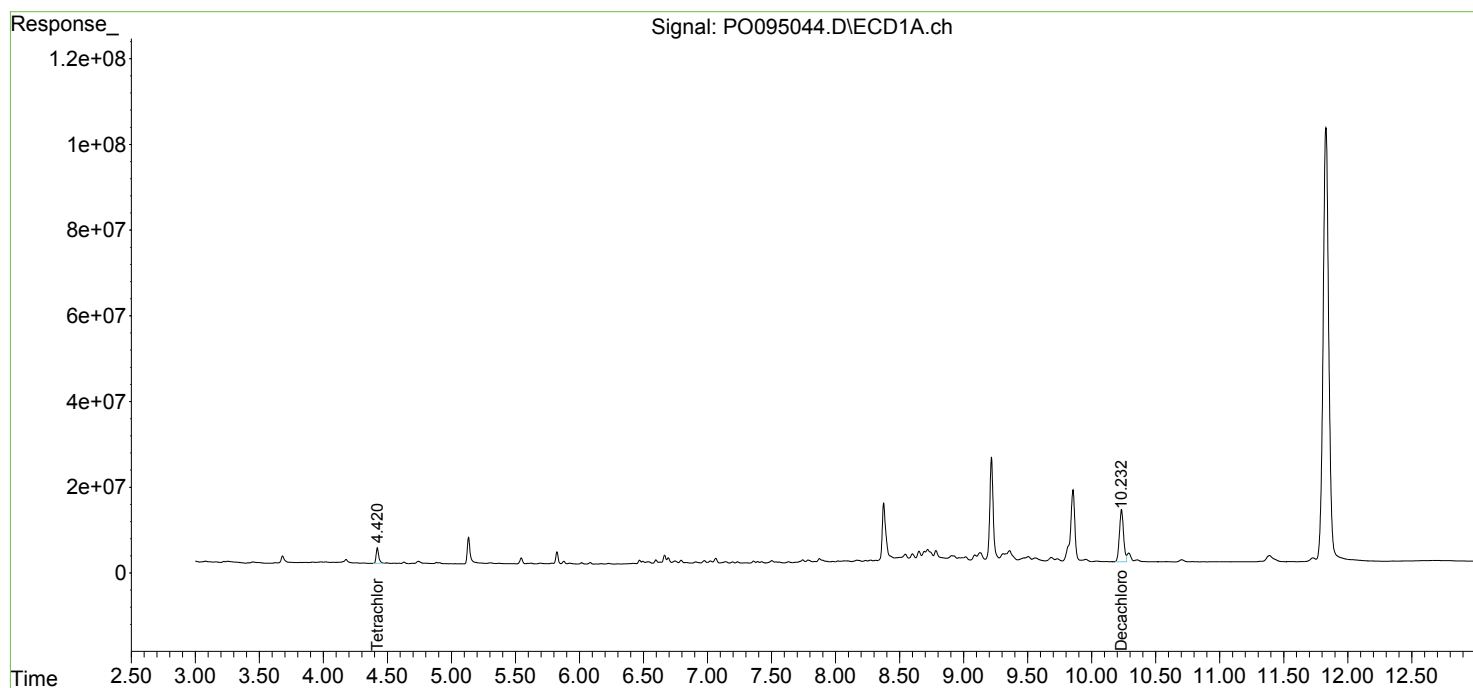

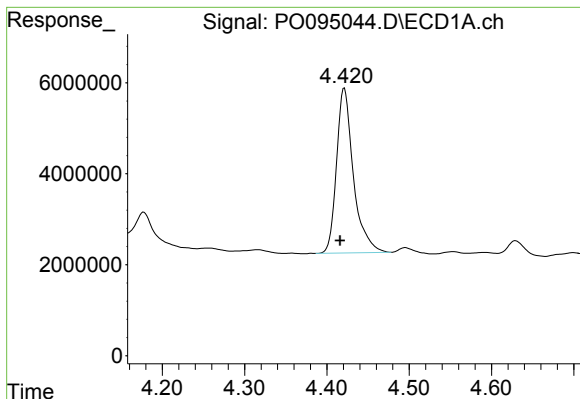


#1 Tetrachloro-m-xylene

R.T.: 4.421 min
Delta R.T.: 0.005 min
Response: 51549786
Conc: 14.97 ng/ml

Instrument :
ECD_O
ClientSampleId :
D3034


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2023
Supervised By :Ankita Jodhani 05/16/2023

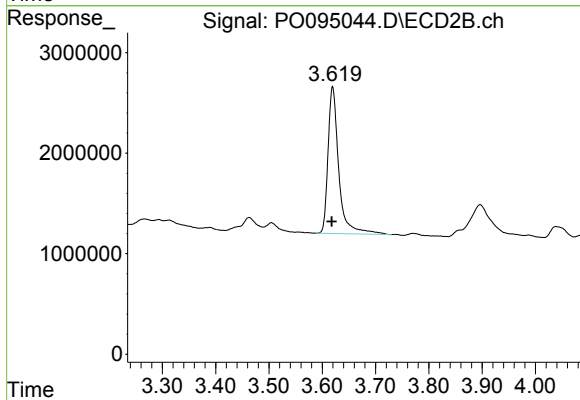


#1 Tetrachloro-m-xylene

R.T.: 3.619 min
Delta R.T.: 0.002 min
Response: 20426928
Conc: 15.27 ng/ml

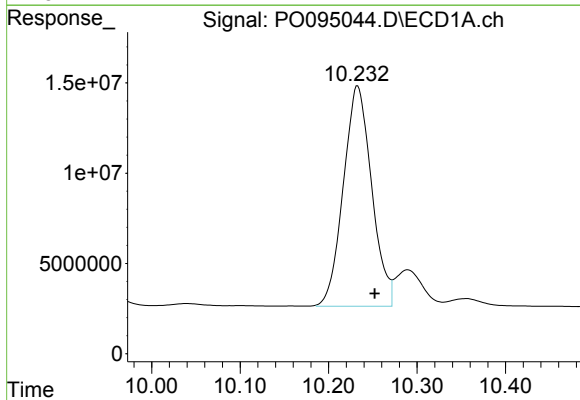

#2 Decachlorobiphenyl

R.T.: 10.232 min
Delta R.T.: -0.020 min
Response: 272777467
Conc: 112.40 ng/ml m

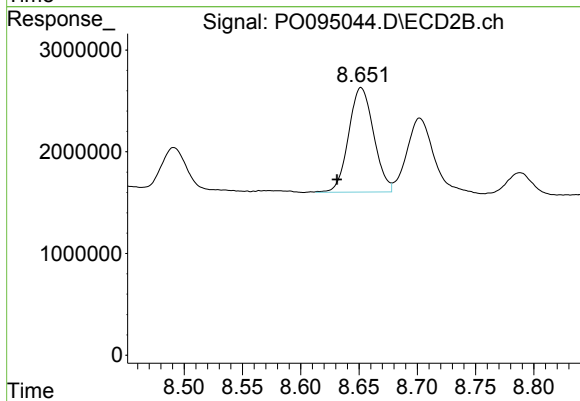

#2 Decachlorobiphenyl

R.T.: 8.651 min
Delta R.T.: 0.020 min
Response: 15351175
Conc: 13.64 ng/ml m