

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051523\
 Data File : P0095089.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2023 07:03
 Operator : YP/AJ
 Sample : 02795-01
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 PCB-HA-01

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 07:36:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.412	3.612	72527651	29295739	21.055	21.894
2)	SA Decachlor...	10.252	8.621	56980027	26666619	23.479	23.691
Target Compounds							
26)	L6 AR-1254-1	6.457	5.494	4000945	2045993	31.579	28.224
27)	L6 AR-1254-2	6.678	5.641	4751926	1011682	24.862	15.505 #
28)	L6 AR-1254-3	7.048	6.046	4065250	2527943	21.553	25.458
29)	L6 AR-1254-4	7.336	6.273	1256679	716512	11.096	14.516 #
30)	L6 AR-1254-5	7.759	6.692	3530330	2219752	25.208	26.384



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051523\
Data File : PO095089.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2023 07:03
Operator : YP/AJ
Sample : 02795-01
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
PCB-HA-01

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 07:36:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

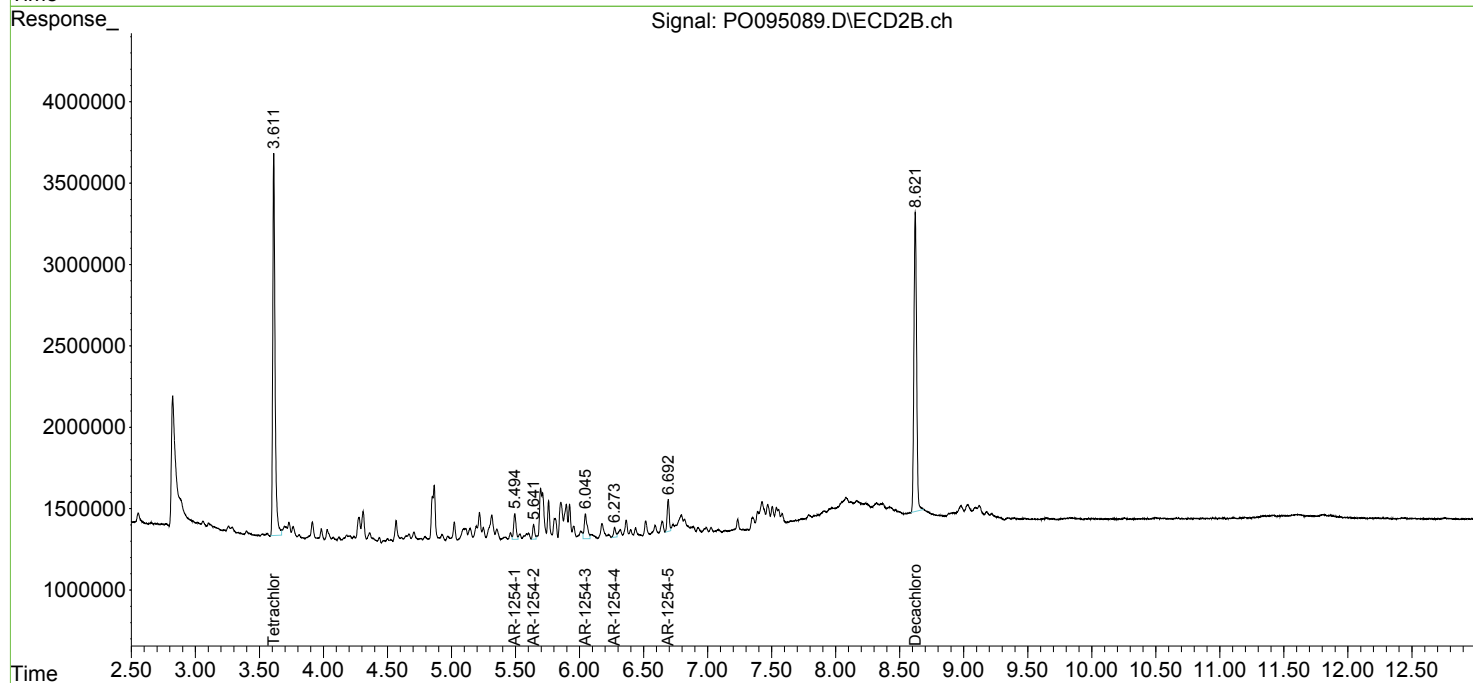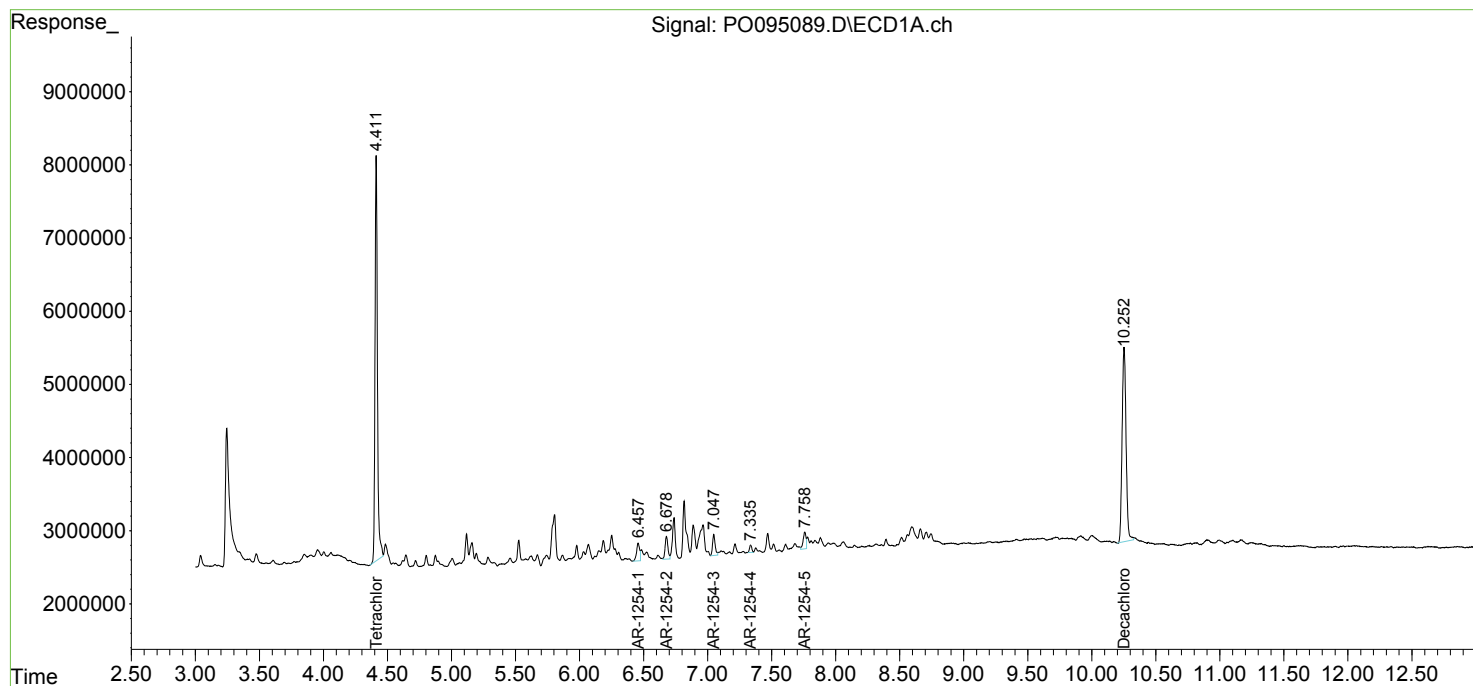


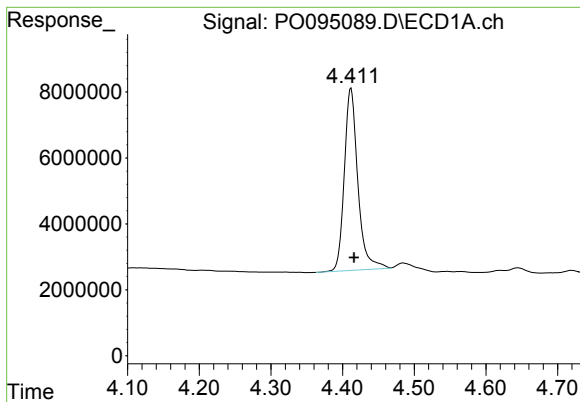

#1 Tetrachloro-m-xylene


R.T.: 4.412 min
Delta R.T.: -0.004 min
Response: 72527651
Conc: 21.06 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-HA-01

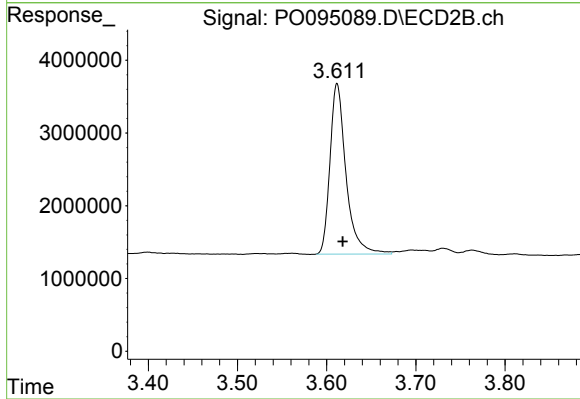


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: -0.006 min
Response: 29295739
Conc: 21.89 ng/ml

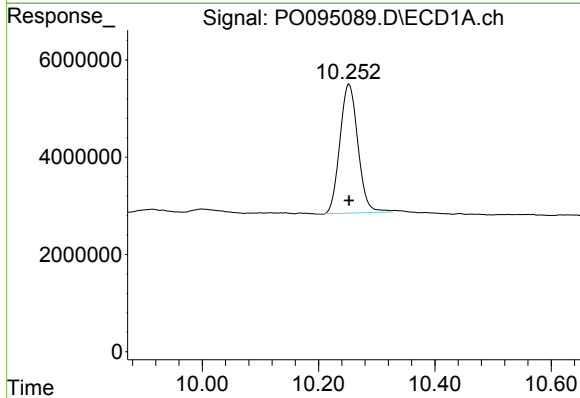


#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: 0.000 min
Response: 56980027
Conc: 23.48 ng/ml

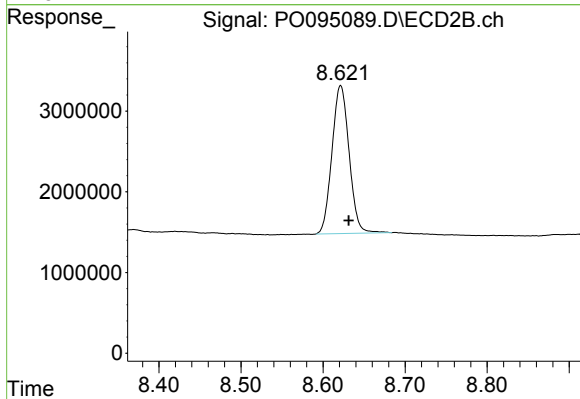

#2 Decachlorobiphenyl


R.T.: 8.621 min
Delta R.T.: -0.010 min
Response: 26666619
Conc: 23.69 ng/ml

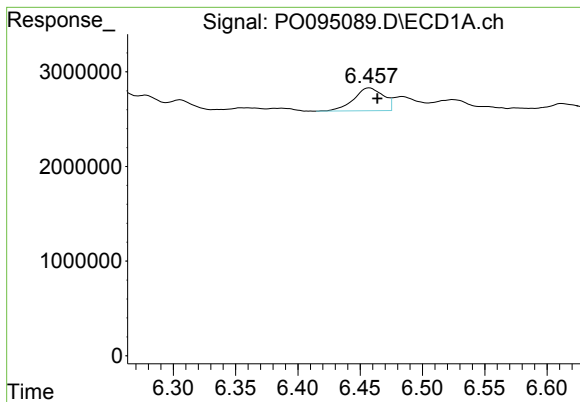

#26 AR-1254-1


R.T.: 6.457 min
Delta R.T.: -0.006 min
Response: 4000945
Conc: 31.58 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-HA-01

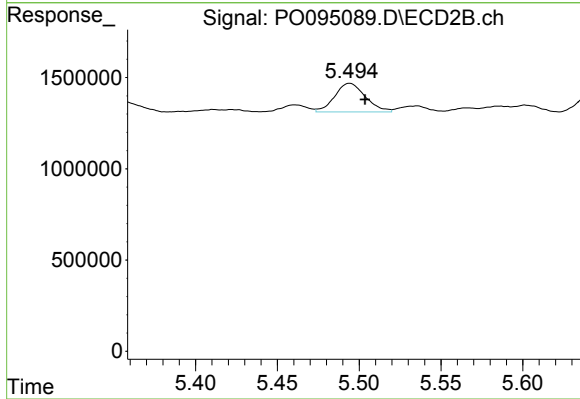


#26 AR-1254-1

R.T.: 5.494 min
Delta R.T.: -0.009 min
Response: 2045993
Conc: 28.22 ng/ml

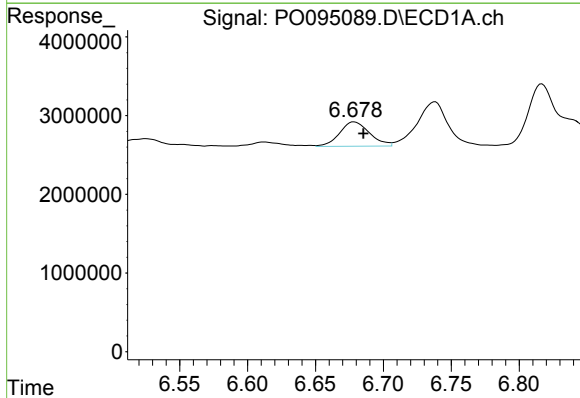


#27 AR-1254-2

R.T.: 6.678 min
Delta R.T.: -0.007 min
Response: 4751926
Conc: 24.86 ng/ml

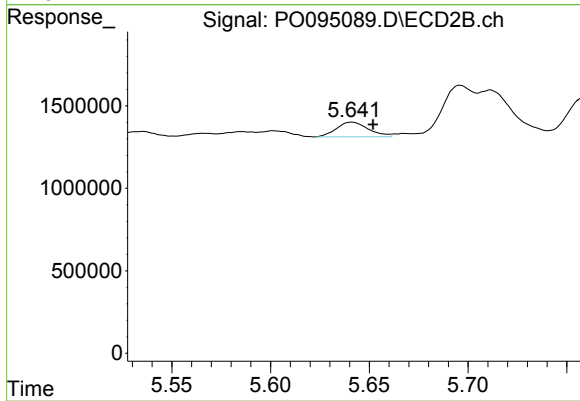

#27 AR-1254-2


R.T.: 5.641 min
Delta R.T.: -0.011 min
Response: 1011682
Conc: 15.50 ng/ml

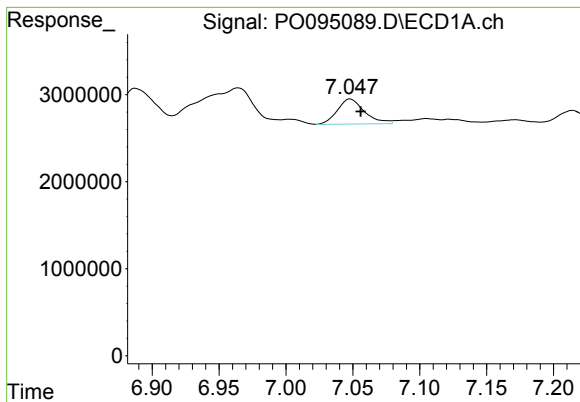

#28 AR-1254-3


R.T.: 7.048 min
Delta R.T.: -0.008 min
Response: 4065250
Conc: 21.55 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-HA-01

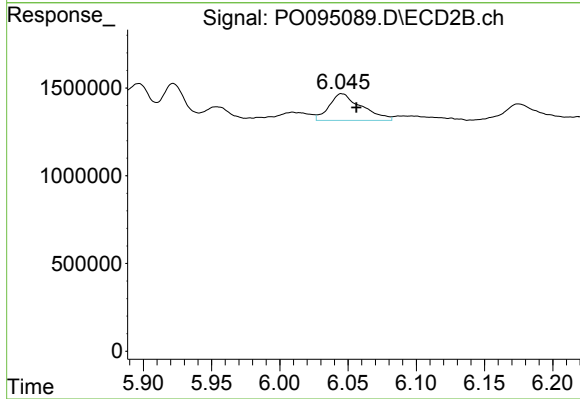


#28 AR-1254-3

R.T.: 6.046 min
Delta R.T.: -0.010 min
Response: 2527943
Conc: 25.46 ng/ml

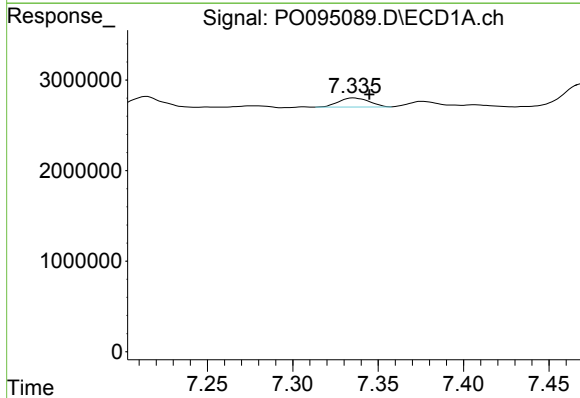


#29 AR-1254-4

R.T.: 7.336 min
Delta R.T.: -0.009 min
Response: 1256679
Conc: 11.10 ng/ml

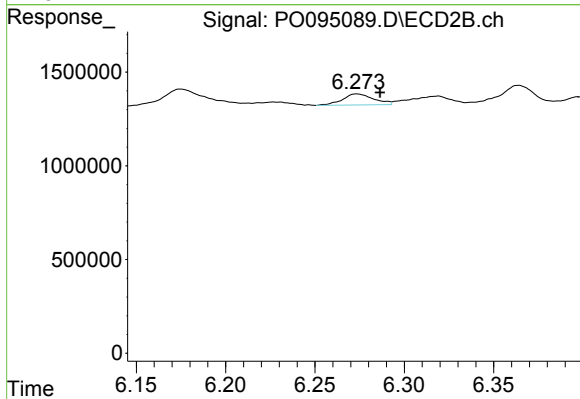

#29 AR-1254-4


R.T.: 6.273 min
Delta R.T.: -0.013 min
Response: 716512
Conc: 14.52 ng/ml

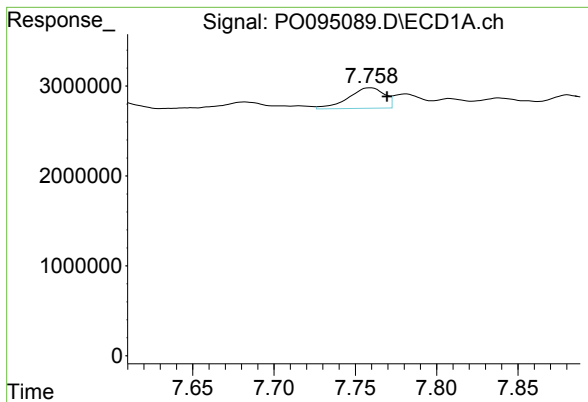

#30 AR-1254-5

R.T.: 7.759 min
Delta R.T.: -0.010 min
Response: 3530330
Conc: 25.21 ng/ml

Instrument :
ECD_O
ClientSampleId :
PCB-HA-01

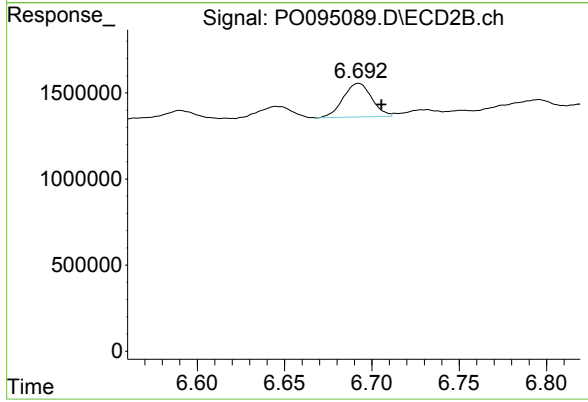

#30 AR-1254-5

R.T.: 6.692 min
Delta R.T.: -0.013 min
Response: 2219752
Conc: 26.38 ng/ml