Quantitation Report (QT Reviewed)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051523\
Data File : PO095091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2023 07:37
Operator : YP/AJ
Sample : 02776-02 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC283069-1-2

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 05/16/2023
Supervised By :Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 08:45:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
	System Monitoring Compounds						
1)	SA Tetrachlo...	4.412	3.612	5066123	1984760	1.471	1.483
2)	SA Decachlor...	10.254	8.622	5254155	2549324	2.165m	2.265
	Target Compounds						

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051523\
Data File : PO095091.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2023 07:37
Operator : YP/AJ
Sample : 02776-02 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
BC283069-1-2

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 05/16/2023
Supervised By :Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 08:45:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

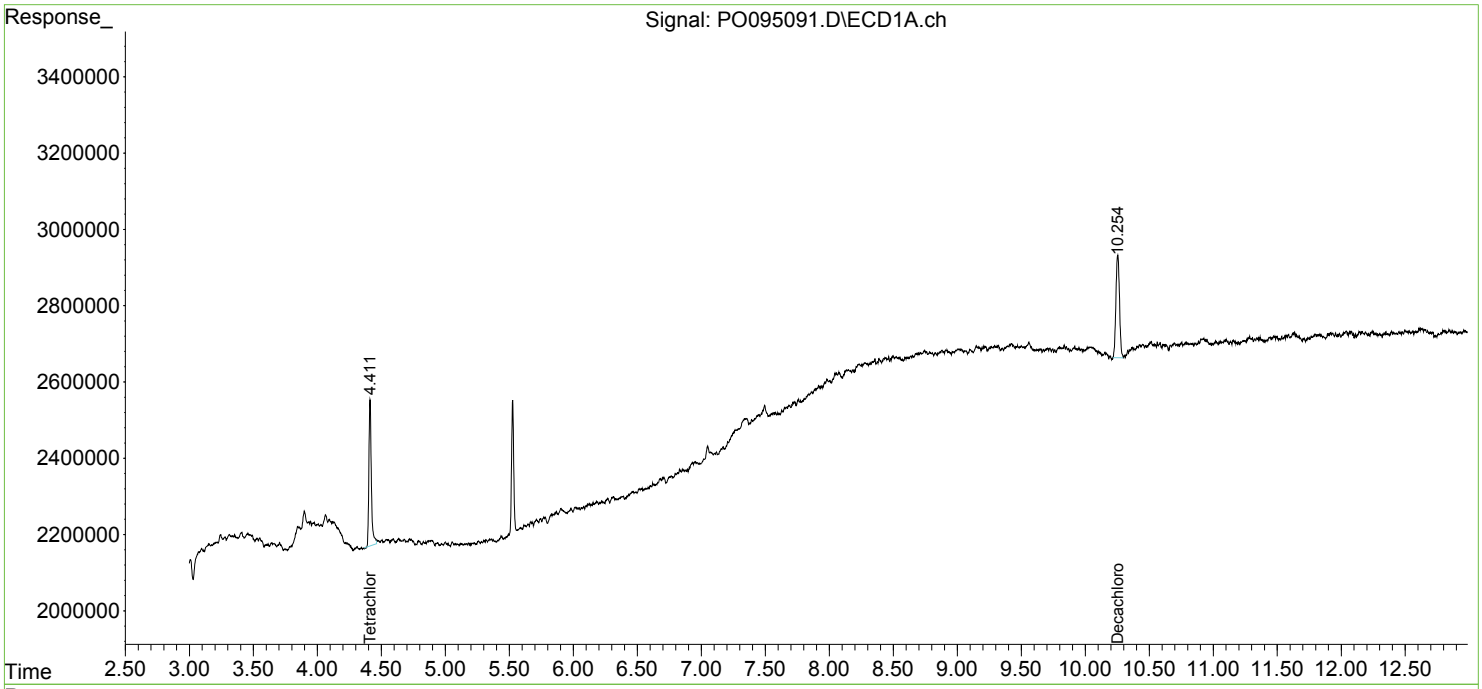

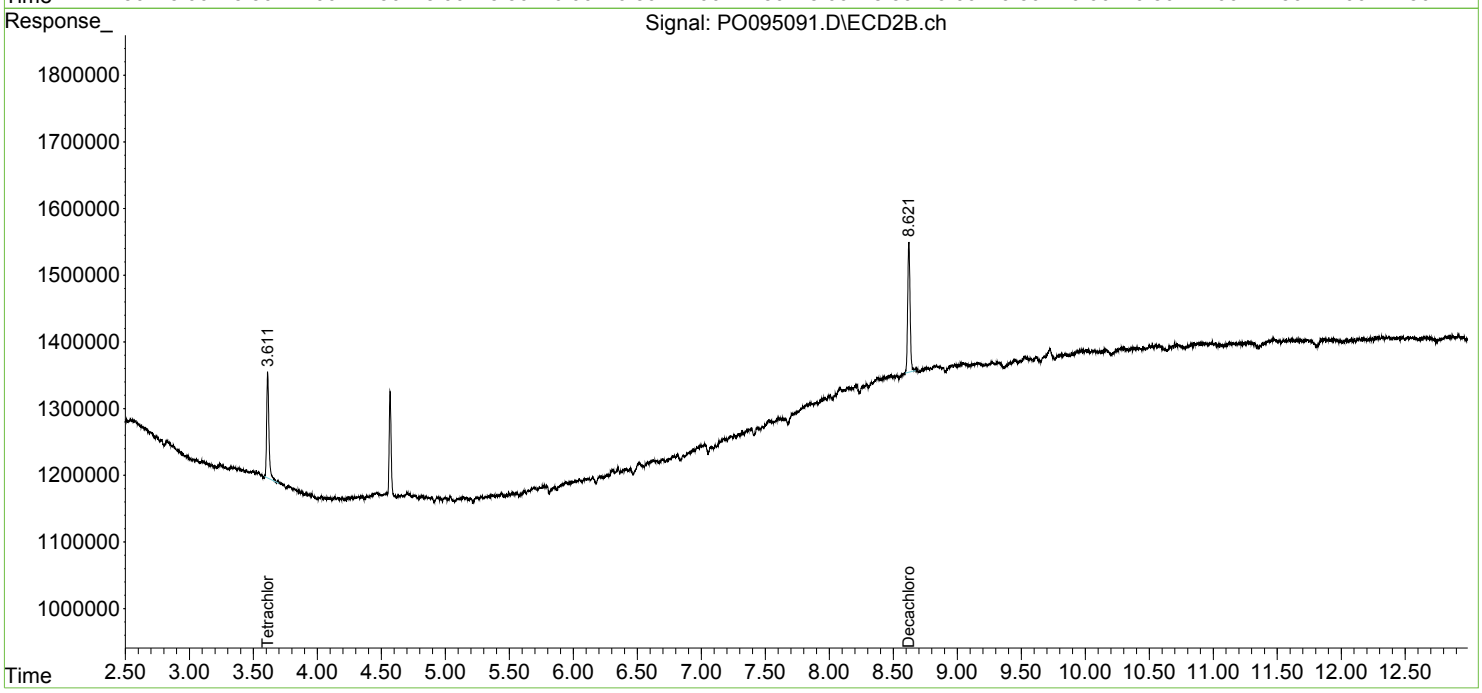

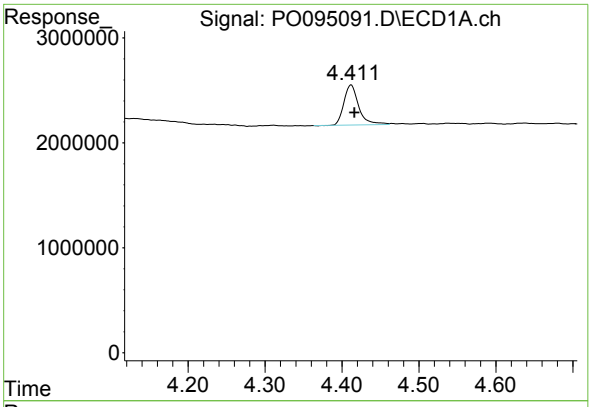

#1 Tetrachloro-m-xylene

R.T.: 4.412 min
Delta R.T.: -0.004 min
Response: 5066123
Conc: 1.47 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC283069-1-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2023
Supervised By :Ankita Jodhani 05/16/2023

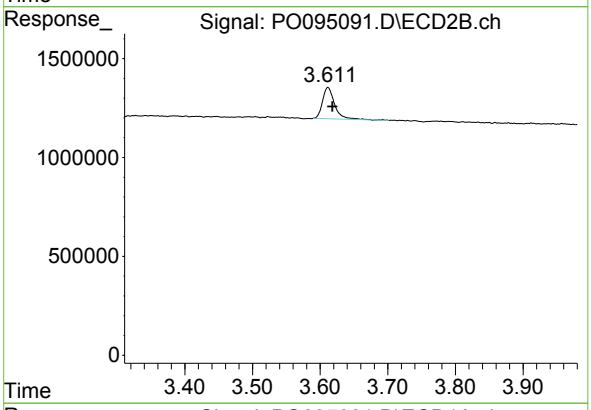

#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: -0.006 min
Response: 1984760
Conc: 1.48 ng/ml

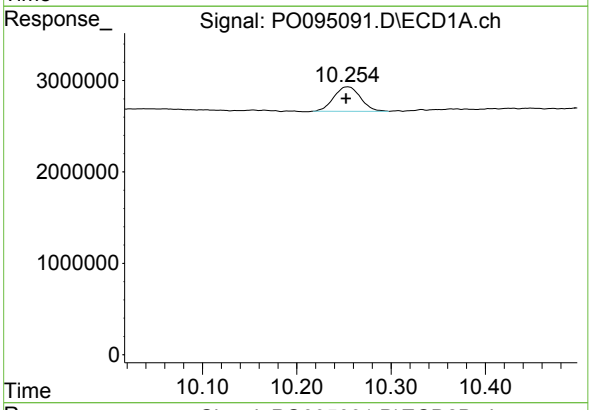

#2 Decachlorobiphenyl

R.T.: 10.254 min
Delta R.T.: 0.002 min
Response: 5254155
Conc: 2.17 ng/ml m

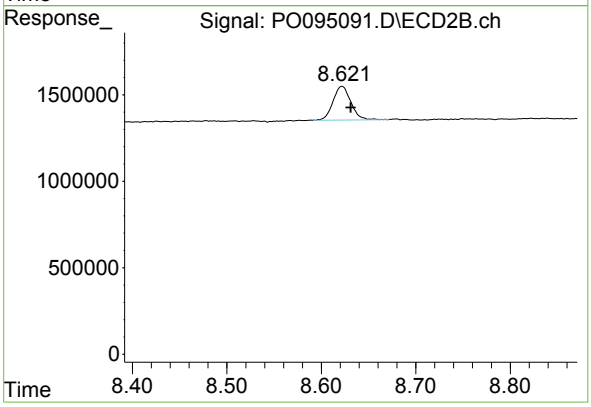

#2 Decachlorobiphenyl

R.T.: 8.622 min
Delta R.T.: -0.009 min
Response: 2549324
Conc: 2.26 ng/ml