

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051523\
 Data File : P0095094.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2023 08:29
 Operator : YP/AJ
 Sample : 02783-01 10X
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 ECD_0
 ClientSampleId :
 KMH4447Y-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2023
 Supervised By :Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 08:52:47 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.412	3.612	5993059	2438744	1.740	1.823
2) SA Decachlor...	10.252	8.623	6426971	2904916	2.648	2.581m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051523\
Data File : P0095094.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2023 08:29
Operator : YP/AJ
Sample : 02783-01 10X
Misc :
ALS Vial : 46 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH4447Y-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2023
Supervised By :Ankita Jodhani 05/16/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 08:52:47 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

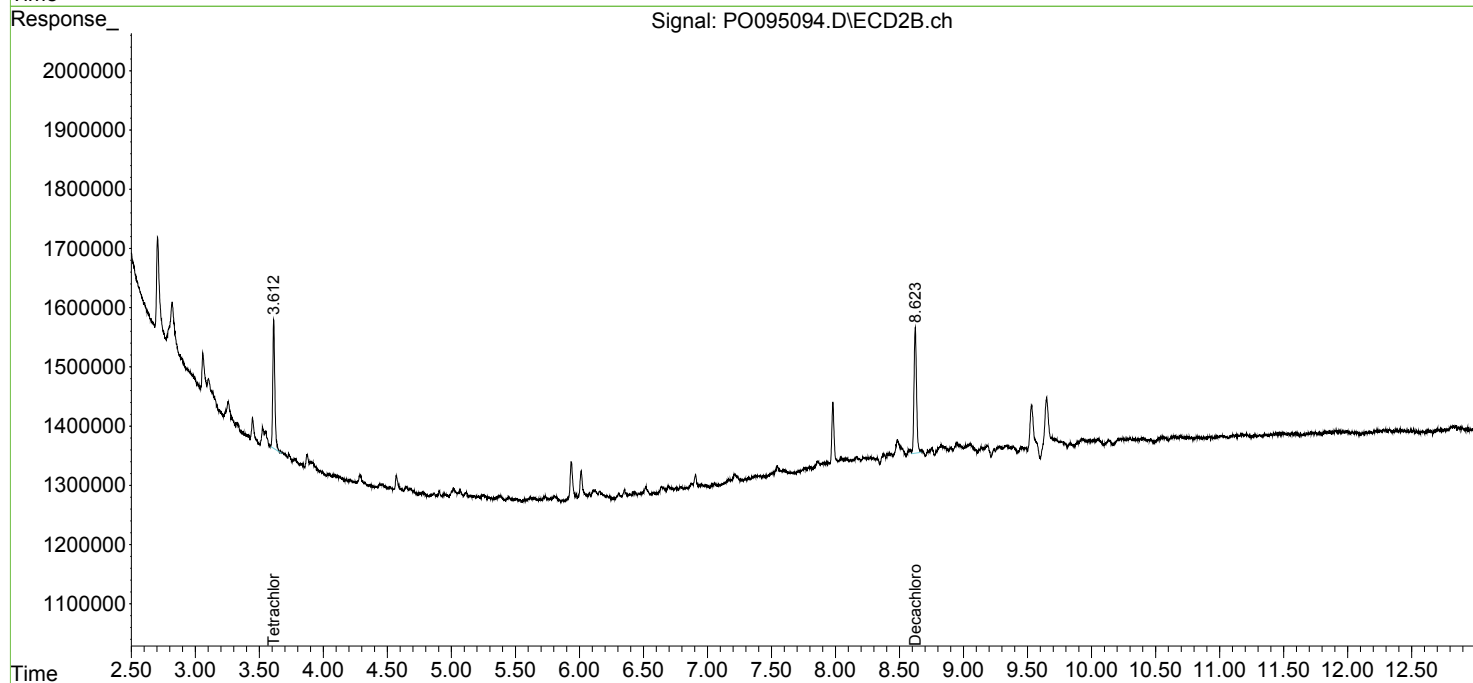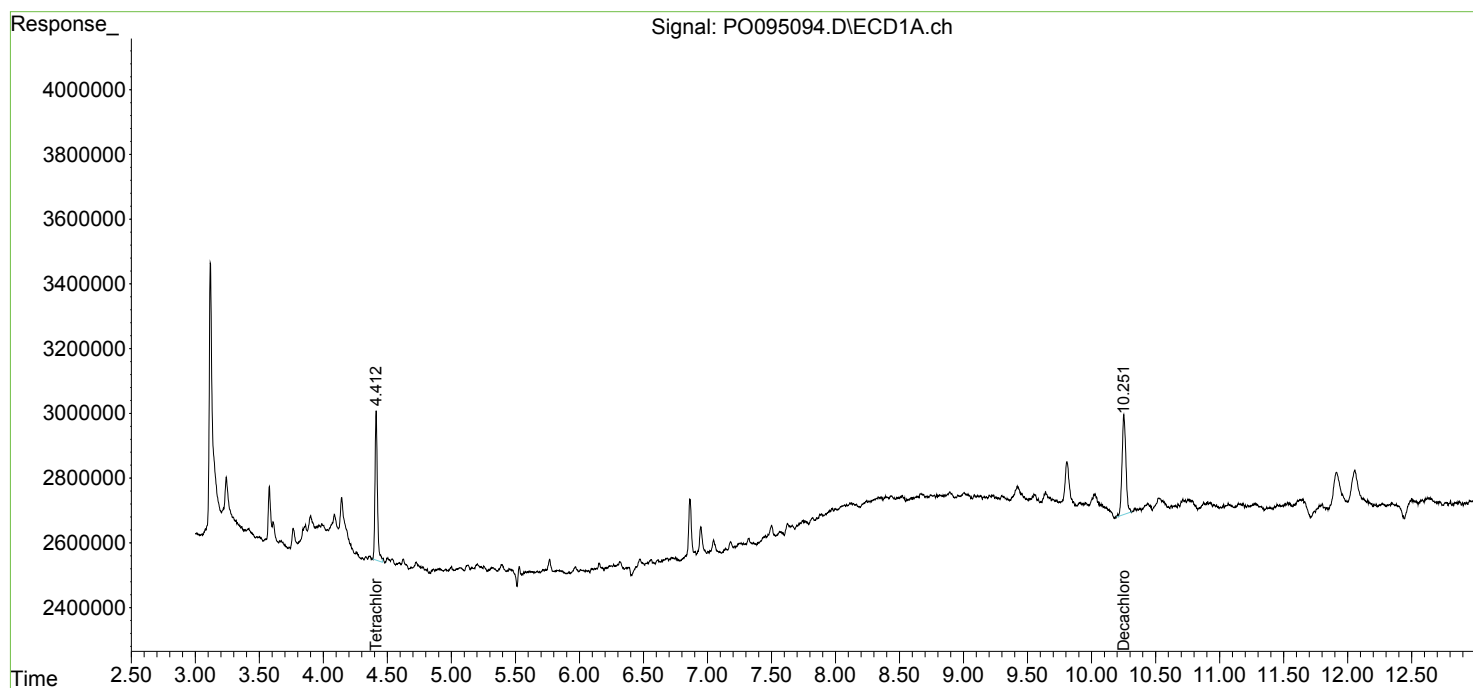

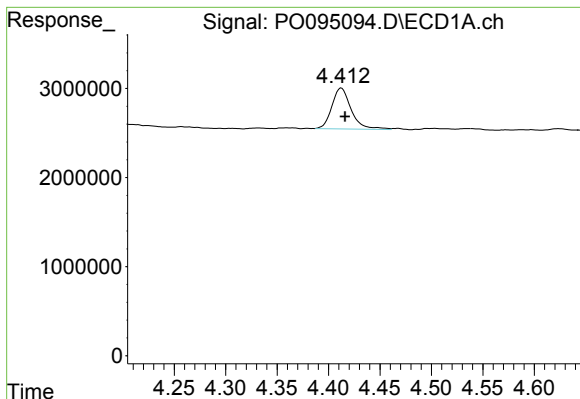

#1 Tetrachloro-m-xylene

R.T.: 4.412 min
Delta R.T.: -0.004 min
Response: 5993059
Conc: 1.74 ng/ml

Instrument :

ECD_O


ClientSampleId :

KMH4447Y-1-1

Manual Integrations


APPROVED

Reviewed By :Yogesh Patel 05/16/2023
Supervised By :Ankita Jodhani 05/16/2023

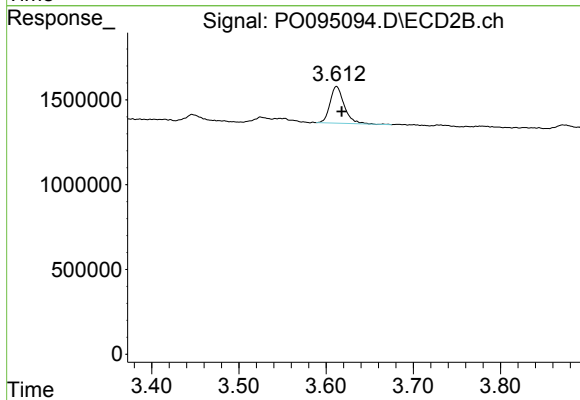


#1 Tetrachloro-m-xylene

R.T.: 3.612 min
Delta R.T.: -0.006 min
Response: 2438744
Conc: 1.82 ng/ml

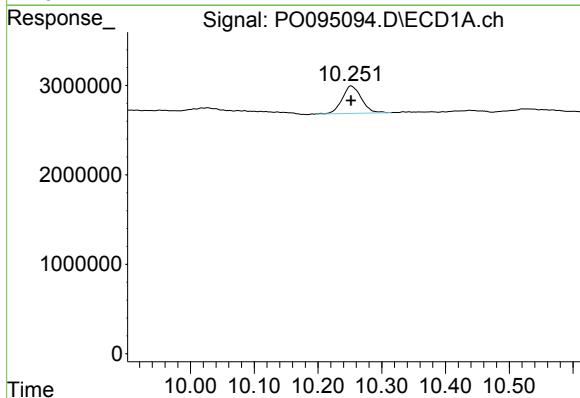

#2 Decachlorobiphenyl

R.T.: 10.252 min
Delta R.T.: 0.000 min
Response: 6426971
Conc: 2.65 ng/ml

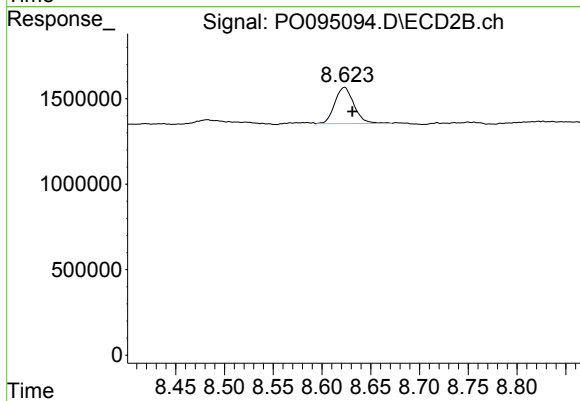

#2 Decachlorobiphenyl

R.T.: 8.623 min
Delta R.T.: -0.008 min
Response: 2904916
Conc: 2.58 ng/ml m