

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051619\
 Data File : P0056285.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 May 2019 12:26
 Operator : SM/SJ
 Sample : K2836-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 CULVER-CBTC-WC1-051019

Manual Integrations
 APPROVED

Ankita
 5/17/2019 1:24:27 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 12:50:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.274	3.577	510807	502435	17.069	17.789
2) SA Decachlor...	9.866	8.526	564059	463724	15.075m	17.148

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051619\
Data File : P0056285.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 May 2019 12:26
Operator : SM/SJ
Sample : K2836-02
Misc :
ALS Vial : 4 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
CULVER-CBTC-WC1-051019


Manual Integrations
APPROVED

Ankita
5/17/2019 1:24:27 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 12:50:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

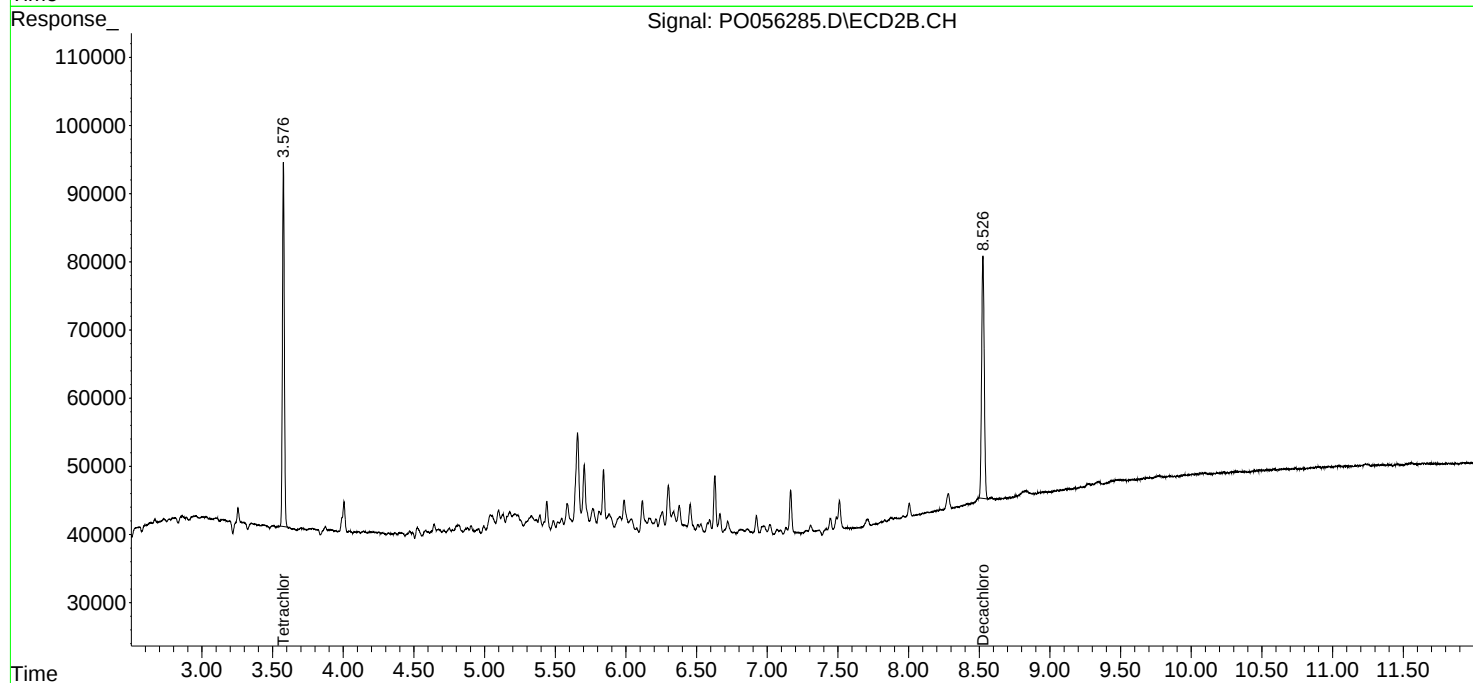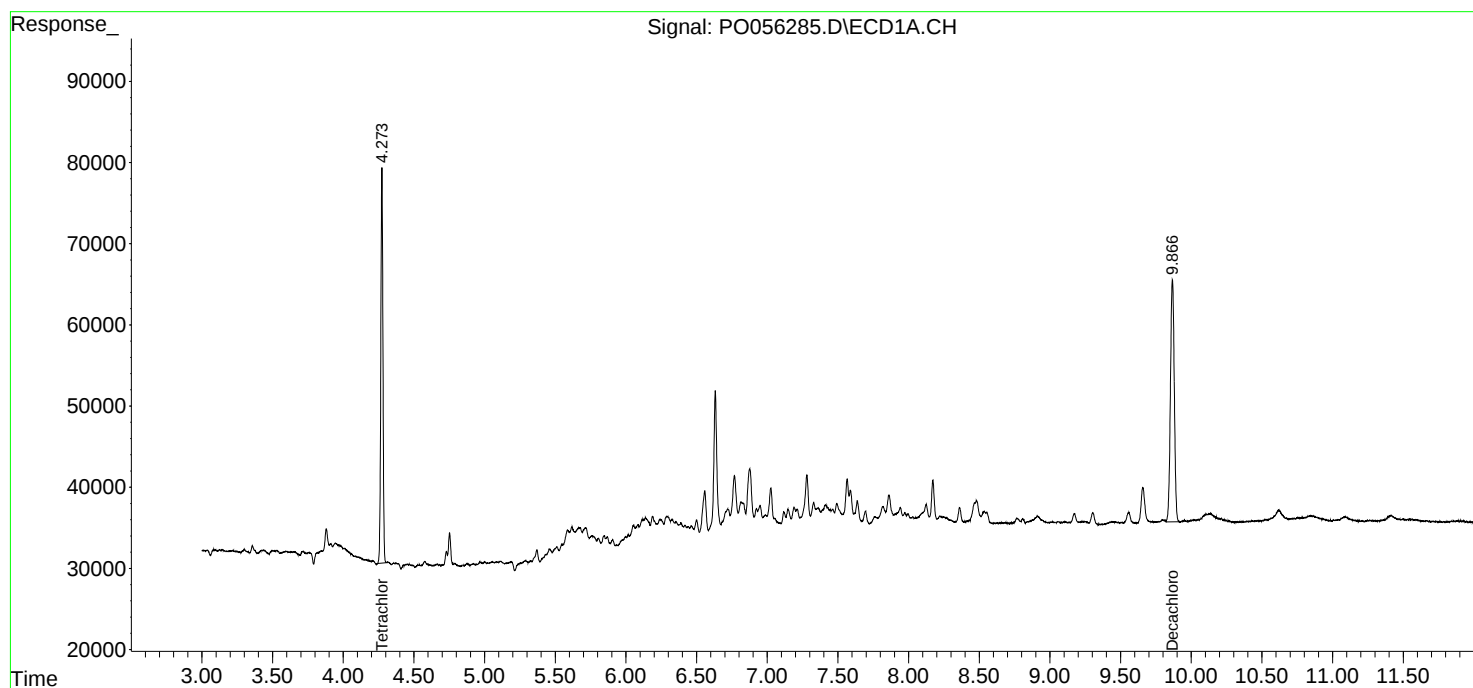

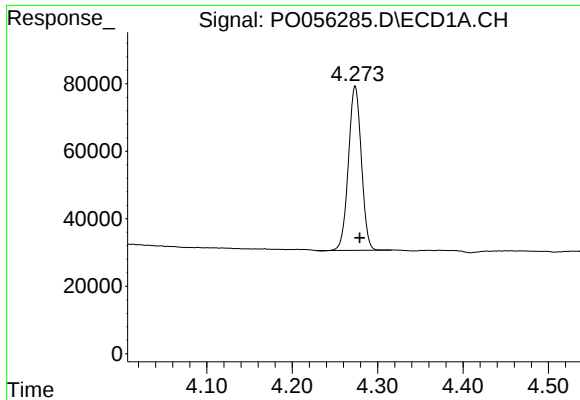


#1 Tetrachloro-m-xylene

R.T.: 4.274 min
Delta R.T.: -0.005 min
Response: 510807
Conc: 17.07 ng/ml

Instrument :
ECD_O
ClientSampleId :
CULVER-CBTC-WC1-051019


Manual Integrations
APPROVED

Ankita
5/17/2019 1:24:27 PM

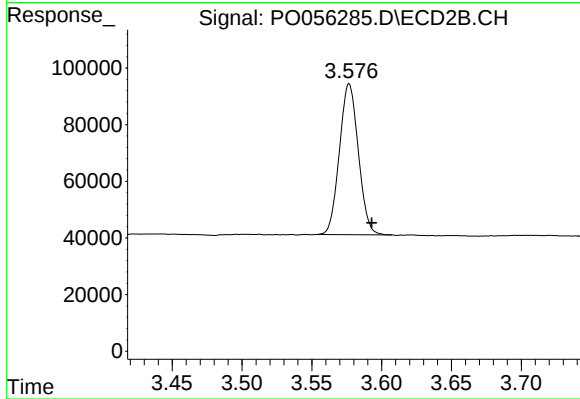


#1 Tetrachloro-m-xylene

R.T.: 3.577 min
Delta R.T.: -0.016 min
Response: 502435
Conc: 17.79 ng/ml

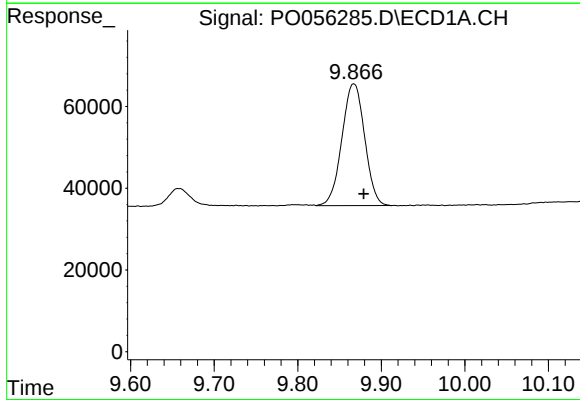

#2 Decachlorobiphenyl

R.T.: 9.866 min
Delta R.T.: -0.013 min
Response: 564059
Conc: 15.07 ng/ml m

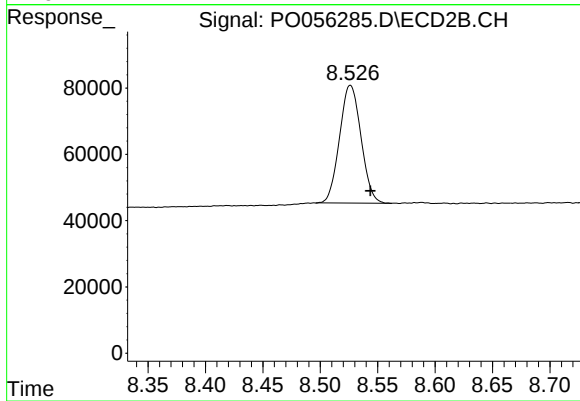

#2 Decachlorobiphenyl

R.T.: 8.526 min
Delta R.T.: -0.017 min
Response: 463724
Conc: 17.15 ng/ml