

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051619\
 Data File : P0056299.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 May 2019 17:34
 Operator : SM/SJ
 Sample : K2861-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-001-IDWGW-20190514

Manual Integrations
 APPROVED

Ankita
 5/17/2019 1:24:44 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 00:52:00 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 03 15:20:04 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.260	3.578	427502	400024	14.285	14.163
2) SA Decachlor...	9.844	8.522	143758	118657	3.842	4.388m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051619\
Data File : P0056299.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 May 2019 17:34
Operator : SM/SJ
Sample : K2861-02
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
TT-001-IDWGW-20190514


Manual Integrations
APPROVED

Ankita
5/17/2019 1:24:44 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 00:52:00 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050319.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 03 15:20:04 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

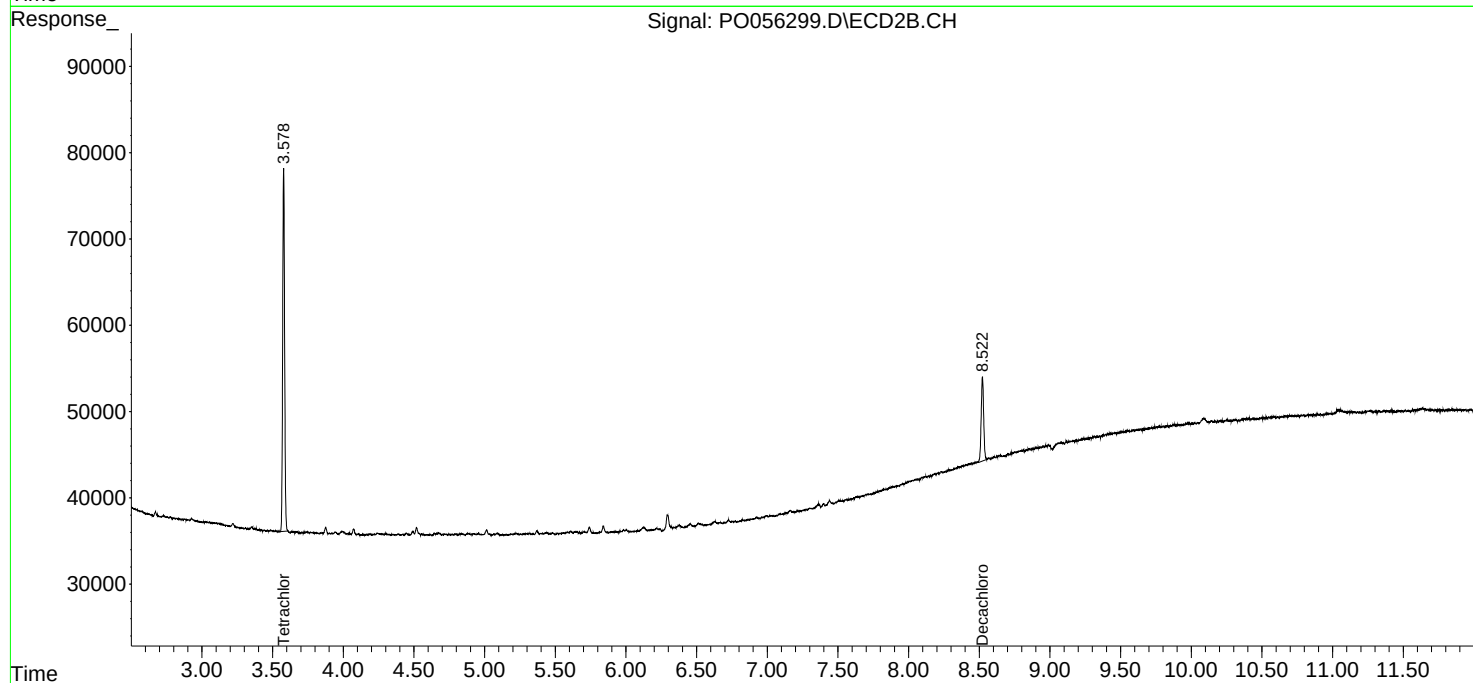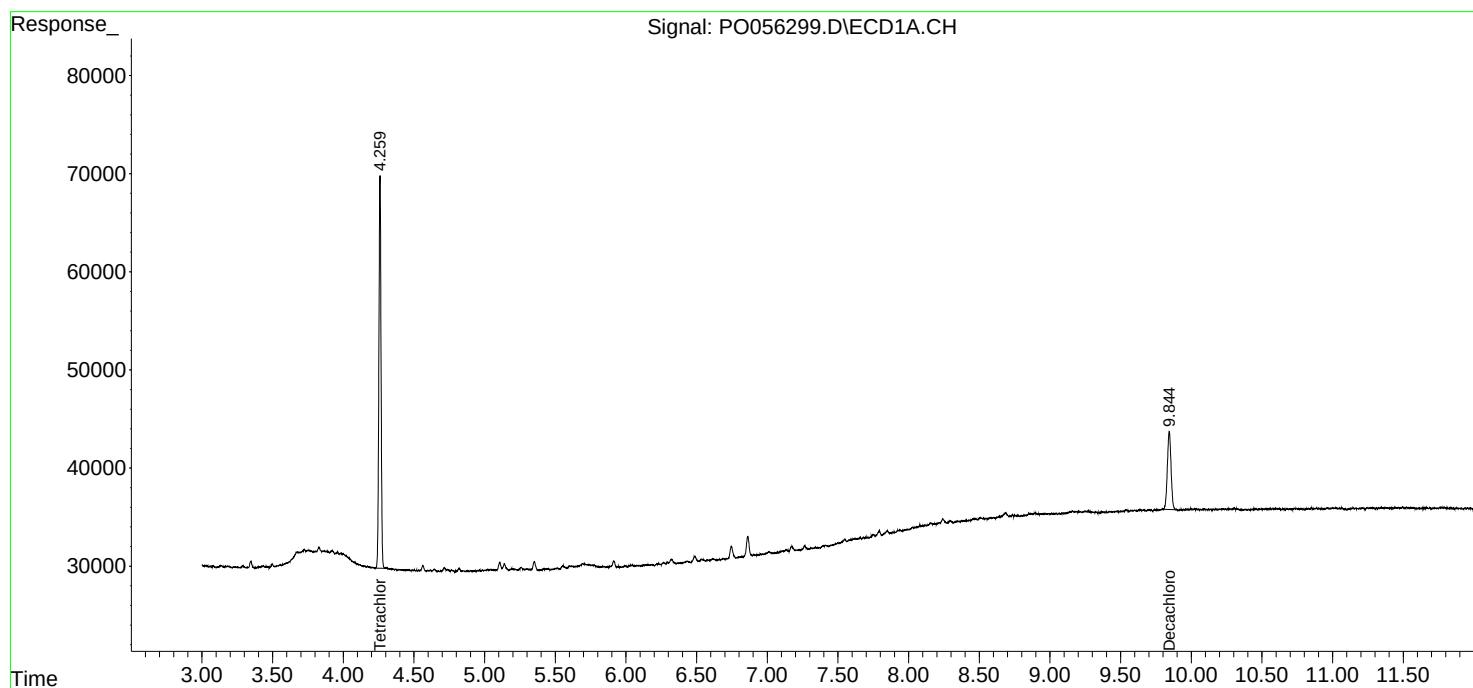

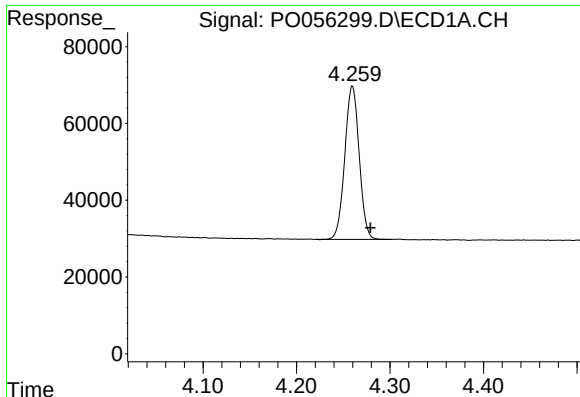


#1 Tetrachloro-m-xylene

R.T.: 4.260 min
Delta R.T.: -0.019 min
Response: 427502
Conc: 14.29 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-001-IDWGW-20190514


Manual Integrations
APPROVED

Ankita
5/17/2019 1:24:44 PM

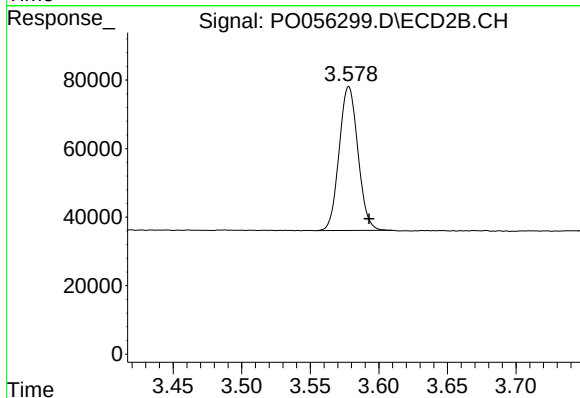


#1 Tetrachloro-m-xylene

R.T.: 3.578 min
Delta R.T.: -0.015 min
Response: 400024
Conc: 14.16 ng/ml

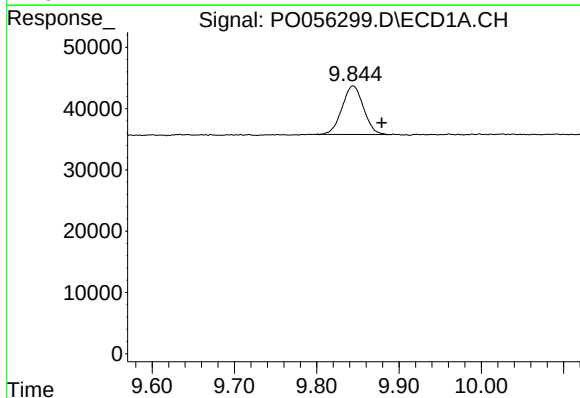

#2 Decachlorobiphenyl

R.T.: 9.844 min
Delta R.T.: -0.035 min
Response: 143758
Conc: 3.84 ng/ml

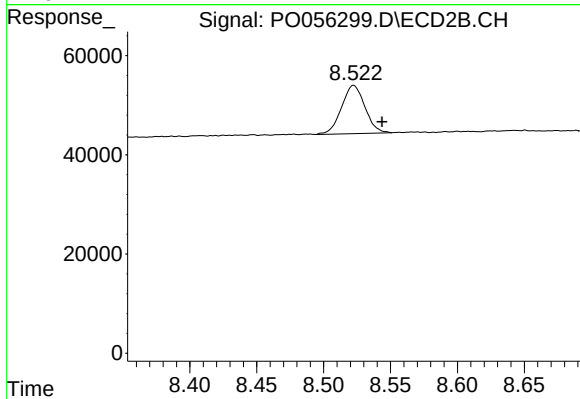

#2 Decachlorobiphenyl

R.T.: 8.522 min
Delta R.T.: -0.022 min
Response: 118657
Conc: 4.39 ng/ml m