

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051622\
 Data File : P0086060.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 May 2022 13:10
 Operator : YP\AJ
 Sample : N2832-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 SB21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 01:55:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.481	3.682	2581884	995865	25.424	22.850
2) SA Decachlor...	10.342	8.749	1313416	704654	24.785	20.761

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051622\
Data File : P0086060.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 May 2022 13:10
Operator : YP\AJ
Sample : N2832-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
SB21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:55:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

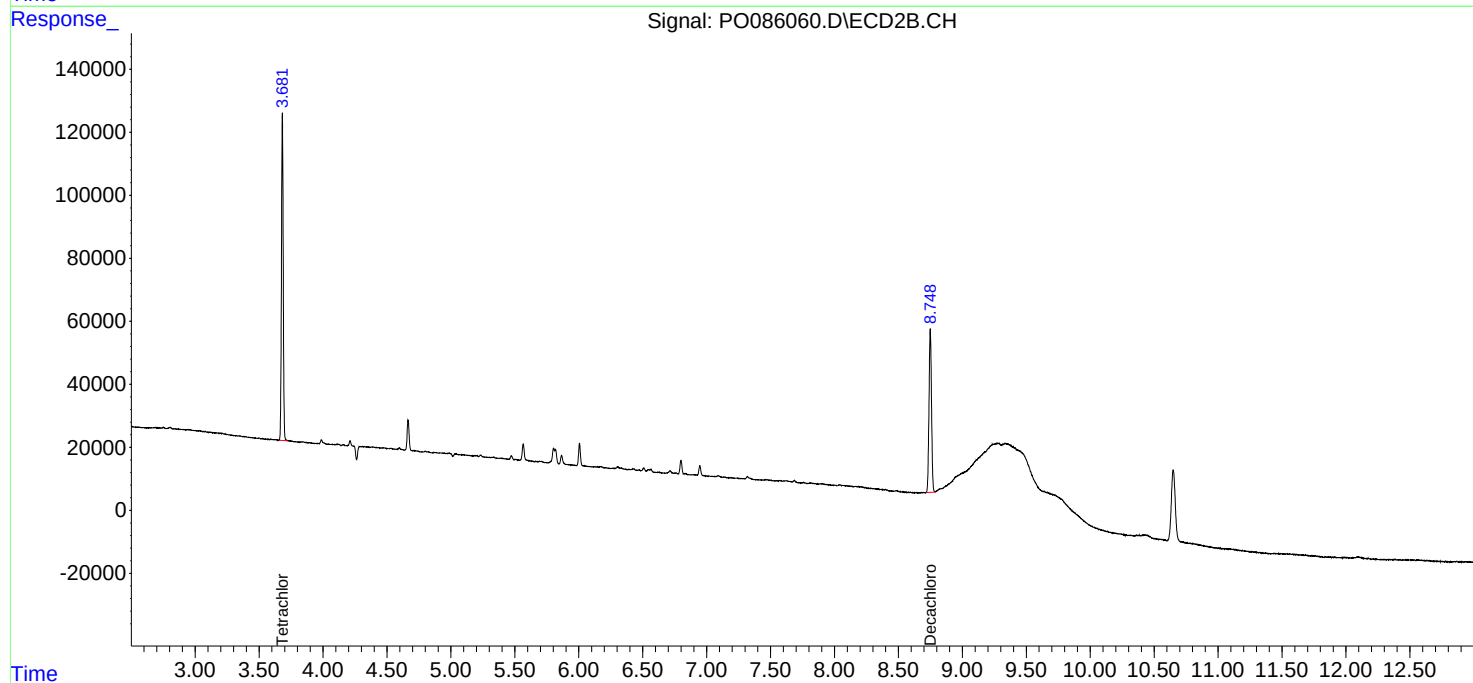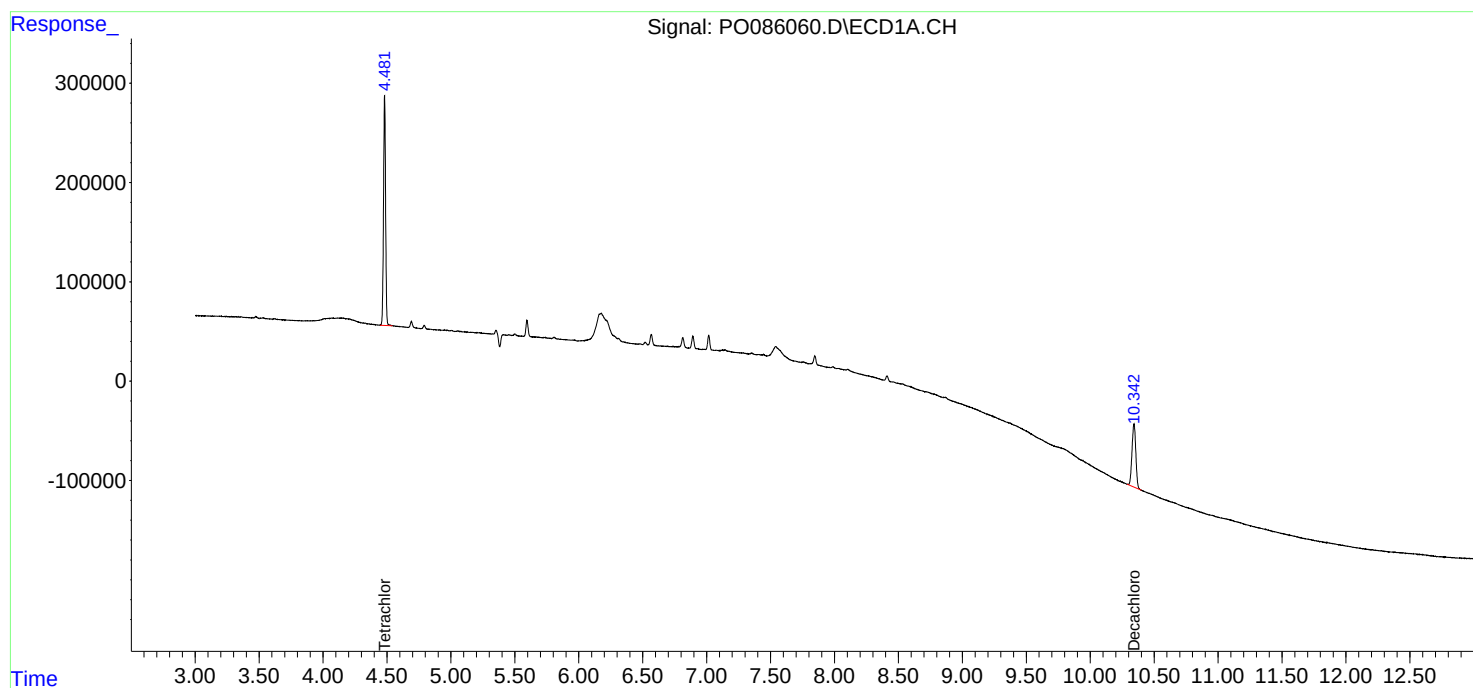


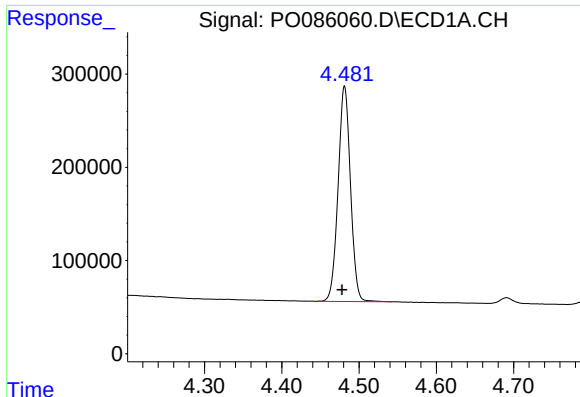

#1 Tetrachloro-m-xylene


R.T.: 4.481 min
Delta R.T.: 0.003 min
Response: 2581884
Conc: 25.42 ng/ml

Instrument :
ECD_O
ClientSampleId :
SB21

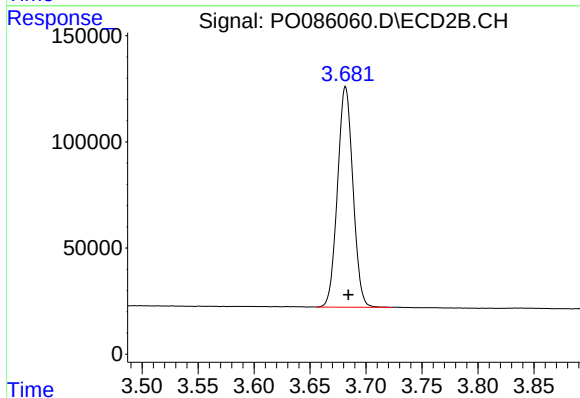


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.002 min
Response: 995865
Conc: 22.85 ng/ml

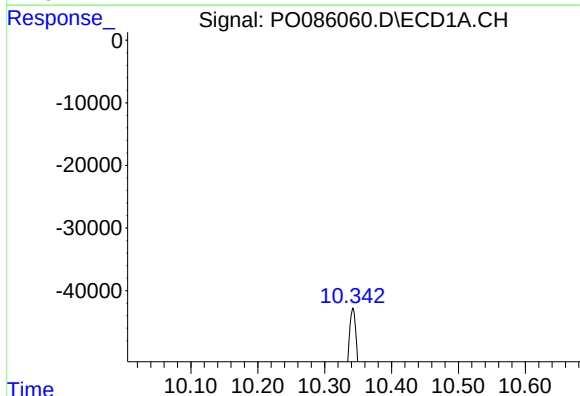

#2 Decachlorobiphenyl

R.T.: 10.342 min
Delta R.T.: 0.015 min
Response: 1313416
Conc: 24.78 ng/ml

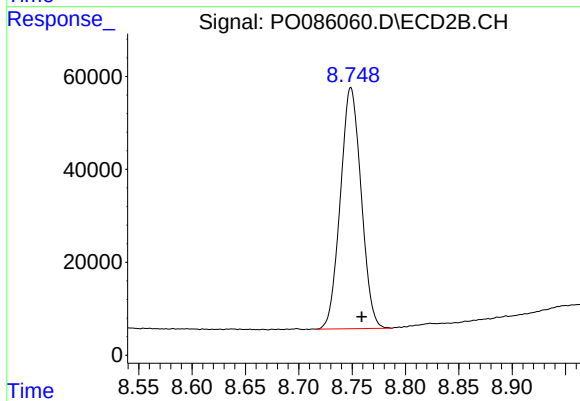

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.010 min
Response: 704654
Conc: 20.76 ng/ml