

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051622\
 Data File : P0086087.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 16 May 2022 23:29
 Operator : YP\AJ
 Sample : N2838-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 TT-044-IDWGW-20220511

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 02:08:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 12 05:35:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.482	3.682	2347879	927147	23.120	21.273
2) SA Decachlor...	10.340	8.746	766966	396773	14.473	11.690

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051622\
Data File : P0086087.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 16 May 2022 23:29
Operator : YP\AJ
Sample : N2838-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
TT-044-IDWGW-20220511

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 02:08:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051122.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 12 05:35:26 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

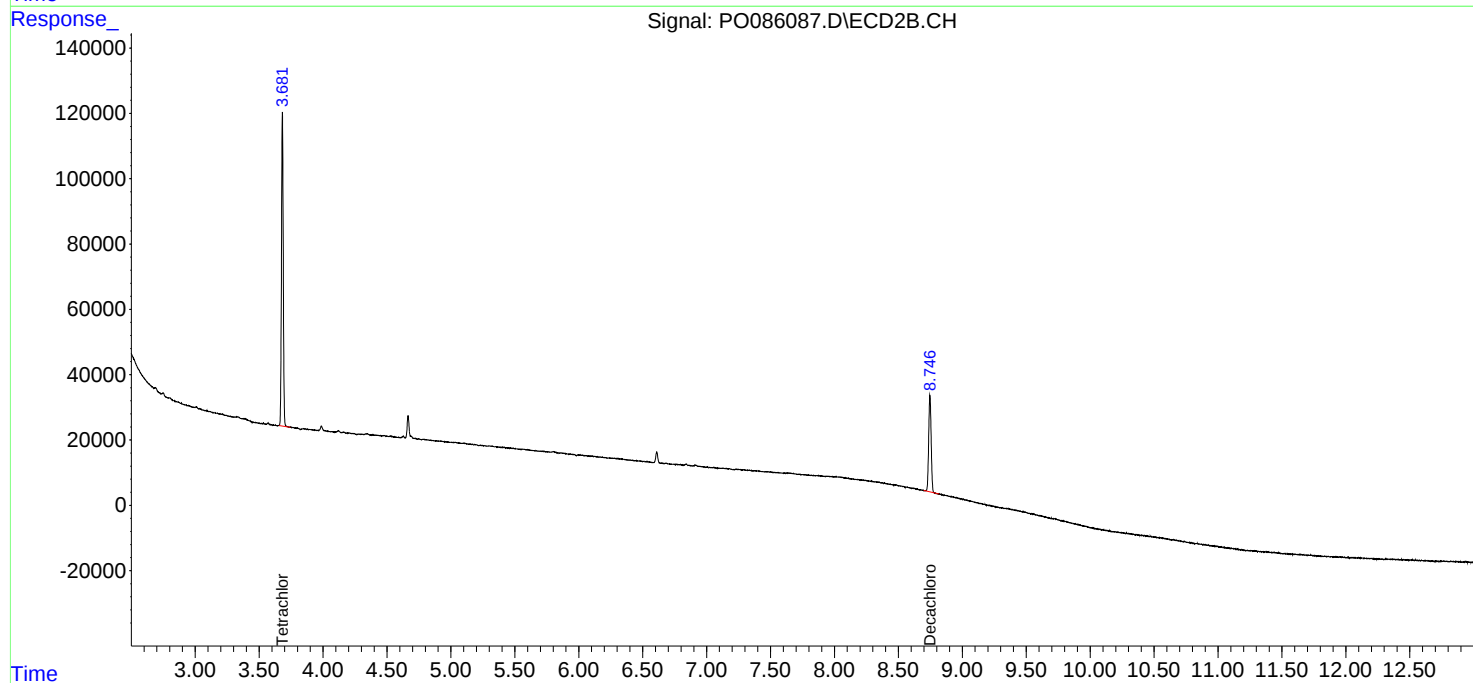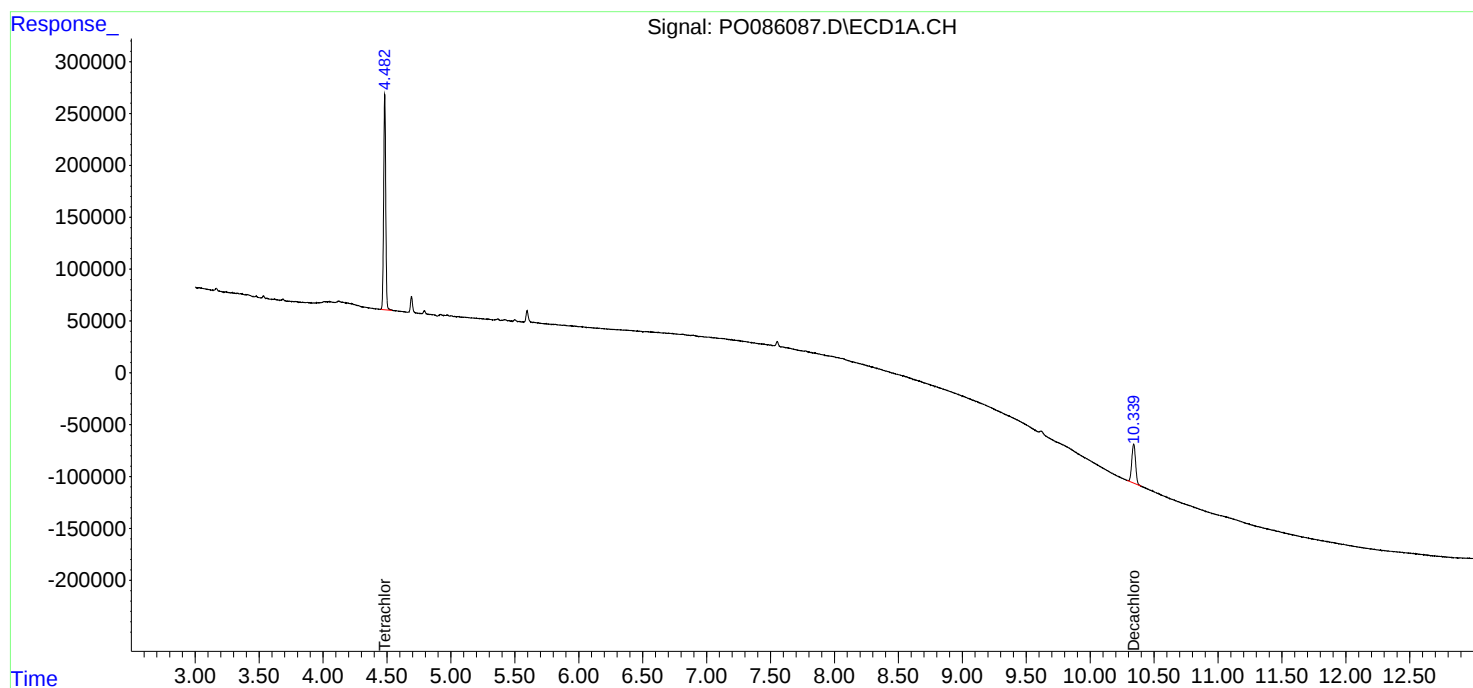


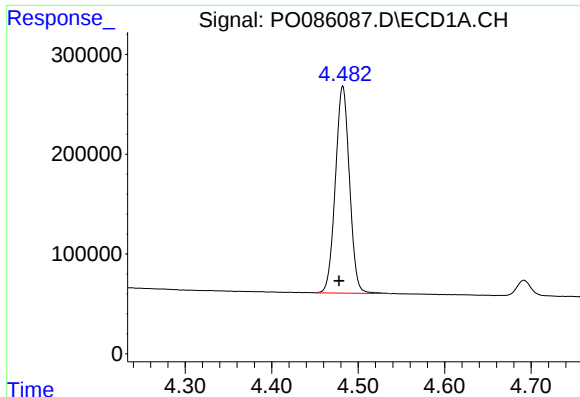

#1 Tetrachloro-m-xylene


R.T.: 4.482 min
Delta R.T.: 0.004 min
Response: 2347879
Conc: 23.12 ng/ml

Instrument :
ECD_O
ClientSampleId :
TT-044-IDWGW-20220511

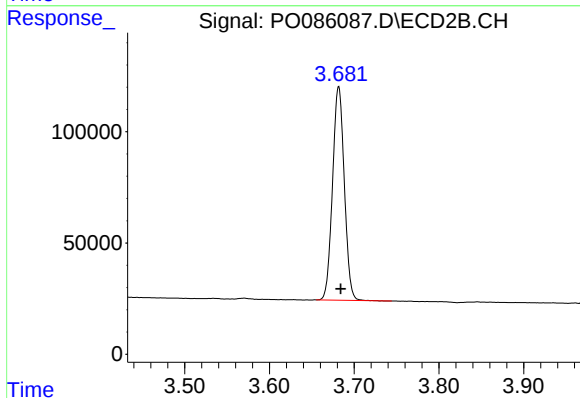


#1 Tetrachloro-m-xylene

R.T.: 3.682 min
Delta R.T.: -0.002 min
Response: 927147
Conc: 21.27 ng/ml

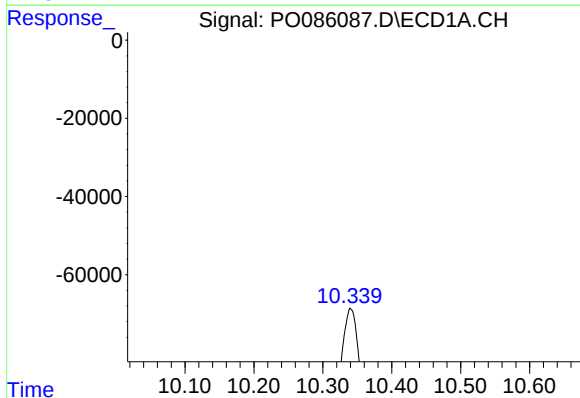

#2 Decachlorobiphenyl

R.T.: 10.340 min
Delta R.T.: 0.013 min
Response: 766966
Conc: 14.47 ng/ml

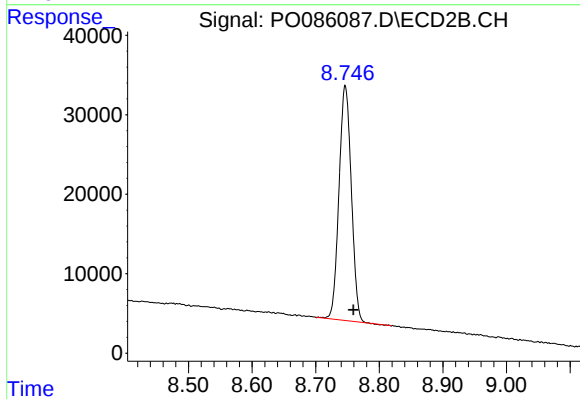

#2 Decachlorobiphenyl

R.T.: 8.746 min
Delta R.T.: -0.013 min
Response: 396773
Conc: 11.69 ng/ml