

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051623\
 Data File : P0095128.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2023 19:22
 Operator : YP/AJ
 Sample : 02783-02 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH4447Y-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/17/2023
 Supervised By :Ankita Jodhani 05/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 21:37:07 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.420	3.618	5133705	2073644	1.490m	1.550m
2) SA Decachlor...	10.282	8.641	5256191	2341022	2.166m	2.080m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051623\
Data File : PO095128.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2023 19:22
Operator : YP/AJ
Sample : 02783-02 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH4447Y-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/17/2023
Supervised By :Ankita Jodhani 05/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 21:37:07 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

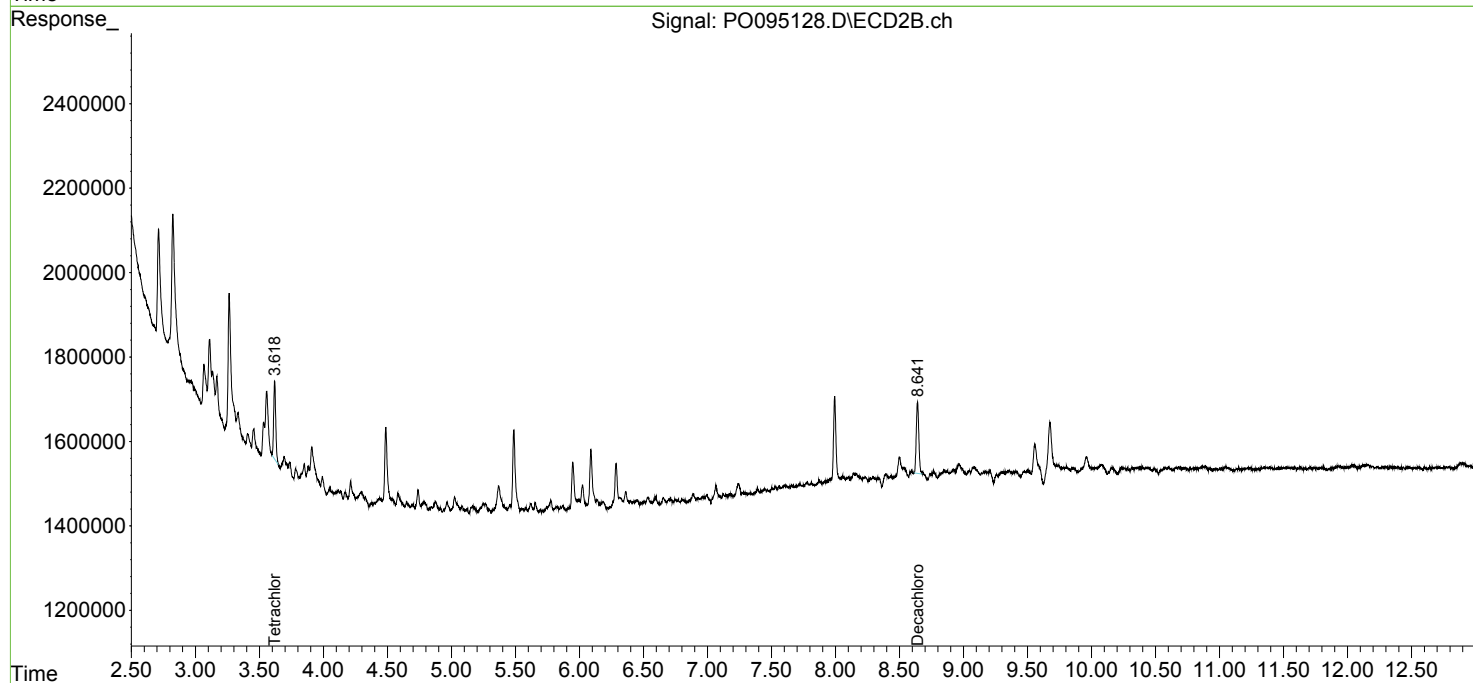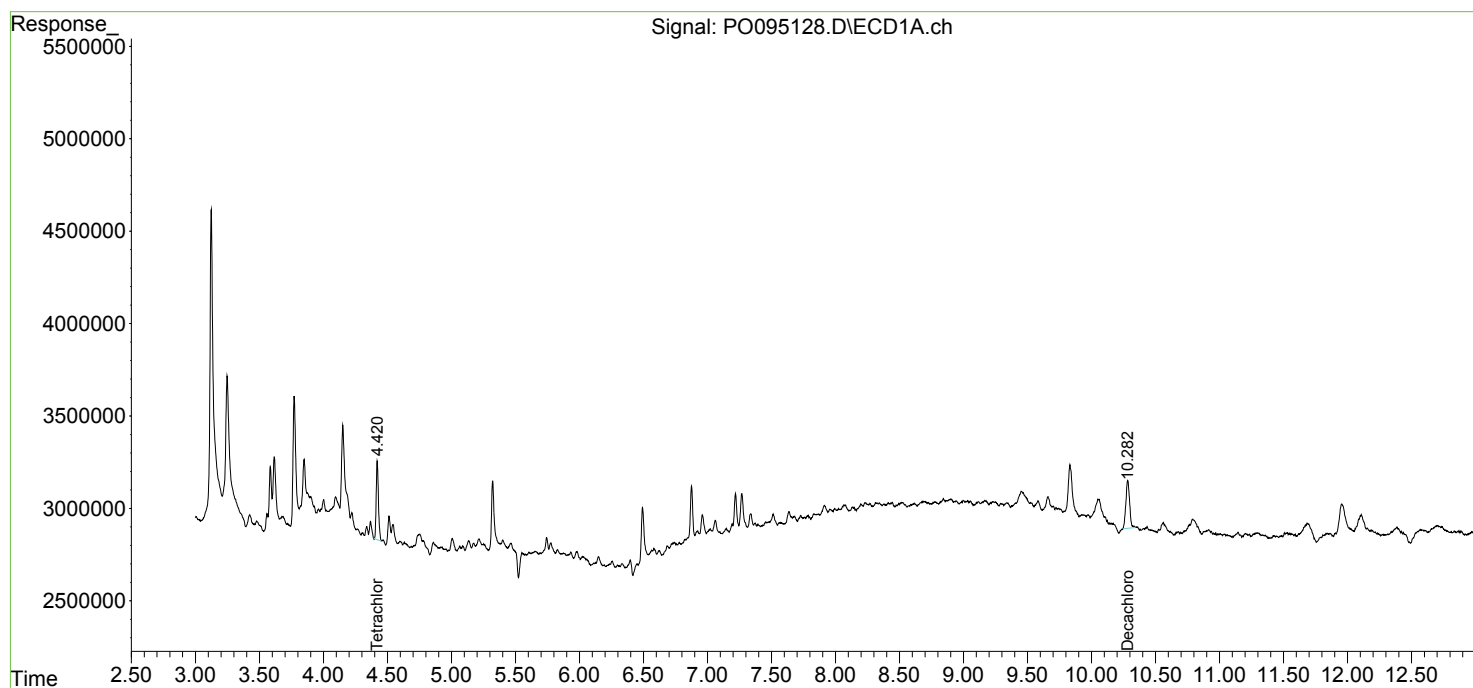

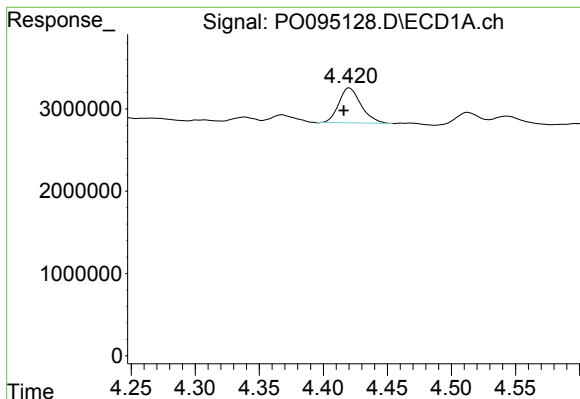


#1 Tetrachloro-m-xylene

R.T.: 4.420 min
Delta R.T.: 0.003 min
Response: 5133705
Conc: 1.49 ng/ml

Instrument :
ECD_O
ClientSampleId :
KMH4447Y-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/17/2023
Supervised By :Ankita Jodhani 05/17/2023

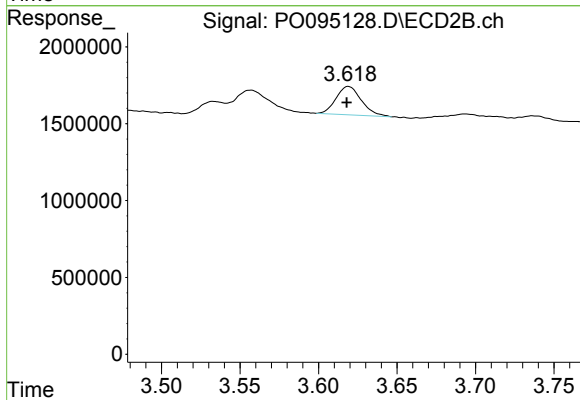


#1 Tetrachloro-m-xylene

R.T.: 3.618 min
Delta R.T.: 0.000 min
Response: 2073644
Conc: 1.55 ng/ml m

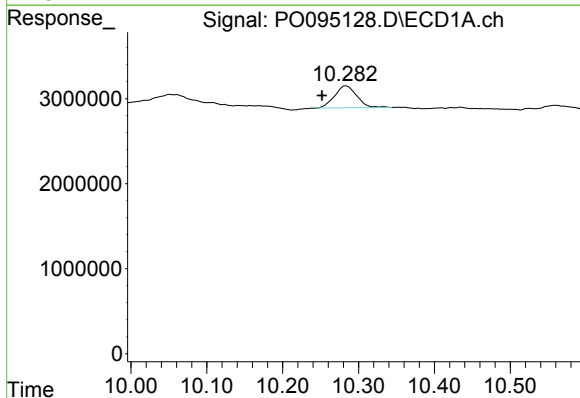

#2 Decachlorobiphenyl

R.T.: 10.282 min
Delta R.T.: 0.030 min
Response: 5256191
Conc: 2.17 ng/ml m

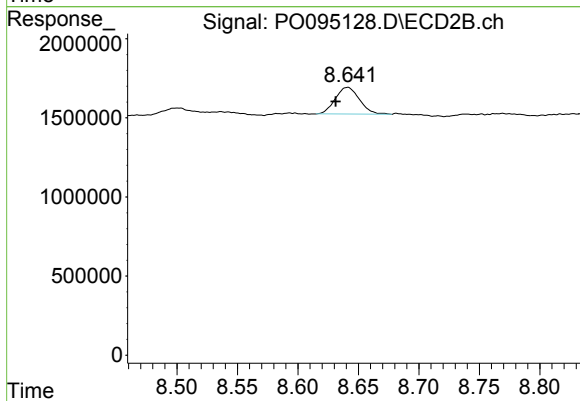

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.010 min
Response: 2341022
Conc: 2.08 ng/ml m