

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051623\
 Data File : P0095129.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 May 2023 19:39
 Operator : YP/AJ
 Sample : 02783-03 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 KMH359L-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/17/2023
 Supervised By :Ankita Jodhani 05/17/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 16 21:38:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0042623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon May 01 11:12:50 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.425	3.623	5813761	2314564	1.688	1.730
2) SA Decachlor...	10.265	8.650	342217	2754200	0.141m	2.447 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0051623\
Data File : P0095129.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2023 19:39
Operator : YP/AJ
Sample : 02783-03 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
KMH359L-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/17/2023
Supervised By :Ankita Jodhani 05/17/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 16 21:38:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0042623.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon May 01 11:12:50 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

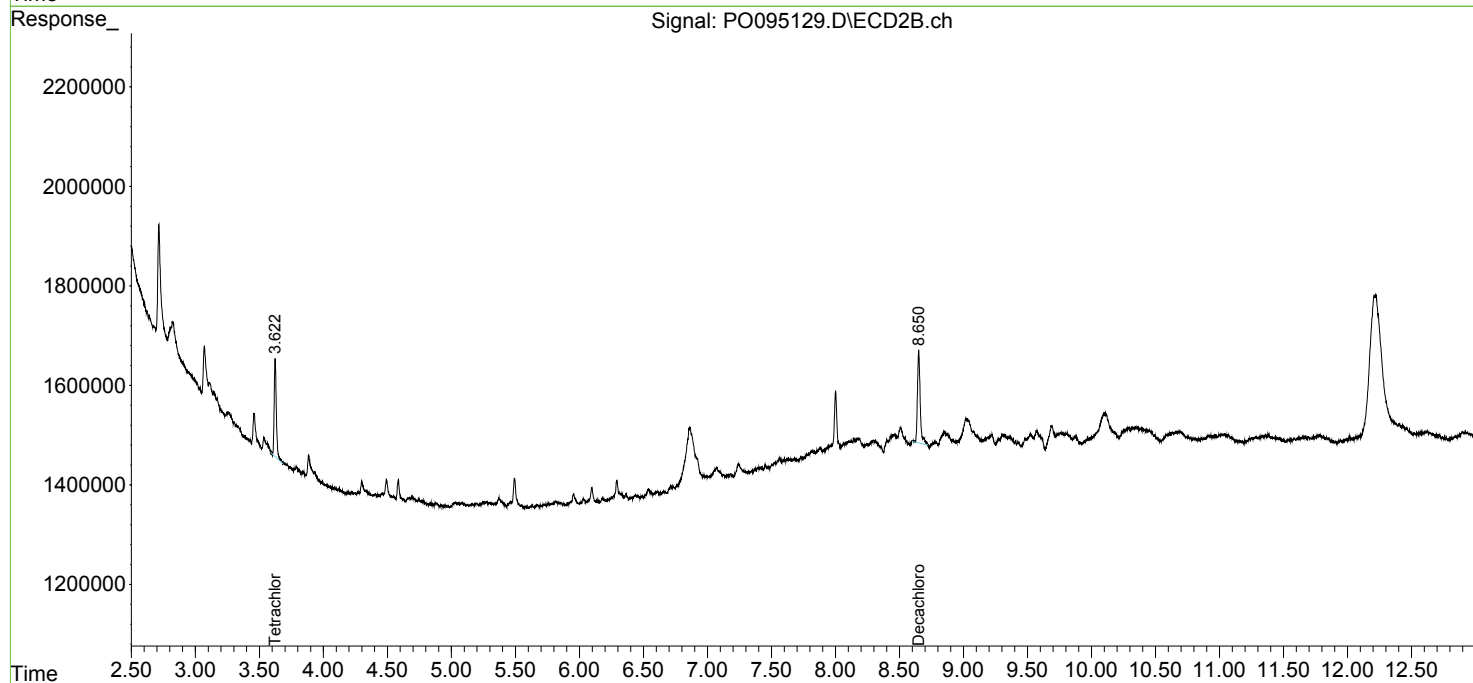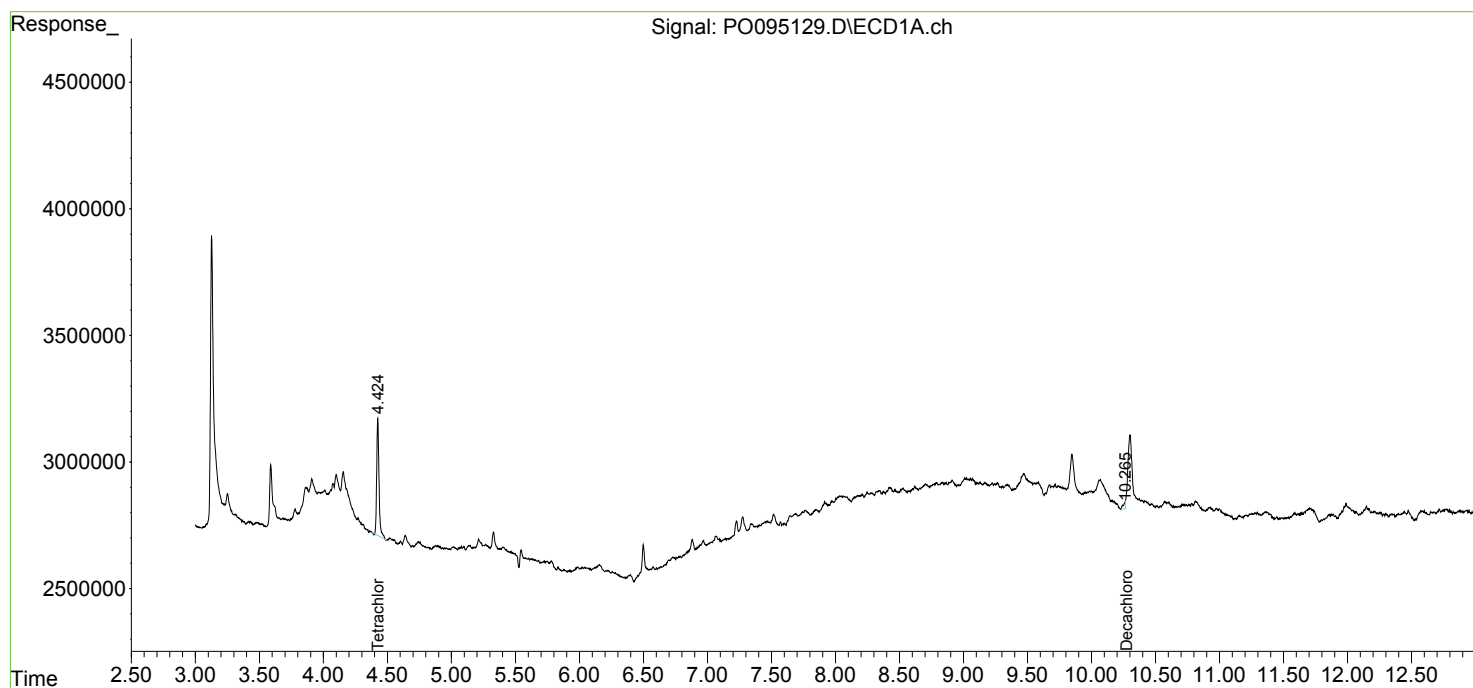

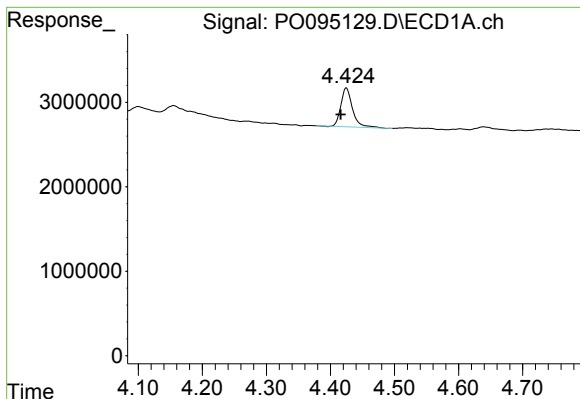

#1 Tetrachloro-m-xylene

R.T.: 4.425 min
Delta R.T.: 0.009 min
Response: 5813761
Conc: 1.69 ng/ml

Instrument :

ECD_O

ClientSampleId :


KMH359L-1-1

Manual Integrations

APPROVED


Reviewed By :Yogesh Patel 05/17/2023

Supervised By :Ankita Jodhani 05/17/2023

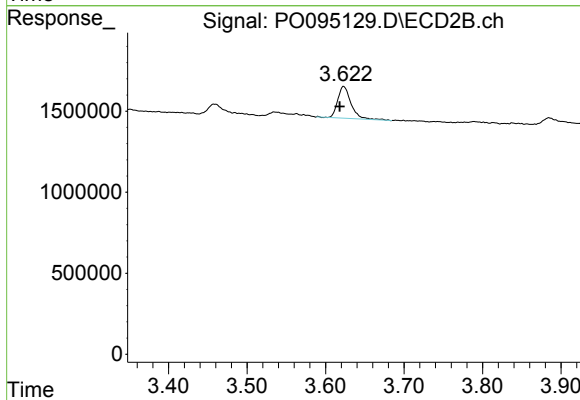


#1 Tetrachloro-m-xylene

R.T.: 3.623 min
Delta R.T.: 0.005 min
Response: 2314564
Conc: 1.73 ng/ml

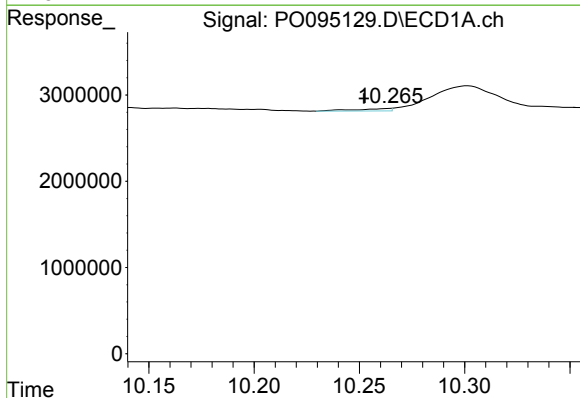

#2 Decachlorobiphenyl

R.T.: 10.265 min
Delta R.T.: 0.013 min
Response: 342217
Conc: 0.14 ng/ml m

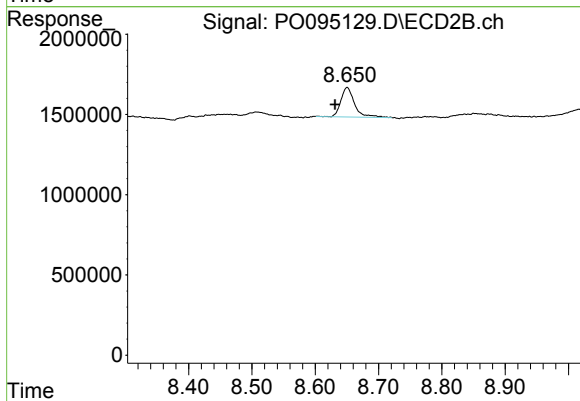

#2 Decachlorobiphenyl

R.T.: 8.650 min
Delta R.T.: 0.019 min
Response: 2754200
Conc: 2.45 ng/ml