

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051624\
Data File : P0103852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 20:20
Operator : YP/AJ
Sample : P2491-03 (Sig #1); P2491-05 (Sig #2)
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2988

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:43:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 16 04:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.450	3.583	161.0E6	55476323	20.925	22.021
2) SA Decachlor...	10.205	8.538	56426542	13988412	11.904	10.753

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\PO051624\
Data File : PO103852.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 May 2024 20:20
Operator : YP/AJ
Sample : P2491-03 (Sig #1); P2491-05 (Sig #2)
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
2988

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 01:43:07 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 16 04:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

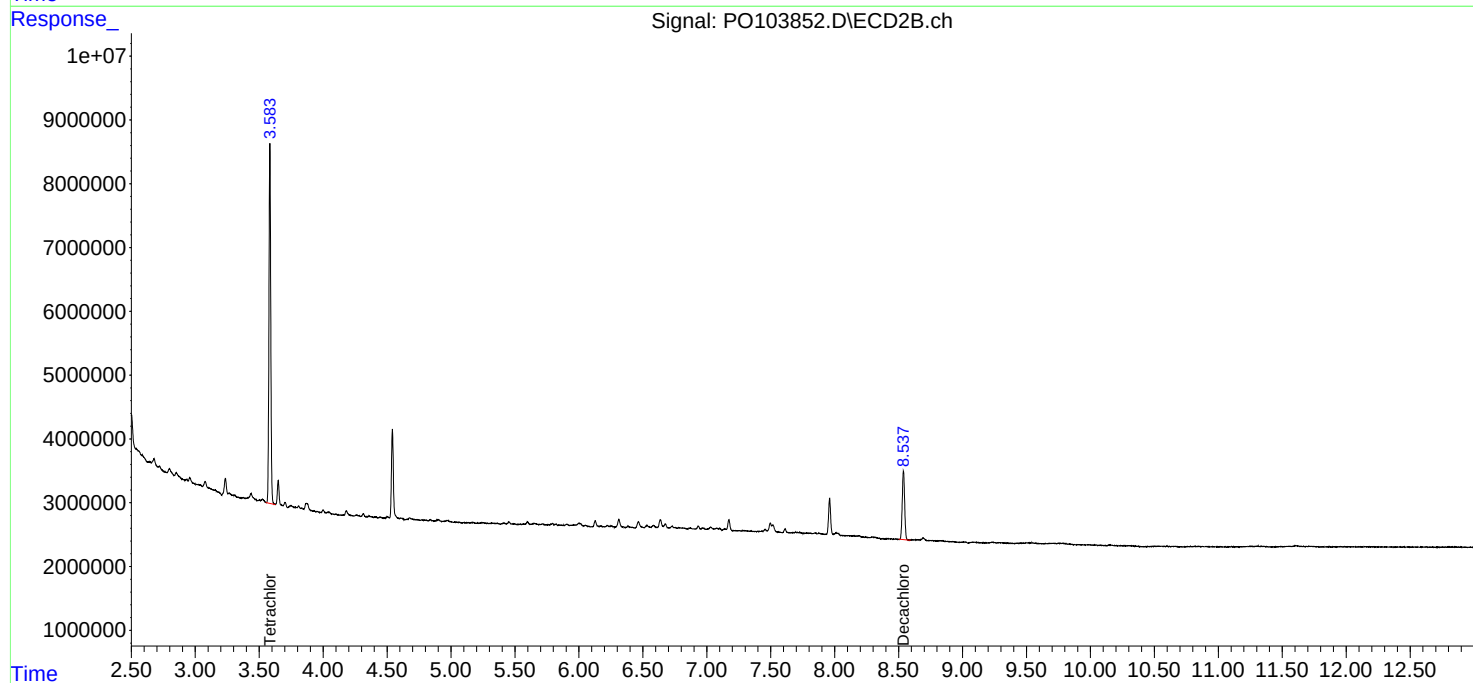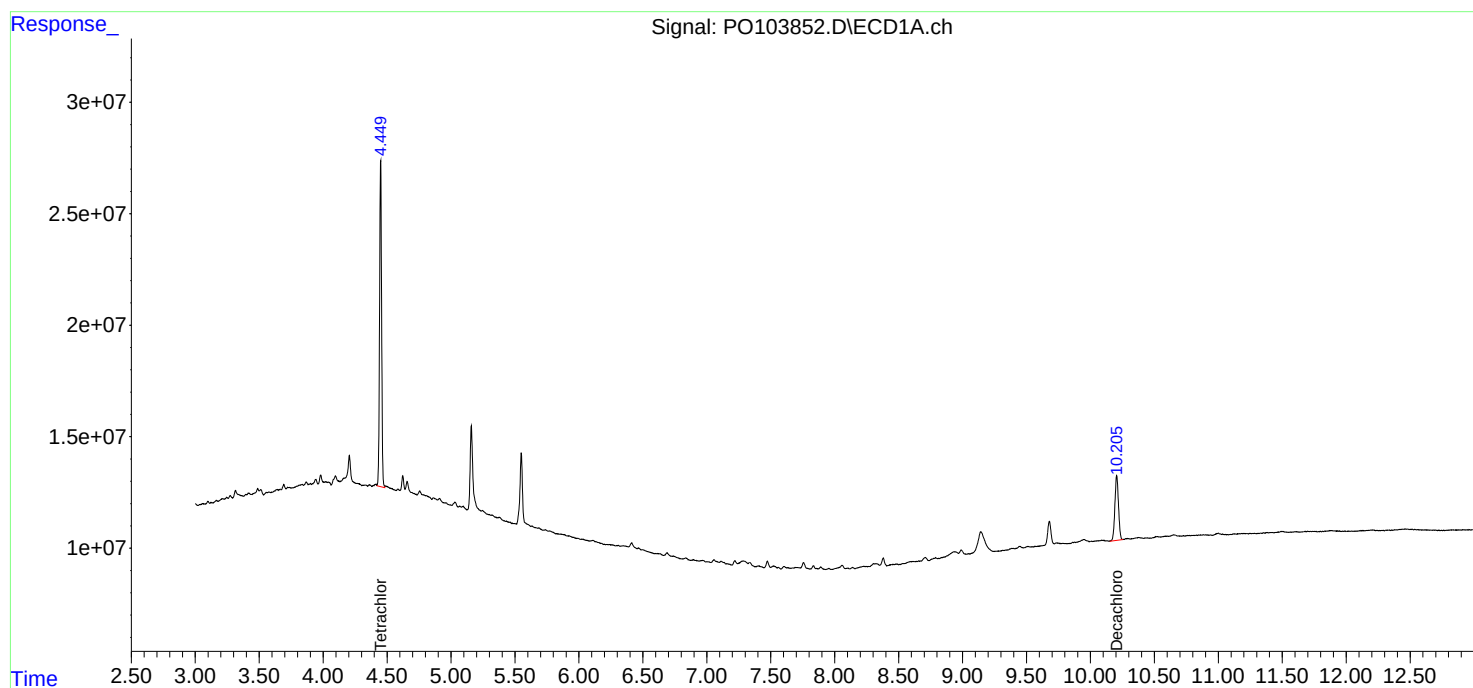


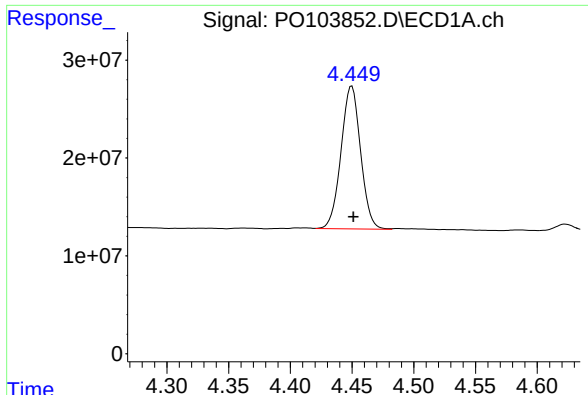

#1 Tetrachloro-m-xylene


R.T.: 4.450 min
Delta R.T.: -0.001 min
Response: 161034940
Conc: 20.93 ng/ml

Instrument :
ECD_O
ClientSampleId :
2988

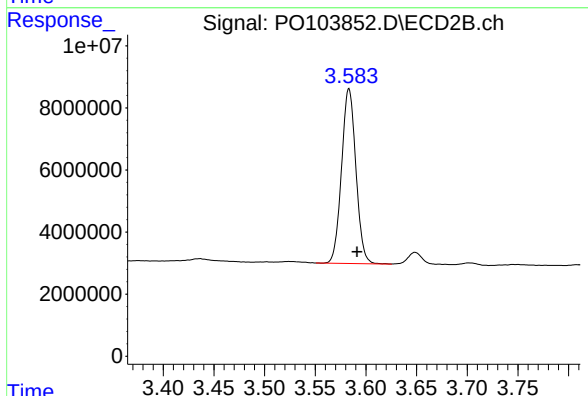


#1 Tetrachloro-m-xylene

R.T.: 3.583 min
Delta R.T.: -0.008 min
Response: 55476323
Conc: 22.02 ng/ml

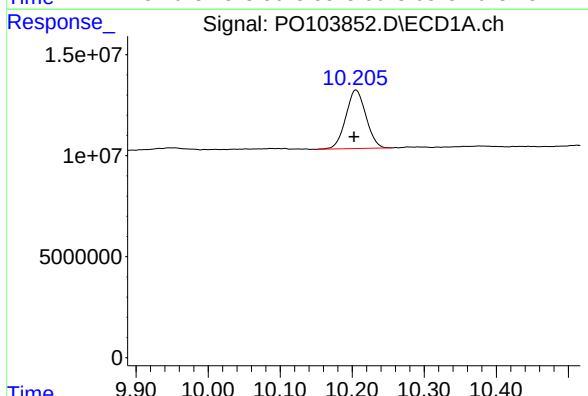

#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.003 min
Response: 56426542
Conc: 11.90 ng/ml

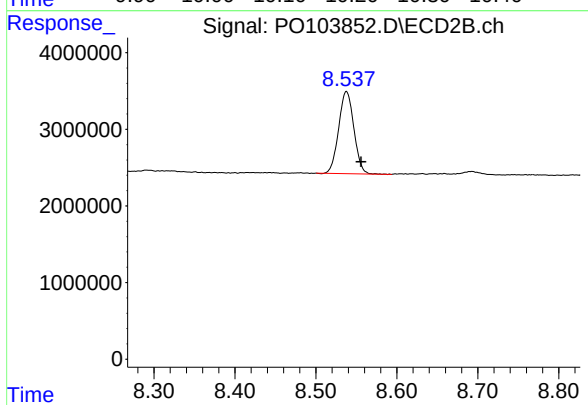

#2 Decachlorobiphenyl

R.T.: 8.538 min
Delta R.T.: -0.018 min
Response: 13988412
Conc: 10.75 ng/ml