

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051624\
 Data File : P0103872.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2024 02:57
 Operator : YP/AJ
 Sample : P2403-09
 Misc : AR1221 MDL 25 PPB
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 03:54:55 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 16 04:14:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.449	3.583	151.2E6	49845488	19.650	19.786
2)	SA Decachlor...	10.207	8.537	105.6E6	25751534	22.282	19.795
Target Compounds							
8)	L2 AR-1221-1	4.659	3.796	2797586	432707	31.518m	14.051 #
9)	L2 AR-1221-2	4.755	3.880	2854812	1054420	42.412m	43.352
10)	L2 AR-1221-3	4.819	3.956	6604216	1348399	32.880m	18.814m#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051624\
Data File : PO103872.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 02:57
Operator : YP/AJ
Sample : P2403-09
Misc : AR1221 MDL 25 PPB
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 03:54:55 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 16 04:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

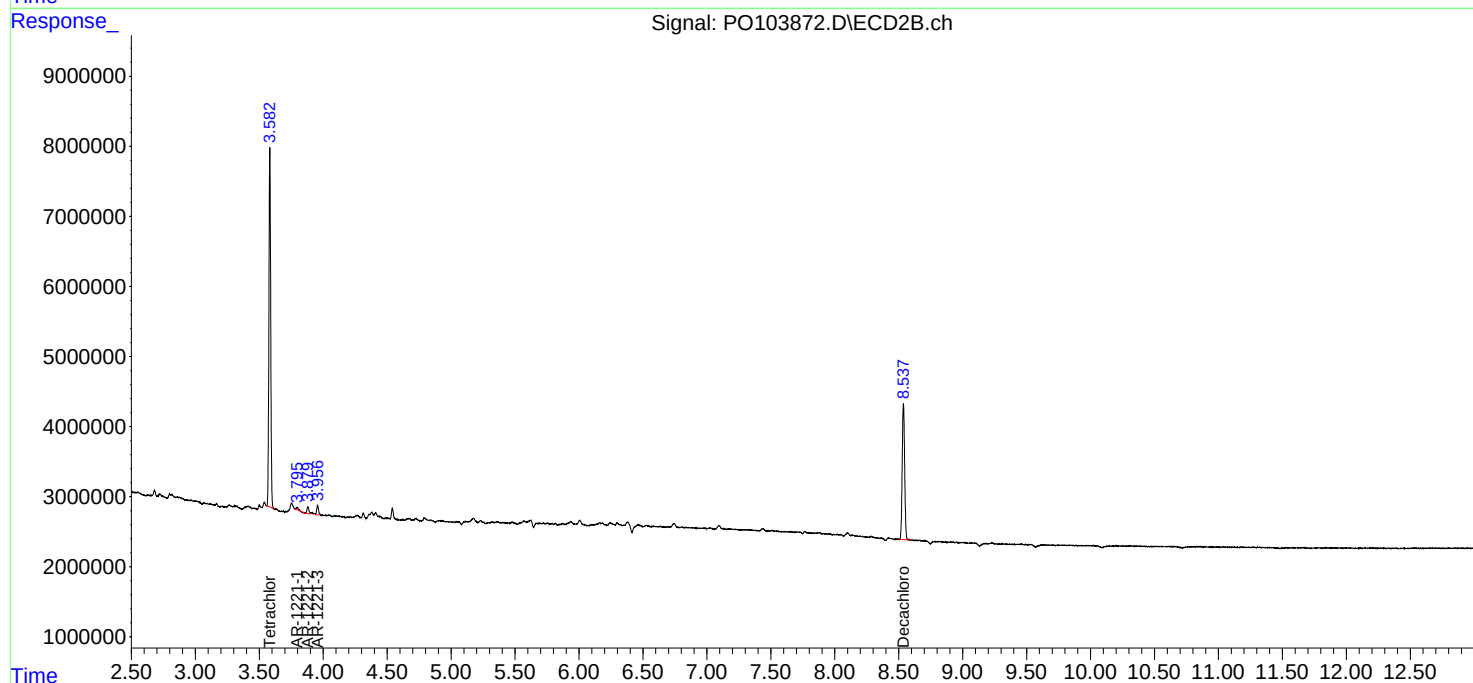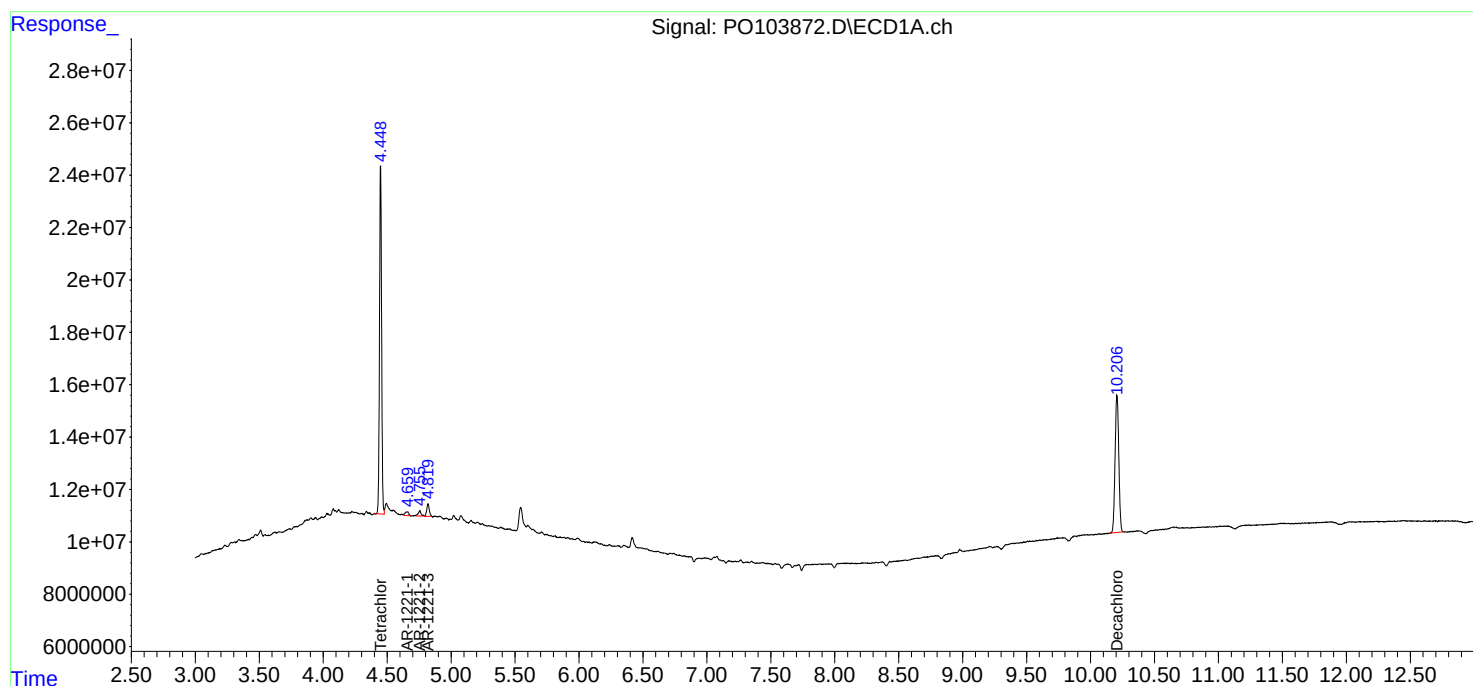


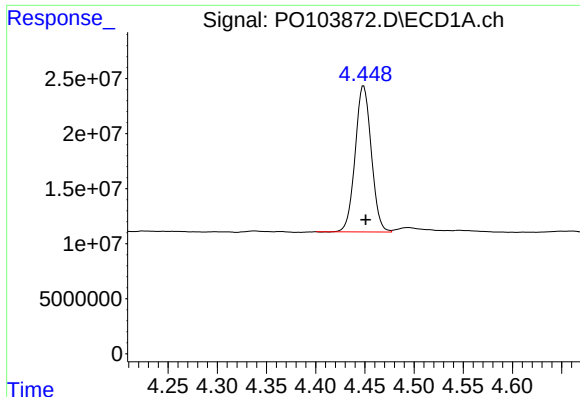

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 151218373
Conc: 19.65 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

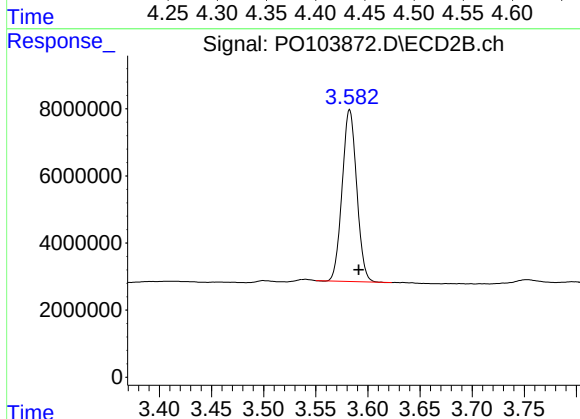


#1 Tetrachloro-m-xylene

R.T.: 3.583 min
Delta R.T.: -0.009 min
Response: 49845488
Conc: 19.79 ng/ml

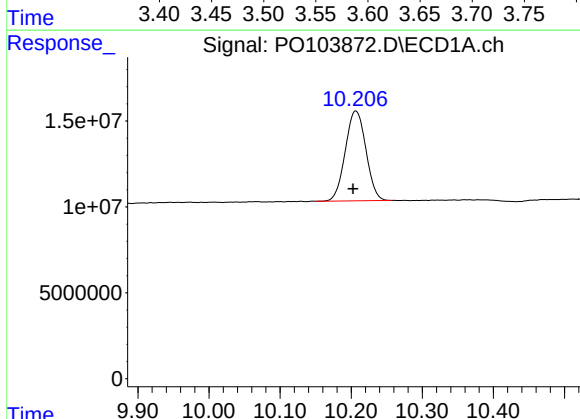


#2 Decachlorobiphenyl

R.T.: 10.207 min
Delta R.T.: 0.004 min
Response: 105622670
Conc: 22.28 ng/ml

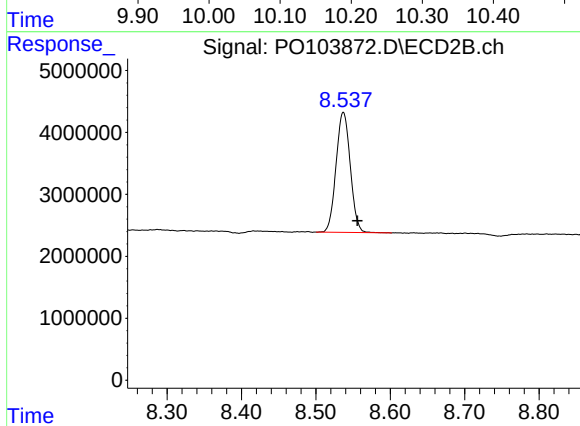

#2 Decachlorobiphenyl


R.T.: 8.537 min
Delta R.T.: -0.019 min
Response: 25751534
Conc: 19.80 ng/ml

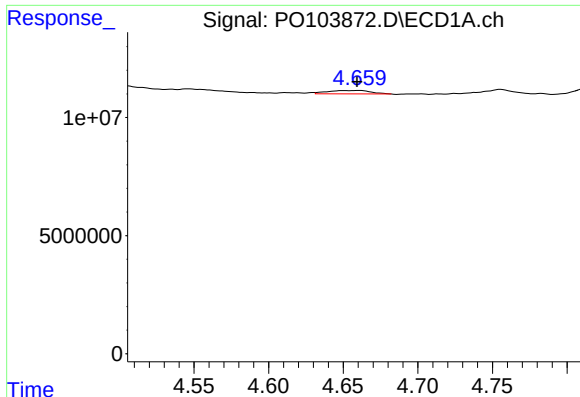

#8 AR-1221-1


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 2797586
Conc: 31.52 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

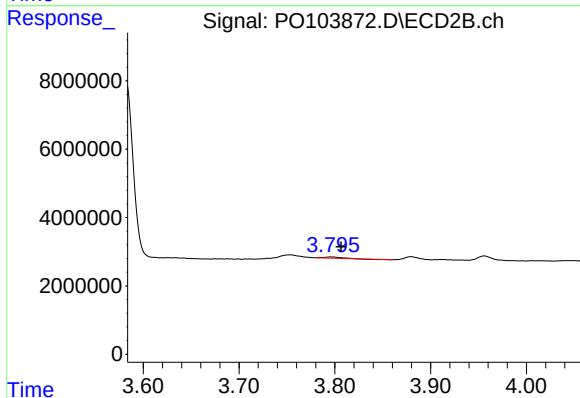


#8 AR-1221-1

R.T.: 3.796 min
Delta R.T.: -0.011 min
Response: 432707
Conc: 14.05 ng/ml

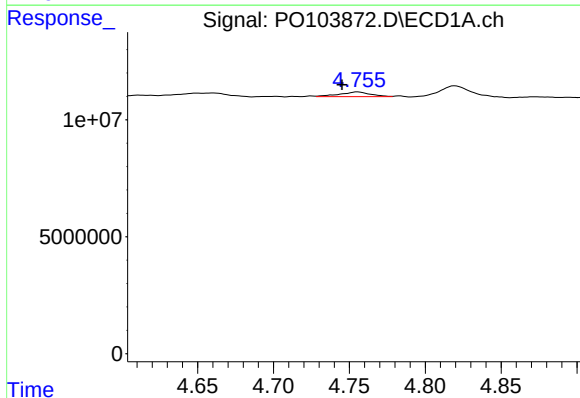


#9 AR-1221-2

R.T.: 4.755 min
Delta R.T.: 0.009 min
Response: 2854812
Conc: 42.41 ng/ml m

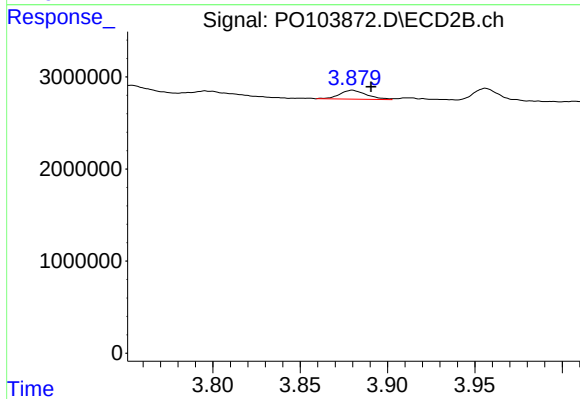

#9 AR-1221-2


R.T.: 3.880 min
Delta R.T.: -0.011 min
Response: 1054420
Conc: 43.35 ng/ml

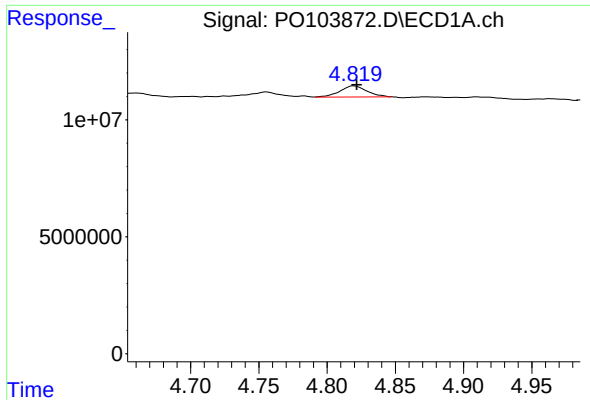

#10 AR-1221-3

R.T.: 4.819 min
Delta R.T.: -0.003 min
Response: 6604216
Conc: 32.88 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

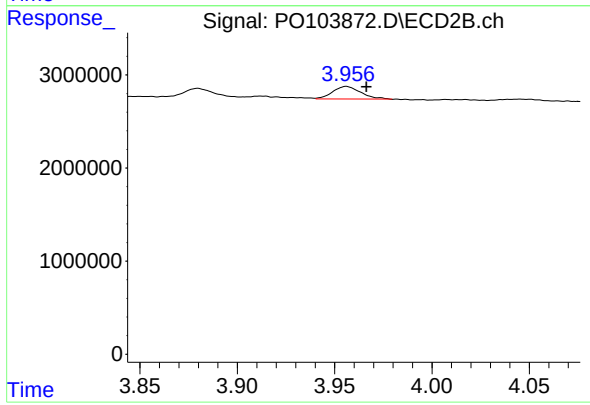

#10 AR-1221-3

R.T.: 3.956 min
Delta R.T.: -0.011 min
Response: 1348399
Conc: 18.81 ng/ml m