

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051624\
 Data File : P0103877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 May 2024 04:22
 Operator : YP/AJ
 Sample : P2403-09
 Misc : AR1262 MDL 25 PPB
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 17 05:24:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0050624.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 16 04:14:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.449	3.582	104.6E6	35000995	13.592	13.894m
2)	SA Decachlor...	10.205	8.536	71433349	17958498	15.070	13.805
Target Compounds							
36)	L8 AR-1262-1	7.753	6.636	3503894	1384415	15.217	18.056
37)	L8 AR-1262-2	8.379	6.932	11133451	2165439	17.150	18.376
38)	L8 AR-1262-3	8.694	7.454	7003848	1506588	16.338	16.674
39)	L8 AR-1262-4	8.784	7.517	5749487	2915054	17.110	17.449
40)	L8 AR-1262-5	9.443	8.007	3795324	1154388	16.005	16.001



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051624\
Data File : PO103877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 May 2024 04:22
Operator : YP/AJ
Sample : P2403-09
Misc : AR1262 MDL 25 PPB
ALS Vial : 43 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 17 05:24:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO050624.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 16 04:14:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

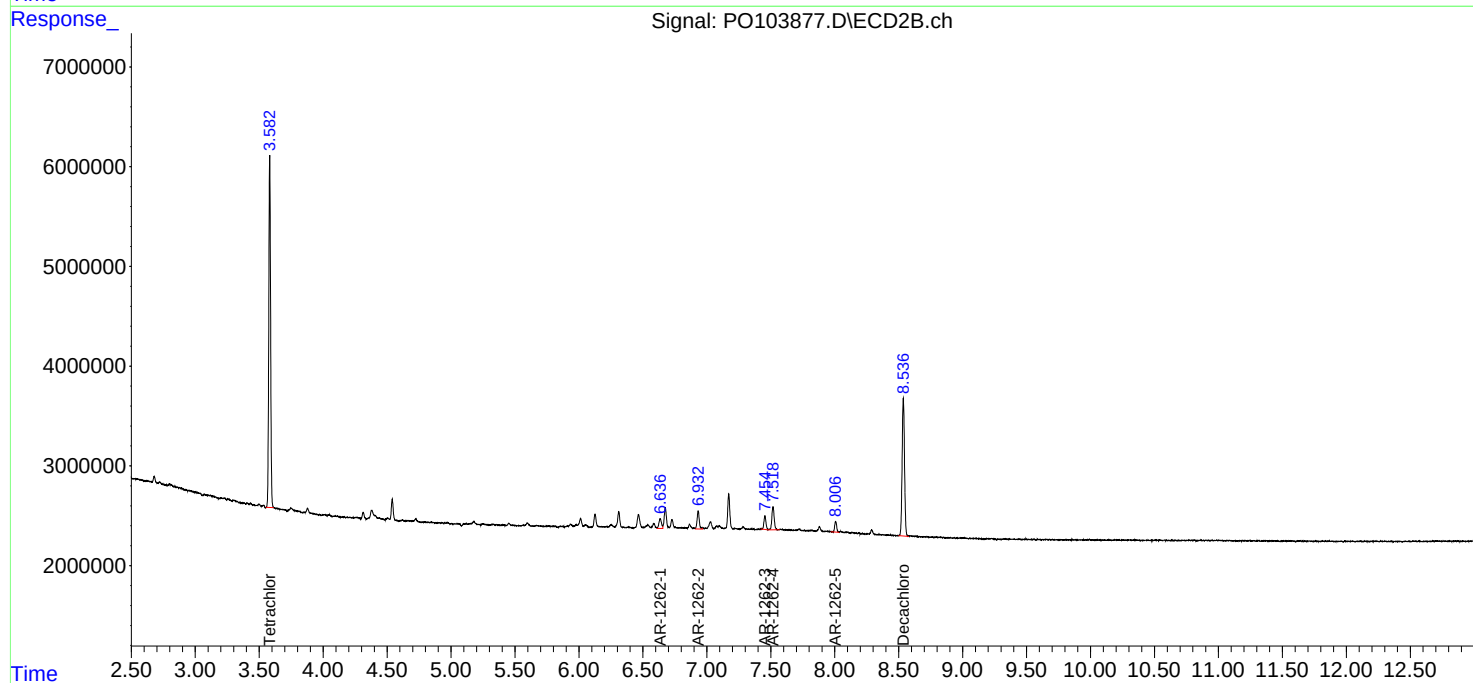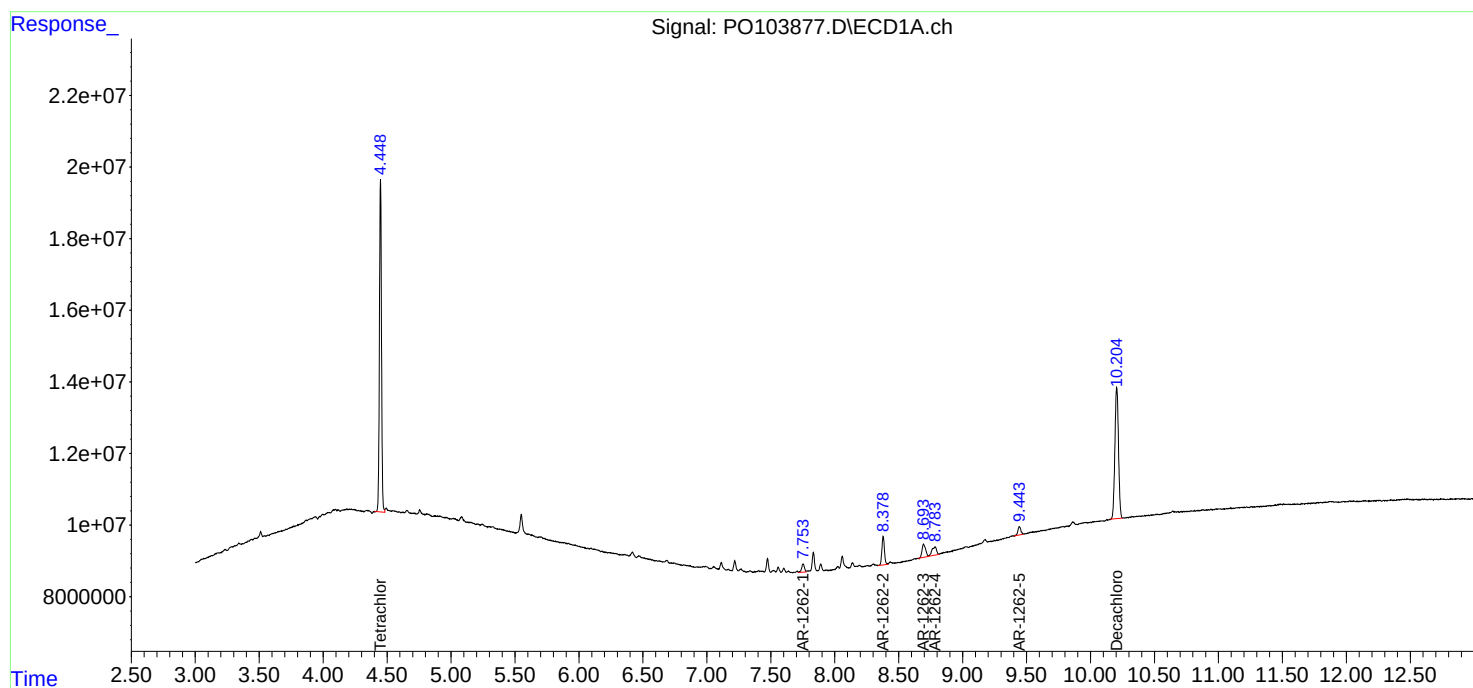


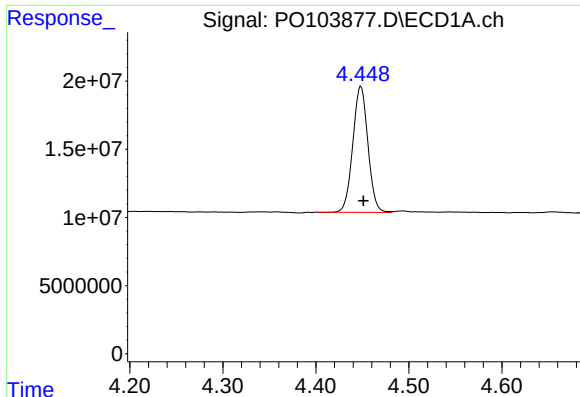

#1 Tetrachloro-m-xylene


R.T.: 4.449 min
Delta R.T.: -0.002 min
Response: 104600710
Conc: 13.59 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

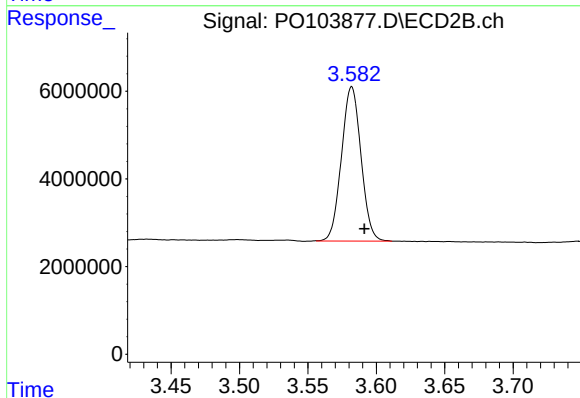


#1 Tetrachloro-m-xylene

R.T.: 3.582 min
Delta R.T.: -0.010 min
Response: 35000995
Conc: 13.89 ng/ml m

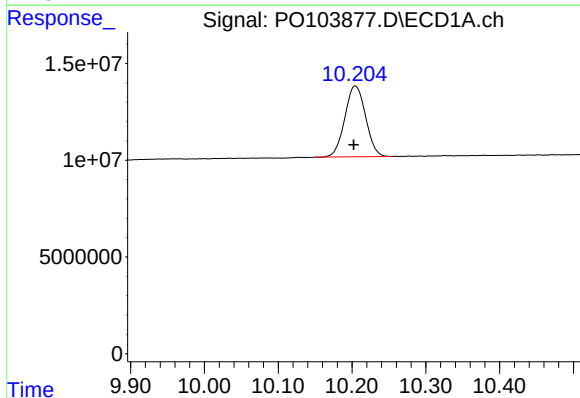


#2 Decachlorobiphenyl

R.T.: 10.205 min
Delta R.T.: 0.002 min
Response: 71433349
Conc: 15.07 ng/ml

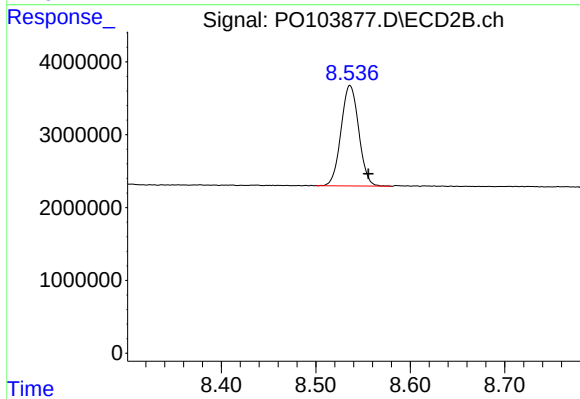

#2 Decachlorobiphenyl


R.T.: 8.536 min
Delta R.T.: -0.020 min
Response: 17958498
Conc: 13.80 ng/ml

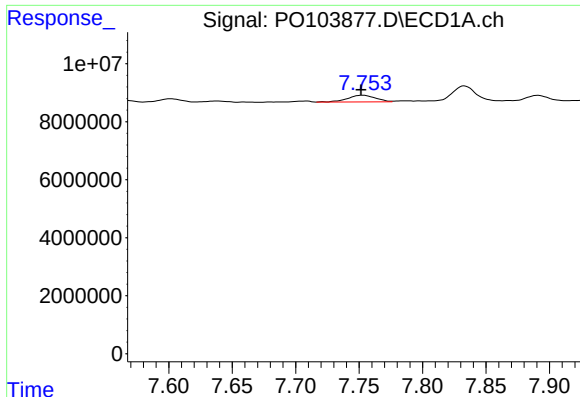

#36 AR-1262-1


R.T.: 7.753 min
Delta R.T.: 0.002 min
Response: 3503894
Conc: 15.22 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

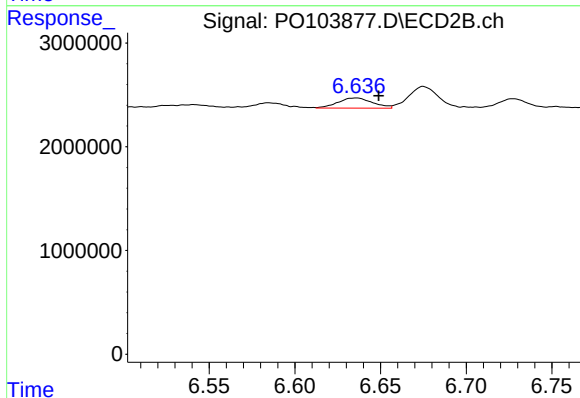


#36 AR-1262-1

R.T.: 6.636 min
Delta R.T.: -0.013 min
Response: 1384415
Conc: 18.06 ng/ml

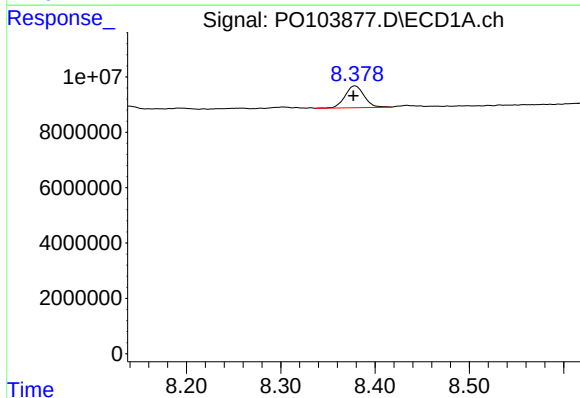


#37 AR-1262-2

R.T.: 8.379 min
Delta R.T.: 0.002 min
Response: 11133451
Conc: 17.15 ng/ml

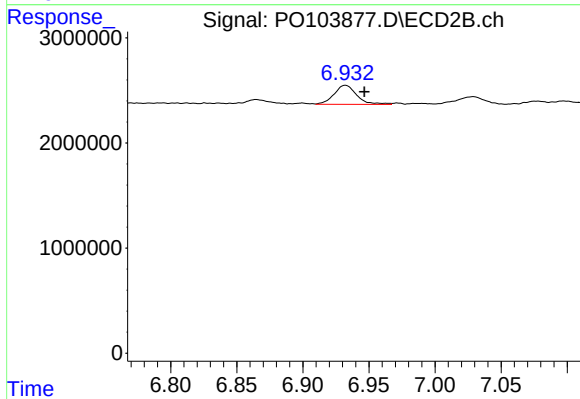

#37 AR-1262-2


R.T.: 6.932 min
Delta R.T.: -0.014 min
Response: 2165439
Conc: 18.38 ng/ml

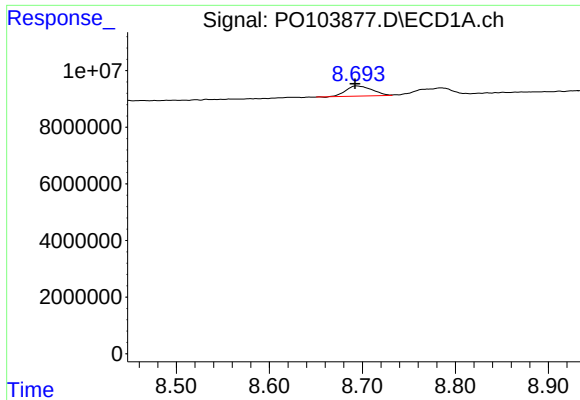

#38 AR-1262-3


R.T.: 8.694 min
Delta R.T.: 0.001 min
Response: 7003848
Conc: 16.34 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

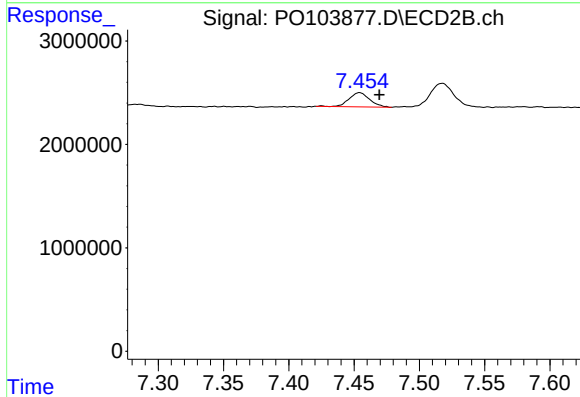


#38 AR-1262-3

R.T.: 7.454 min
Delta R.T.: -0.015 min
Response: 1506588
Conc: 16.67 ng/ml

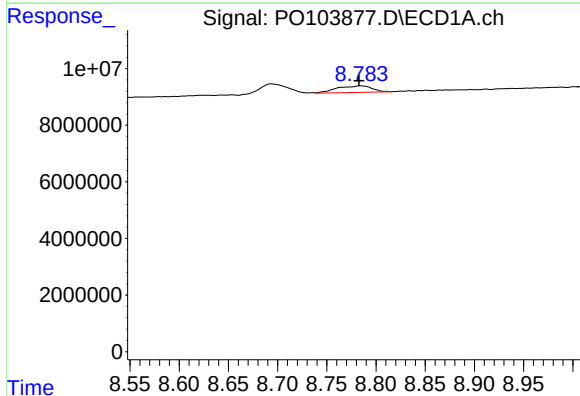


#39 AR-1262-4

R.T.: 8.784 min
Delta R.T.: 0.001 min
Response: 5749487
Conc: 17.11 ng/ml

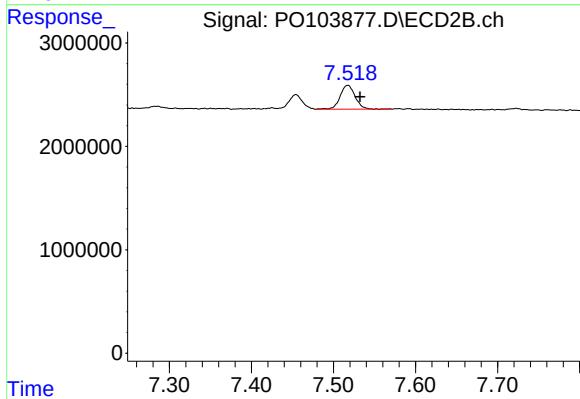

#39 AR-1262-4


R.T.: 7.517 min
Delta R.T.: -0.015 min
Response: 2915054
Conc: 17.45 ng/ml

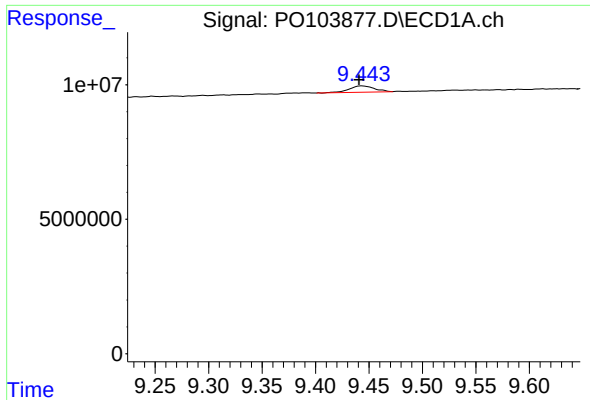

#40 AR-1262-5

R.T.: 9.443 min
Delta R.T.: 0.003 min
Response: 3795324
Conc: 16.00 ng/ml

Instrument :
ECD_O
ClientSampleId :
MDL-WATER-03-QT2-2024

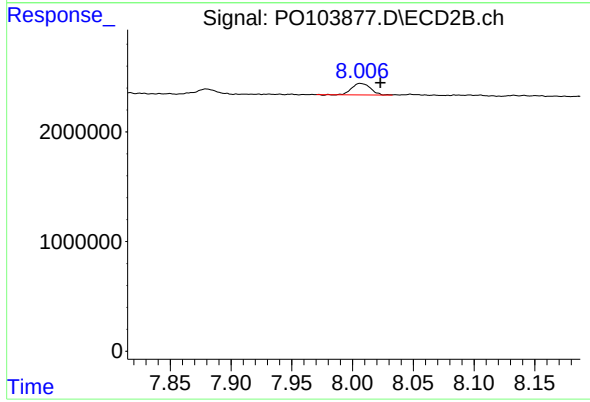

#40 AR-1262-5

R.T.: 8.007 min
Delta R.T.: -0.016 min
Response: 1154388
Conc: 16.00 ng/ml