

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051625\
 Data File : P0111100.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 May 2025 11:46
 Operator : YP/AJ
 Sample : Q2046-01 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 BC136902-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 05/16/2025
 Supervised By :mohammad ahmed 05/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 15 12:31:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051525.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu May 15 07:11:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.683	3.679	9249696	6179605	1.572	1.134m#
2) SA Decachlor...	8.726	8.674	5509984	1980942	1.067m	1.071m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\PO051625\
Data File : PO111100.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 May 2025 11:46
Operator : YP/AJ
Sample : Q2046-01 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
BC136902-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2025
Supervised By :mohammad ahmed 05/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 15 12:31:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\PO051525.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu May 15 07:11:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

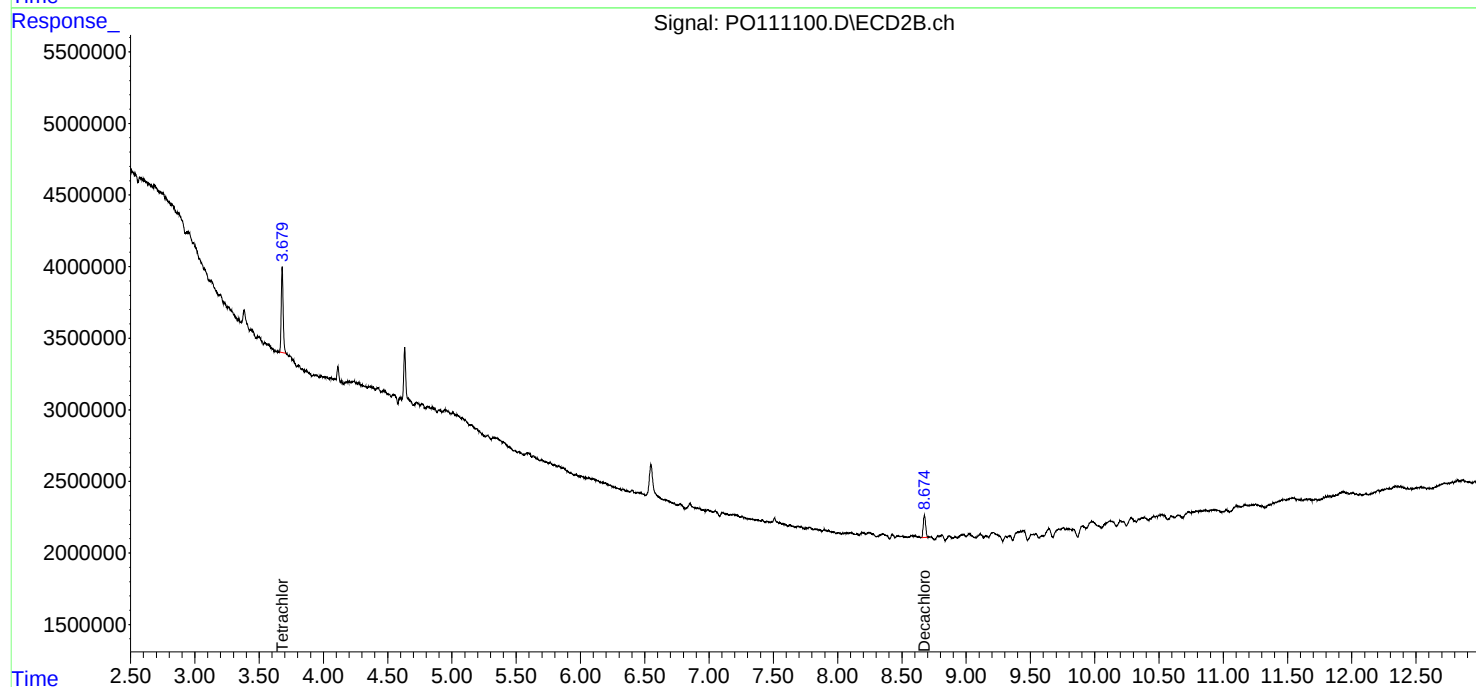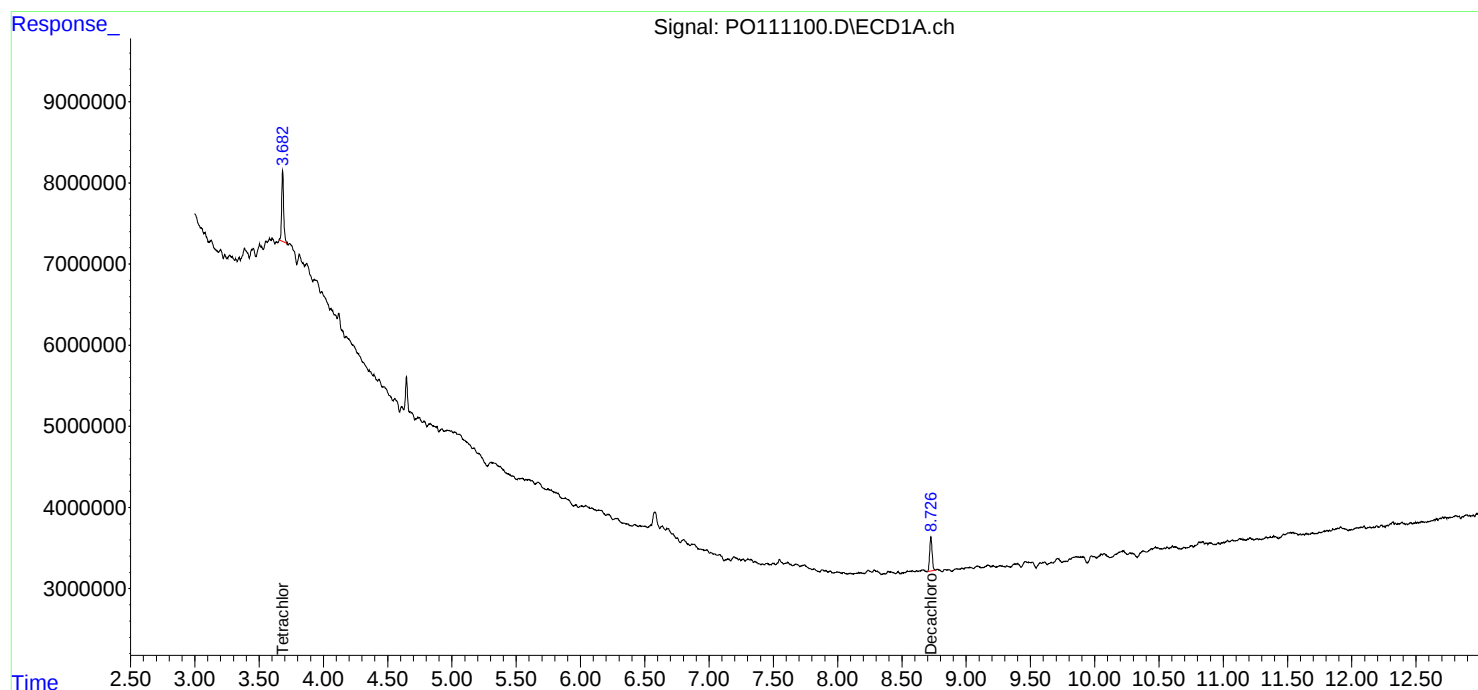

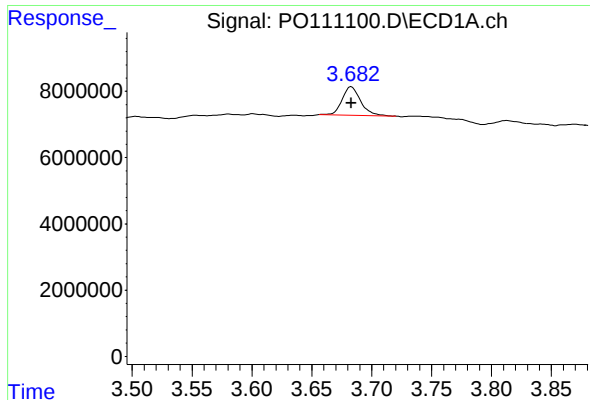


#1 Tetrachloro-m-xylene

R.T.: 3.683 min
Delta R.T.: 0.000 min
Response: 9249696
Conc: 1.57 ng/ml

Instrument :
ECD_O
ClientSampleId :
BC136902-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 05/16/2025
Supervised By :mohammad ahmed 05/19/2025

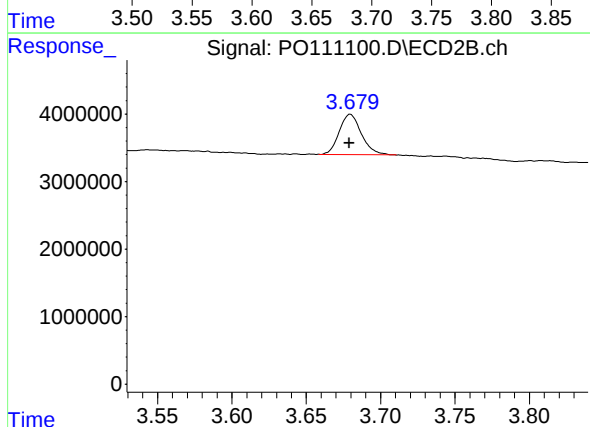


#1 Tetrachloro-m-xylene

R.T.: 3.679 min
Delta R.T.: 0.000 min
Response: 6179605
Conc: 1.13 ng/ml m

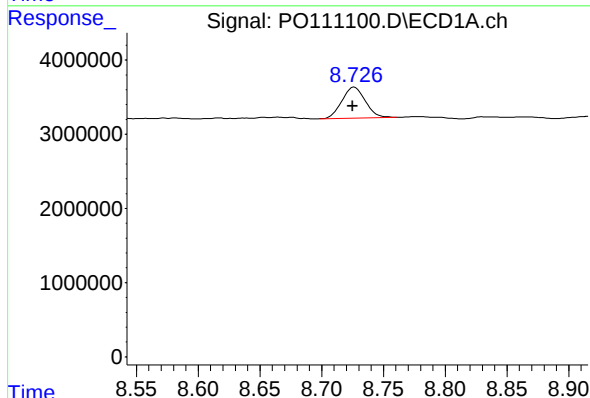

#2 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: 0.000 min
Response: 5509984
Conc: 1.07 ng/ml m

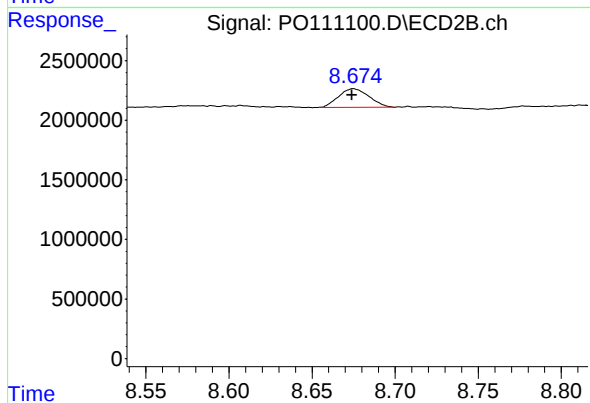

#2 Decachlorobiphenyl

R.T.: 8.674 min
Delta R.T.: 0.000 min
Response: 1980942
Conc: 1.07 ng/ml m