

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
 Data File : P0077892.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 May 2021 19:00
 Operator : DD\AJ
 Sample : M2415-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: May 18 04:25:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri May 14 05:52:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.349	3.630	1512989	681424	25.775	26.780
2)	SA Decachlor...	9.965	8.823	1014015	634215	24.528	26.390
Target Compounds							
8)	L2 AR-1221-1	4.594	0.000	32861	0	47.544	N.D. #
9)	L2 AR-1221-2	4.692	3.972	17869	10048	35.129	42.090
29)	L6 AR-1254-4	0.000	6.508f	0	7556	N.D.	6.036 #
34)	L7 AR-1260-4	8.152	7.273f	35091	9888	16.069	8.173 #
35)	L7 AR-1260-5	8.469	0.000	3920	0	0.906	N.D. #
37)	L8 AR-1262-2	8.469	0.000	3920	0	0.763	N.D. #
45)	L9 AR-1268-5	0.000	8.604	0	5345	N.D.	0.622 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_O\Data\P0051721\
Data File : P0077892.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 May 2021 19:00
Operator : DD\AJ
Sample : M2415-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: May 18 04:25:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_O\methods\P0051321.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri May 14 05:52:29 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

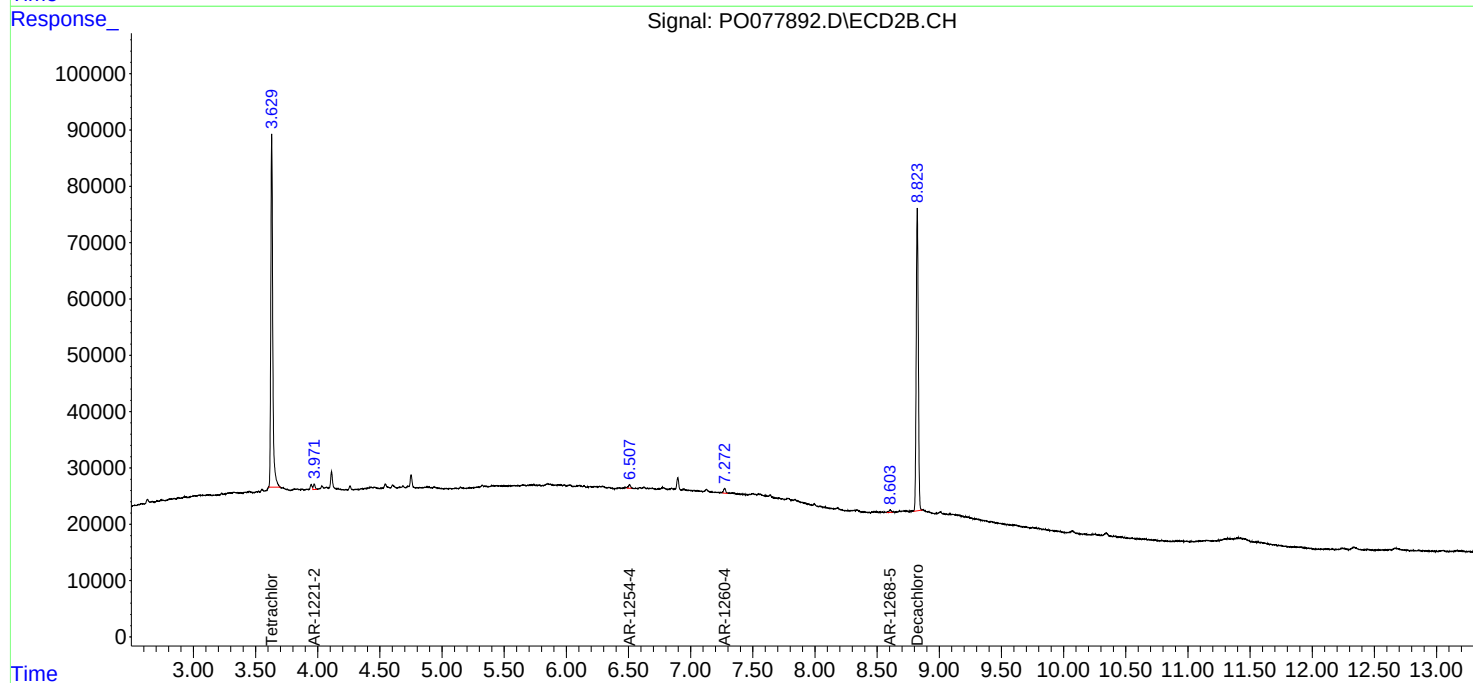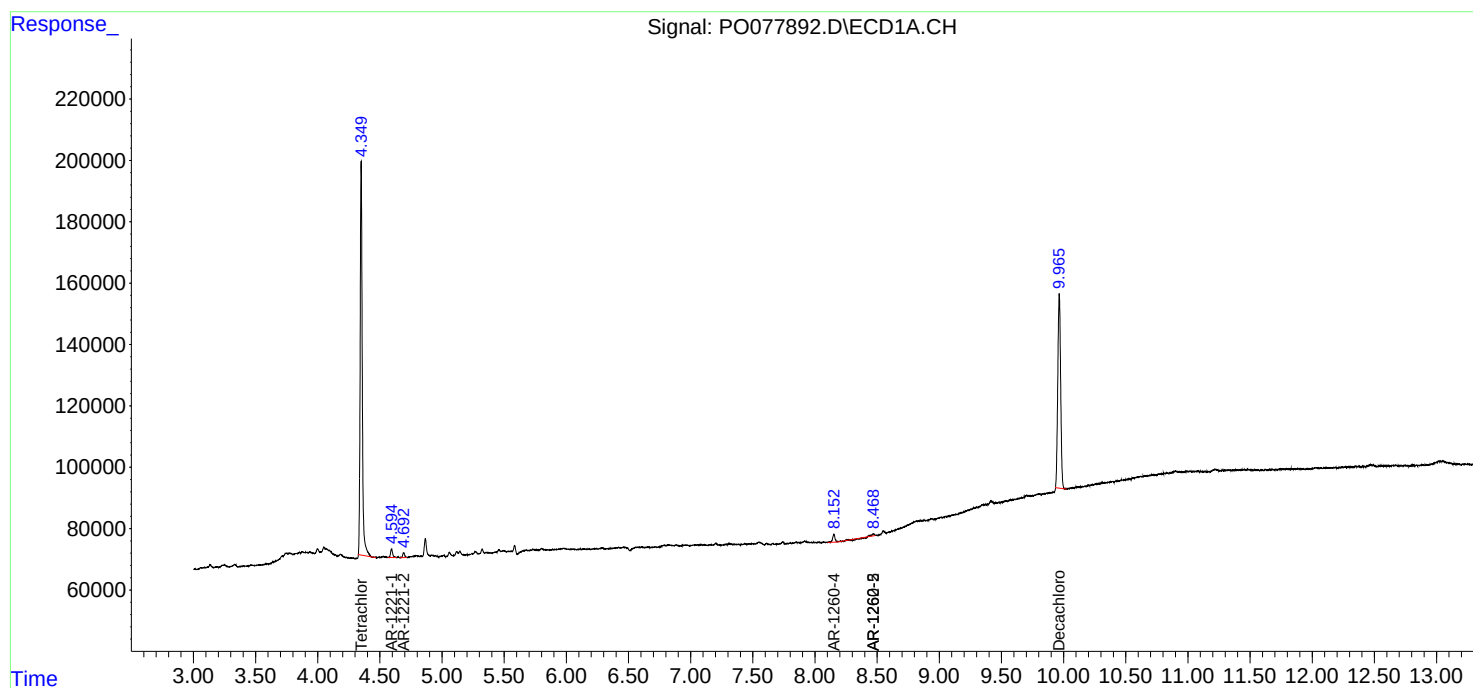


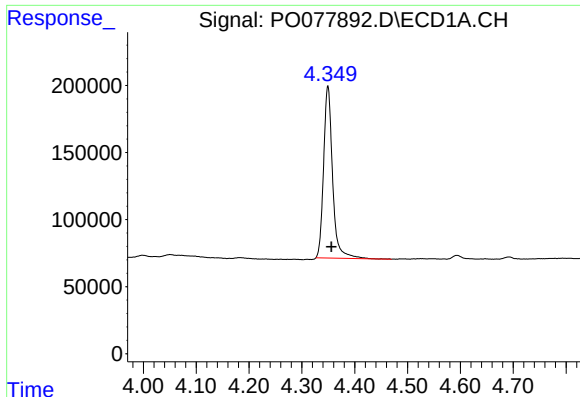

#1 Tetrachloro-m-xylene


R.T.: 4.349 min
Delta R.T.: -0.007 min
Response: 1512989
Conc: 25.77 ng/ml

Instrument :
ECD_O
ClientSampleId :

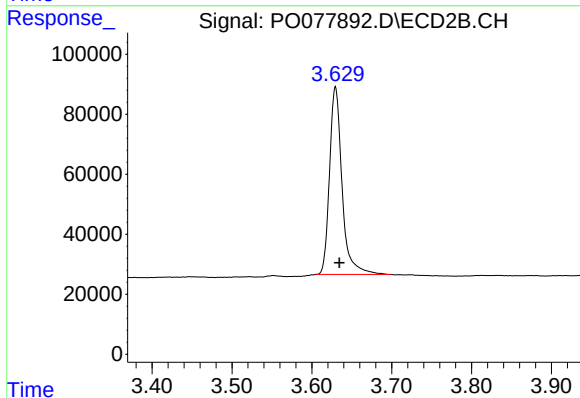


#1 Tetrachloro-m-xylene

R.T.: 3.630 min
Delta R.T.: -0.005 min
Response: 681424
Conc: 26.78 ng/ml

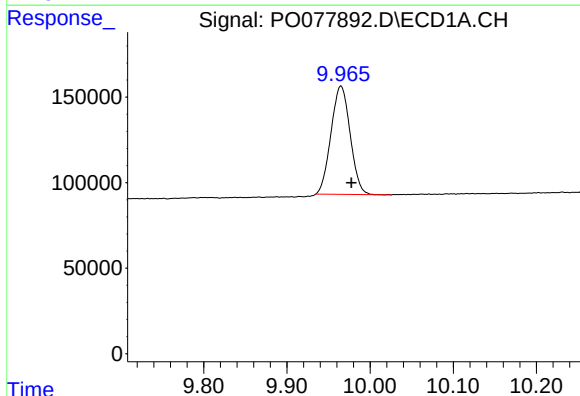


#2 Decachlorobiphenyl

R.T.: 9.965 min
Delta R.T.: -0.013 min
Response: 1014015
Conc: 24.53 ng/ml

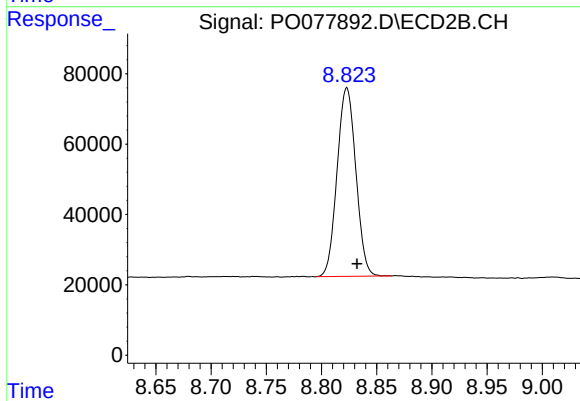

#2 Decachlorobiphenyl


R.T.: 8.823 min
Delta R.T.: -0.009 min
Response: 634215
Conc: 26.39 ng/ml

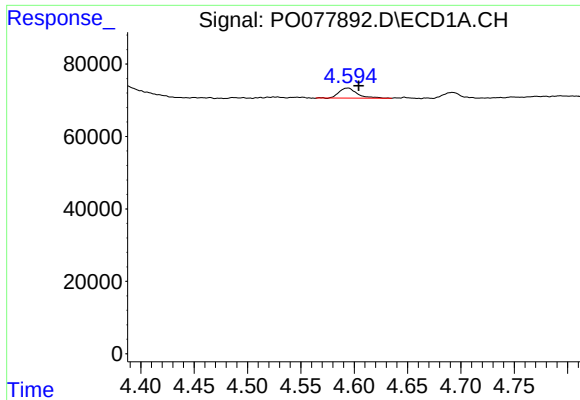

#8 AR-1221-1


R.T.: 4.594 min
Delta R.T.: -0.011 min
Response: 32861
Conc: 47.54 ng/ml

Instrument :
ECD_O
ClientSampleId :

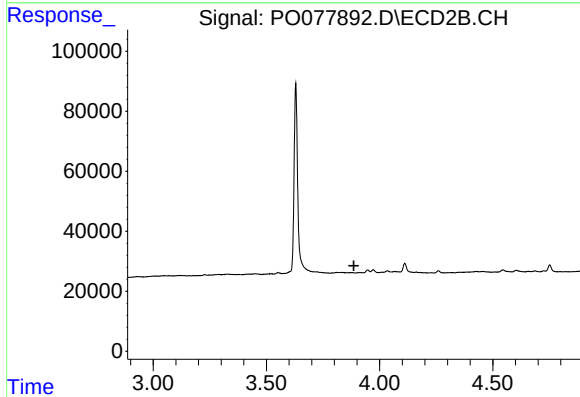


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 3.886 min
Response: 0
Conc: N.D.

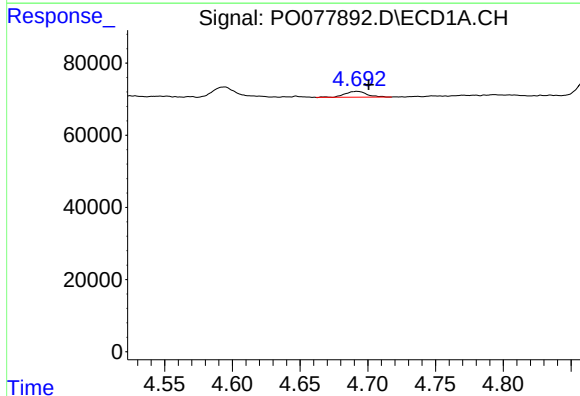


#9 AR-1221-2

R.T.: 4.692 min
Delta R.T.: -0.009 min
Response: 17869
Conc: 35.13 ng/ml

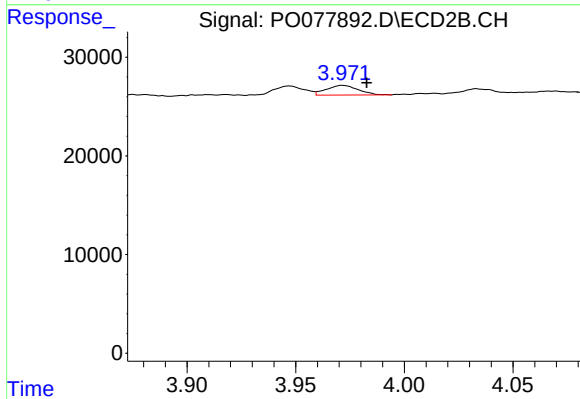

#9 AR-1221-2


R.T.: 3.972 min
Delta R.T.: -0.011 min
Response: 10048
Conc: 42.09 ng/ml

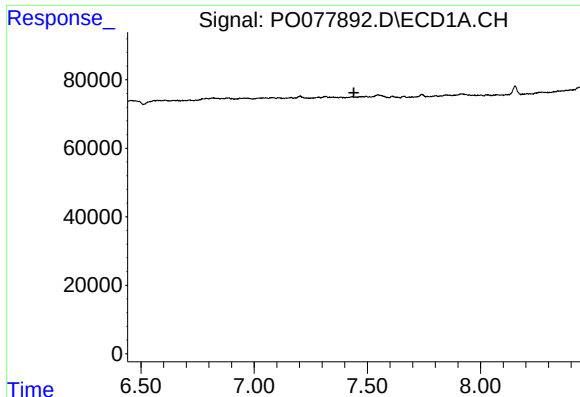

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.441 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

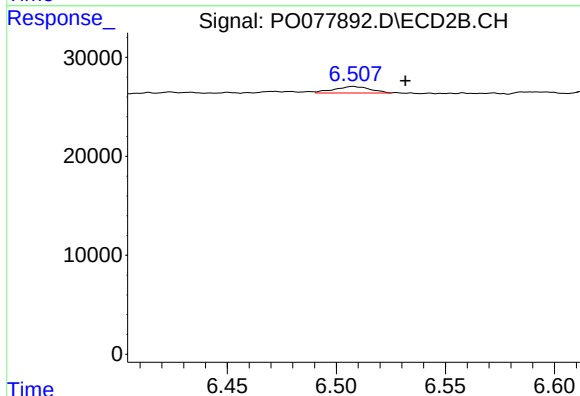


#29 AR-1254-4

R.T.: 6.508 min
Delta R.T.: -0.024 min
Response: 7556
Conc: 6.04 ng/ml

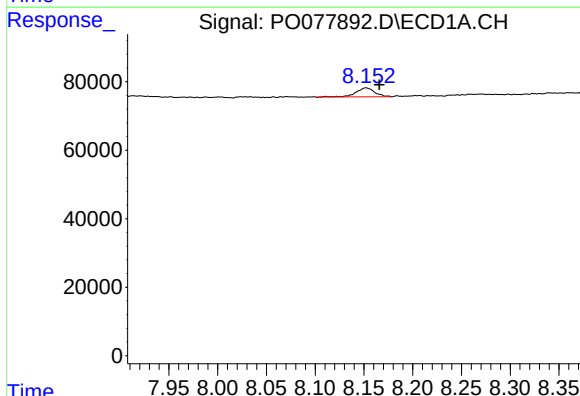


#34 AR-1260-4

R.T.: 8.152 min
Delta R.T.: -0.014 min
Response: 35091
Conc: 16.07 ng/ml

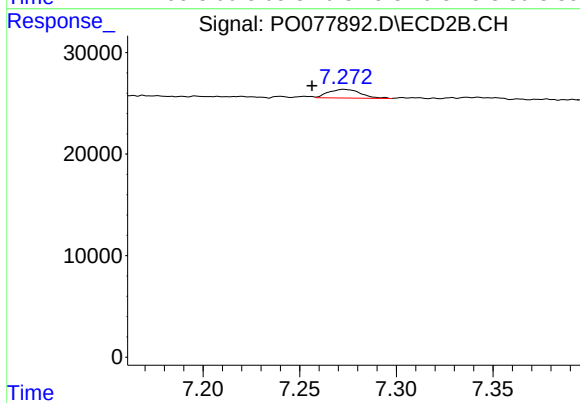

#34 AR-1260-4


R.T.: 7.273 min
Delta R.T.: 0.016 min
Response: 9888
Conc: 8.17 ng/ml

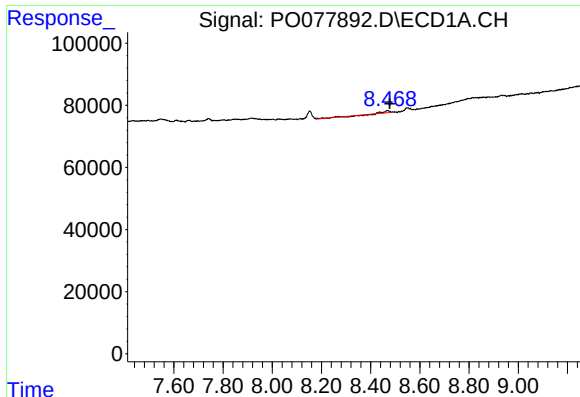

#35 AR-1260-5


R.T.: 8.469 min
Delta R.T.: -0.009 min
Response: 3920
Conc: 0.91 ng/ml

Instrument :
ECD_O
ClientSampleId :

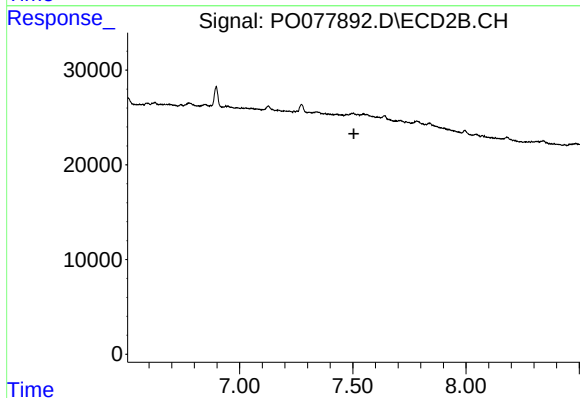


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.504 min
Response: 0
Conc: N.D.

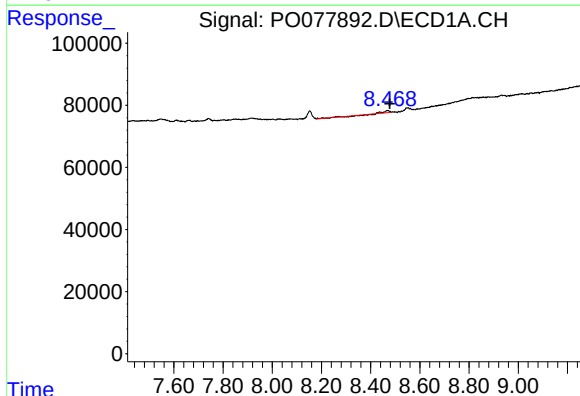


#37 AR-1262-2

R.T.: 8.469 min
Delta R.T.: -0.009 min
Response: 3920
Conc: 0.76 ng/ml

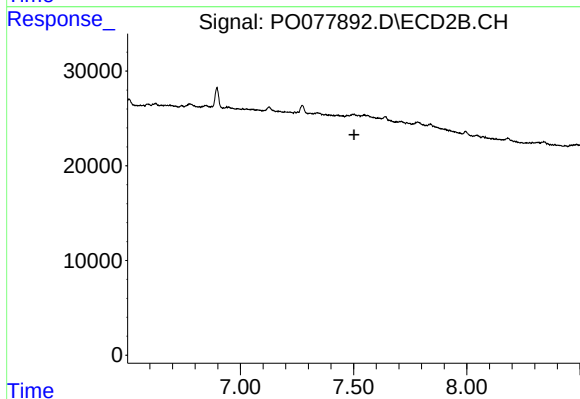

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 7.502 min
Response: 0
Conc: N.D.

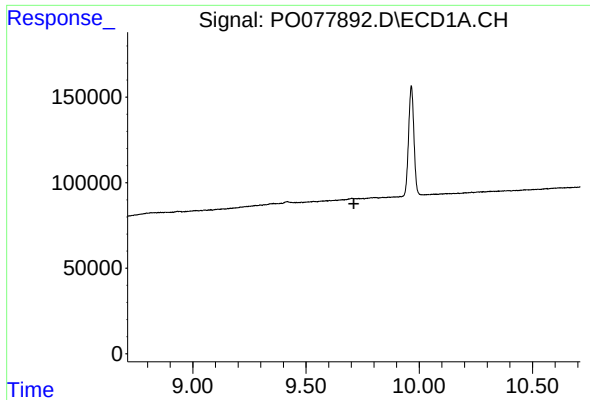

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.711 min
Response: 0
Conc: N.D.

Instrument :
ECD_O
ClientSampleId :

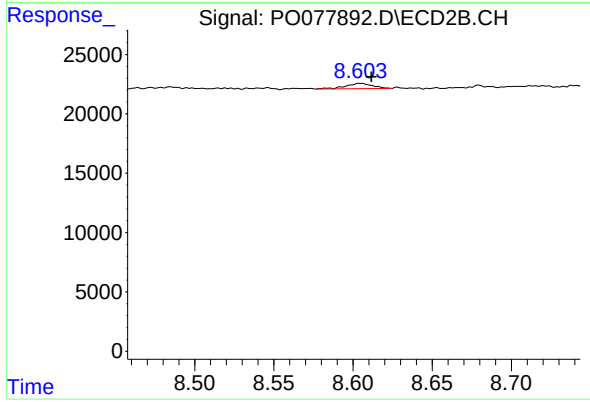

#45 AR-1268-5

R.T.: 8.604 min
Delta R.T.: -0.008 min
Response: 5345
Conc: 0.62 ng/ml